

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG072315\
 Data File : BG018067.D
 Acq On : 23 Jul 2015 16:47
 Operator : TP/UM
 Sample : G3035-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C01H6

Quant Time: Jul 24 01:07:27 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG072315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 23 16:20:02 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.51	152	53561	20.00	ng/ul	0.00
18) Naphthalene-d8	10.29	136	256239	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.18	164	168400	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.93	188	397882	20.00	ng/ul	0.00
78) Chrysene-d12	21.14	240	425907	20.00	ng/ul	0.00
86) Perylene-d12	23.32	264	415497	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.02	96	4258	4.97	ng/uL	0.00
5) Phenol-d5	6.69	99	94563	22.89	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.85	67	53718	26.34	ng/ul	0.00
9) 2-Chlorophenol-d4	7.05	132	90554	24.71	ng/ul	0.00
13) 4-Methylphenol-d8	8.23	113	85817	23.42	ng/ul	0.00
19) Nitrobenzene-d5	8.66	128	49346	24.36	ng/ul	0.00
22) 2-Nitrophenol-d4	9.39	143	54095	25.29	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.92	165	84382	22.67	ng/ul	0.00
29) 4-Chloroaniline-d4	10.44	131	130386	30.11	ng/ul	0.00
44) Dimethylphthalate-d6	13.60	166	313222	26.49	ng/ul	0.00
47) Acenaphthylene-d8	13.87	160	372391	25.63	ng/ul	0.00
52) 4-Nitrophenol-d4	14.40	143	56834	22.85	ng/ul	0.00
58) Fluorene-d10	15.18	176	283430	25.94	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.31	200	41348	16.25	ng/ul	0.00
71) Anthracene-d10	17.03	188	438134	25.42	ng/ul	0.00
79) Pyrene-d10	19.34	212	490646	25.15	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.18	264	432679	21.82	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.65	163	81453	6.85	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG072315\
Data File : BG018067.D
Acq On : 23 Jul 2015 16:47
Operator : TP/UM
Sample : G3035-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C01H6

Quant Time: Jul 24 01:07:27 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG072315.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 23 16:20:02 2015
Response via : Initial Calibration

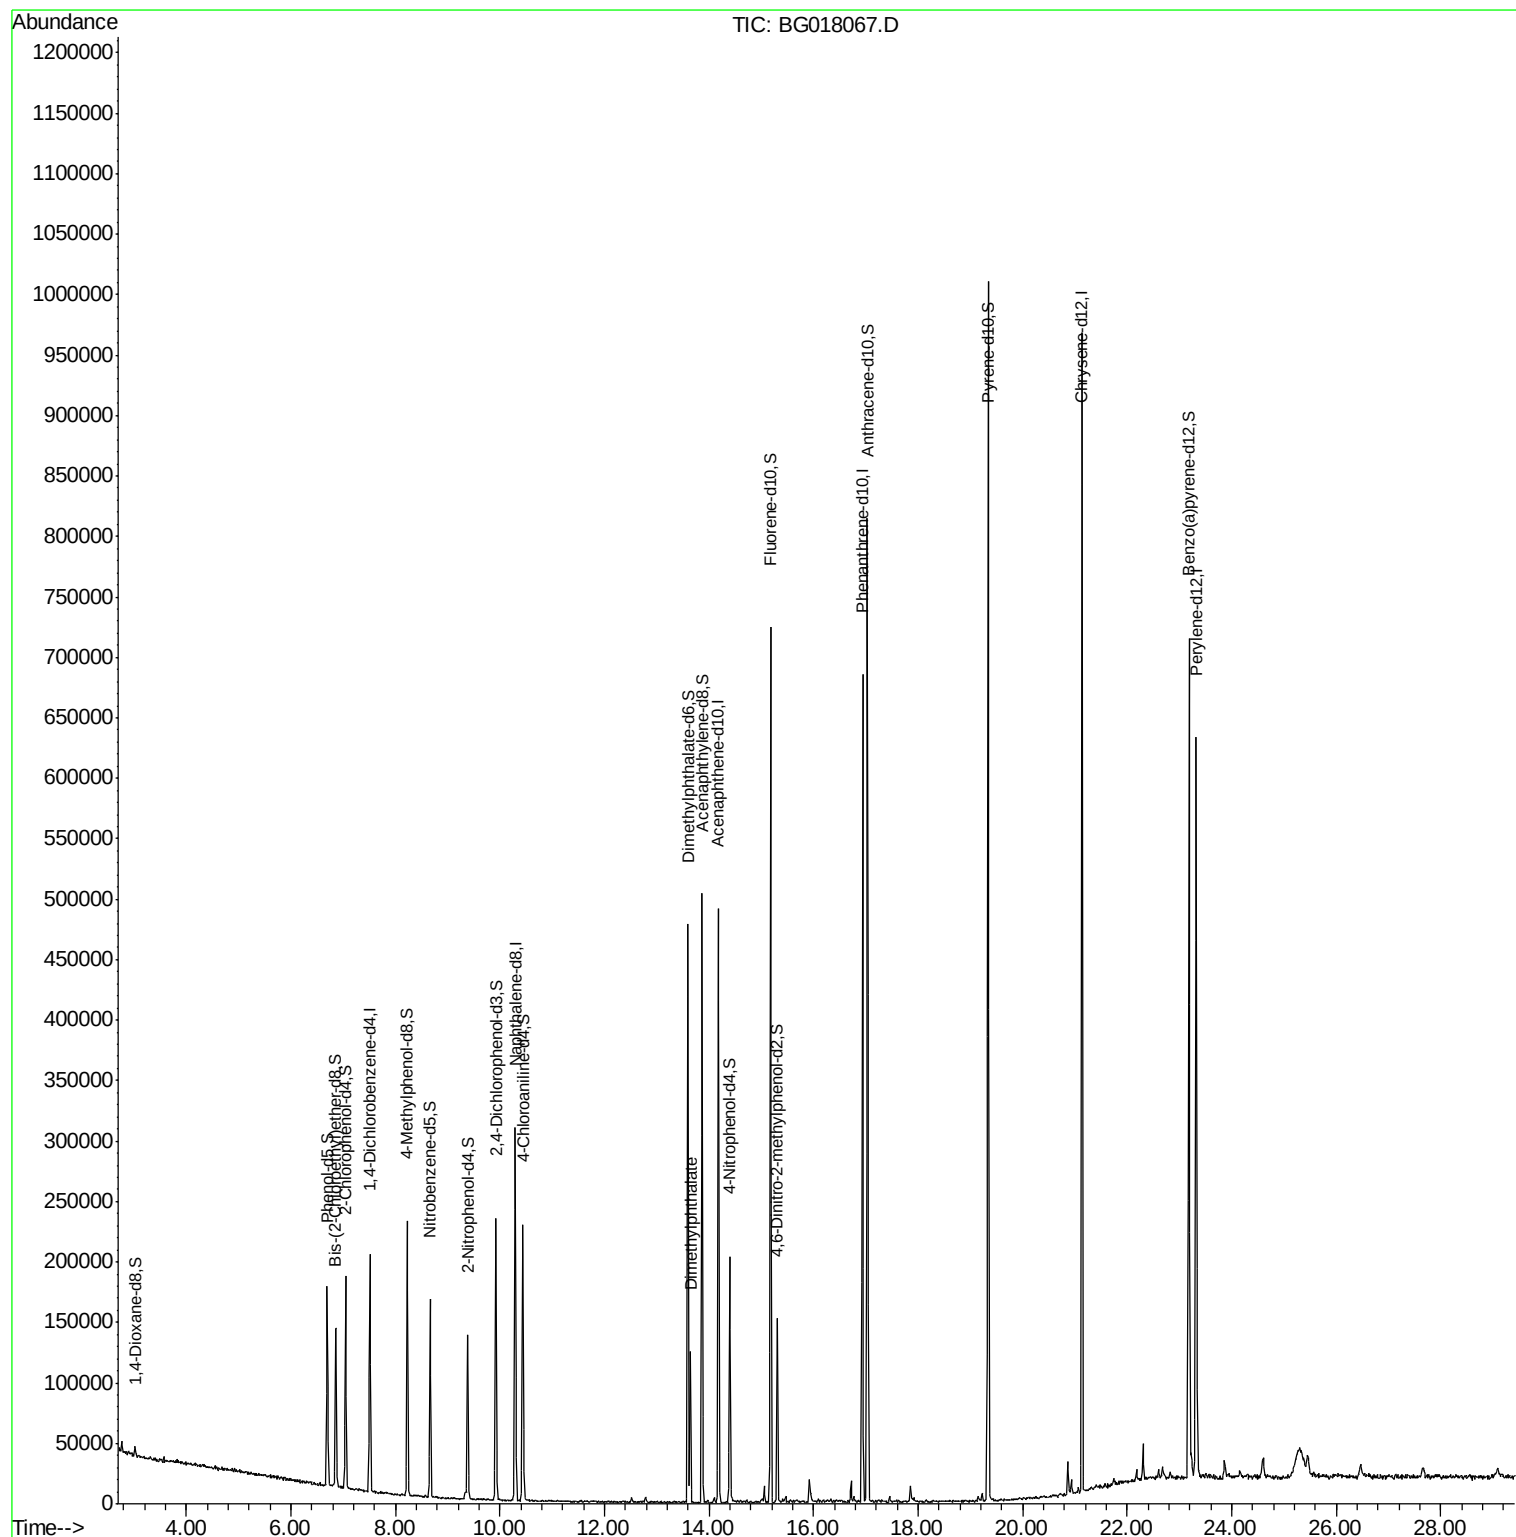

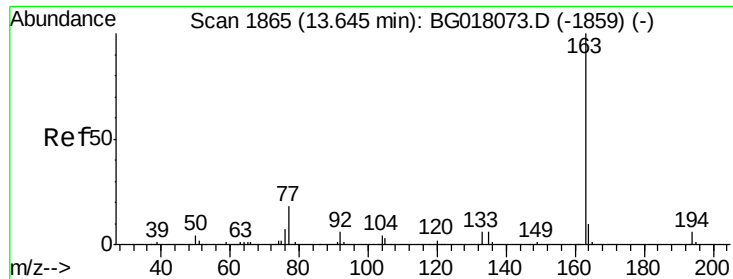

#45

Dimethylphthalate

Concen: 6.85 ng/ul

RT: 13.65 min Scan# 1865

Delta R.T. 0.00 min

Lab File: BG018067.D


Acq: 23 Jul 2015 16:47

Instrument :

BNA_G

ClientSampleId :

C01H6

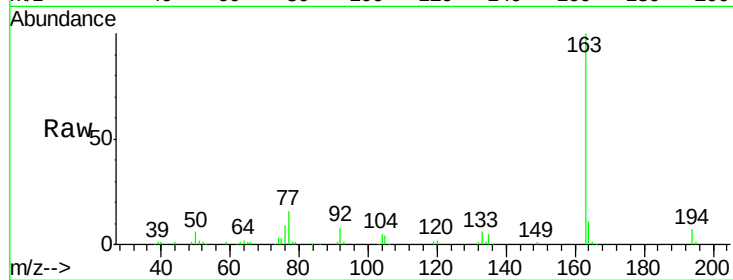

Tgt Ion:163 Resp: 81453

Ion Ratio Lower Upper

163 100

194 6.7 5.4 8.2

164 10.5 8.7 13.1

