

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG072315\
 Data File : BG018069.D
 Acq On : 23 Jul 2015 17:57
 Operator : TP/UM
 Sample : G3035-11
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C02E3

Quant Time: Jul 24 01:07:39 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG072315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 23 16:20:02 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.51	152	43248	20.00	ng/ul	0.00
18) Naphthalene-d8	10.29	136	209207	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.18	164	141324	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.94	188	341612	20.00	ng/ul	0.00
78) Chrysene-d12	21.14	240	360842	20.00	ng/ul	0.00
86) Perylene-d12	23.32	264	349902	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.02	96	1070	1.55	ng/uL	0.00
5) Phenol-d5	6.69	99	22110	6.63	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.85	67	11604	7.05	ng/ul	0.00
9) 2-Chlorophenol-d4	7.04	132	19686	6.65	ng/ul	0.00
13) 4-Methylphenol-d8	8.23	113	20379	6.89	ng/ul	0.00
19) Nitrobenzene-d5	8.66	128	11799	7.13	ng/ul	0.00
22) 2-Nitrophenol-d4	9.38	143	13610	7.79	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.92	165	21134	6.95	ng/ul	0.00
29) 4-Chloroaniline-d4	10.44	131	28766	8.14	ng/ul	0.00
44) Dimethylphthalate-d6	13.60	166	175145	17.65	ng/ul	0.00
47) Acenaphthylene-d8	13.87	160	130655	10.72	ng/ul	0.00
52) 4-Nitrophenol-d4	14.40	143	47484	22.75	ng/ul	0.00
58) Fluorene-d10	15.18	176	149214	16.27	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.31	200	34438	15.77	ng/ul	0.00
71) Anthracene-d10	17.03	188	319350	21.58	ng/ul	0.00
79) Pyrene-d10	19.34	212	439864	26.61	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.18	264	422619	25.31	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.65	163	57210	5.73	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG072315\
Data File : BG018069.D
Acq On : 23 Jul 2015 17:57
Operator : TP/UM
Sample : G3035-11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C02E3

Quant Time: Jul 24 01:07:39 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG072315.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 23 16:20:02 2015
Response via : Initial Calibration

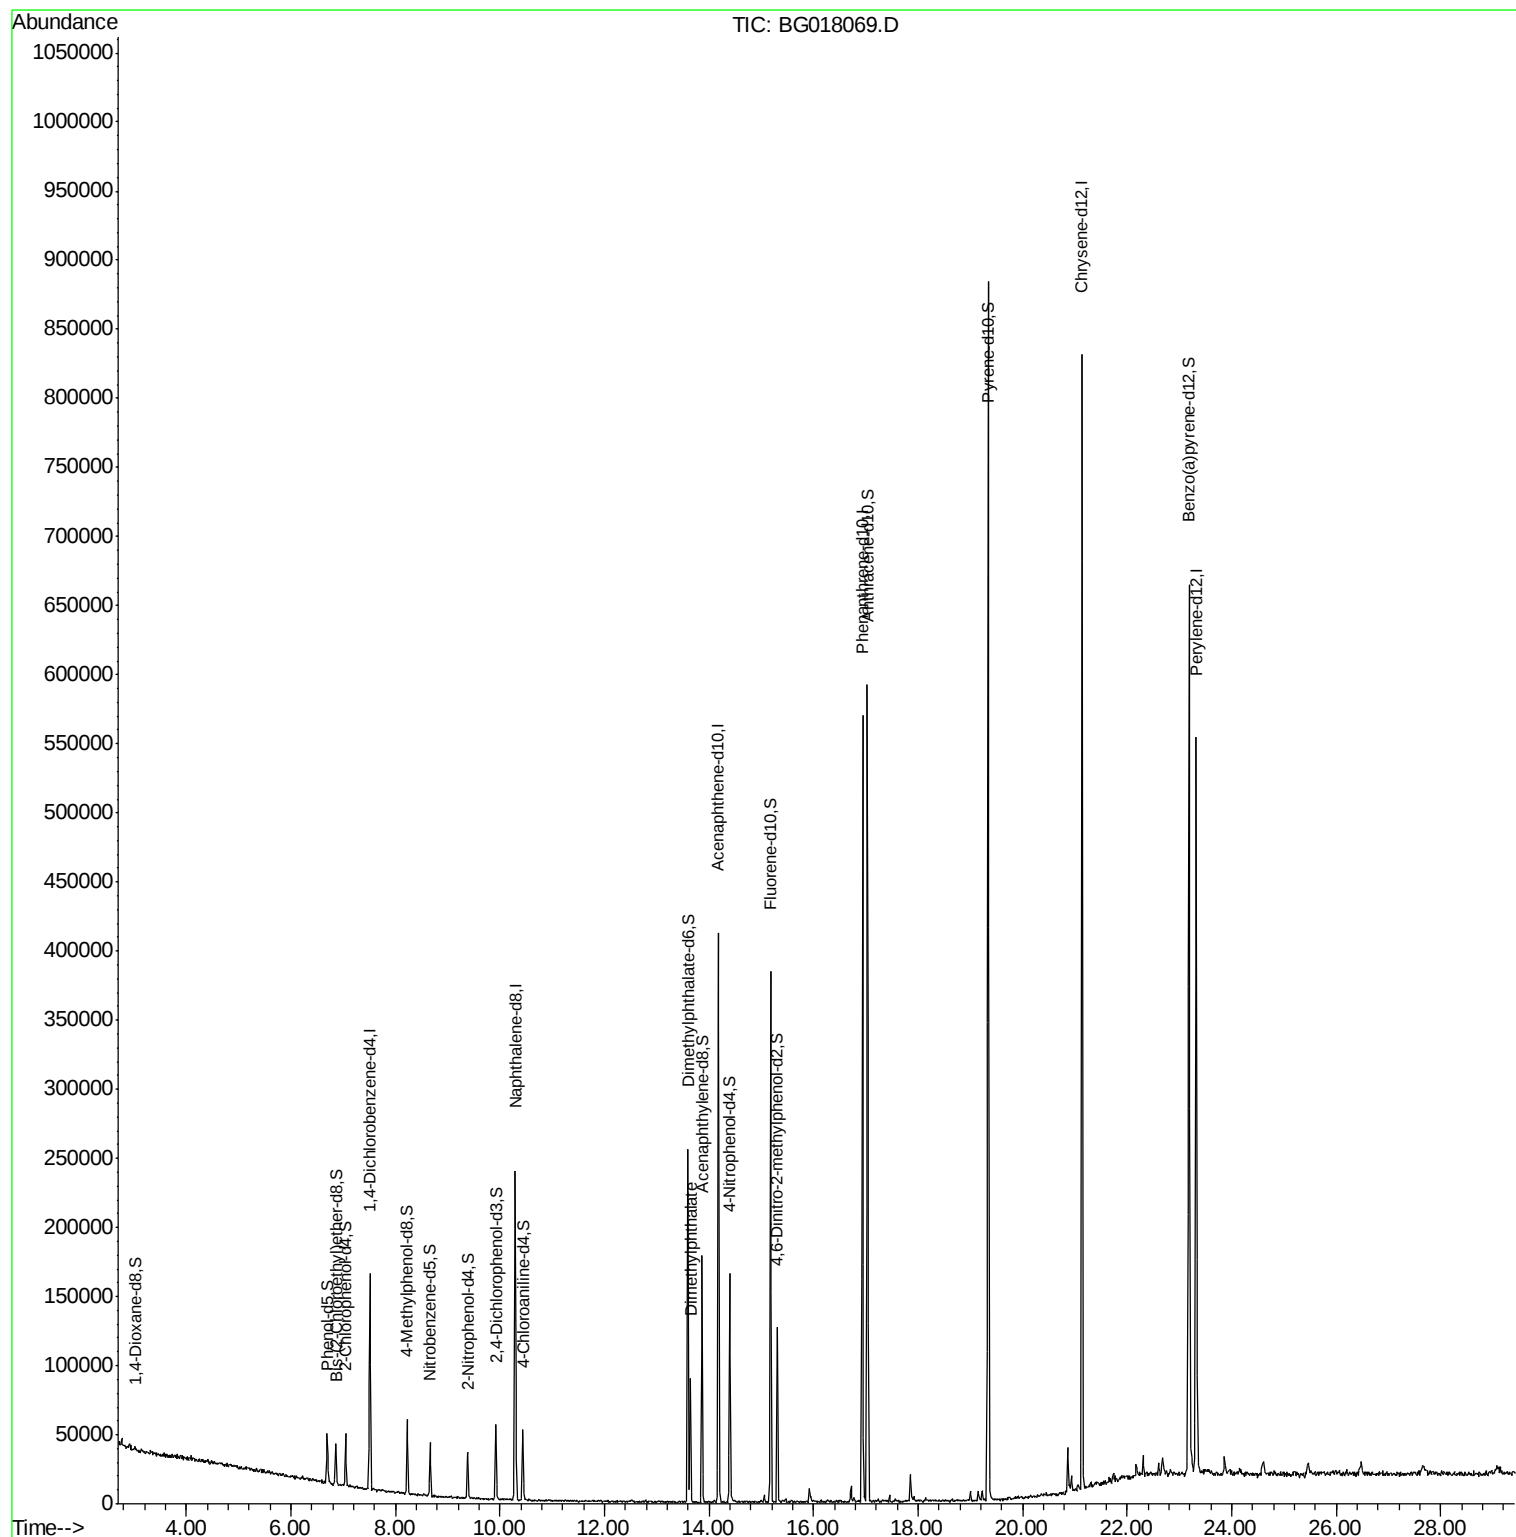

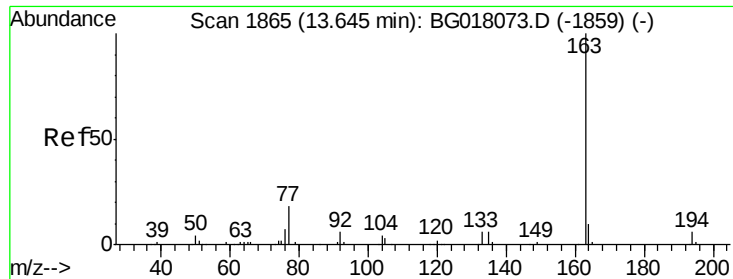

#45

Dimethylphthalate

Concen: 5.73 ng/ul

RT: 13.65 min Scan# 1865

Delta R.T. 0.00 min

Lab File: BG018069.D


Acq: 23 Jul 2015 17:57

Instrument :

BNA_G

ClientSampleId :

C02E3

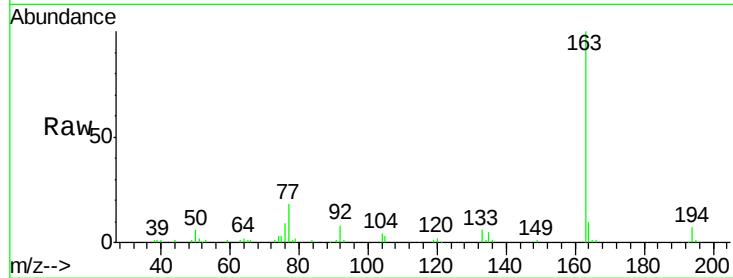

Tgt Ion:	163	Resp:	57210
Ion	Ratio	Lower	Upper
163	100		
194	6.8	5.4	8.2
164	9.6	8.7	13.1

