

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG072315\
 Data File : BG018072.D
 Acq On : 23 Jul 2015 19:43
 Operator : TP/UM
 Sample : G3035-21
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C02E0

Quant Time: Jul 24 01:23:58 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG072315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 23 16:20:02 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.51	152	42855	20.00	ng/ul	0.00
18) Naphthalene-d8	10.29	136	205135	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.18	164	138427	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.93	188	336099	20.00	ng/ul	0.00
78) Chrysene-d12	21.14	240	349320	20.00	ng/ul	0.00
86) Perylene-d12	23.32	264	340590	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.02	96	4250	6.20	ng/uL	0.00
5) Phenol-d5	6.70	99	102894	31.12	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.85	67	55754	34.16	ng/ul	0.00
9) 2-Chlorophenol-d4	7.05	132	94042	32.08	ng/ul	0.00
13) 4-Methylphenol-d8	8.23	113	94675	32.29	ng/ul	0.00
19) Nitrobenzene-d5	8.66	128	54775	33.78	ng/ul	0.00
22) 2-Nitrophenol-d4	9.38	143	57215	33.42	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.92	165	94360	31.66	ng/ul	0.00
29) 4-Chloroaniline-d4	10.44	131	132663	38.26	ng/ul	0.00
44) Dimethylphthalate-d6	13.60	166	344210	35.42	ng/ul	0.00
47) Acenaphthylene-d8	13.87	160	419965	35.17	ng/ul	0.00
52) 4-Nitrophenol-d4	14.40	143	71799	35.12	ng/ul	0.00
58) Fluorene-d10	15.18	176	321684	35.81	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.30	200	55402	25.78	ng/ul	0.00
71) Anthracene-d10	17.03	188	507620	34.87	ng/ul	0.00
79) Pyrene-d10	19.34	212	554666	34.66	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	492472	30.30	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.65	163	103529	10.59	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG072315\
Data File : BG018072.D
Acq On : 23 Jul 2015 19:43
Operator : TP/UM
Sample : G3035-21
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C02E0

Quant Time: Jul 24 01:23:58 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG072315.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 23 16:20:02 2015
Response via : Initial Calibration

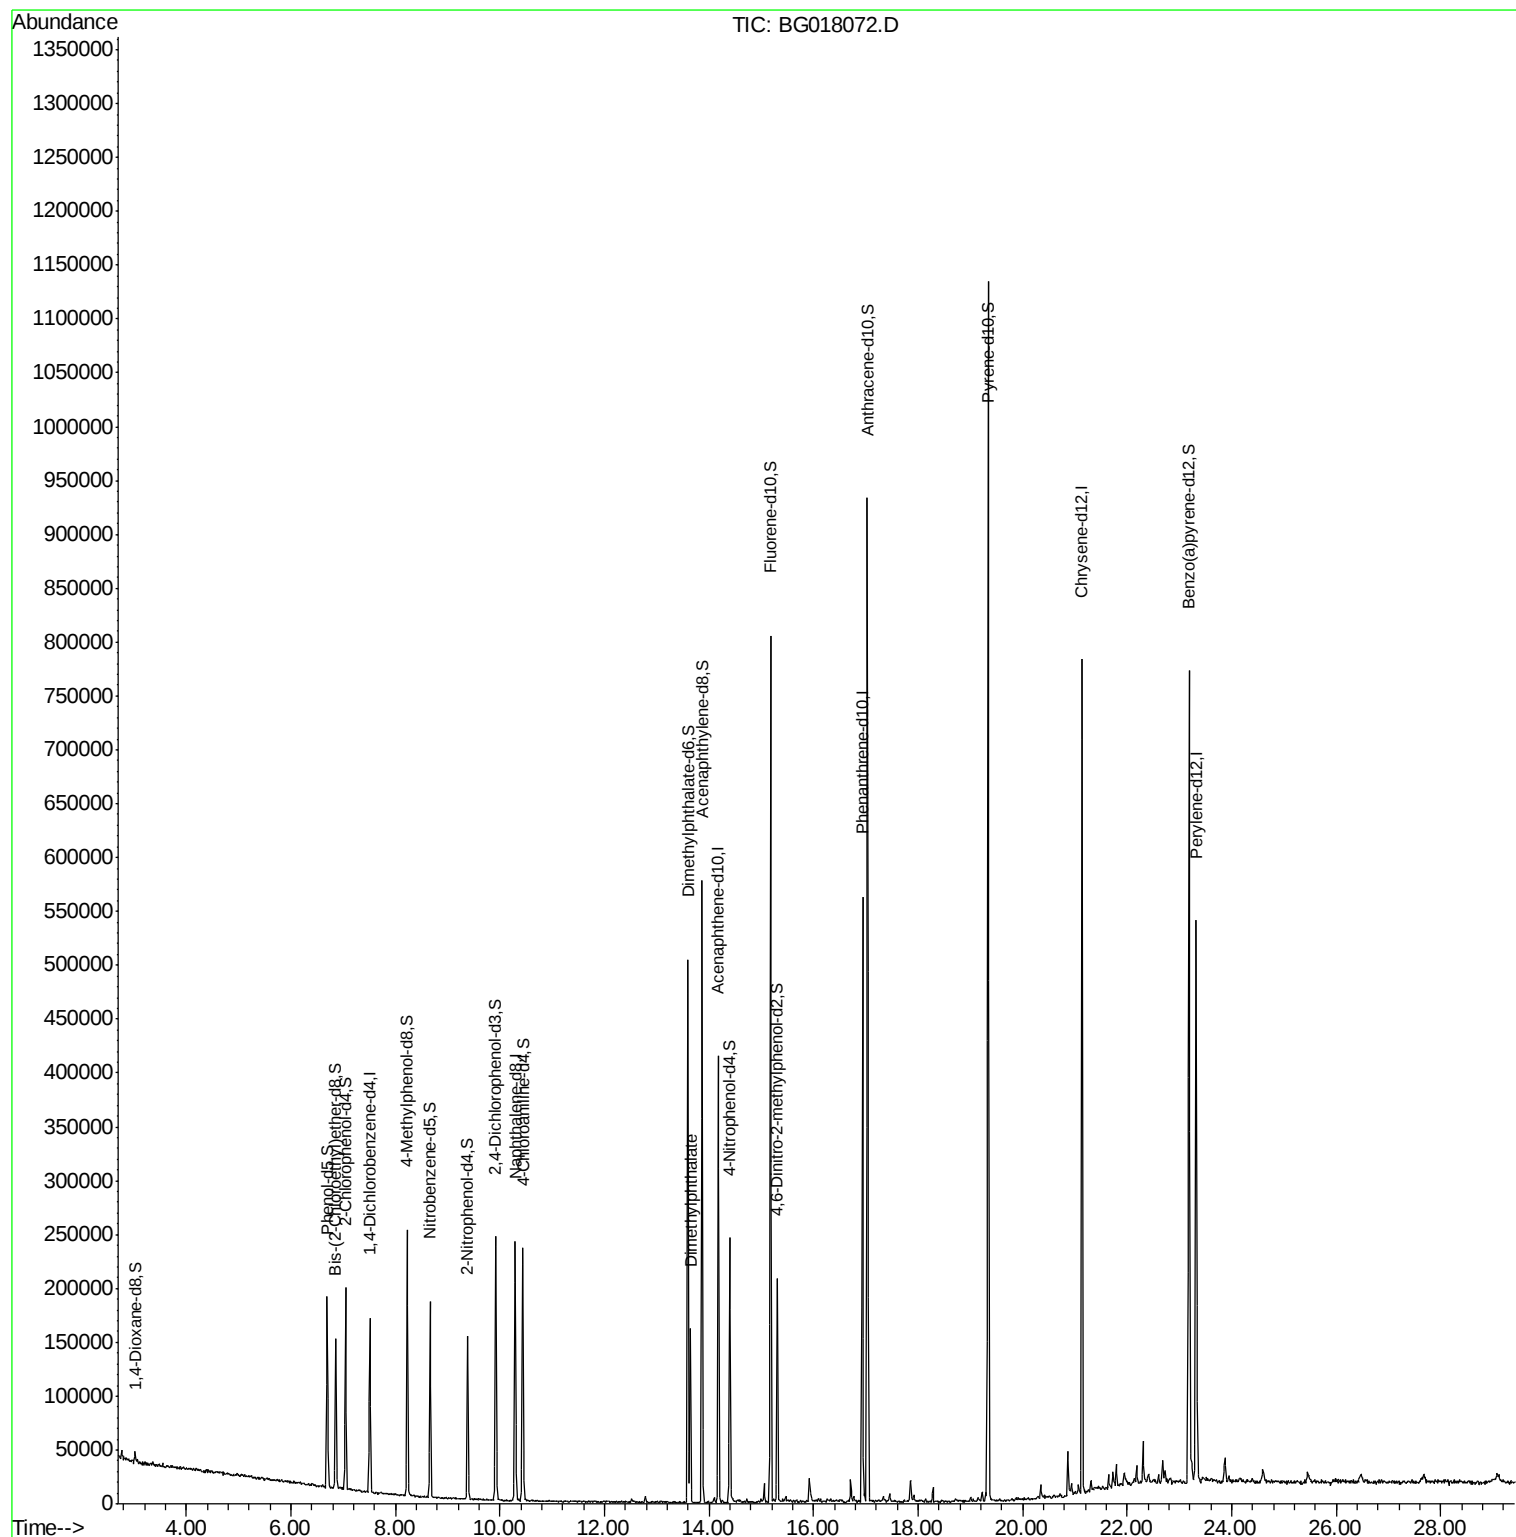

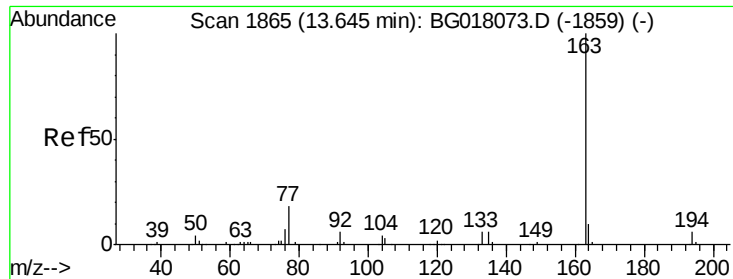

#45

Dimethylphthalate

Concen: 10.59 ng/ul

RT: 13.65 min Scan# 1865

Delta R.T. 0.00 min

Lab File: BG018072.D


Acq: 23 Jul 2015 19:43

Instrument :

BNA_G

ClientSampleId :

C02E0

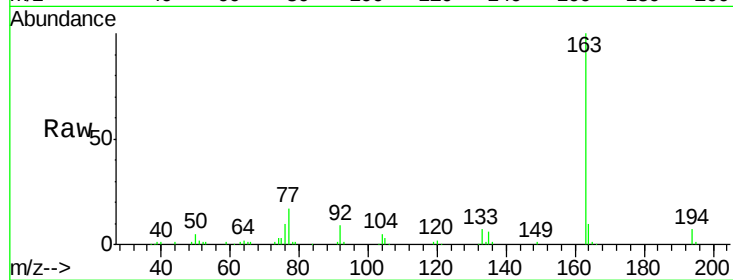

Tgt Ion:	163	Resp:	103529
Ion	Ratio	Lower	Upper
163	100		
194	7.2	5.4	8.2
164	9.5	8.7	13.1

