

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG072315\
 Data File : BG018076.D
 Acq On : 23 Jul 2015 22:03
 Operator : TP/UM
 Sample : G3035-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C01K0

Manual Integrations
 APPROVED

apatel
 7/24/2015 4:50:53 PM

Quant Time: Jul 24 01:55:36 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG072315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 24 01:33:04 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.51	152	45228	20.00	ng/ul	0.00
18) Naphthalene-d8	10.29	136	226099	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.18	164	153083	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.93	188	341743	20.00	ng/ul	0.00
78) Chrysene-d12	21.14	240	349840	20.00	ng/ul	0.00
86) Perylene-d12	23.32	264	347731	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.02	96	962	1.33	ng/uL	0.00
5) Phenol-d5	6.70	99	28503	8.17	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.86	67	16457	9.55	ng/ul	0.00
9) 2-Chlorophenol-d4	7.04	132	27833	9.00	ng/ul	0.00
13) 4-Methylphenol-d8	8.22	113	13293	4.30	ng/ul	0.00
19) Nitrobenzene-d5	8.66	128	16287	9.11	ng/ul	0.00
22) 2-Nitrophenol-d4	9.38	143	17563	9.31	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.92	165	27809	8.47	ng/ul	0.00
29) 4-Chloroaniline-d4	10.43	131	20083	5.26	ng/ul	0.00
44) Dimethylphthalate-d6	13.59	166	105852	9.85	ng/ul	0.00
47) Acenaphthylene-d8	13.86	160	133831	10.13	ng/ul	0.00
52) 4-Nitrophenol-d4	14.39	143	16923	7.48	ng/ul	0.00
58) Fluorene-d10	15.17	176	101293	10.20	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.30	200	13470	6.16	ng/ul	0.00
71) Anthracene-d10	17.03	188	144992	9.80	ng/ul	0.00
79) Pyrene-d10	19.34	212	153038	9.55	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.18	264	139682	8.42	ng/ul	0.00

Target Compounds

						Qvalue
14) Acetophenone	8.34	105	21758	4.99	ng/ul	99
45) Dimethylphthalate	13.64	163	32557	3.01	ng/ul	98
50) Acenaphthene	14.25	153	19529	2.15	ng/ul	97
54) Dibenzofuran	14.58	168	15980	1.24	ng/ul	94
59) Fluorene	15.23	166	20039	1.80	ng/ul#	93
70) Phenanthrene	16.98	178	365741	21.30	ng/ul	99
72) Anthracene	17.07	178	85885	4.93	ng/ul	98
75) Carbazole	17.34	167	34471	2.28	ng/ul	98
77) Fluoranthene	19.01	202	609779	33.34	ng/ul	99
80) Pyrene	19.37	202	631679	31.53	ng/ul	99
83) Benzo(a)anthracene	21.12	228	346439	18.72	ng/ul	100
85) Chrysene	21.17	228	348825	20.02	ng/ul	98
88) Benzo(b)fluoranthene	22.67	252	443365	23.27	ng/ul	99
89) Benzo(k)fluoranthene	22.71	252	126501m	6.86	ng/ul	
91) Benzo(a)pyrene	23.23	252	308366	16.71	ng/ul	99
92) Indeno(1,2,3-cd)pyrene	25.53	276	189114	8.88	ng/ul	94
93) Dibenzo(a,h)anthracene	25.53	278	53857	2.96	ng/ul#	79
94) Benzo(g,h,i)perylene	26.20	276	132860	7.55	ng/ul	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG072315\
Data File : BG018076.D
Acq On : 23 Jul 2015 22:03
Operator : TP/UM
Sample : G3035-04
Misc :
ALS Vial : 17 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
C01K0

Manual Integrations
APPROVED

apatel
7/24/2015 4:50:53 PM

Quant Time: Jul 24 01:55:36 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG072315.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 24 01:33:04 2015
Response via : Initial Calibration

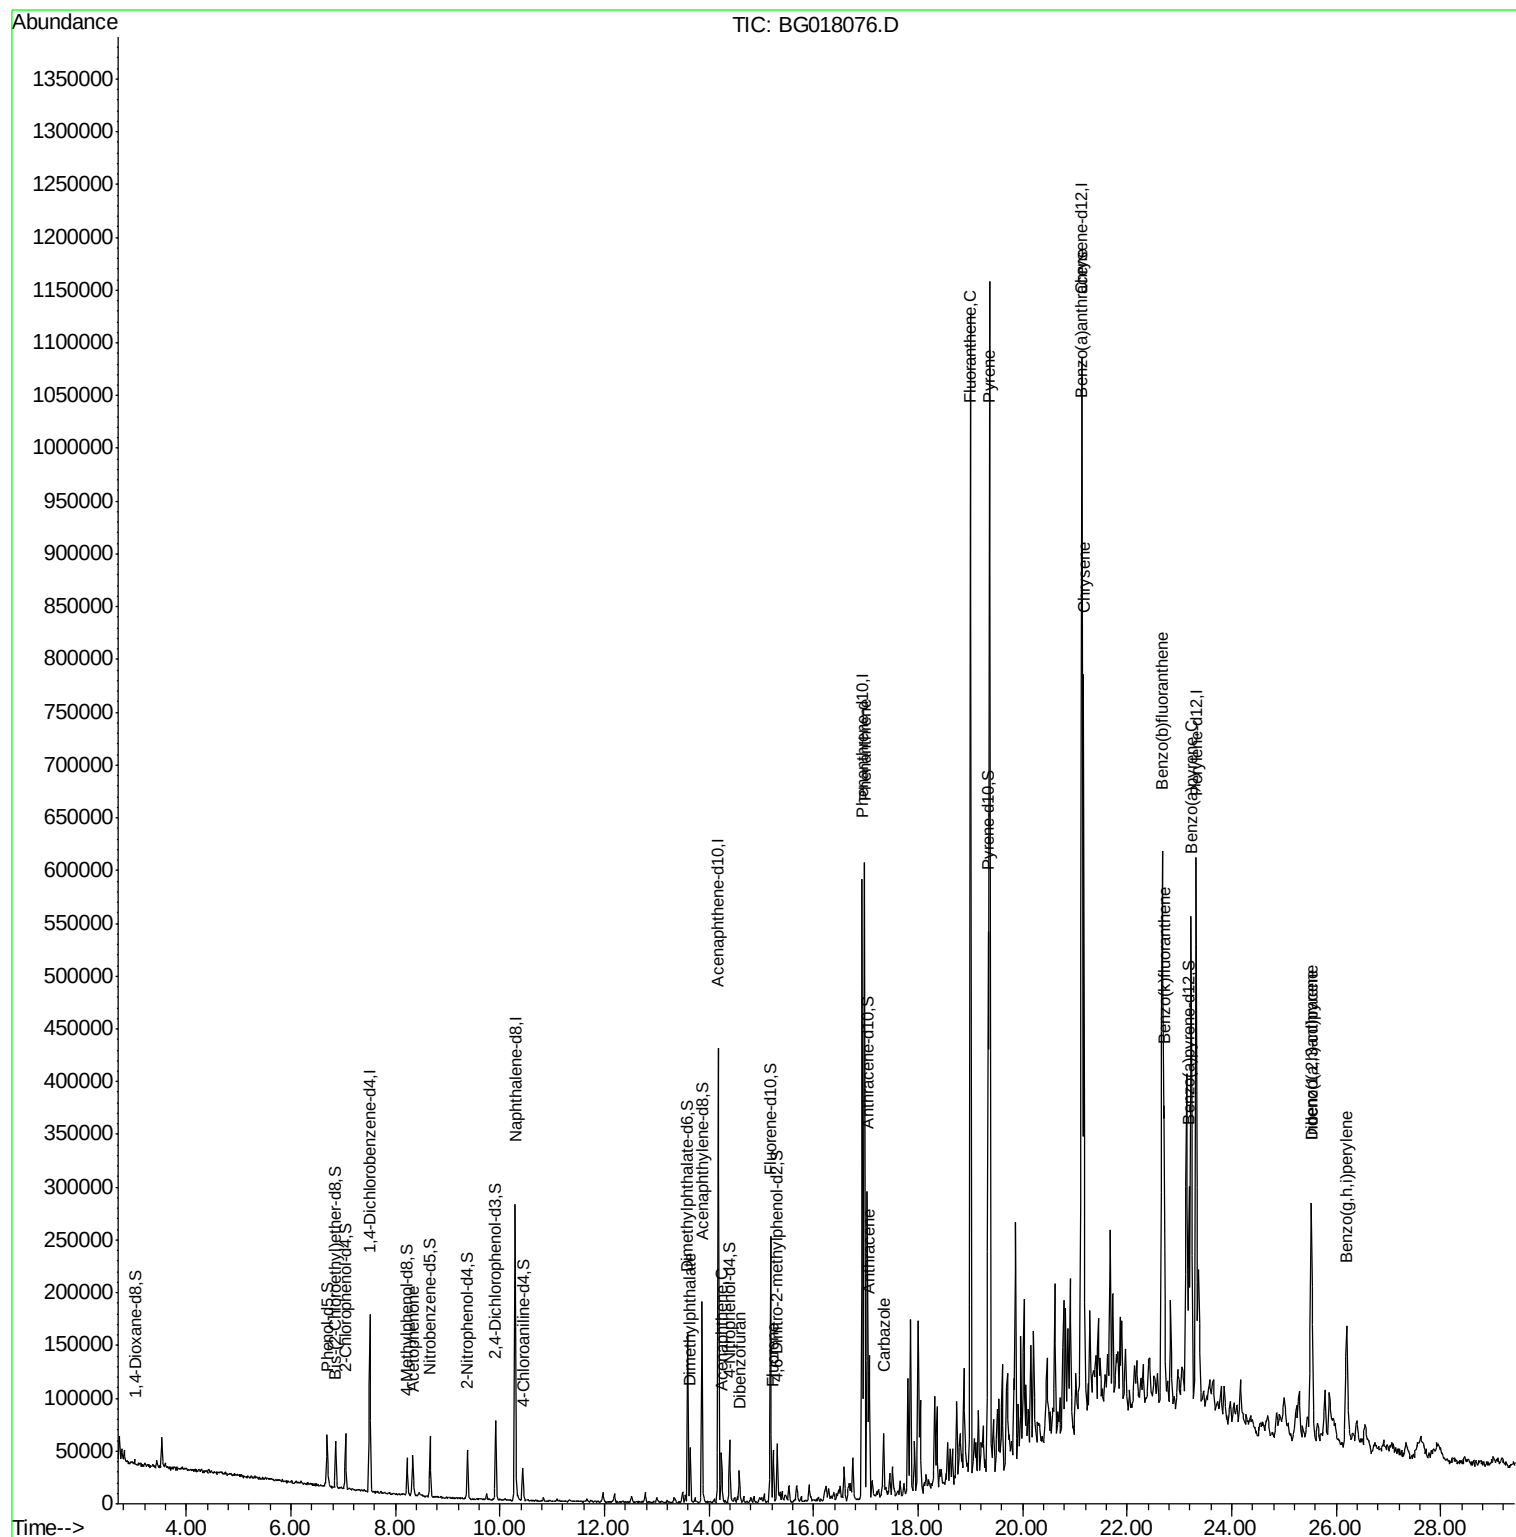

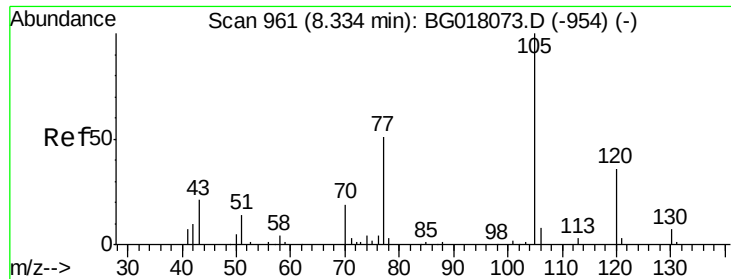

#14

Acetophenone

Concen: 4.99 ng/ul

RT: 8.34 min Scan# 961

Delta R.T. 0.00 min

Lab File: BG018076.D


Acq: 23 Jul 2015 22:03

Instrument :

BNA_G

ClientSampleId :




C01K0

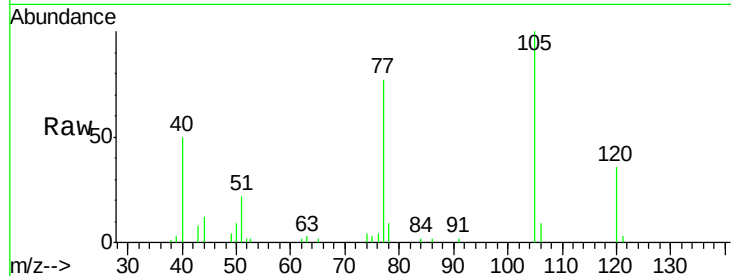

Tgt Ion:	105	Resp:	21758
Ion Ratio	Lower	Upper	
105	100		
77	76.6	61.7	92.5
51	22.2	18.1	27.1

Manual Integrations
APPROVED

apatel
7/24/2015 4:50:53 PM

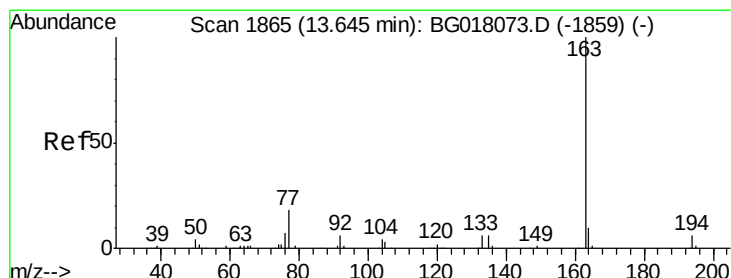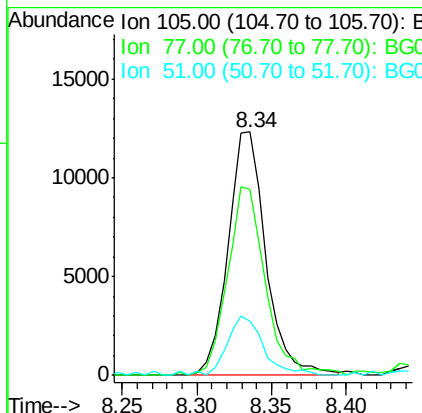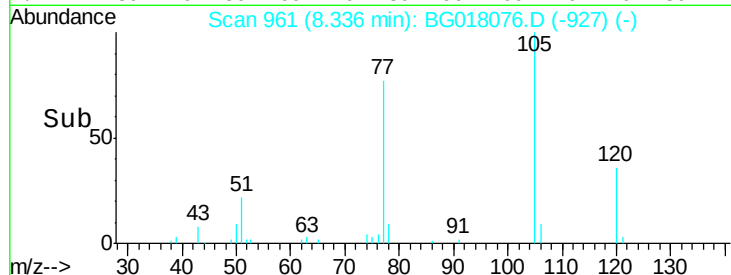

#45

Dimethylphthalate

Concen: 3.01 ng/ul




RT: 13.64 min Scan# 1864


Delta R.T. -0.00 min

Lab File: BG018076.D

Acq: 23 Jul 2015 22:03

Tgt Ion:	163	Resp:	32557
Ion Ratio	Lower	Upper	
163	100		
194	6.3	5.4	8.2
164	9.8	8.7	13.1

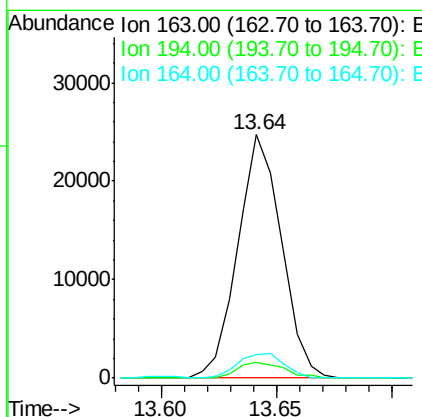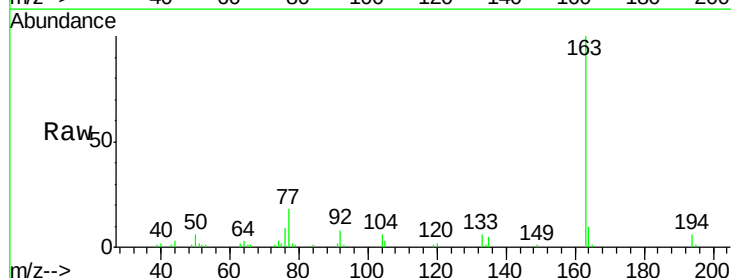

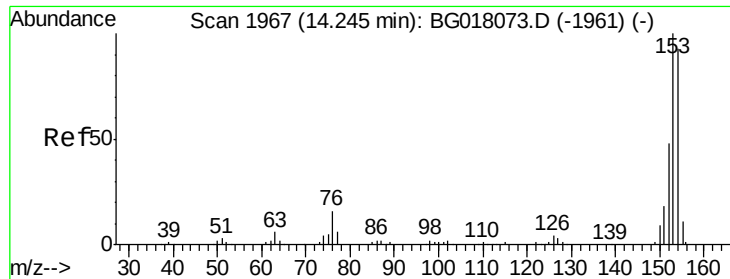

#50

Acenaphthene

Concen: 2.15 ng/ul

RT: 14.25 min Scan# 1967

Delta R.T. 0.00 min

Lab File: BG018076.D


Acq: 23 Jul 2015 22:03

Instrument :

BNA_G

ClientSampleId :

C01K0

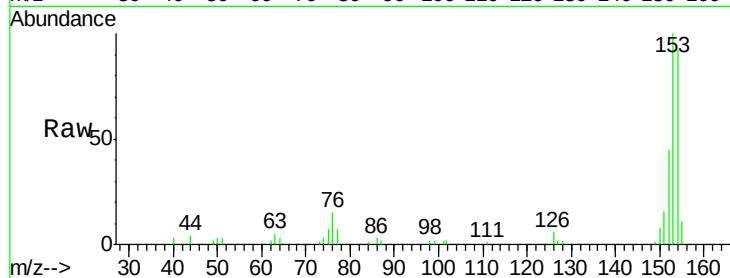

Tgt Ion:153 Resp: 19529

Ion Ratio Lower Upper


153 100

152 44.6 38.9 58.3

154 92.2 72.6 108.8

Manual Integrations
APPROVED



apatel
7/24/2015 4:50:53 PM

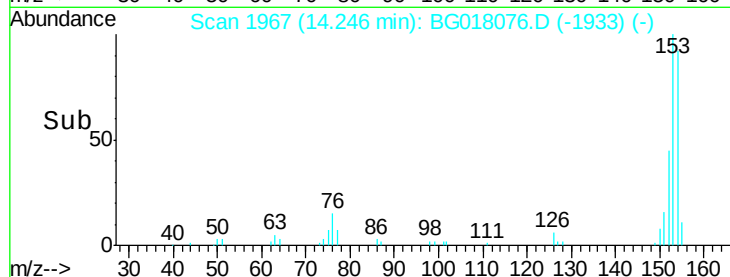

Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

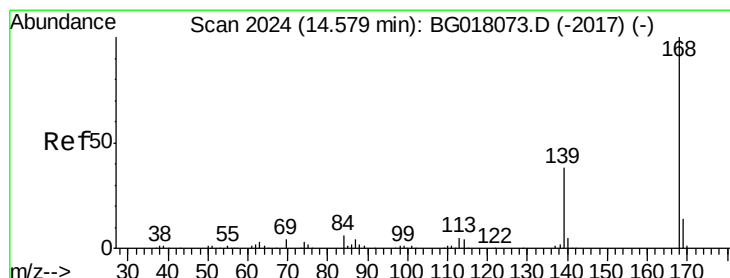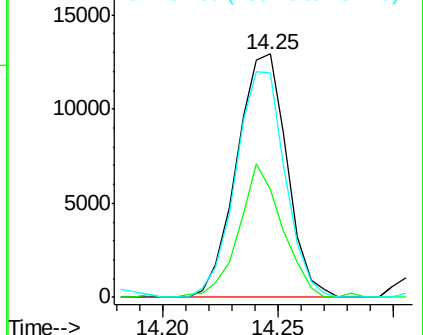

#54

Dibenzofuran

Concen: 1.24 ng/ul

RT: 14.58 min Scan# 2024

Delta R.T. 0.00 min

Lab File: BG018076.D


Acq: 23 Jul 2015 22:03

Tgt Ion:168 Resp: 15980

Ion Ratio Lower Upper



168 100


139 41.7 30.6 46.0

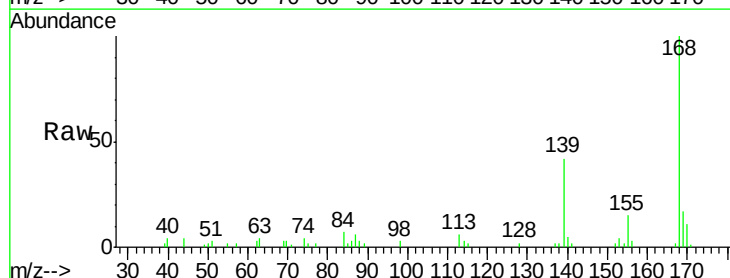

Abundance Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E

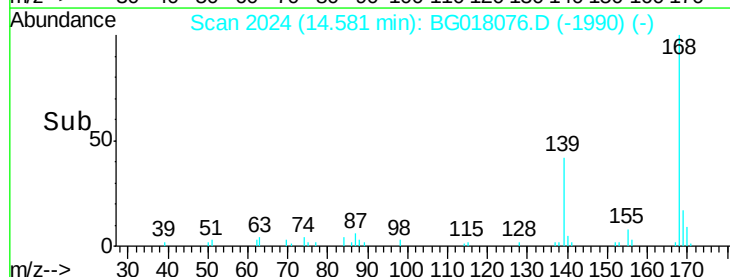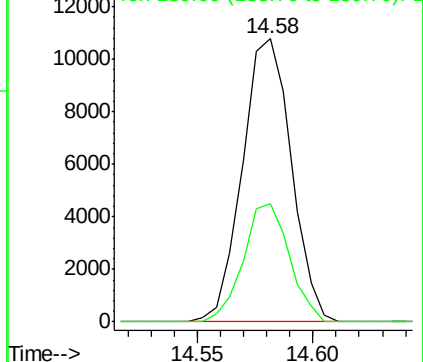

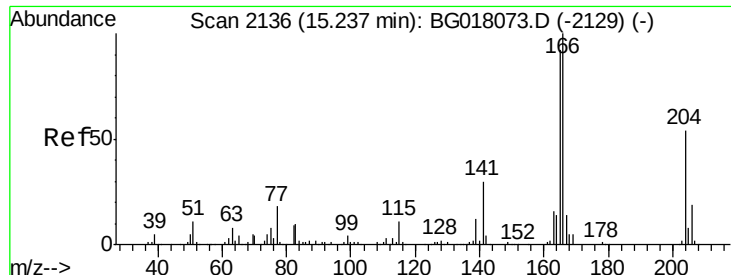





#59
 Fluorene
 Concen: 1.80 ng/ul
 RT: 15.23 min Scan# 2135
 Delta R.T. -0.00 min
 Lab File: BG018076.D
 Acq: 23 Jul 2015 22:03

Instrument :
 BNA_G
 ClientSampleId :
 C01K0

Tgt Ion	Ratio	Resp	Lower	Upper
166	100	20039		
165	98.8	73.6	110.4	
167	16.7	10.8	16.2	




Manual Integrations
 APPROVED


apatel
 7/24/2015 4:50:53 PM

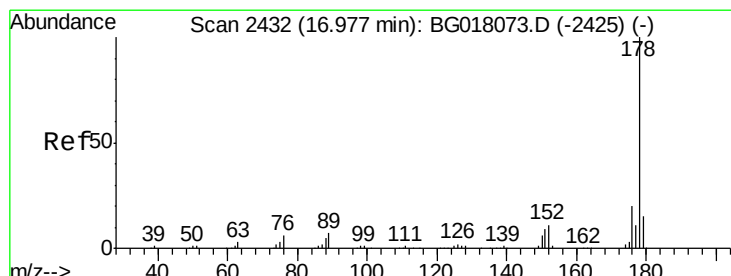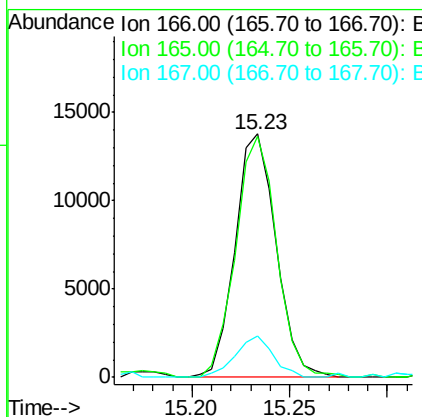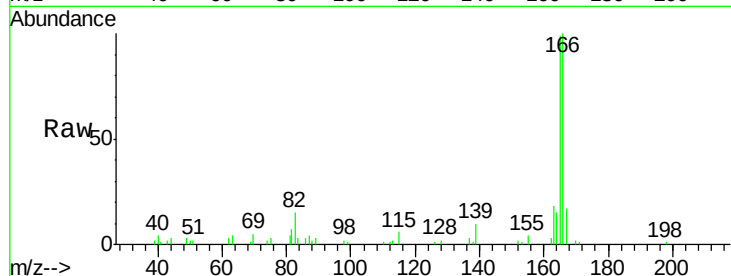

#70
 Phenanthrene
 Concen: 21.30 ng/ul
 RT: 16.98 min Scan# 2432
 Delta R.T. 0.00 min
 Lab File: BG018076.D
 Acq: 23 Jul 2015 22:03

Tgt Ion	Ratio	Resp	Lower	Upper
178	100	365741		
179	15.6	13.0	19.6	
176	19.5	15.8	23.8	

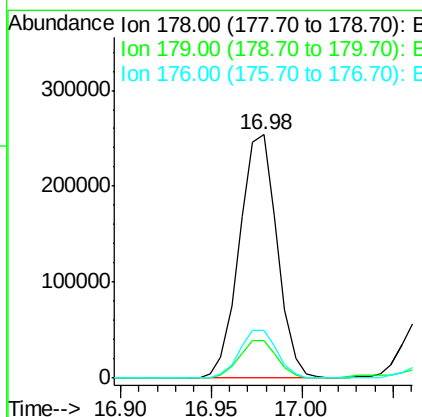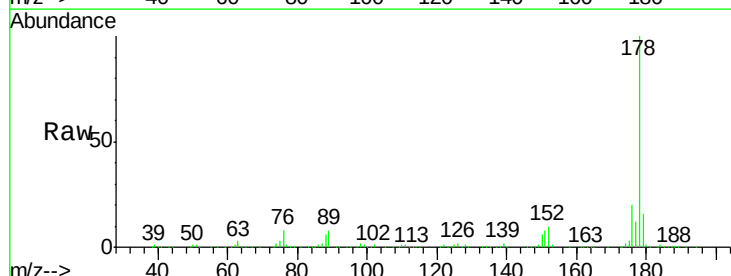

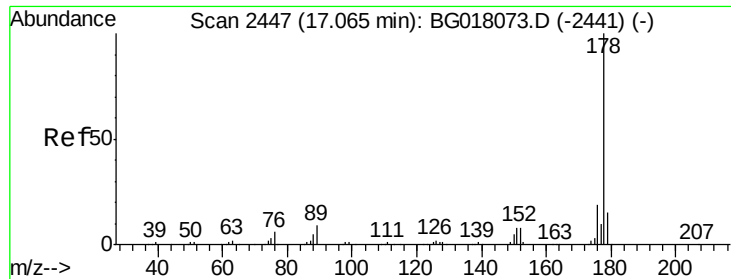

#72

Anthracene

Concen: 4.93 ng/ul

RT: 17.07 min Scan# 2447

Delta R.T. 0.00 min

Lab File: BG018076.D


Acq: 23 Jul 2015 22:03

Instrument :

BNA_G

ClientSampleId :




C01K0

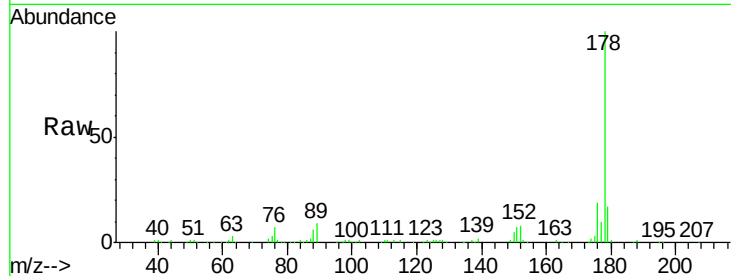

Tgt Ion:	178	Resp:	85885
Ion Ratio	Lower	Upper	
178	100		
179	16.8	12.4	18.6
176	19.2	15.8	23.8

Manual Integrations
APPROVED

apatel
7/24/2015 4:50:53 PM

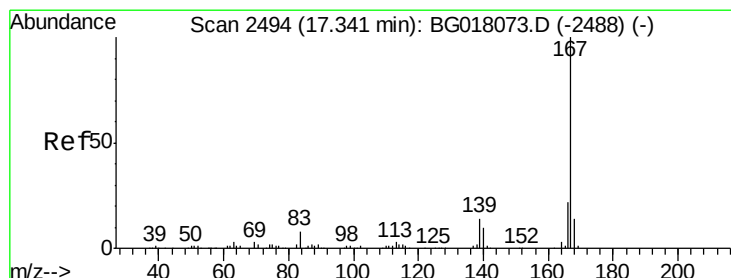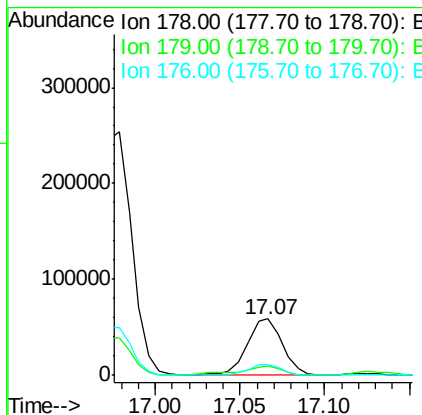

#75

Carbazole

Concen: 2.28 ng/ul




RT: 17.34 min Scan# 2494


Delta R.T. 0.00 min

Lab File: BG018076.D

Acq: 23 Jul 2015 22:03

Tgt Ion:	167	Resp:	34471
Ion Ratio	Lower	Upper	
167	100		
166	22.7	17.4	26.2
139	13.9	10.6	15.8

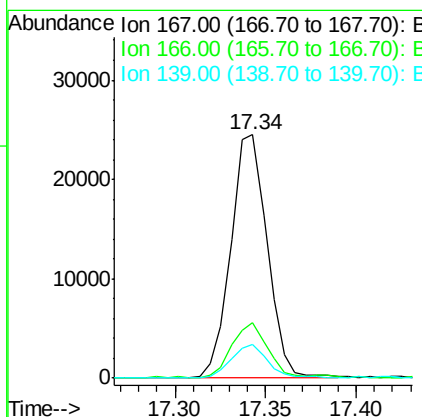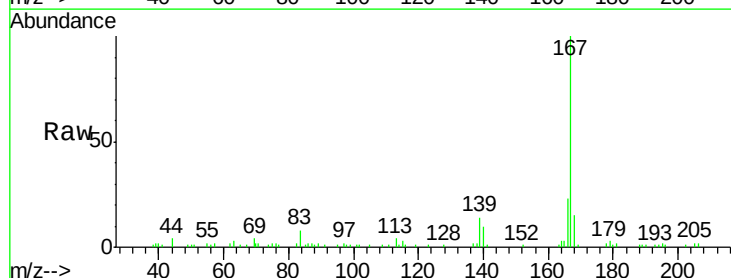

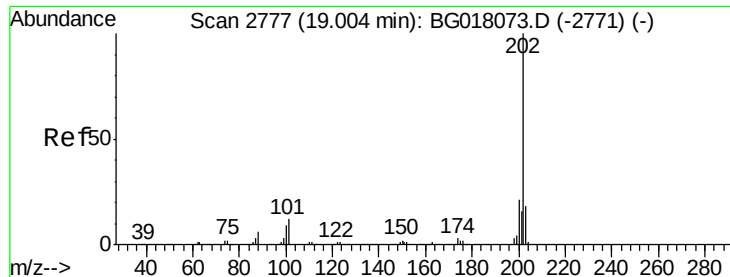

#77

Fluoranthene

Concen: 33.34 ng/ul

RT: 19.01 min Scan# 2777

Delta R.T. 0.00 min

Lab File: BG018076.D


Acq: 23 Jul 2015 22:03

Instrument :

BNA_G

ClientSampleId :




C01K0

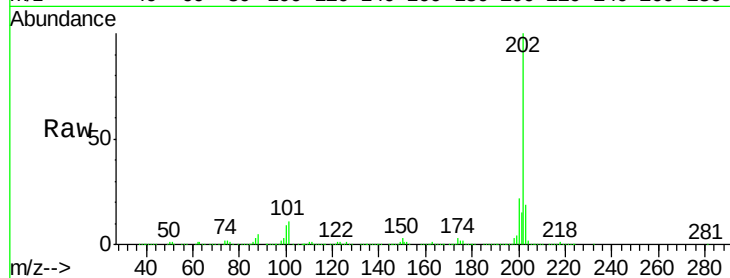

Tgt Ion	Ratio	Resp	Lower	Upper
202	100	609779		
101	11.5	9.1	13.7	
100	8.7	7.5	11.3	

Manual Integrations
APPROVED

apatel
7/24/2015 4:50:53 PM

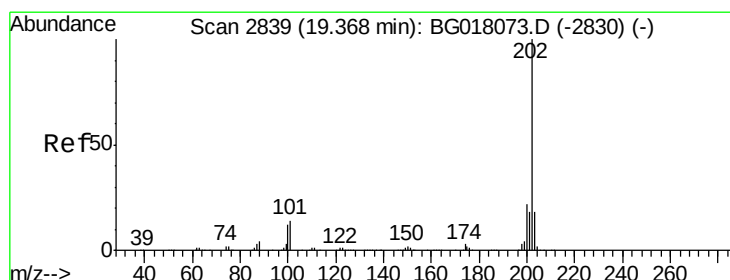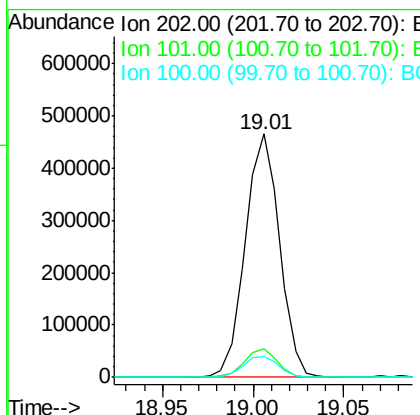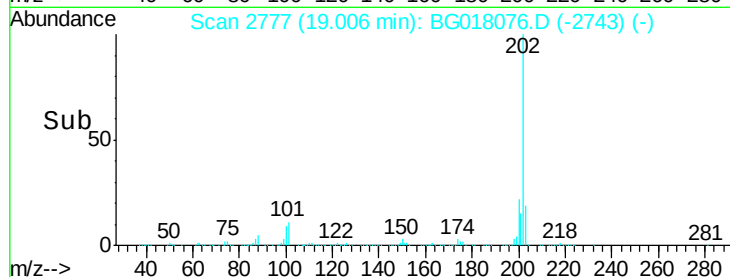

#80

Pyrene

Concen: 31.53 ng/ul




RT: 19.37 min Scan# 2839


Delta R.T. 0.00 min

Lab File: BG018076.D

Acq: 23 Jul 2015 22:03

Tgt Ion	Ratio	Resp	Lower	Upper
202	100	631679		
101	13.2	10.9	16.3	
100	11.1	8.5	12.7	

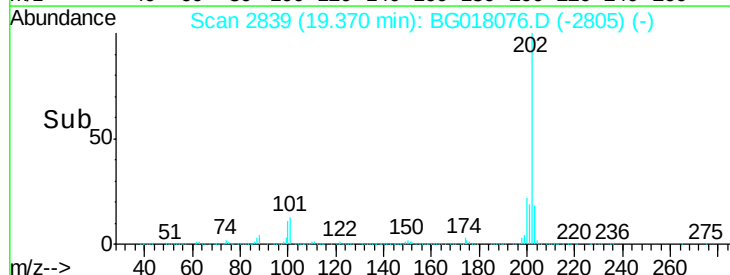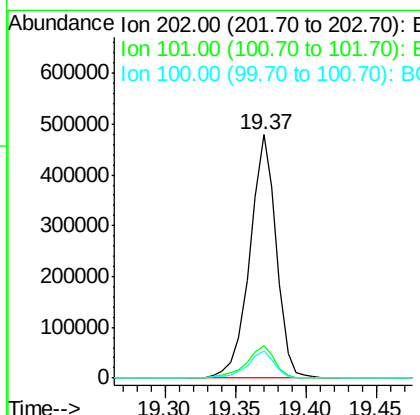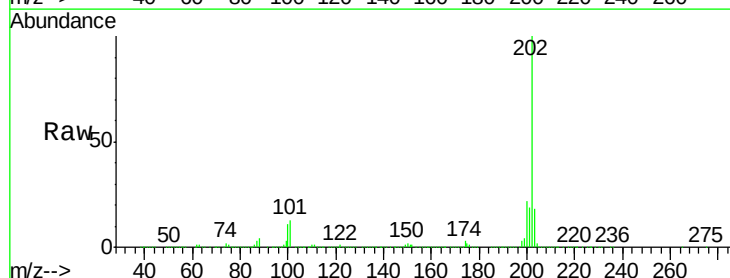

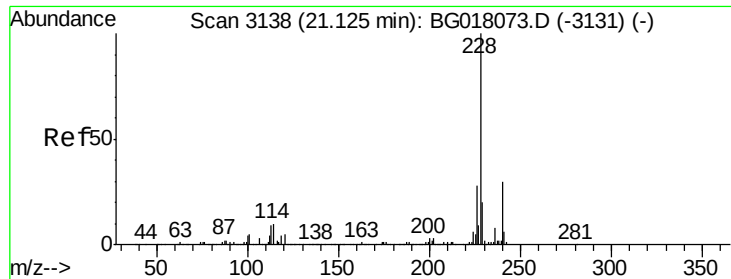

#83

Benzo(a)anthracene

Concen: 18.72 ng/ul

RT: 21.12 min Scan# 3137

Delta R.T. -0.00 min

Lab File: BG018076.D

Acq: 23 Jul 2015 22:03

Instrument :

BNA_G





ClientSampleId :

C01K0

Tgt	Ion	Ratio	Resp	Lower	Upper
228	100		346439		
229	20.4		16.6	24.8	
226	26.4		21.1	31.7	

Manual Integrations
APPROVED

apatel
7/24/2015 4:50:53 PM

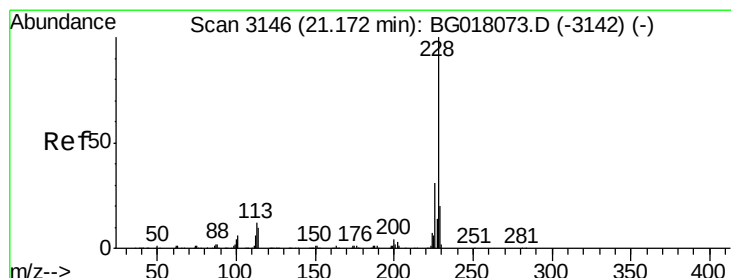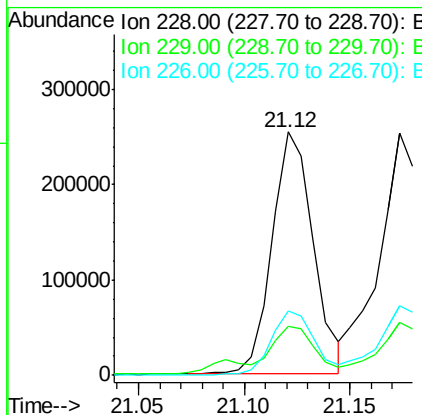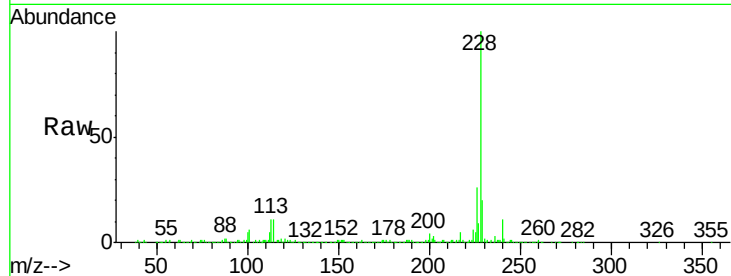

#85

Chrysene

Concen: 20.02 ng/ul




RT: 21.17 min Scan# 3146


Delta R.T. 0.00 min

Lab File: BG018076.D

Acq: 23 Jul 2015 22:03

Tgt	Ion	Ratio	Resp	Lower	Upper
228	100		348825		
226	28.6		22.9	34.3	
229	21.9		15.6	23.4	

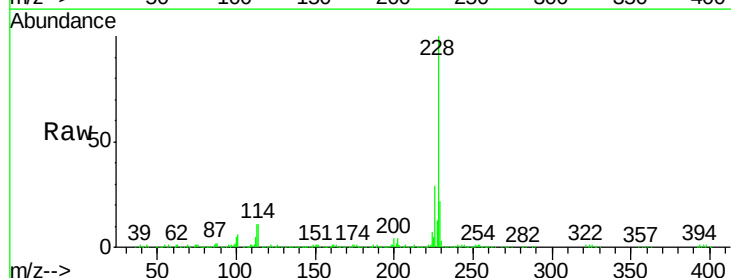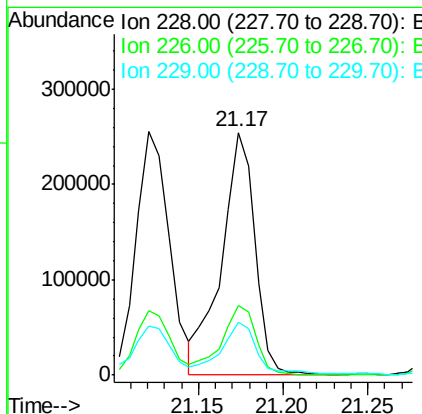

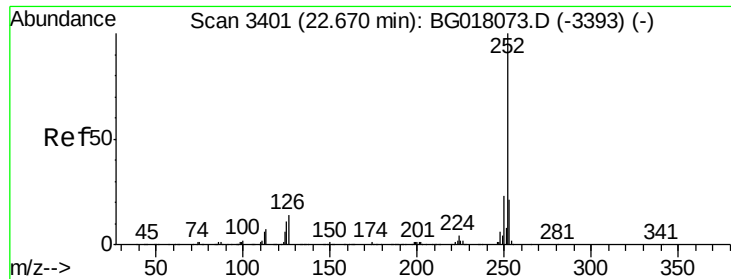





#88
Benzo(b)fluoranthene
Concen: 23.27 ng/ul
RT: 22.67 min Scan# 3401
Delta R.T. 0.00 min
Lab File: BG018076.D
Acq: 23 Jul 2015 22:03

Instrument :
BNA_G
ClientSampled :
C01K0

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.5	18.5	27.7
125	11.8	9.1	13.7




Manual Integrations
APPROVED


apatel
7/24/2015 4:50:53 PM

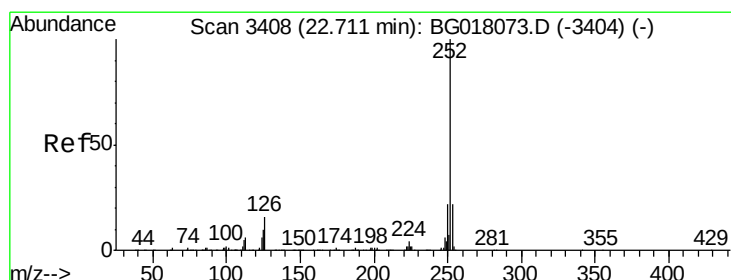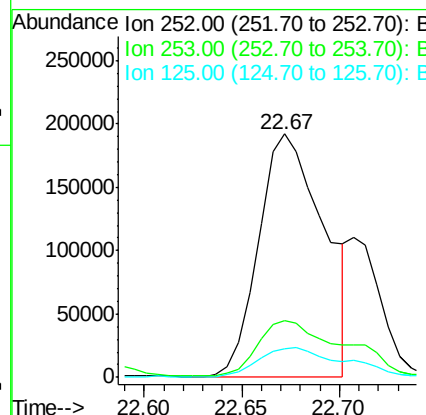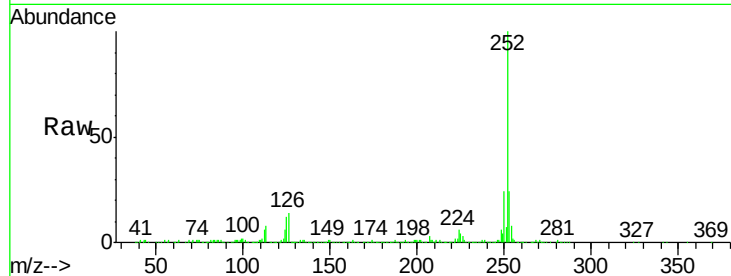

#89
Benzo(k)fluoranthene
Concen: 6.86 ng/ul m
RT: 22.71 min Scan# 3407
Delta R.T. -0.00 min
Lab File: BG018076.D
Acq: 23 Jul 2015 22:03

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.0	17.8	26.8
125	12.0	9.3	13.9

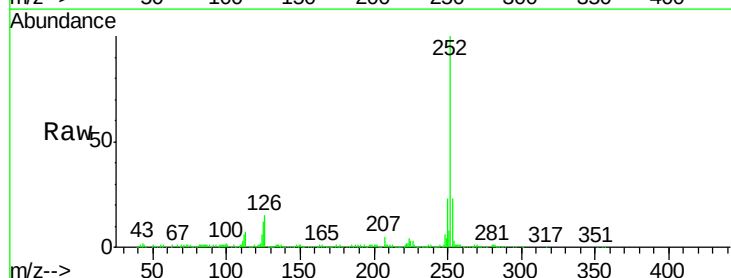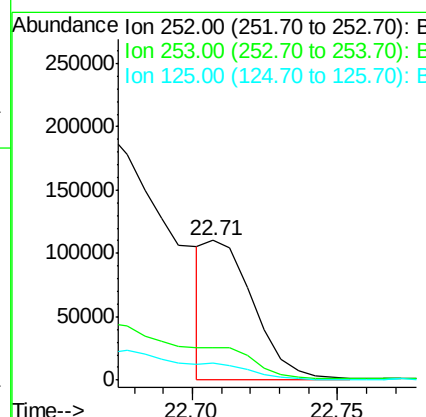

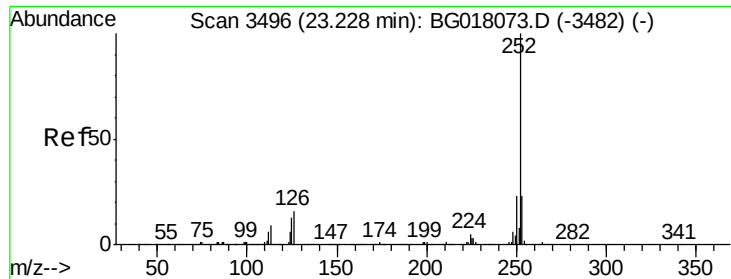





#91
Benzo(a)pyrene
Concen: 16.71 ng/ul
RT: 23.23 min Scan# 3496
Delta R.T. 0.00 min
Lab File: BG018076.D
Acq: 23 Jul 2015 22:03

Instrument :
BNA_G
ClientSampleId :
C01K0

Tgt Ion	Ratio	Resp Lower	Resp Upper
252	100		
253	22.7	18.0	27.0
125	12.3	10.2	15.2




Manual Integrations
APPROVED


apatel
7/24/2015 4:50:53 PM

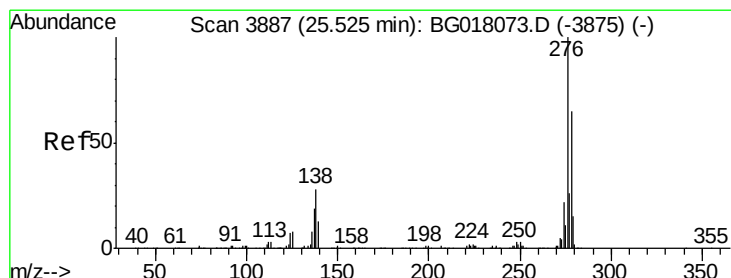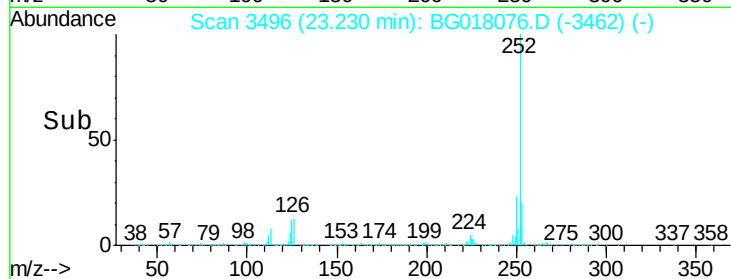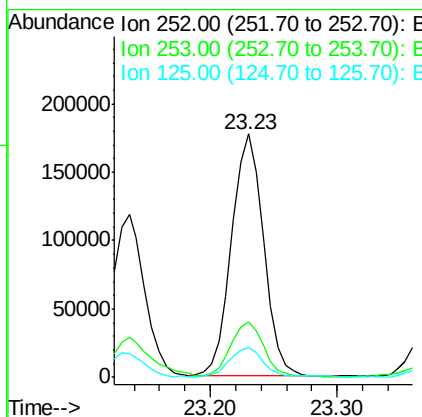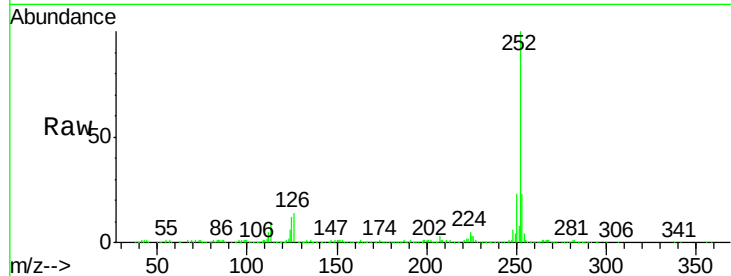

#92
Indeno(1,2,3-cd)pyrene
Concen: 8.88 ng/ul
RT: 25.53 min Scan# 3887
Delta R.T. 0.00 min
Lab File: BG018076.D
Acq: 23 Jul 2015 22:03

Tgt Ion	Ratio	Resp Lower	Resp Upper
276	100		
138	22.9	22.6	33.8
277	24.6	19.8	29.8

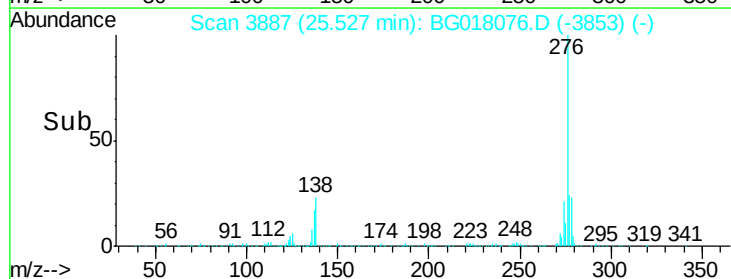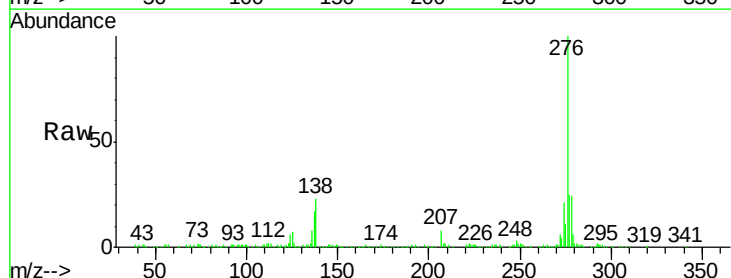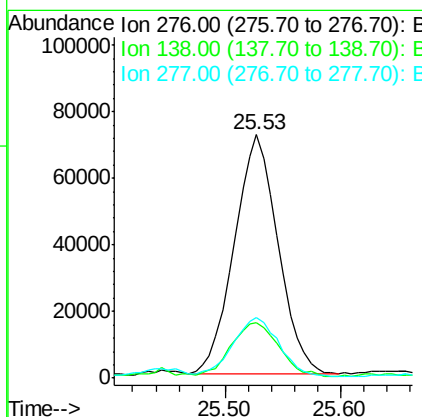

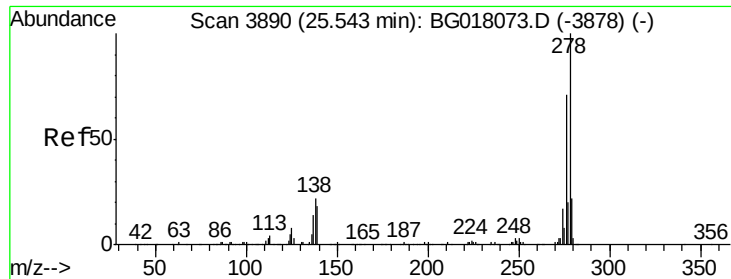





#93
Dibenzo(a,h)anthracene
Concen: 2.96 ng/ul
RT: 25.53 min Scan# 3887
Delta R.T. -0.02 min
Lab File: BG018076.D
Acq: 23 Jul 2015 22:03

Instrument :
BNA_G
ClientSampleId :
C01K0

Tgt Ion	Ratio	Lower	Upper
278	100		
139	0.0	13.7	20.5#
279	25.9	18.1	27.1

Manual Integrations
APPROVED

apatel
7/24/2015 4:50:53 PM

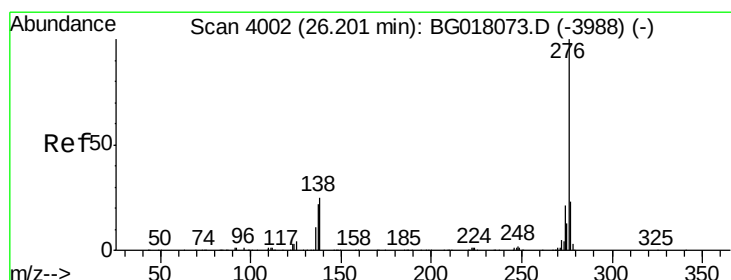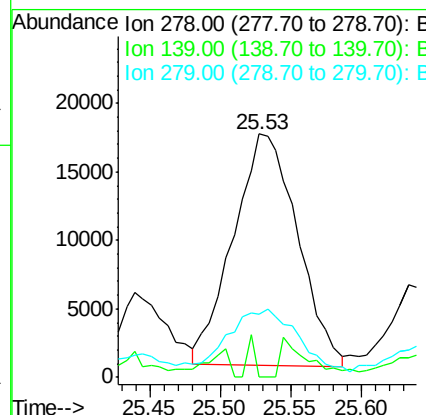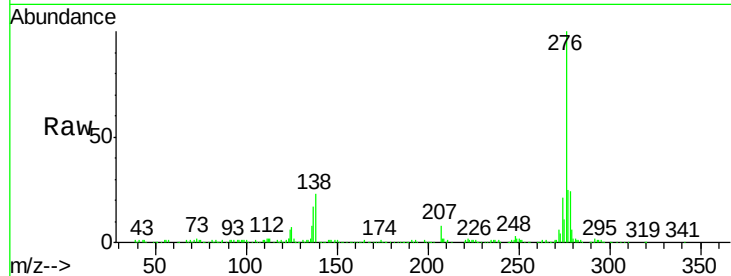

#94
Benzo(g,h,i)perylene
Concen: 7.55 ng/ul
RT: 26.20 min Scan# 4001
Delta R.T. -0.00 min
Lab File: BG018076.D
Acq: 23 Jul 2015 22:03

Tgt Ion	Ratio	Lower	Upper
276	100		
138	26.9	18.8	28.2
277	22.1	19.3	28.9

