

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG072316\
 Data File : BG023233.D
 Acq On : 23 Jul 2016 2:48
 Operator : UM/SJ
 Sample : H4131-28
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 D-15

Quant Time: Jul 23 04:30:58 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 19 15:46:37 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.14	152	110460	20.00	ng	0.00
21) Naphthalene-d8	10.98	136	509685	20.00	ng	0.00
38) Acenaphthene-d10	14.81	164	365129	20.00	ng	0.01
63) Phenanthrene-d10	17.57	188	933763	20.00	ng	0.02
75) Chrysene-d12	21.89	240	992827	20.00	ng	0.01
86) Perylene-d12	25.30	264	963622	20.00	ng	0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.68	112	892827	132.19	ng	0.00
7) Phenol-d6	7.29	99	1255584	118.70	ng	0.00
23) Nitrobenzene-d5	9.32	82	1037478	87.16	ng	0.00
41) 2,4,6-Tribromophenol	16.31	330	616803	93.99	ng	0.01
44) 2-Fluorobiphenyl	13.43	172	1924612	83.03	ng	0.01
78) Terphenyl-d14	20.18	244	2858732	95.87	ng	0.02
Target Compounds						
76) Benzidine	19.81	184	878933	30.88	ng	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG072316\
Data File : BG023233.D
Acq On : 23 Jul 2016 2:48
Operator : UM/SJ
Sample : H4131-28
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
D-15

Quant Time: Jul 23 04:30:58 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 19 15:46:37 2016
Response via : Initial Calibration

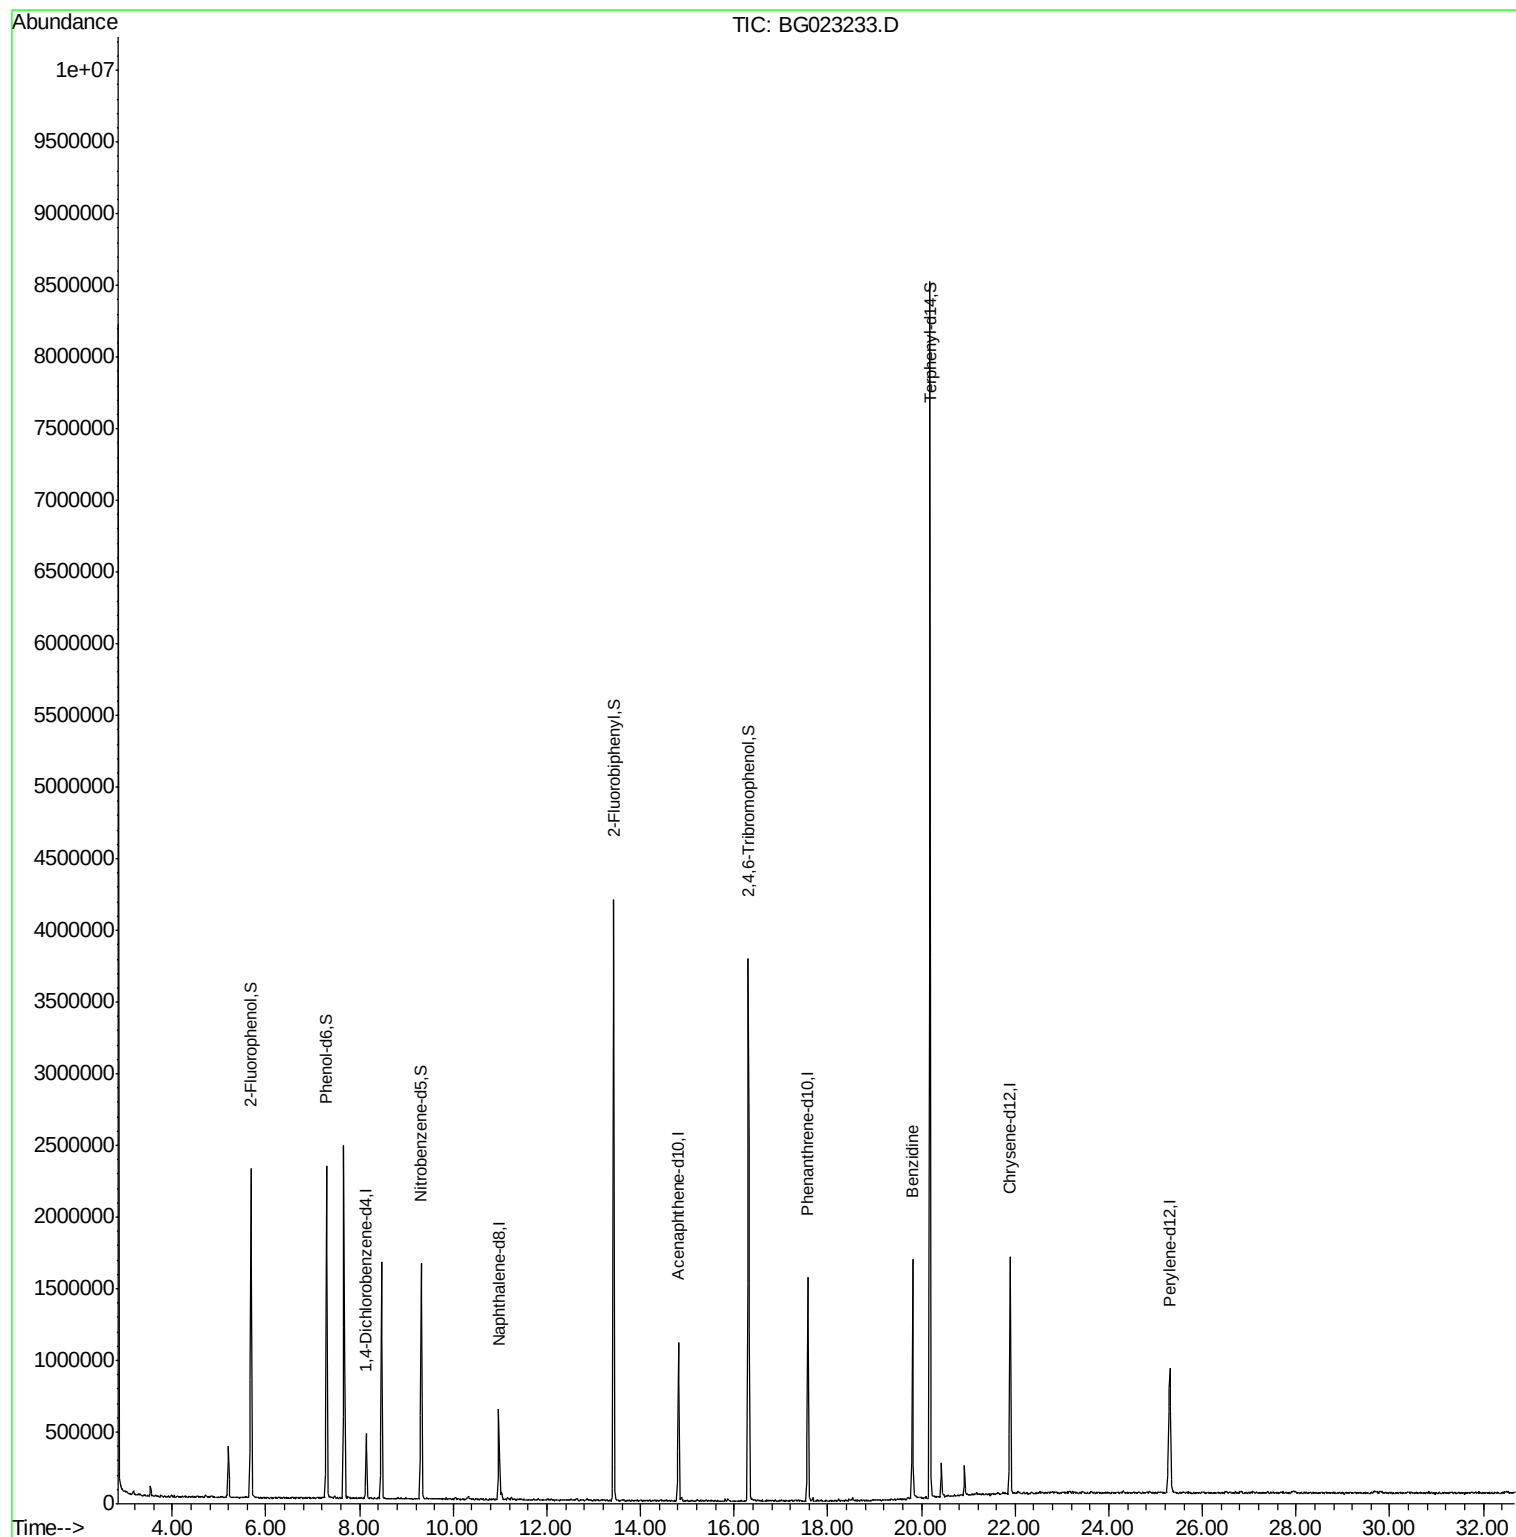

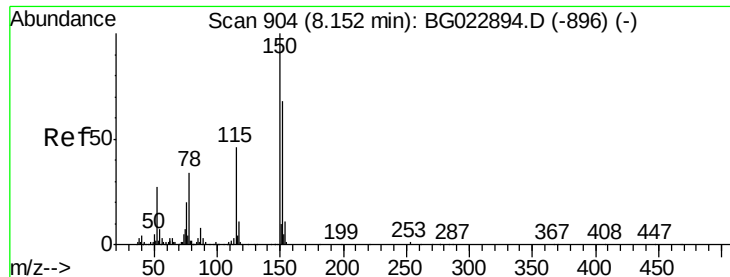

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 8.14 min Scan# 903

Delta R.T. -0.00 min

Lab File: BG023233.D

Acq: 23 Jul 2016 2:48

Instrument :

BNA_G

ClientSampled :

D-15


Tgt Ion:152 Resp: 110460

Ion Ratio Lower Upper

152 100

150 157.0 144.7 217.1




115 63.8 64.0 96.0#

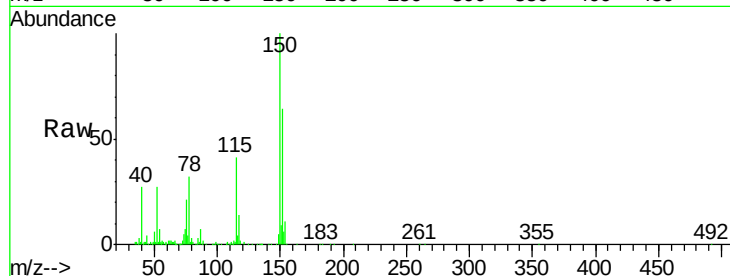

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

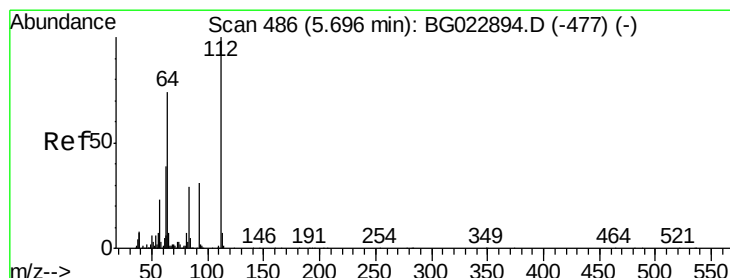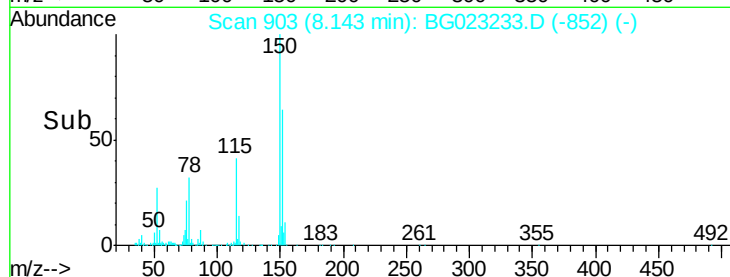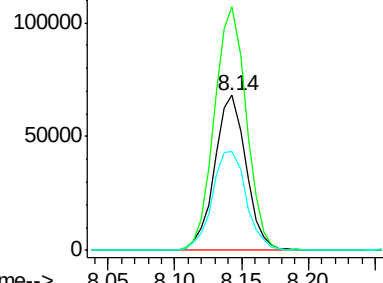

#5

2-Fluorophenol

Concen: 132.19 ng

RT: 5.68 min Scan# 484

Delta R.T. 0.01 min

Lab File: BG023233.D

Acq: 23 Jul 2016 2:48


Tgt Ion:112 Resp: 892827

Ion Ratio Lower Upper

112 100

64 72.0 59.0 88.4



63 43.5 37.8 56.8

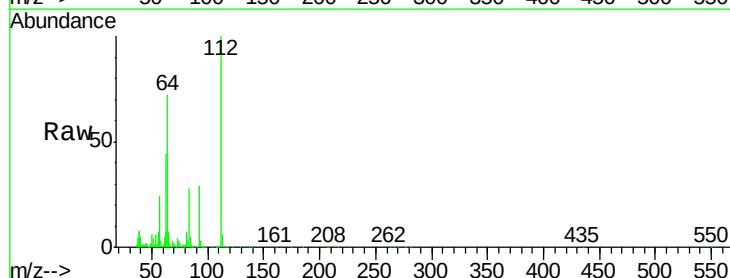


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

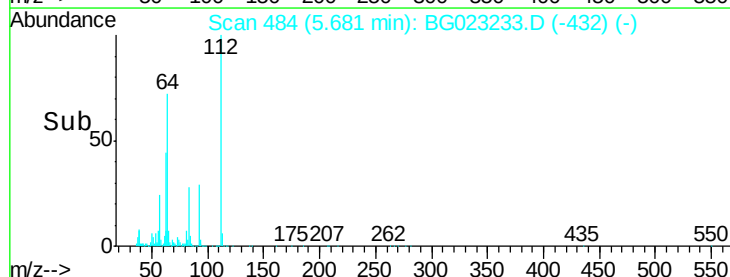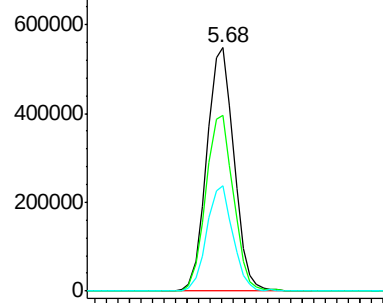

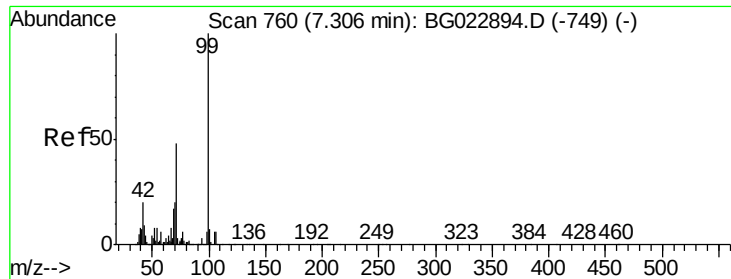

#7

Phenol-d6

Concen: 118.70 ng

RT: 7.29 min Scan# 758

Delta R.T. -0.01 min

Lab File: BG023233.D

Acq: 23 Jul 2016 2:48

Instrument :

BNA_G

ClientSampleId :

D-15


Tgt Ion: 99 Resp: 1255584

Ion Ratio Lower Upper




99 100

42 21.4 17.8 26.6

71 49.1 41.5 62.3

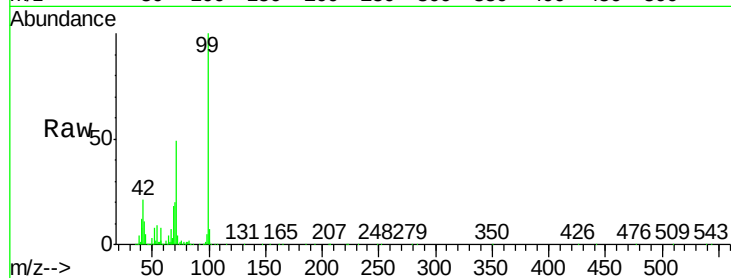

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

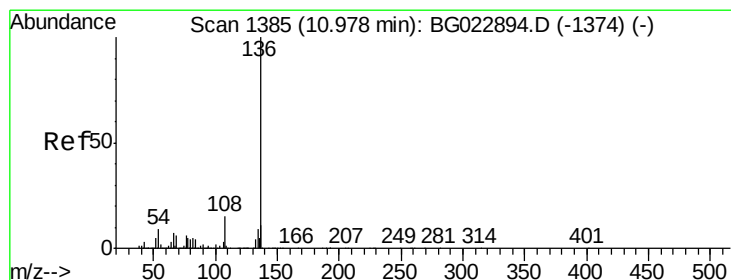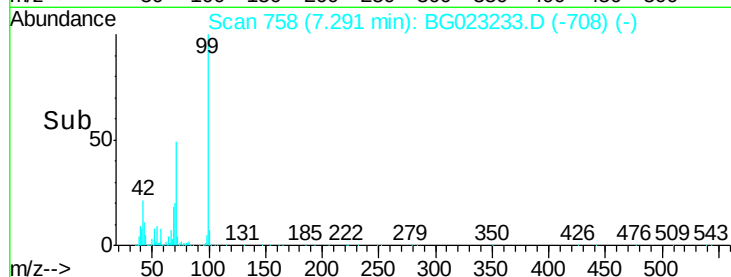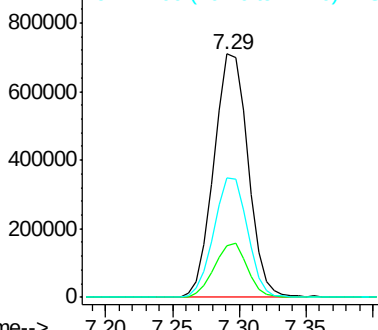

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.98 min Scan# 1385

Delta R.T. -0.00 min

Lab File: BG023233.D

Acq: 23 Jul 2016 2:48

Tgt Ion: 136 Resp: 509685


Ion Ratio Lower Upper

136 100



137 11.1 9.6 14.4


54 8.5 7.3 10.9

68 6.4 5.3 7.9

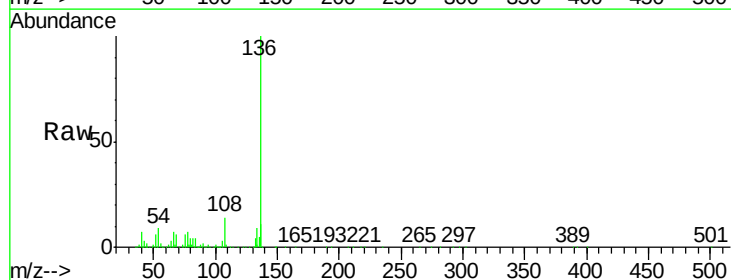

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



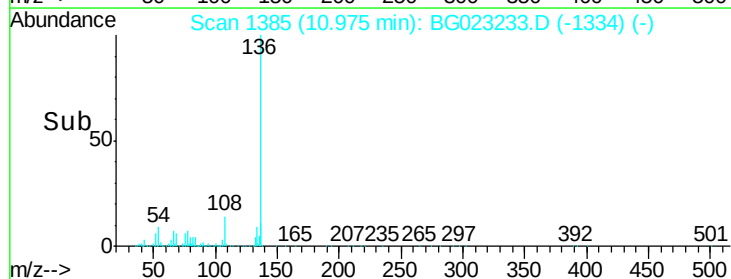
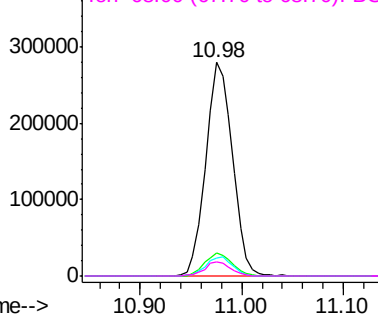


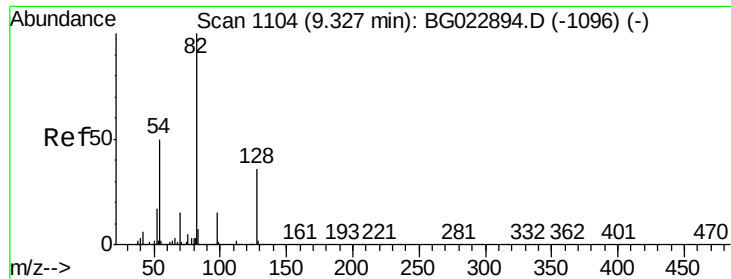

#23
Nitrobenzene-d5
Concen: 87.16 ng
RT: 9.32 min Scan# 1103
Delta R.T. -0.00 min
Lab File: BG023233.D
Acq: 23 Jul 2016 2:48




Instrument :
BNA_G
ClientSampleId :
D-15


Tgt Ion: 82 Resp: 1037478
Ion Ratio Lower Upper
82 100
128 31.6 24.4 36.6
54 52.1 41.4 62.0

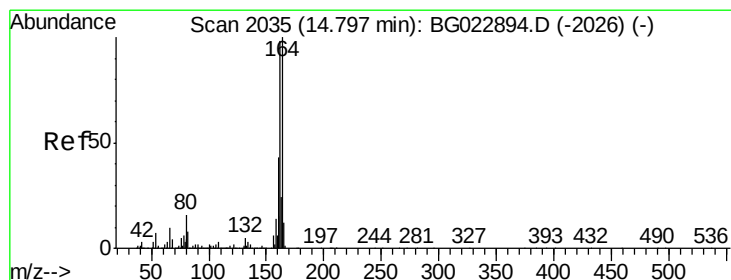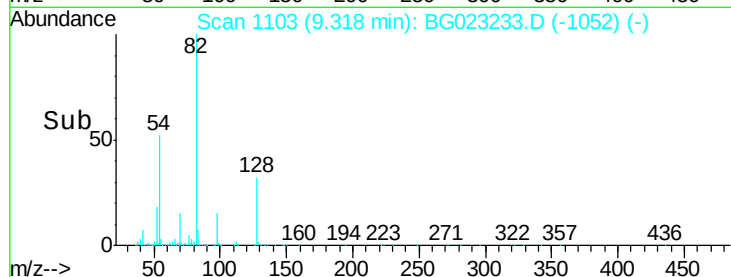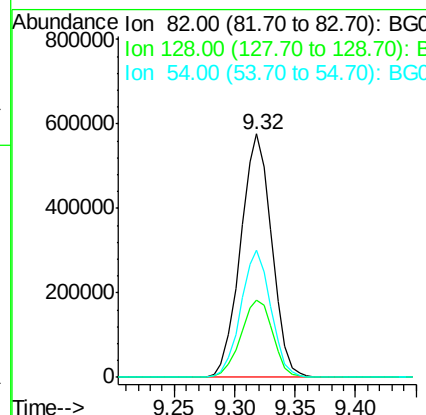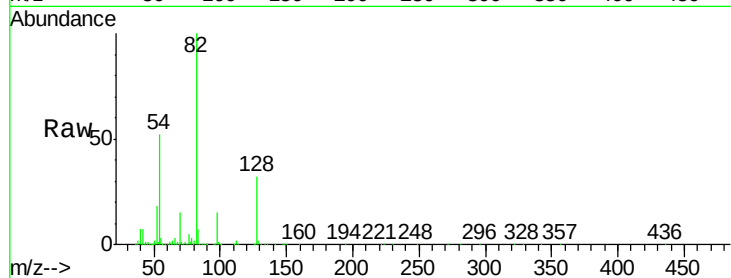

#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.81 min Scan# 2038
Delta R.T. 0.01 min
Lab File: BG023233.D
Acq: 23 Jul 2016 2:48

Tgt Ion: 164 Resp: 365129
Ion Ratio Lower Upper
164 100
162 103.0 87.7 131.5
160 46.2 37.2 55.8


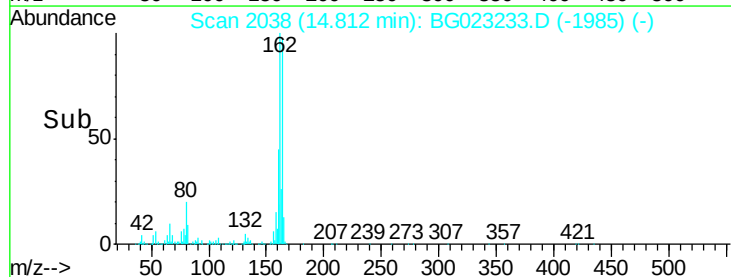
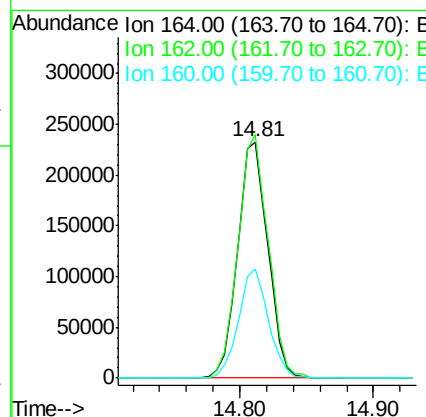
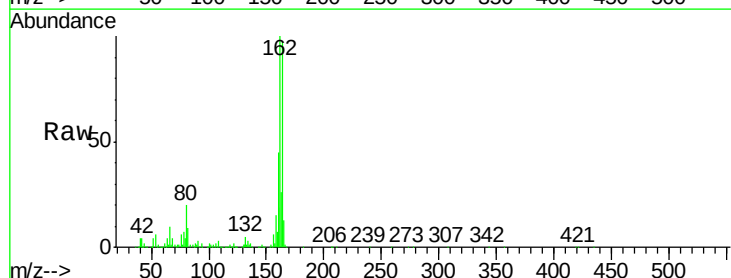


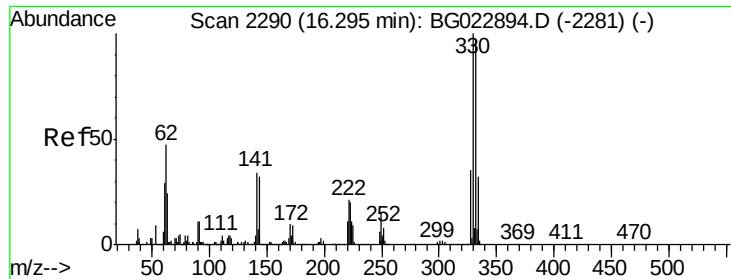

#41
 2,4,6-Tribromophenol
 Concen: 93.99 ng
 RT: 16.31 min Scan# 2293
 Delta R.T. 0.01 min
 Lab File: BG023233.D
 Acq: 23 Jul 2016 2:48




Instrument :
 BNA_G
 ClientSampleId :
 D-15


Tgt Ion:330 Resp: 616803
 Ion Ratio Lower Upper
 330 100
 332 99.0 77.4 116.2
 141 46.0 31.7 47.5

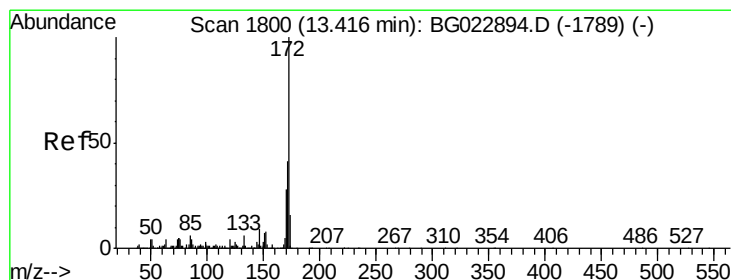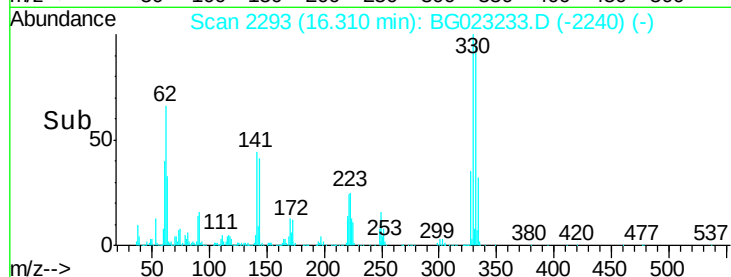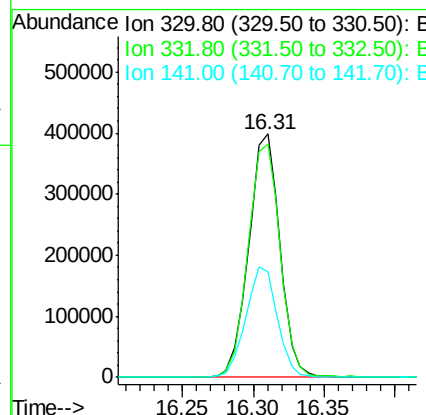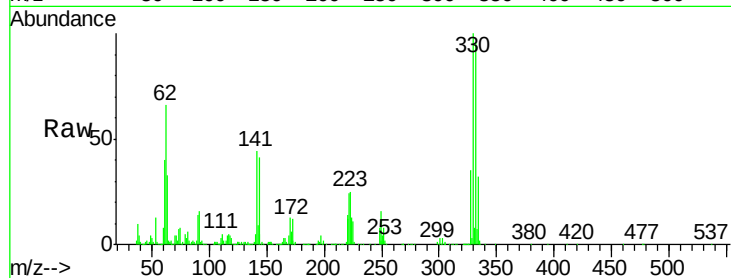

#44
 2-Fluorobiphenyl
 Concen: 83.03 ng
 RT: 13.43 min Scan# 1802
 Delta R.T. 0.01 min
 Lab File: BG023233.D
 Acq: 23 Jul 2016 2:48

Tgt Ion:172 Resp: 1924612
 Ion Ratio Lower Upper
 172 100
 171 40.7 31.6 47.4
 170 29.1 21.3 31.9

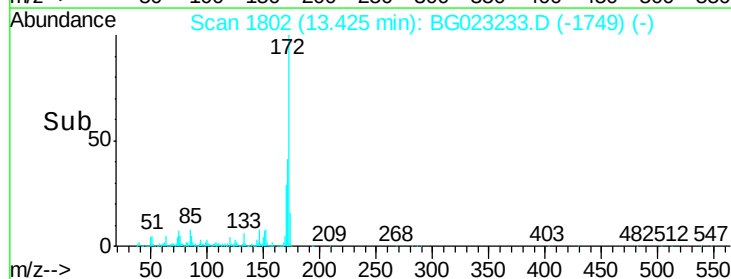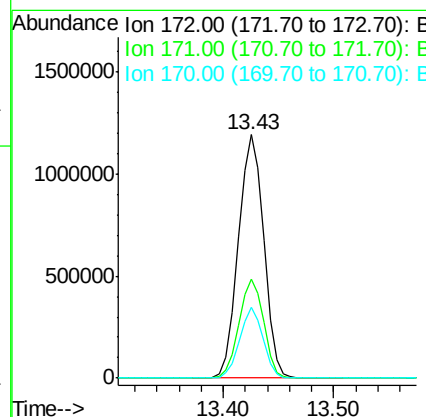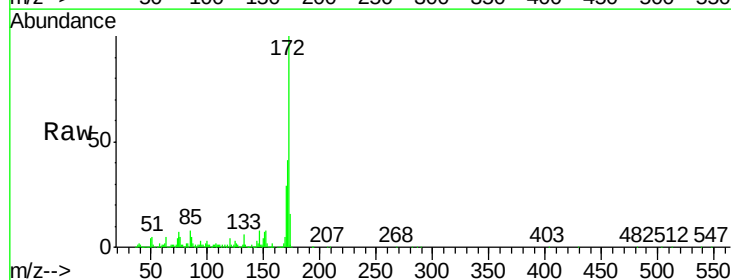

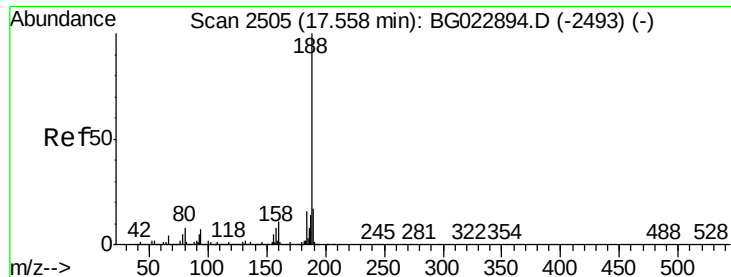

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.57 min Scan# 2508

Delta R.T. 0.02 min

Lab File: BG023233.D

Acq: 23 Jul 2016 2:48

Instrument :

BNA_G

ClientSampleId :

D-15


Tgt Ion:188 Resp: 933763

Ion Ratio Lower Upper

188 100

94 8.1 5.2 7.8#




80 11.2 7.2 10.8#

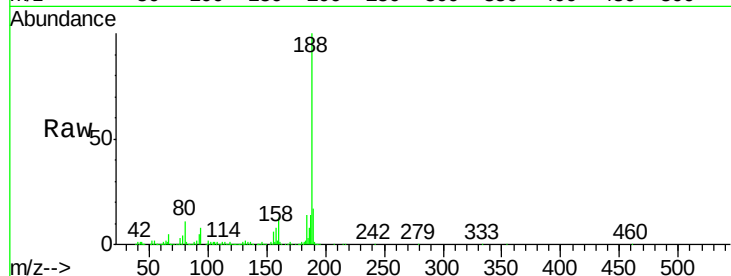

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

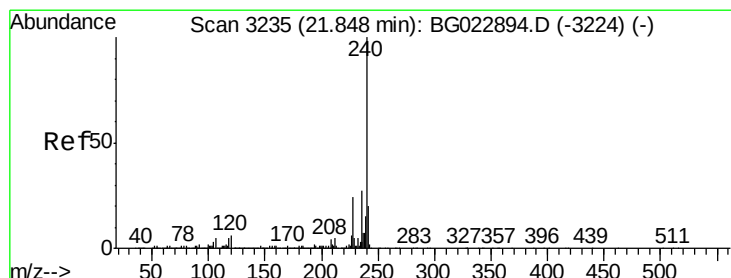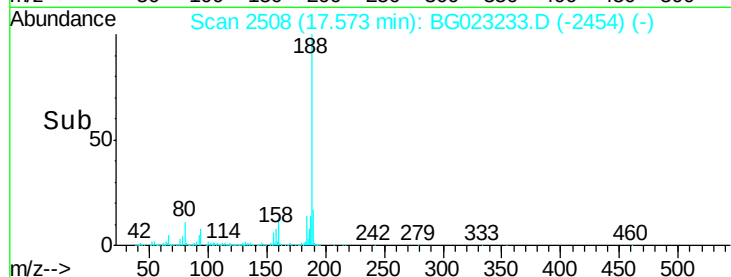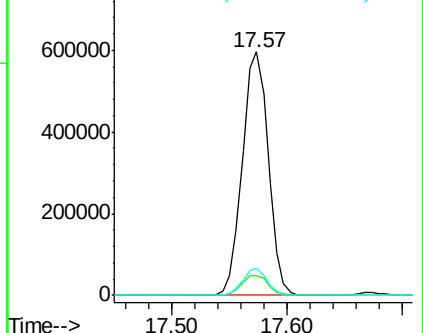

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.89 min Scan# 3243

Delta R.T. 0.01 min

Lab File: BG023233.D

Acq: 23 Jul 2016 2:48


Tgt Ion:240 Resp: 992827

Ion Ratio Lower Upper

240 100

120 6.8 4.1 6.1#



236 25.7 21.1 31.7

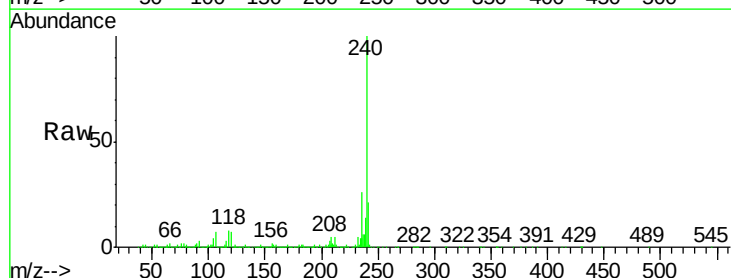


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

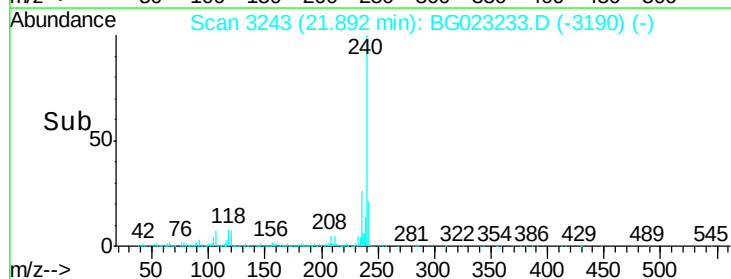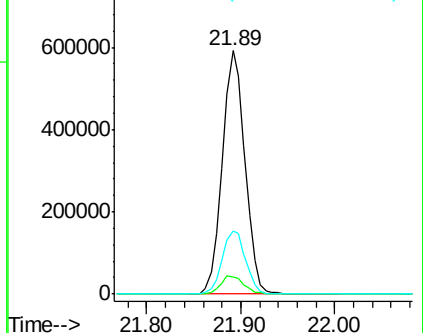

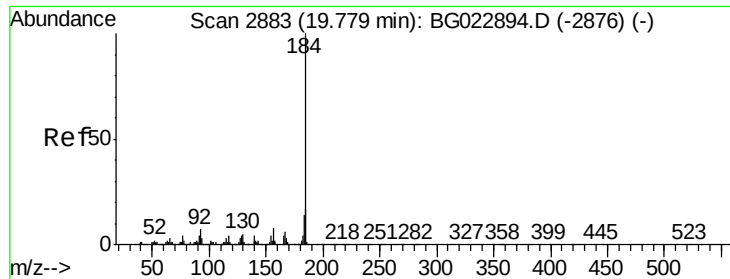

#76

Benzidine

Concen: 30.88 ng

RT: 19.81 min Scan# 2888

Delta R.T. 0.02 min

Lab File: BG023233.D

Acq: 23 Jul 2016 2:48

Instrument :

BNA_G

ClientSampleId :

D-15


Tgt Ion:184 Resp: 878933

Ion Ratio Lower Upper

184 100

185 16.8 12.6 19.0

183 12.8 10.7 16.1

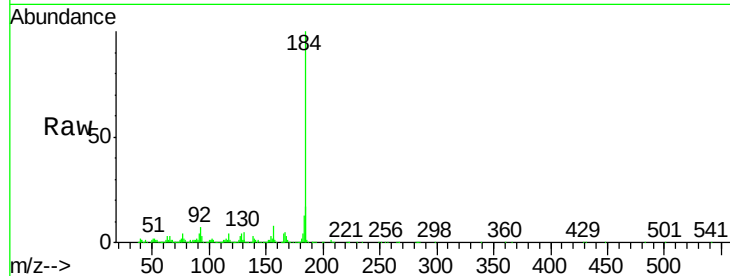

Abundance Ion 184.00 (183.70 to 184.70): E

Ion 185.00 (184.70 to 185.70): E

Ion 183.00 (182.70 to 183.70): E

800000

600000

400000

200000

0

19.81

19.80

19.81

19.82

19.83

19.84

19.85

19.86

19.87

19.88

19.89

19.90

19.91

19.92

19.93

19.94

19.95

19.96

19.97

19.98

19.99

20.00

20.01

20.02

20.03

20.04

20.05

20.06

20.07

20.08

20.09

20.10

20.11

20.12

20.13

20.14

20.15

20.16

20.17

20.18

20.19

20.20

20.21

20.22

20.23

20.24

20.25

20.26

20.27

20.28

20.29

20.30

20.31

20.32

20.33

20.34

20.35

20.36

20.37

20.38

20.39

20.40

20.41

20.42

20.43

20.44

20.45

20.46

20.47

20.48

20.49

20.50

20.51

20.52

20.53

20.54

20.55

20.56

20.57

20.58

20.59

20.60

20.61

20.62

20.63

20.64

20.65

20.66

20.67

20.68

20.69

20.70

20.71

20.72

20.73

20.74

20.75

20.76

20.77

20.78

20.79

20.80

20.81

20.82

20.83

20.84

20.85

20.86

20.87

20.88

20.89

20.90

20.91

20.92

20.93

20.94

20.95

20.96

20.97

20.98

20.99

21.00

21.01

21.02

21.03

21.04

21.05

21.06

21.07

21.08

21.09

21.10

21.11

21.12

21.13

21.14

21.15

21.16

21.17

21.18

21.19

21.20

21.21

21.22

21.23

21.24

21.25

21.26

21.27

21.28

21.29

21.30

21.31

21.32

21.33

21.34

21.35

21.36

21.37

21.38

21.39

21.40

21.41

21.42

21.43

21.44

21.45

21.46

21.47

21.48

21.49

21.50

21.51

21.52

21.53

21.54

21.55

21.56

21.57

21.58

21.59

21.60

21.61

21.62

21.63

21.64

21.65

21.66

21.67

21.68

21.69

21.70

21.71

21.72

21.73

21.74

21.75

21.76

21.77

21.78

21.79

21.80

21.81

21.82

21.83

21.84

21.85

21.86

21.87

21.88

21.89

21.90

21.91

21.92

21.93

21.94

21.95

21.96

21.97

21.98

21.99

22.00

22.01

22.02

22.03

22.04

22.05

22.06

22.07

22.08

22.09

22.10

22.11

22.12

22.13

22.14

22.15

22.16

22.17

22.18

22.19

22.20

22.21

22.22

22.23

22.24


22.25

22.26

22.27

22.28

22.29

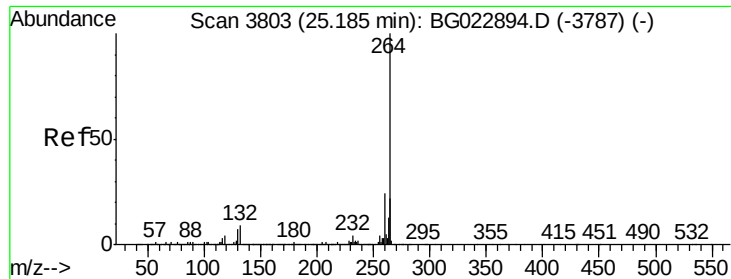

#86
Perylene-d12
Concen: 20.00 ng
RT: 25.30 min Scan# 3823
Delta R.T. 0.03 min
Lab File: BG023233.D
Acq: 23 Jul 2016 2:48

Instrument :
BNA_G
ClientSampleId :
D-15

Tgt Ion	Ratio	Lower	Upper
264	100		
260	25.6	18.4	27.6
265	23.3	18.9	28.3

