
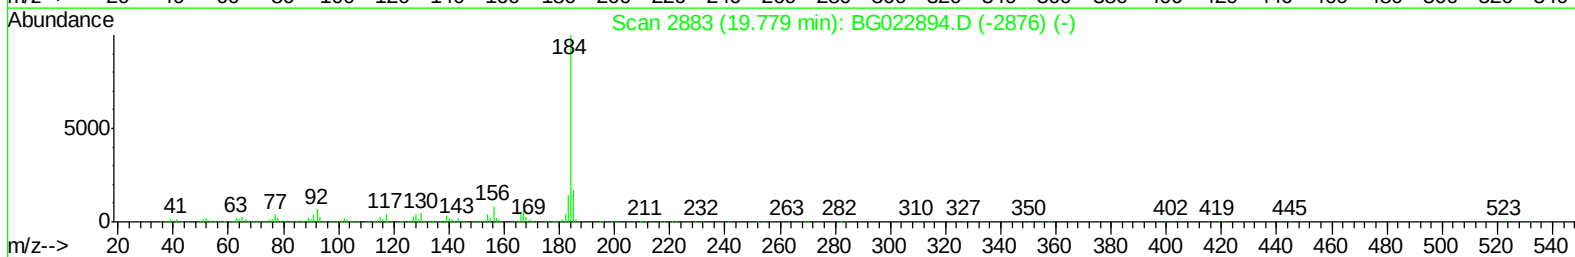
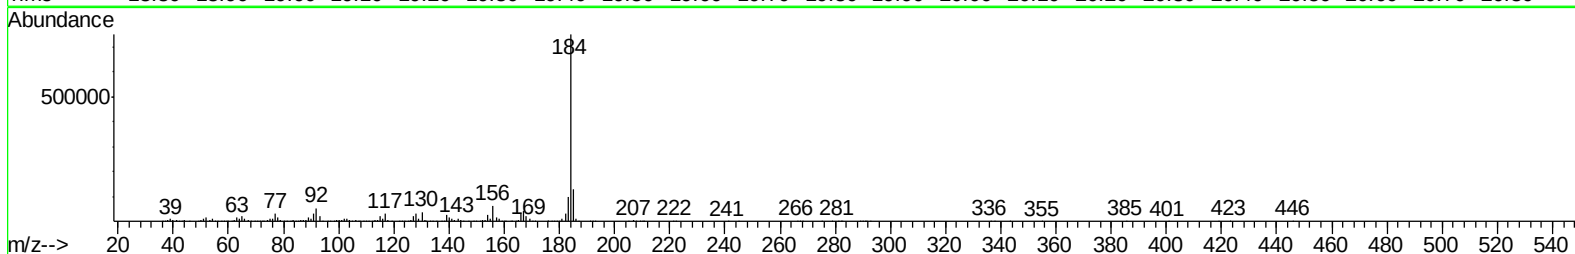


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG072316\
Data File : BG023219.D
Acq On : 22 Jul 2016 16:31
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 23 07:07:38 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 19 15:46:37 2016
Response via : Initial Calibration

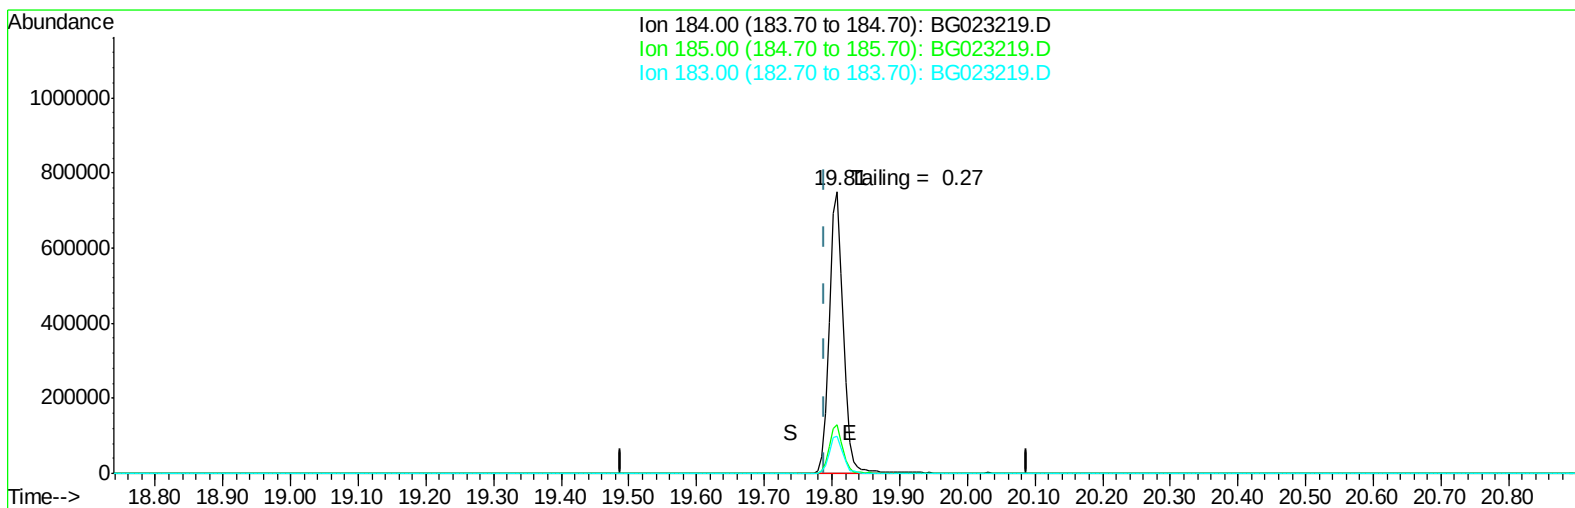

TIC: BG023219.D

(76) Benzidine




19.808min (+0.019) 269384.69ng m

response 1065758

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	17.09
183.00	13.40	13.38
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG072316\
Data File : BG023219.D
Acq On : 22 Jul 2016 16:31
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 23 07:07:38 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 19 15:46:37 2016
Response via : Initial Calibration

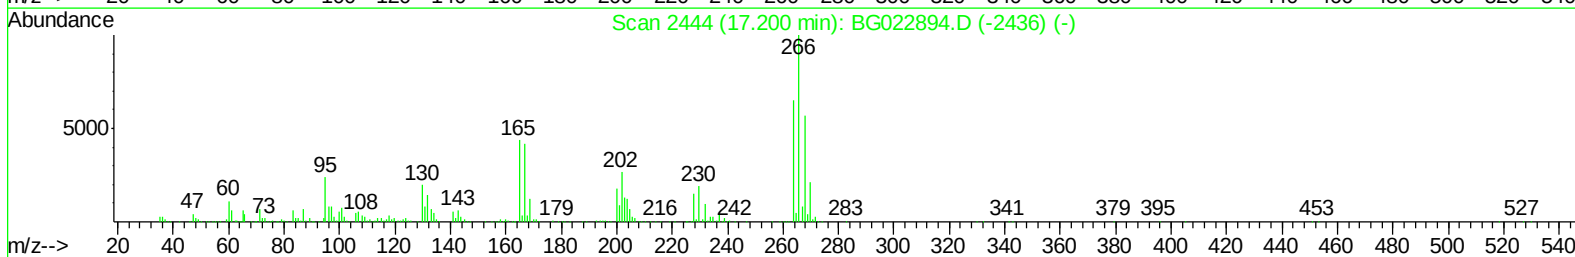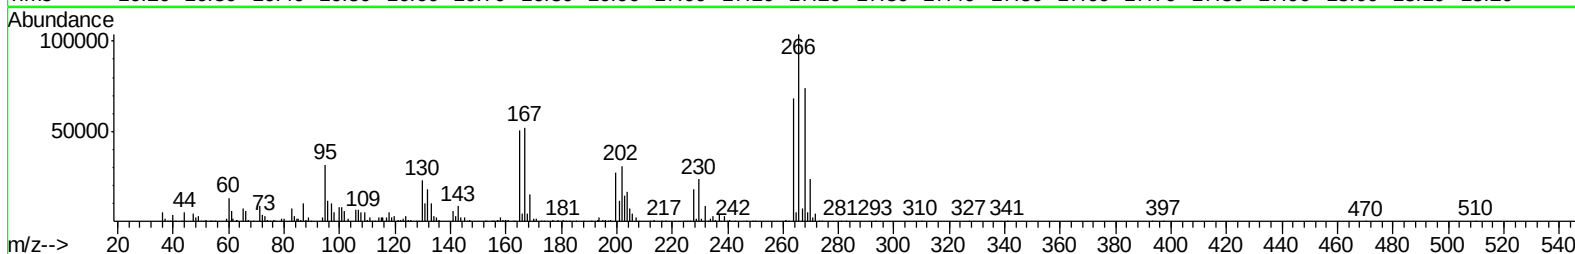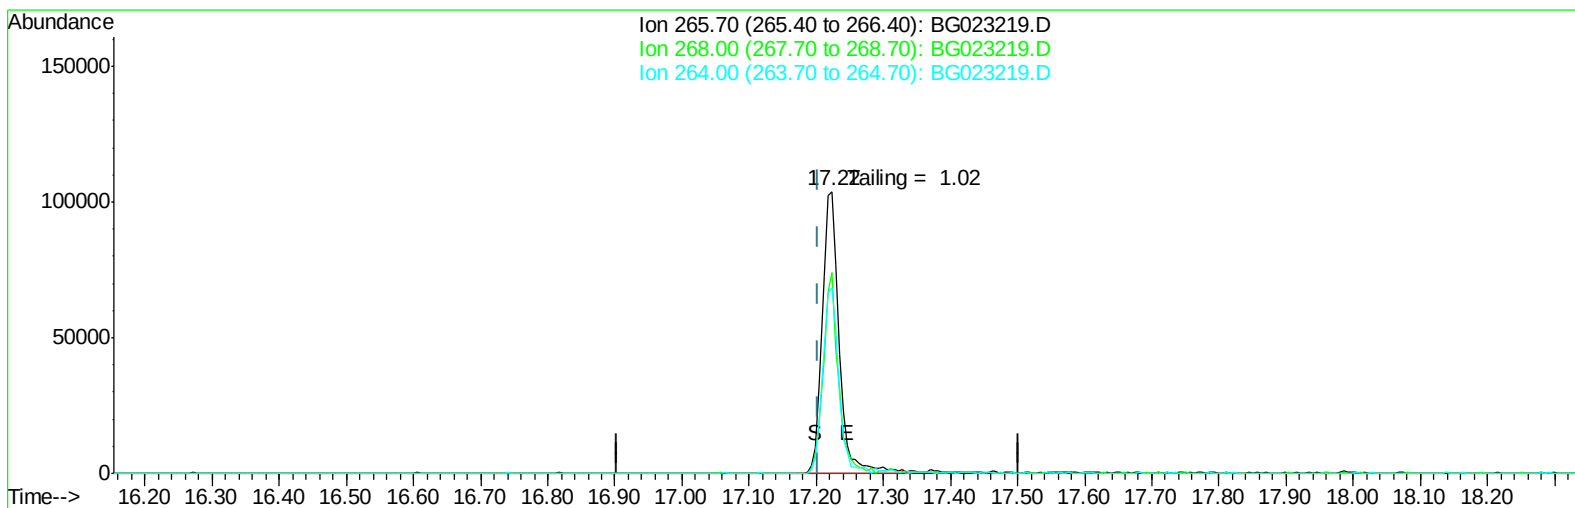

TIC: BG023219.D

(69) Pentachlorophenol (C)

17.223min (+0.019) 263329.53ng

response 180926

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	71.37
264.00	63.20	65.90
0.00	0.00	0.00