


Data Path : Z:\HPCHEM1\BNA_G\Data\BG072316\
 Data File : BG023236.D
 Acq On : 23 Jul 2016 4:50
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 19 15:46:37 2016

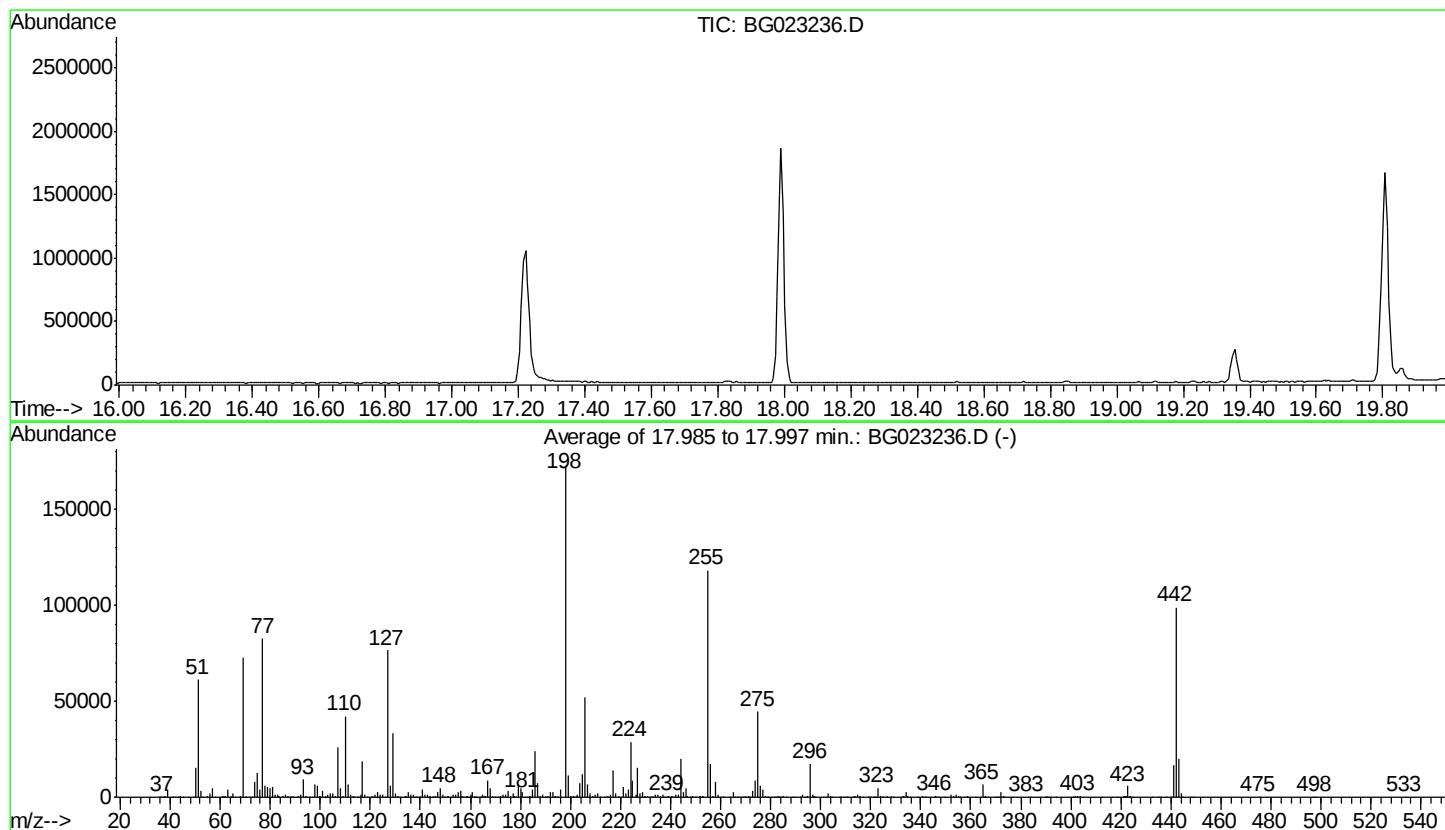

AutoFind: Scans 2578, 2579, 2580; Background Corrected with Scan 2571

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.4	61300	PASS
68	69	0.00	2	1.3	931	PASS
69	198	0.00	100	42.1	72770	PASS
70	69	0.00	2	0.3	246	PASS
127	198	10	80	44.2	76490	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	172992	PASS
199	198	5	9	6.6	11442	PASS
275	198	10	60	25.8	44565	PASS
365	198	1	100	3.8	6585	PASS
441	442	0.01	24	16.9	16700	PASS
442	198	50	100	57.2	98952	PASS
443	442	15	24	20.1	19860	PASS