
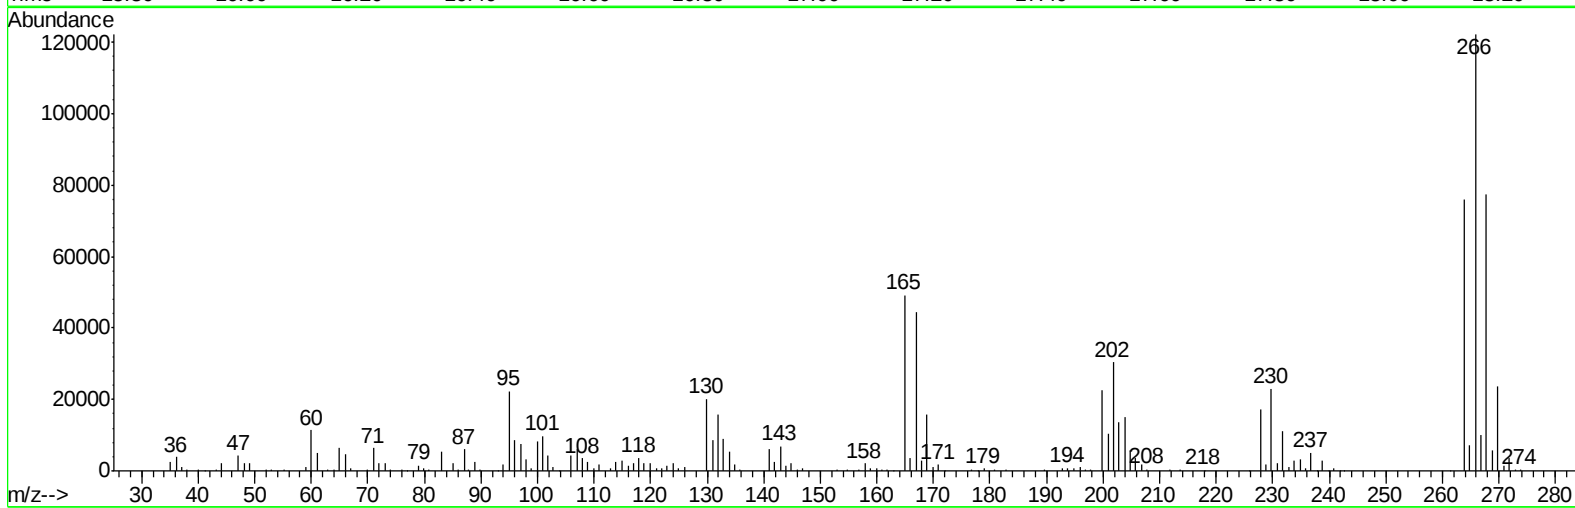


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072319\
Data File : BG041751.D
Acq On : 23 Jul 2019 10:03
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 24 08:39:14 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 15 16:16:21 2019
Response via : Initial Calibration

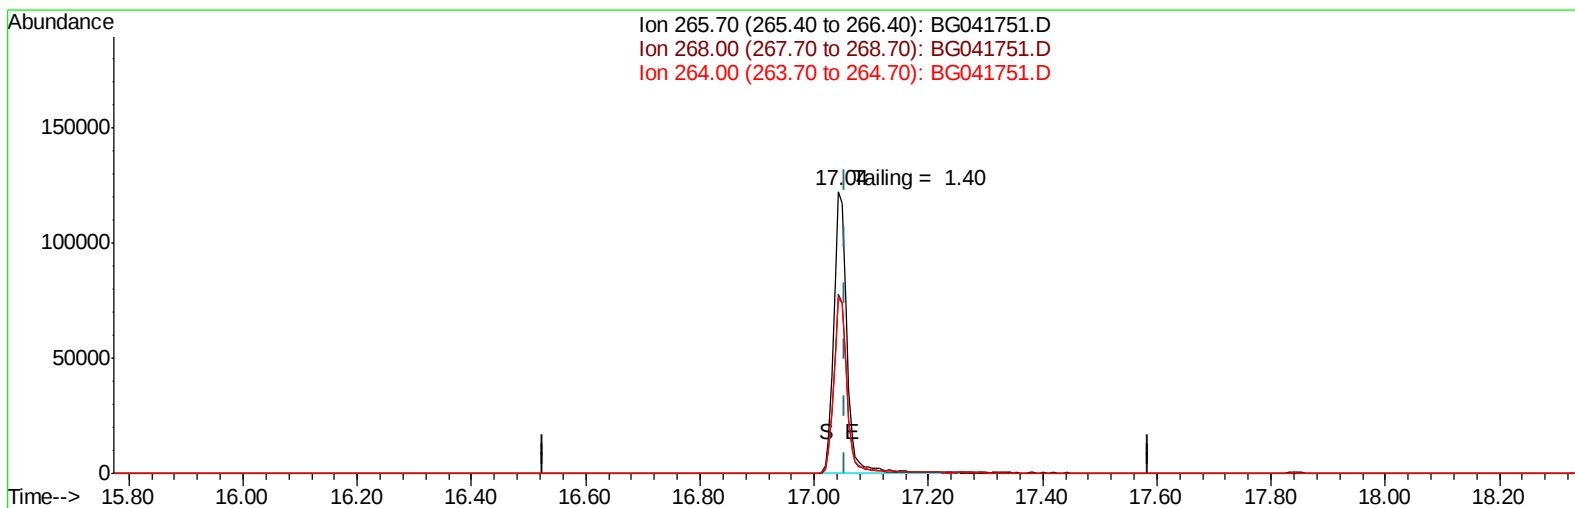

TIC: BG041751.D

(70) Pentachlorophenol (C)



17.043min (-0.013) 122983.39ng

response 192566

Ion	Exp%	Act%
265.70	100	100
268.00	66.10	63.46
264.00	64.30	62.24
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072319\  
Data File : BG041751.D  
Acq On    : 23 Jul 2019  10:03  
Operator  : HP/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Quant Time: Jul 24 08:39:14 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 15 16:16:21 2019
Response via : Initial Calibration

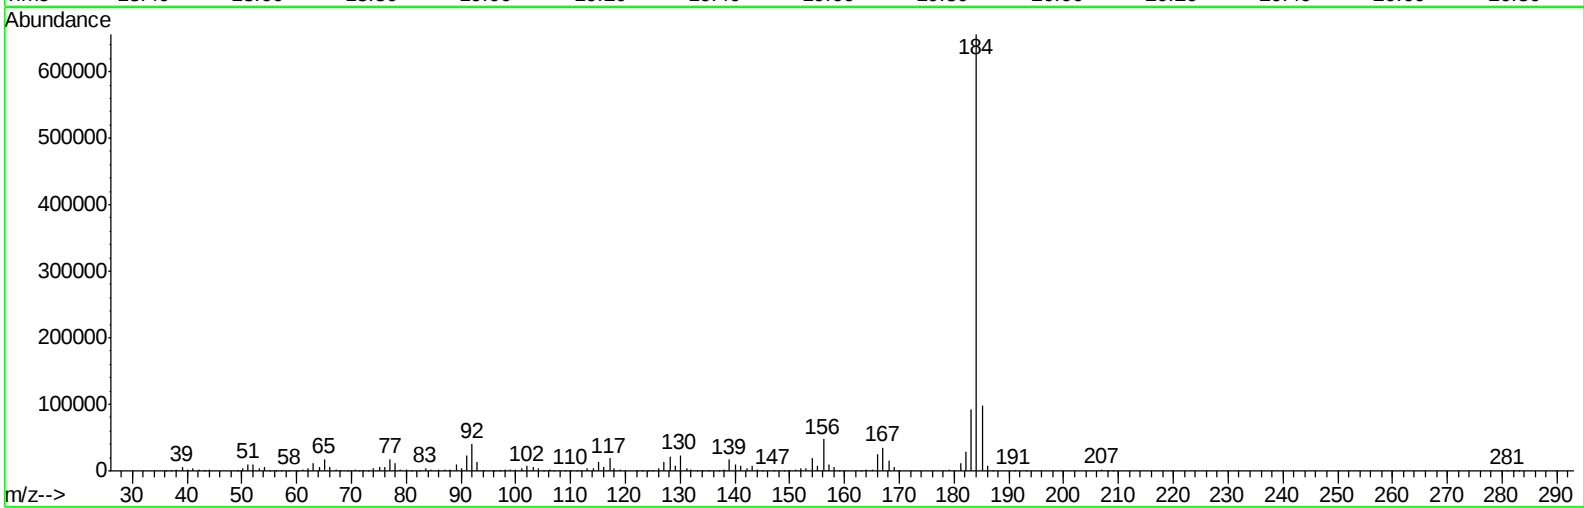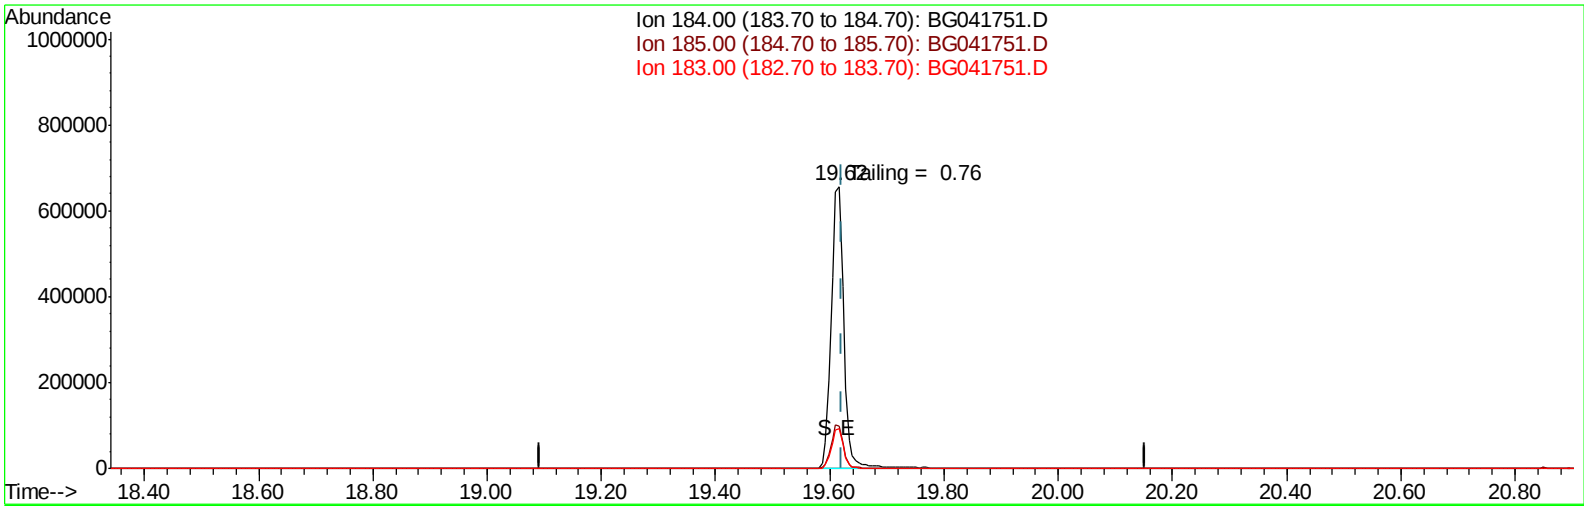

TIC: BG041751.D

(77) Benzidine

19.616min (-0.007) -20.00ng

response 997797

Ion	Exp%	Act%
184.00	100	100
185.00	16.20	15.07
183.00	14.70	14.10
0.00	0.00	0.00