


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG072319\
 Data File : BG041751.D
 Acq On : 23 Jul 2019 10:03
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 15 16:16:21 2019

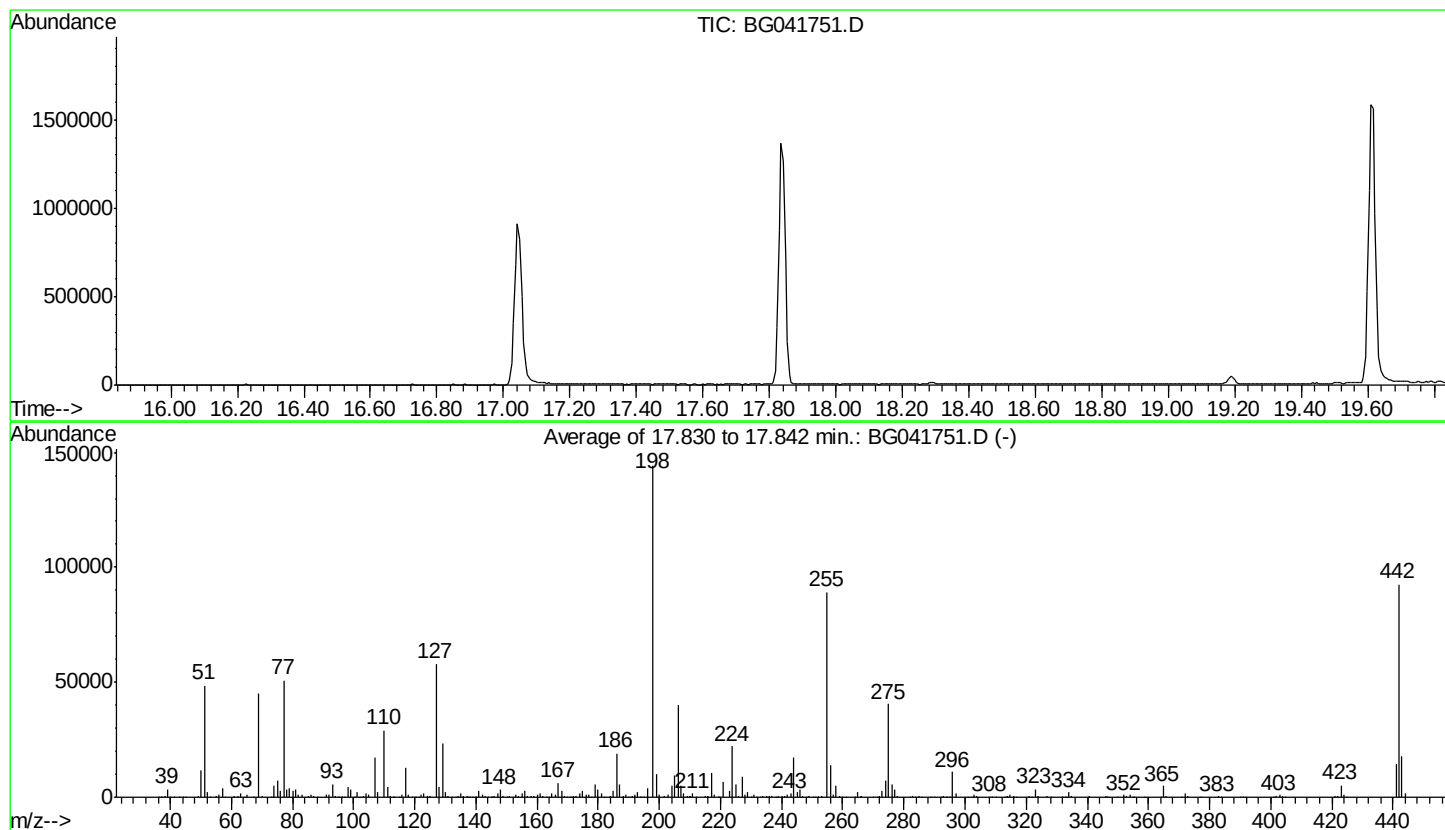

AutoFind: Scans 2509, 2510, 2511; Background Corrected with Scan 2502

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.7	48557	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	31.4	45333	PASS
70	69	0.00	2	0.7	299	PASS
127	198	10	80	40.2	58005	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	144210	PASS
199	198	5	9	6.9	10013	PASS
275	198	10	60	28.1	40573	PASS
365	198	1	100	3.4	4923	PASS
441	198	0.01	100	10.2	14769	PASS
442	198	50	100	64.2	92512	PASS
443	442	15	24	19.4	17904	PASS