
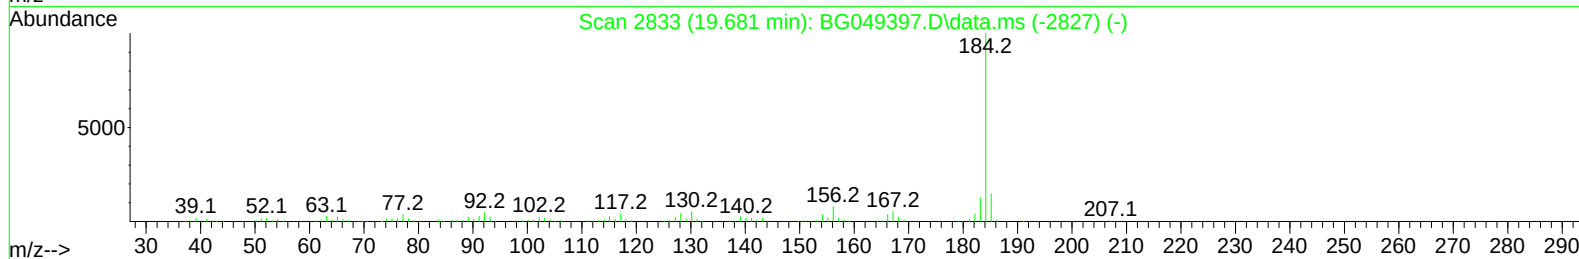
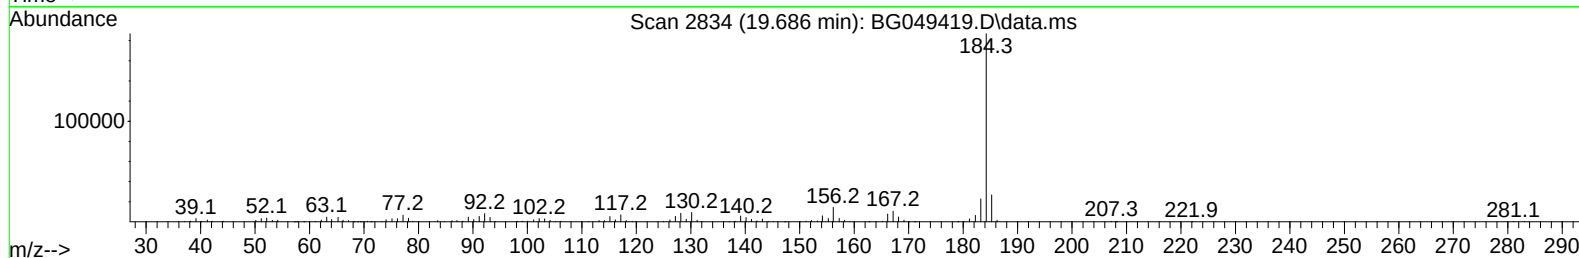


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072321\
Data File : BG049419.D
Acq On : 23 Jul 2021 8:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 23 11:08:38 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG072121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 21 16:57:05 2021
Response via : Initial Calibration

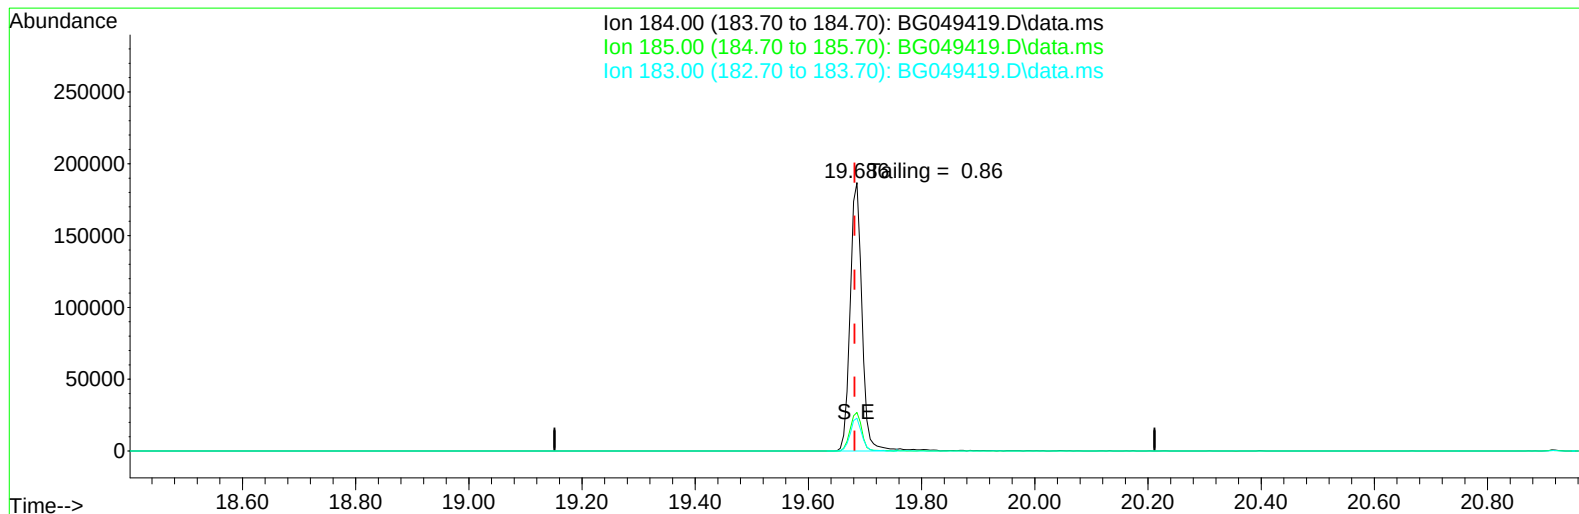




TIC: BG049419.D\data.ms

(77) Benzidine**19.686min (+ 0.004) 155743.99 ng****response 271562**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.40
183.00	11.70	12.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072321\
Data File : BG049419.D
Acq On : 23 Jul 2021 8:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 23 11:08:38 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG072121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 21 16:57:05 2021
Response via : Initial Calibration

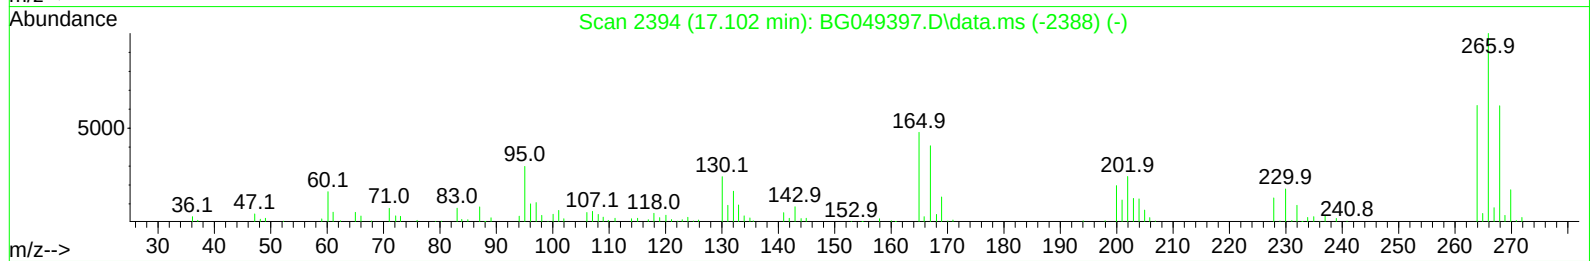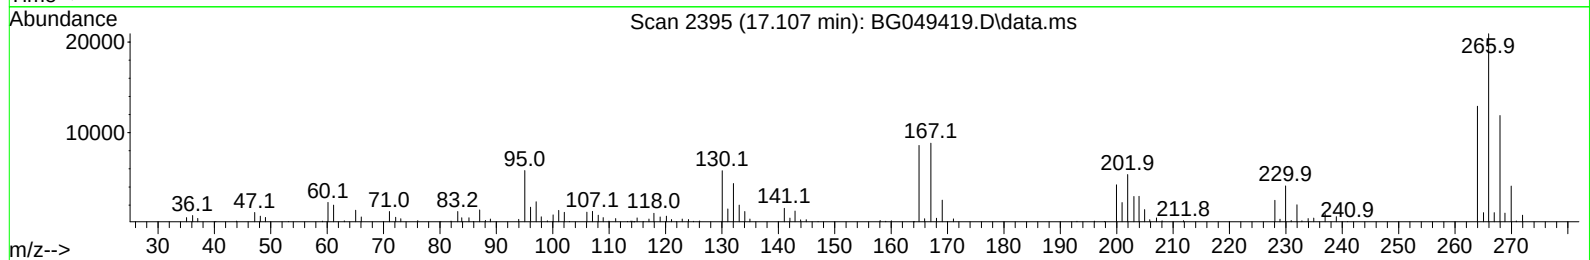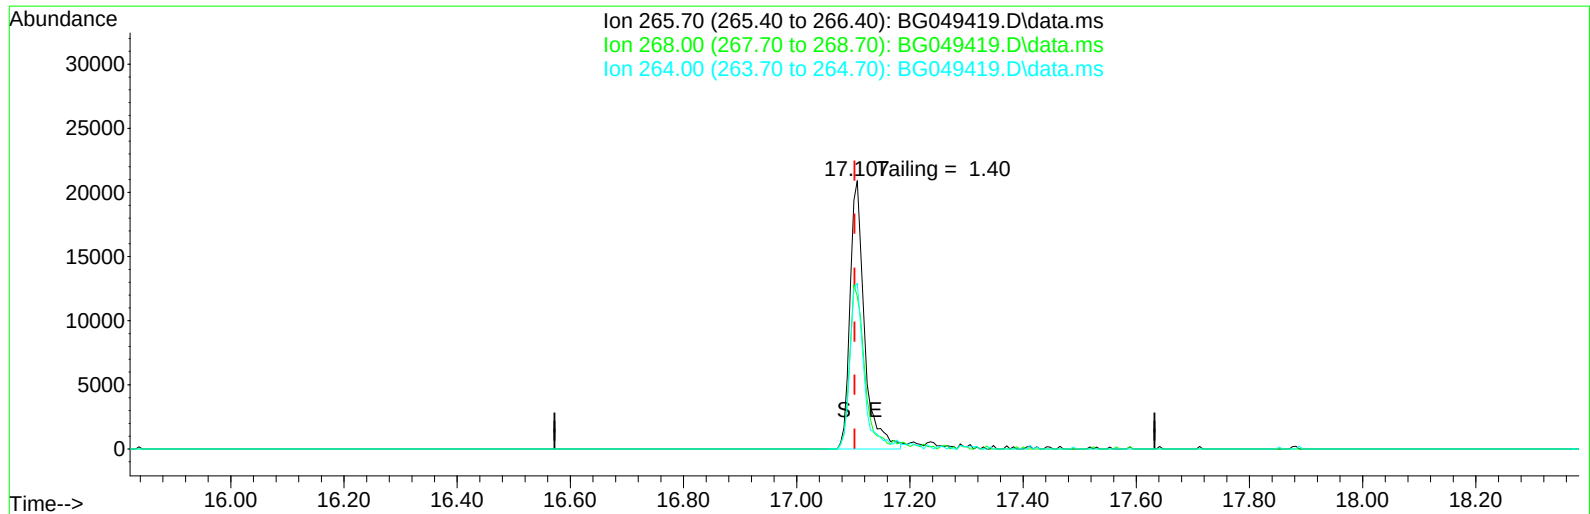

TIC: BG049419.D\data.ms

(70) Pentachlorophenol (C)

17.107min (+ 0.005) 63711.79 ng

response 37549

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	56.86
264.00	61.30	61.75
0.00	0.00	0.00