
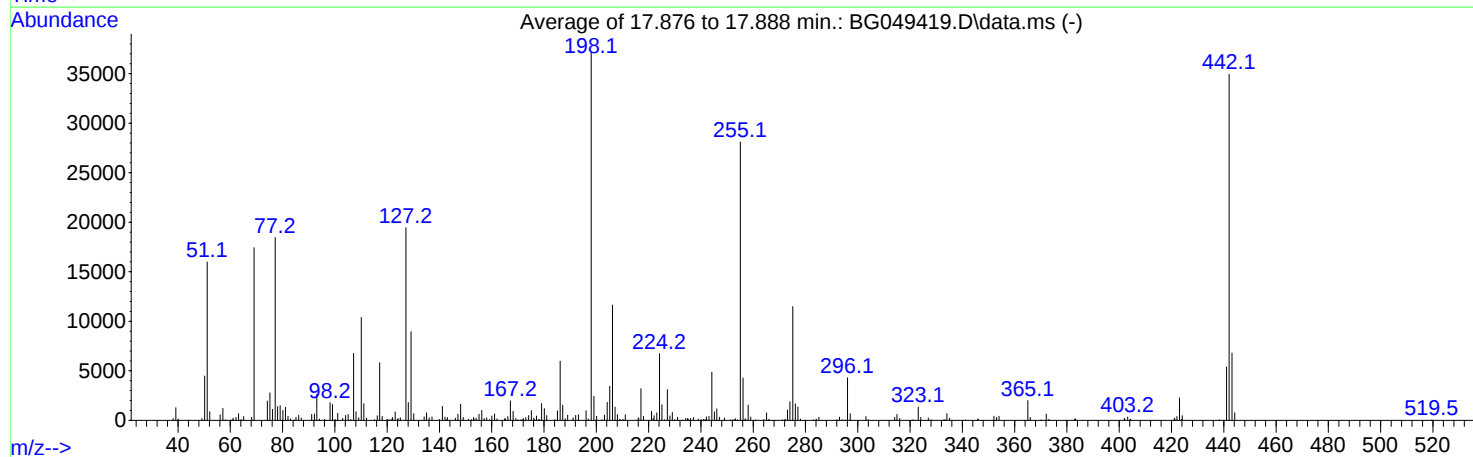


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072321\
 Data File : BG049419.D
 Acq On : 23 Jul 2021 8:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG072121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 21 16:57:05 2021

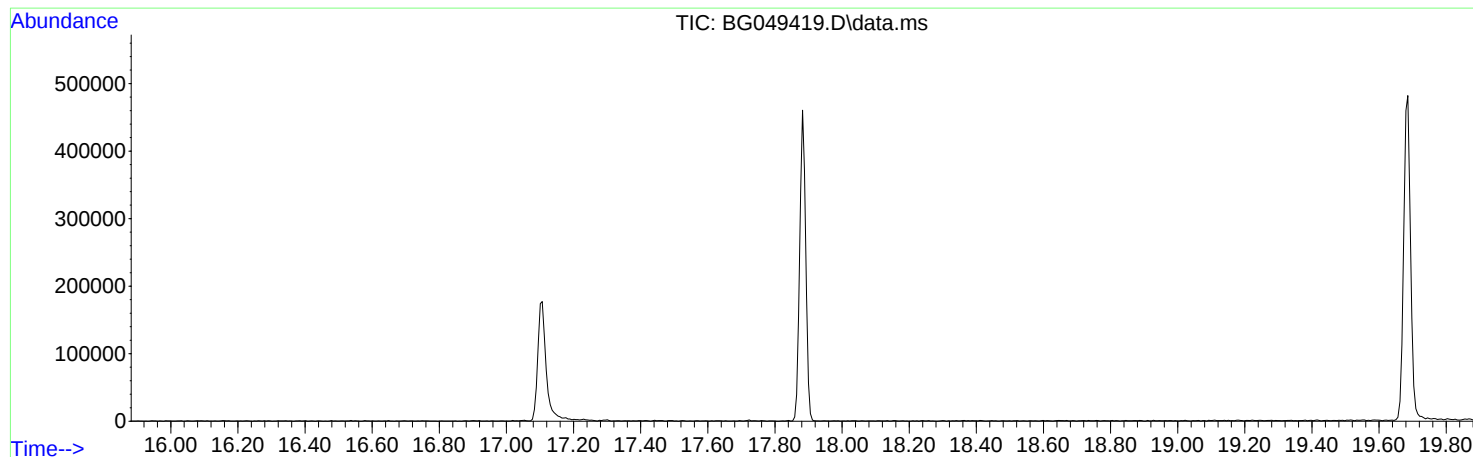




AutoFind: Scans 2526, 2527, 2528; Background Corrected with Scan 2520

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.1	15988	PASS
68	69	0.00	2	1.8	306	PASS
69	198	0.00	100	47.0	17436	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.4	19440	PASS
197	198	0.00	2	0.4	138	PASS
198	198	100	100	100.0	37133	PASS
199	198	5	9	6.6	2433	PASS
275	198	10	60	31.0	11493	PASS
365	198	1	100	5.4	2003	PASS
441	198	0.01	100	14.5	5390	PASS
442	442	100	100	100.0	34941	PASS
443	442	15	24	19.5	6804	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072321\
Data File : BG049419.D
Acq On : 23 Jul 2021 8:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 23 11:08:38 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG072121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 21 16:57:05 2021
Response via : Initial Calibration

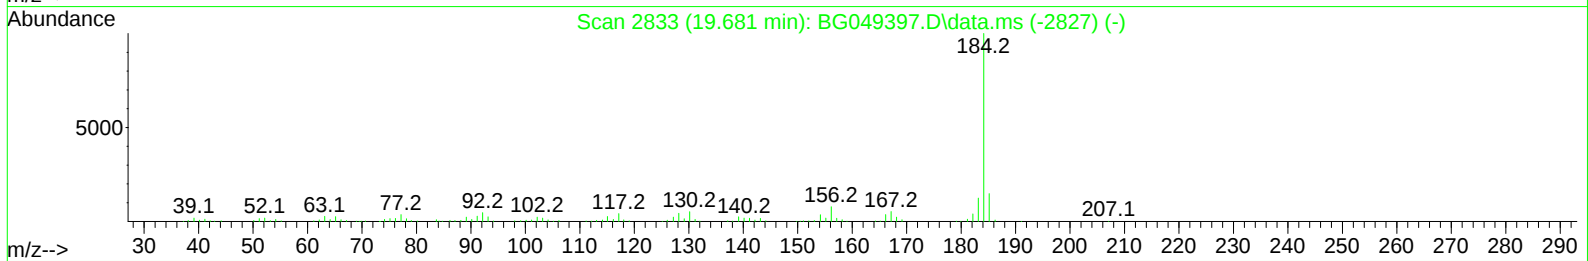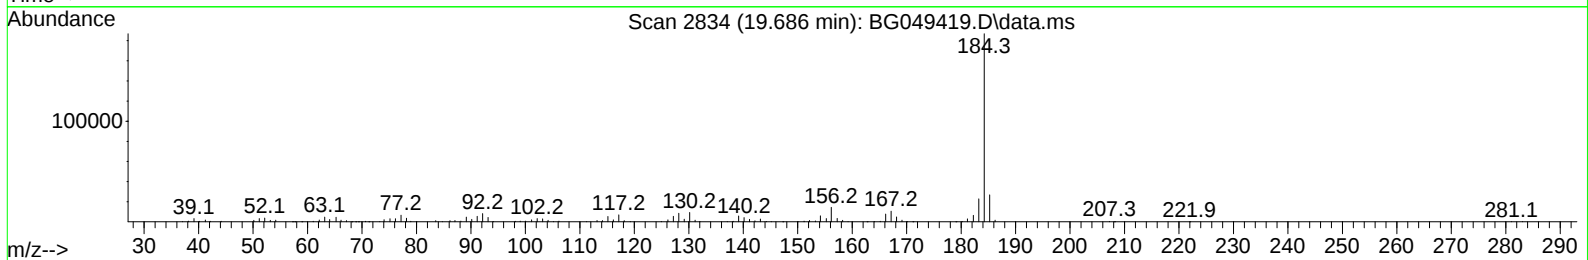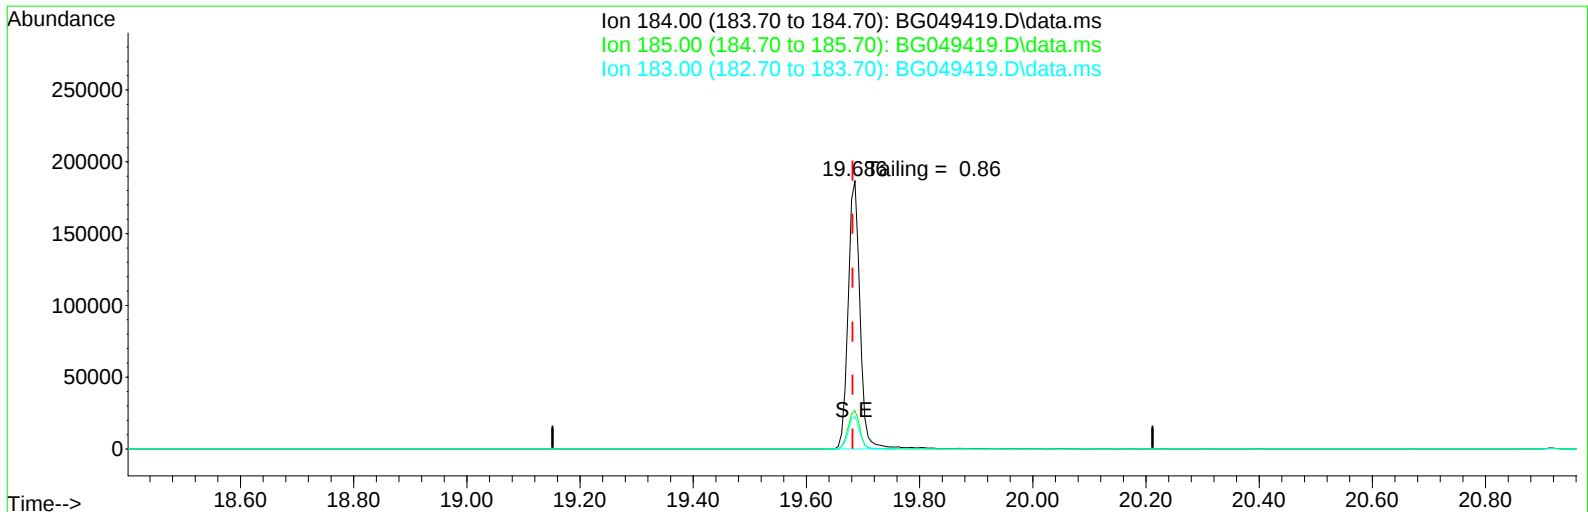

TIC: BG049419.D\data.ms

(77) Benzidine

19.686min (+ 0.004) 155743.99 ng




response 271562

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.40
183.00	11.70	12.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072321\
Data File : BG049419.D
Acq On : 23 Jul 2021 8:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 23 11:08:38 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG072121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 21 16:57:05 2021
Response via : Initial Calibration

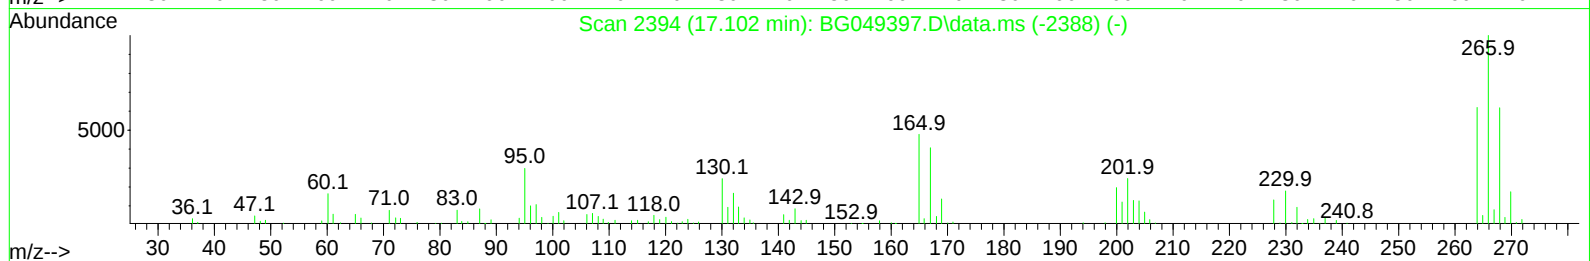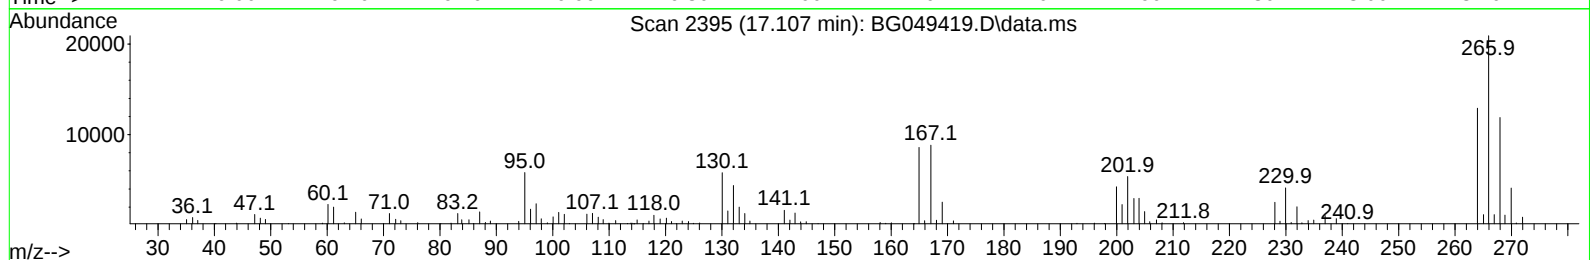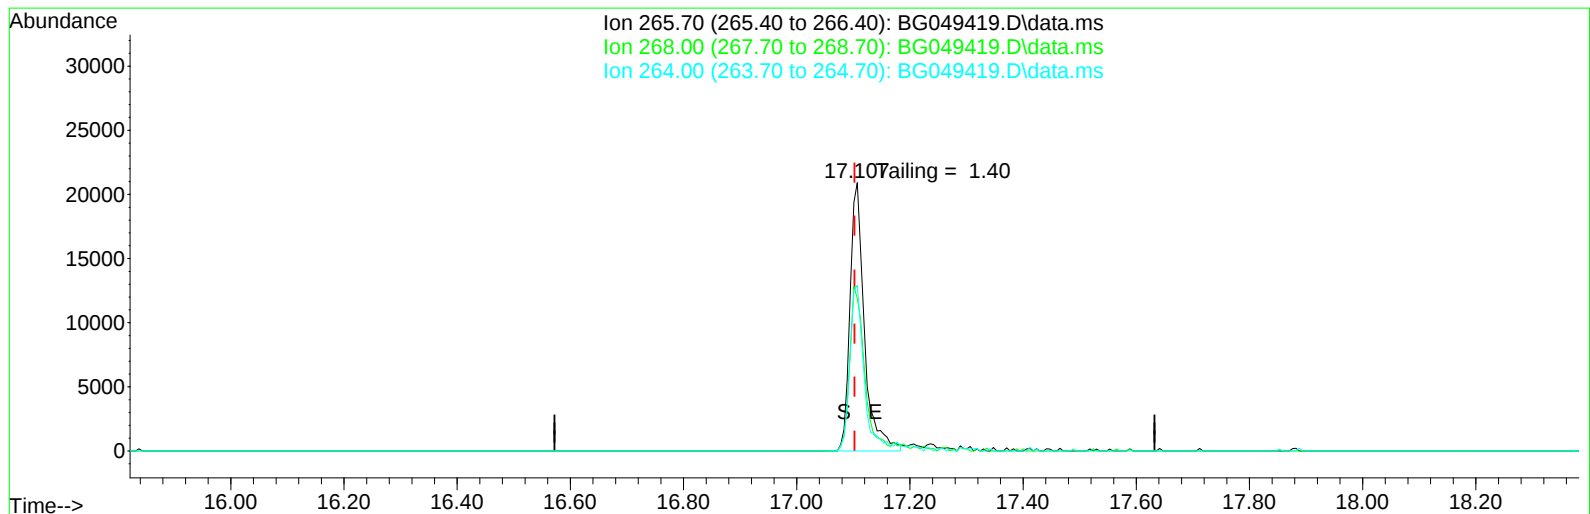

TIC: BG049419.D\data.ms

(70) Pentachlorophenol (C)

17.107min (+ 0.005) 63711.79 ng

response 37549

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	56.86
264.00	61.30	61.75
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/23/2021	BNA_G	BG049419.D
Compound Name	Response	Retention Time
DDT	141114	20.91
DDD	1354	20.47
DDE	0	19.96
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1354	142468	0.95

Instrument :
BNA_G
ClientSampleId :
DFTPP