

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072324\
 Data File : BG062189.D
 Acq On : 23 Jul 2024 17:14
 Operator : MA/JU
 Sample : PB162104BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK104

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062189.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.459	26	29	34	rVB4	9389	12432	0.77%	0.076%
2	3.793	84	86	89	rVB2	2596	2569	0.16%	0.016%
3	3.876	96	100	114	rBV	145657	241709	15.05%	1.487%
4	4.210	155	157	161	rVB	4172	4295	0.27%	0.026%
5	4.604	221	224	230	rBV2	2208	4238	0.26%	0.026%
6	5.009	291	293	296	rBV	2534	2632	0.16%	0.016%
7	5.039	296	298	302	rBV4	1806	2796	0.17%	0.017%
8	6.161	486	489	492	rBV	2022	2709	0.17%	0.017%
9	6.637	567	570	573	rBV	2575	3155	0.20%	0.019%
10	6.783	592	595	597	rBV	1837	2165	0.13%	0.013%
11	7.236	665	672	681	rBV	216216	375325	23.37%	2.309%
12	7.388	690	698	704	rBV	127939	211589	13.18%	1.302%
13	7.600	728	734	742	rBV	189037	314031	19.56%	1.932%
14	7.735	753	757	760	rBV	1654	2188	0.14%	0.013%
15	8.064	806	813	821	rVB	173170	293805	18.30%	1.808%
16	8.781	927	935	947	rBV2	262331	455010	28.33%	2.799%
17	9.233	1004	1012	1020	rBV	204343	367942	22.91%	2.264%
18	9.956	1127	1135	1145	rBV	199715	351138	21.87%	2.160%
19	10.502	1222	1228	1238	rBV	295469	526615	32.79%	3.240%
20	10.878	1285	1292	1302	rVB	254512	464213	28.91%	2.856%
21	11.013	1309	1315	1323	rBV	264367	483250	30.09%	2.973%
22	11.583	1408	1412	1413	rBV	2744	2187	0.14%	0.013%
23	11.700	1430	1432	1436	rBV	2099	3172	0.20%	0.020%
24	12.041	1487	1490	1494	rBV	2009	2207	0.14%	0.014%
25	12.235	1519	1523	1526	rBV	2104	2979	0.19%	0.018%
26	12.452	1556	1560	1564	rBV2	4520	7051	0.44%	0.043%
27	12.605	1584	1586	1589	rBV	1777	2314	0.14%	0.014%
28	12.734	1606	1608	1613	rVB	2303	3096	0.19%	0.019%
29	13.833	1793	1795	1799	rVB	1676	2268	0.14%	0.014%
30	13.980	1817	1820	1824	rVB	1711	2735	0.17%	0.017%
31	14.021	1824	1827	1828	rBV	2001	2178	0.14%	0.013%
32	14.091	1833	1839	1845	rVB	561874	809305	50.40%	4.979%
33	14.338	1877	1881	1883	rBV	1568	2331	0.15%	0.014%
34	14.391	1883	1890	1899	rVV	585492	912479	56.82%	5.614%
35	14.514	1906	1911	1912	rBV	1864	2319	0.14%	0.014%
36	14.690	1934	1941	1950	rBV	488626	760733	47.37%	4.680%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072324\
 Data File : BG062189.D
 Acq On : 23 Jul 2024 17:14
 Operator : MA/JU
 Sample : PB162104BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK104

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071924.MA.M
 Title : SVOA CALIBRATION

37	14.919	1973	1980	1992	rBV	204174	363707	22.65%	2.238%
38	15.372	2051	2057	2058	rBV2	1887	2520	0.16%	0.016%
39	15.466	2070	2073	2074	rBV	2757	2714	0.17%	0.017%
40	15.683	2103	2110	2118	rBV	791612	1196461	74.51%	7.361%
41	15.806	2125	2131	2138	rBV	215657	317023	19.74%	1.950%
42	15.918	2146	2150	2153	rVB2	4304	7572	0.47%	0.047%
43	15.965	2156	2158	2162	rBV	2173	2369	0.15%	0.015%
44	16.135	2185	2187	2192	rVB	2886	3361	0.21%	0.021%
45	16.576	2260	2262	2265	rBV	2302	2287	0.14%	0.014%
46	16.711	2283	2285	2286	rBV	3429	2667	0.17%	0.016%
47	16.840	2304	2307	2308	rBV	2554	2527	0.16%	0.016%
48	16.870	2311	2312	2316	rBV	1762	2285	0.14%	0.014%
49	17.028	2337	2339	2342	rVB	3151	2990	0.19%	0.018%
50	17.105	2349	2352	2357	rVB2	2769	3354	0.21%	0.021%
51	17.340	2390	2392	2394	rBV	2610	2145	0.13%	0.013%
52	17.440	2402	2409	2415	rVB	665919	1027302	63.97%	6.320%
53	17.534	2419	2425	2432	rVV	904457	1381744	86.05%	8.501%
54	17.633	2440	2442	2444	rBV3	3838	3731	0.23%	0.023%
55	17.692	2450	2452	2456	rVB2	2795	2974	0.19%	0.018%
56	17.727	2456	2458	2459	rBV2	3058	2236	0.14%	0.014%
57	17.851	2477	2479	2484	rVB3	3121	3749	0.23%	0.023%
58	17.904	2484	2488	2491	rBV3	2431	3613	0.22%	0.022%
59	18.056	2513	2514	2515	rBV	5633	2494	0.16%	0.015%
60	18.238	2543	2545	2548	rBV3	2871	2244	0.14%	0.014%
61	18.679	2618	2620	2622	rBV3	4631	3807	0.24%	0.023%
62	18.849	2645	2649	2650	rBV3	3886	4231	0.26%	0.026%
63	19.002	2674	2675	2676	rBV	5736	2747	0.17%	0.017%
64	19.819	2808	2814	2822	rVB2	1096689	1605827	100.00%	9.880%
65	21.699	3128	3134	3143	rVB2	678099	1088625	67.79%	6.698%
66	24.712	3638	3647	3656	rVB2	527846	1477194	91.99%	9.088%
67	24.935	3676	3685	3696	rVB2	373278	1086342	67.65%	6.684%


Sum of corrected areas: 16254002

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072324\
Data File : BG062189.D
Acq On : 23 Jul 2024 17:14
Operator : MA/JU
Sample : PB162104BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK104

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

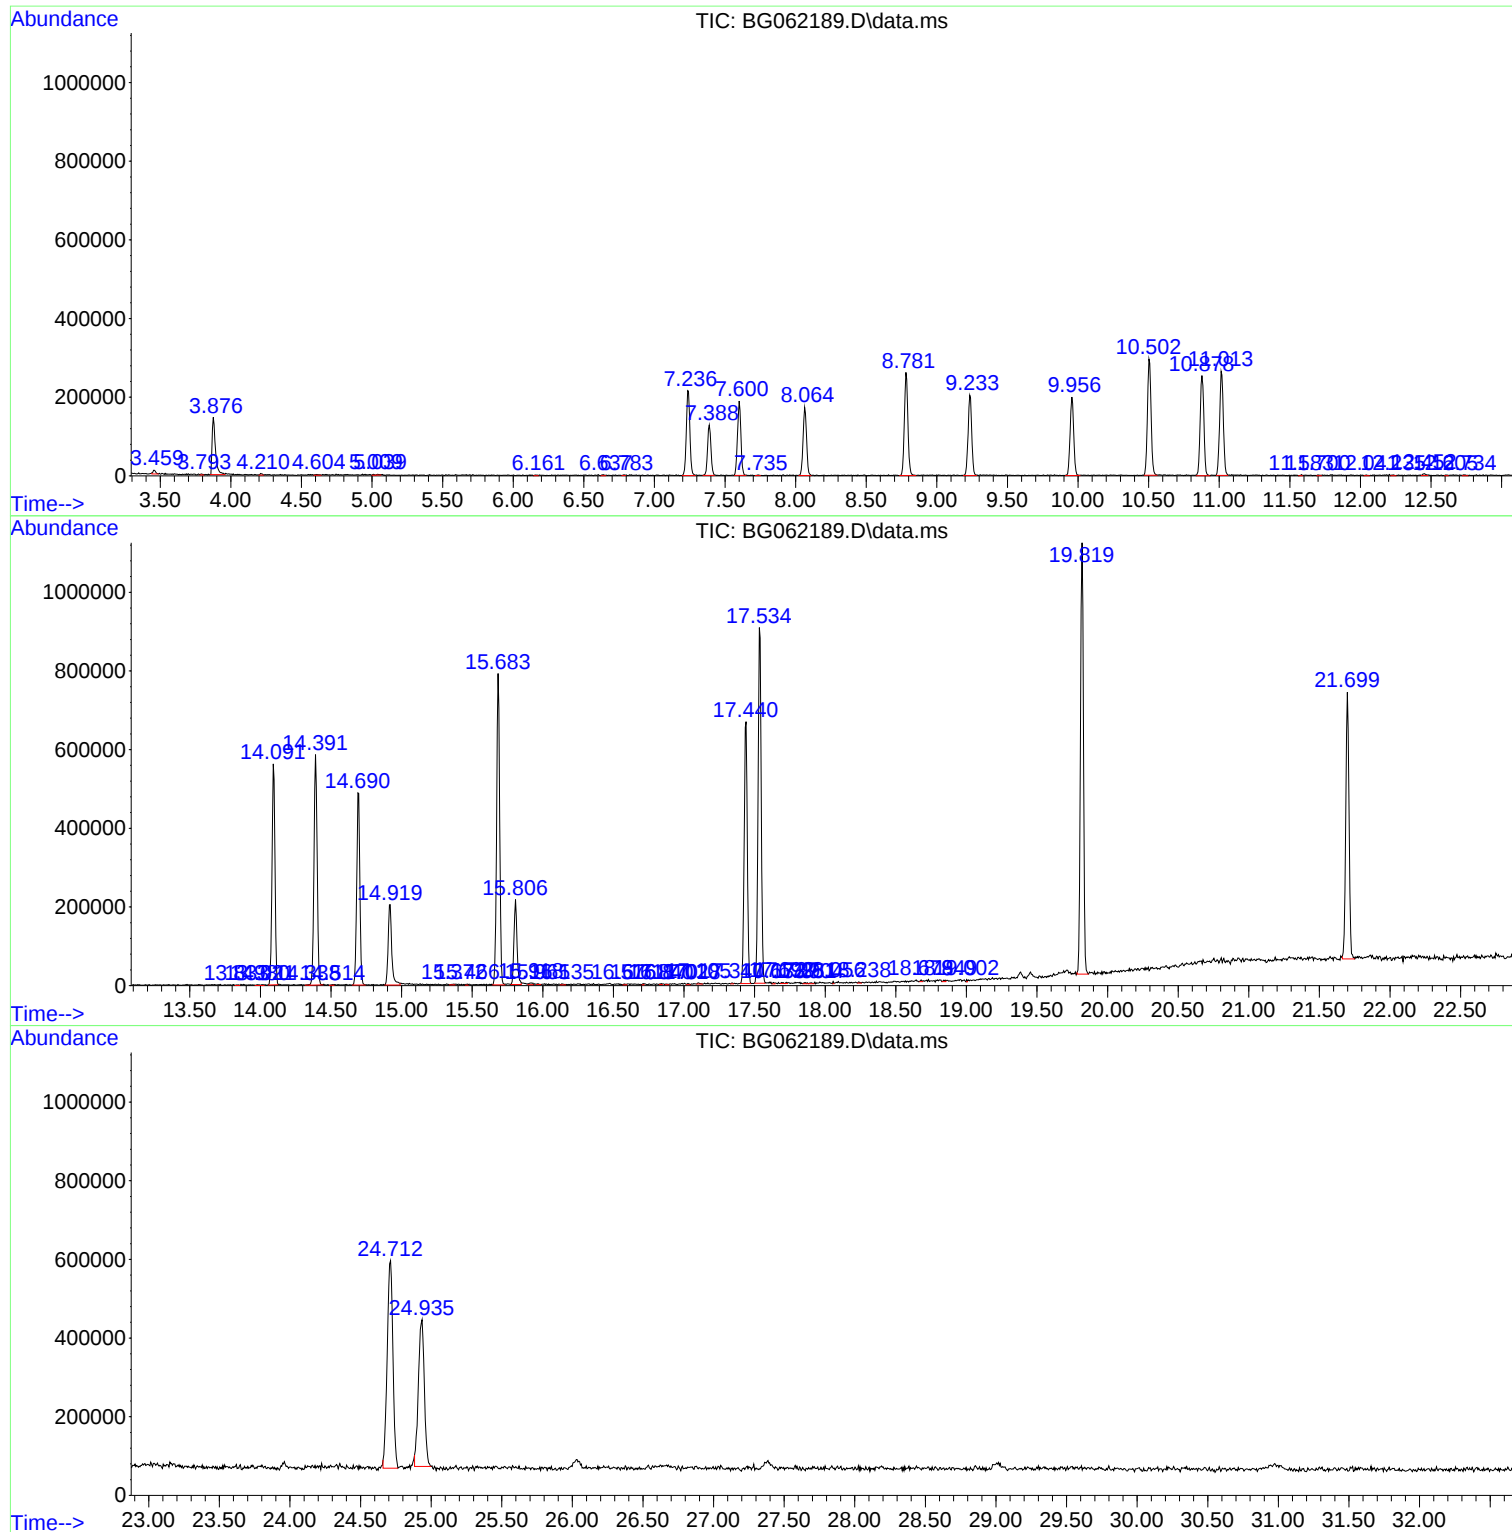

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072324\
Data File : BG062189.D
Acq On : 23 Jul 2024 17:14
Operator : MA/JU
Sample : PB162104BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK104

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072324\
Data File : BG062189.D
Acq On : 23 Jul 2024 17:14
Operator : MA/JU
Sample : PB162104BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK104

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc