

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072324\
 Data File : BG062202.D
 Acq On : 24 Jul 2024 2:05
 Operator : MA/JU
 Sample : P3244-08
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YDZF9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062202.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.458	26	29	36	rVB5	10461	18701	1.30%	0.146%
2	3.805	86	88	90	rBV2	3024	3033	0.21%	0.024%
3	3.887	99	102	111	rBV	62465	101388	7.02%	0.793%
4	4.152	146	147	150	rBV	2513	2445	0.17%	0.019%
5	4.187	150	153	155	rVV3	2495	2769	0.19%	0.022%
6	5.015	292	294	298	rBV	1354	2265	0.16%	0.018%
7	5.133	310	314	316	rBV4	3640	3770	0.26%	0.029%
8	5.315	343	345	348	rBV2	1923	2331	0.16%	0.018%
9	5.779	423	424	428	rVB	3293	2204	0.15%	0.017%
10	6.607	560	565	567	rBV	1304	2072	0.14%	0.016%
11	6.983	626	629	632	rBV	2101	2075	0.14%	0.016%
12	7.253	668	675	681	rBV	71428	122494	8.48%	0.958%
13	7.388	692	698	708	rVB	112666	188830	13.08%	1.476%
14	7.606	727	735	745	rBV2	161846	275754	19.10%	2.156%
15	7.835	770	774	777	rBV2	2241	2863	0.20%	0.022%
16	7.988	797	800	802	rVB2	2562	2327	0.16%	0.018%
17	8.064	807	813	820	rVV	155021	268015	18.56%	2.095%
18	8.140	824	826	830	rVB2	1841	2093	0.14%	0.016%
19	8.311	854	855	859	rBV	2784	2651	0.18%	0.021%
20	8.352	859	862	865	rBV	1649	2235	0.15%	0.017%
21	8.792	930	937	945	rBV	194992	323896	22.43%	2.532%
22	8.875	948	951	954	rVB	2174	2640	0.18%	0.021%
23	8.916	954	958	960	rBV2	1599	2204	0.15%	0.017%
24	8.969	965	967	969	rBV	2525	2196	0.15%	0.017%
25	9.239	1004	1013	1020	rBV	186649	326684	22.63%	2.554%
26	9.350	1030	1032	1034	rBV	2947	2112	0.15%	0.017%
27	9.380	1034	1037	1039	rVB	1906	2179	0.15%	0.017%
28	9.638	1078	1081	1084	rBV2	1684	2245	0.16%	0.018%
29	9.762	1098	1102	1103	rBV	2040	2223	0.15%	0.017%
30	9.785	1103	1106	1108	rVV2	2931	3085	0.21%	0.024%
31	9.961	1127	1136	1143	rVB2	173509	316922	21.95%	2.477%
32	10.267	1184	1188	1191	rBV	1792	2884	0.20%	0.023%
33	10.361	1203	1204	1207	rBV	2392	2095	0.15%	0.016%
34	10.514	1222	1230	1238	rBV	280621	497309	34.45%	3.888%
35	10.566	1238	1239	1242	rVB	3117	2178	0.15%	0.017%
36	10.884	1285	1293	1301	rVB	231185	420421	29.12%	3.287%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072324\
 Data File : BG062202.D
 Acq On : 24 Jul 2024 2:05
 Operator : MA/JU
 Sample : P3244-08
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YDZF9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071924.MA.M
 Title : SVOA CALIBRATION

37	11.025	1309	1317	1329	rVB	202266	378346	26.21%	2.958%
38	11.113	1329	1332	1335	rBV	1506	2043	0.14%	0.016%
39	11.230	1350	1352	1356	rVB	2883	3201	0.22%	0.025%
40	11.265	1356	1358	1361	rBV	1880	2641	0.18%	0.021%
41	11.612	1410	1417	1423	rBV4	12492	26484	1.83%	0.207%
42	11.823	1451	1453	1456	rBV	1966	2836	0.20%	0.022%
43	11.917	1465	1469	1471	rBV2	1673	2043	0.14%	0.016%
44	12.082	1496	1497	1502	rBV	2224	2164	0.15%	0.017%
45	12.229	1520	1522	1526	rVB	2196	2063	0.14%	0.016%
46	12.317	1535	1537	1540	rBV	2868	2909	0.20%	0.023%
47	12.458	1553	1561	1562	rBV2	7070	10235	0.71%	0.080%
48	12.540	1573	1575	1580	rVB2	3354	4033	0.28%	0.032%
49	12.899	1635	1636	1638	rBV	3149	2003	0.14%	0.016%
50	12.951	1642	1645	1647	rBV	2116	2871	0.20%	0.022%
51	13.075	1663	1666	1667	rBV2	1652	2036	0.14%	0.016%
52	13.192	1683	1686	1690	rBV2	2302	3324	0.23%	0.026%
53	13.327	1706	1709	1712	rBV2	2089	2846	0.20%	0.022%
54	13.368	1712	1716	1719	rVB4	2947	3609	0.25%	0.028%
55	13.410	1722	1723	1725	rBV	2741	2276	0.16%	0.018%
56	13.492	1733	1737	1744	rVB2	29527	45434	3.15%	0.355%
57	13.556	1744	1748	1749	rBV	3121	3321	0.23%	0.026%
58	13.650	1761	1764	1768	rBV2	2648	3368	0.23%	0.026%
59	13.727	1774	1777	1779	rBV2	4081	3620	0.25%	0.028%
60	13.768	1783	1784	1788	rVB2	2998	2756	0.19%	0.022%
61	13.838	1793	1796	1797	rBV	2141	2421	0.17%	0.019%
62	14.003	1822	1824	1825	rBV	2731	2244	0.16%	0.018%
63	14.050	1830	1832	1834	rVV	3472	3829	0.27%	0.030%
64	14.097	1834	1840	1848	rVB	525399	772999	53.54%	6.043%
65	14.273	1868	1870	1872	rVB	4000	2010	0.14%	0.016%
66	14.302	1872	1875	1877	rBV4	2504	2508	0.17%	0.020%
67	14.391	1884	1890	1896	rBV2	505144	817262	56.61%	6.389%
68	14.455	1899	1901	1903	rVB	3391	2080	0.14%	0.016%
69	14.561	1915	1919	1925	rVB3	17914	26246	1.82%	0.205%
70	14.614	1927	1928	1931	rBV2	3115	3513	0.24%	0.027%
71	14.696	1936	1942	1950	rVB	414134	649871	45.01%	5.080%
72	14.749	1950	1951	1953	rBV2	3100	2074	0.14%	0.016%
73	14.843	1965	1967	1968	rBV2	3556	2286	0.16%	0.018%
74	14.937	1978	1983	1990	rBV2	40599	72853	5.05%	0.570%
75	15.019	1995	1997	1998	rBV2	5051	3111	0.22%	0.024%
76	15.113	2009	2013	2014	rBV2	2894	3308	0.23%	0.026%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072324\
 Data File : BG062202.D
 Acq On : 24 Jul 2024 2:05
 Operator : MA/JU
 Sample : P3244-08
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YDZF9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071924.MA.M
 Title : SVOA CALIBRATION

77	15.148	2014	2019	2024	rVV2	31383	43483	3.01%	0.340%
78	15.272	2037	2040	2044	rVB4	8126	11332	0.78%	0.089%
79	15.407	2060	2063	2064	rBV3	3281	3454	0.24%	0.027%
80	15.513	2077	2081	2086	rBV4	8331	12293	0.85%	0.096%
81	15.689	2104	2111	2117	rBV	705766	1073681	74.37%	8.393%
82	15.818	2128	2133	2142	rBV2	100239	201653	13.97%	1.576%
83	15.965	2156	2158	2160	rBV3	6774	6791	0.47%	0.053%
84	16.229	2201	2203	2204	rBV2	4981	3689	0.26%	0.029%
85	16.265	2207	2209	2212	rVV4	5708	3733	0.26%	0.029%
86	16.364	2224	2226	2232	rBV6	5020	6309	0.44%	0.049%
87	16.488	2246	2247	2250	rBV2	5161	4866	0.34%	0.038%
88	16.611	2266	2268	2270	rBV3	4871	4616	0.32%	0.036%
89	16.699	2279	2283	2290	rVB2	21307	33392	2.31%	0.261%
90	17.034	2338	2340	2343	rBV4	8652	6709	0.46%	0.052%
91	17.439	2403	2409	2416	rVB	538232	823455	57.04%	6.437%
92	17.539	2420	2426	2433	rBV	830835	1234586	85.51%	9.651%
93	19.824	2809	2815	2821	rVB	972324	1443737	100.00%	11.286%
94	21.704	3130	3135	3141	rVB2	497607	836023	57.91%	6.535%
95	24.718	3642	3648	3657	rVB2	490345	1231734	85.32%	9.629%




Sum of corrected areas: 12792201

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072324\
Data File : BG062202.D
Acq On : 24 Jul 2024 2:05
Operator : MA/JU
Sample : P3244-08
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YDZF9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

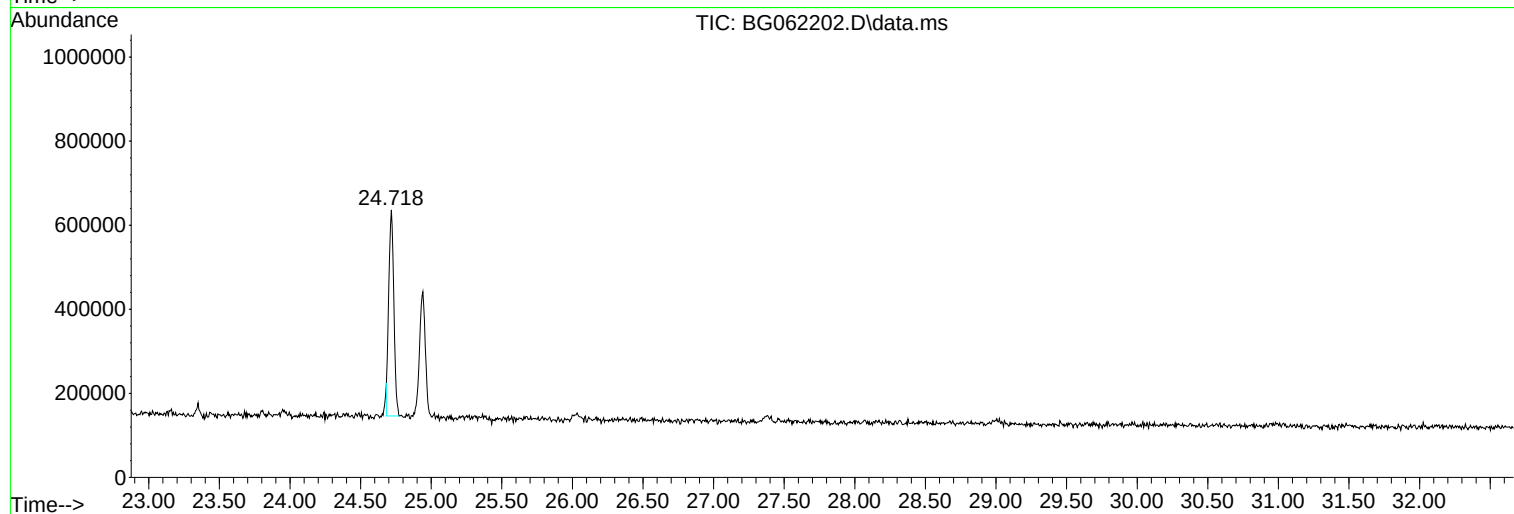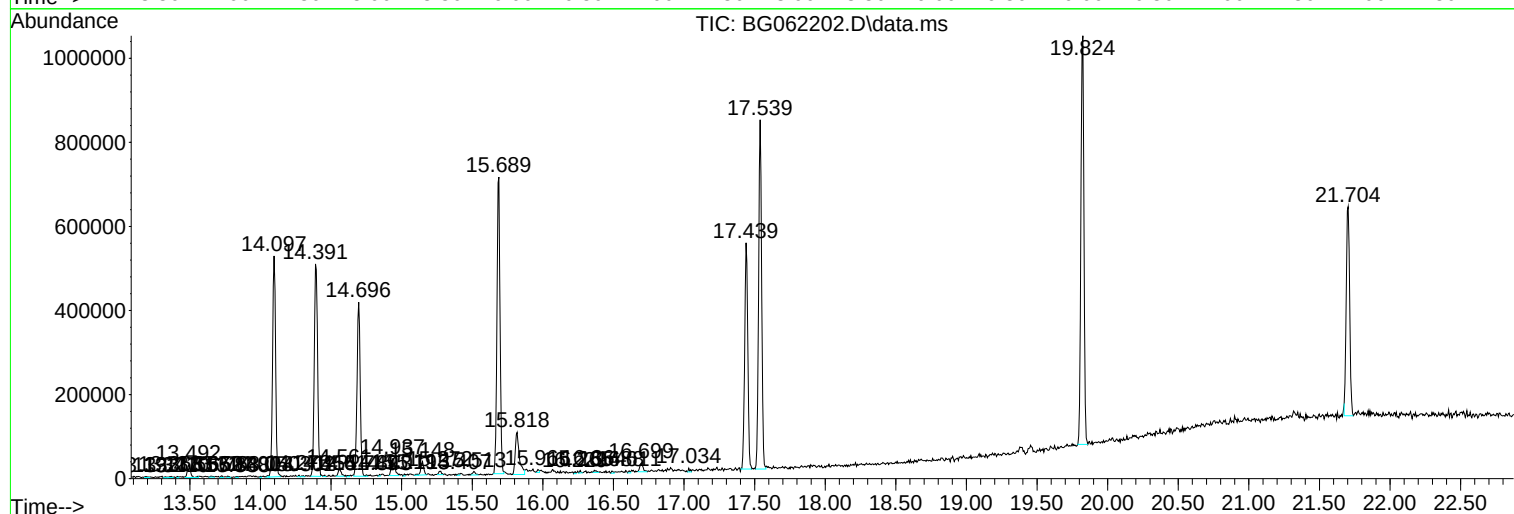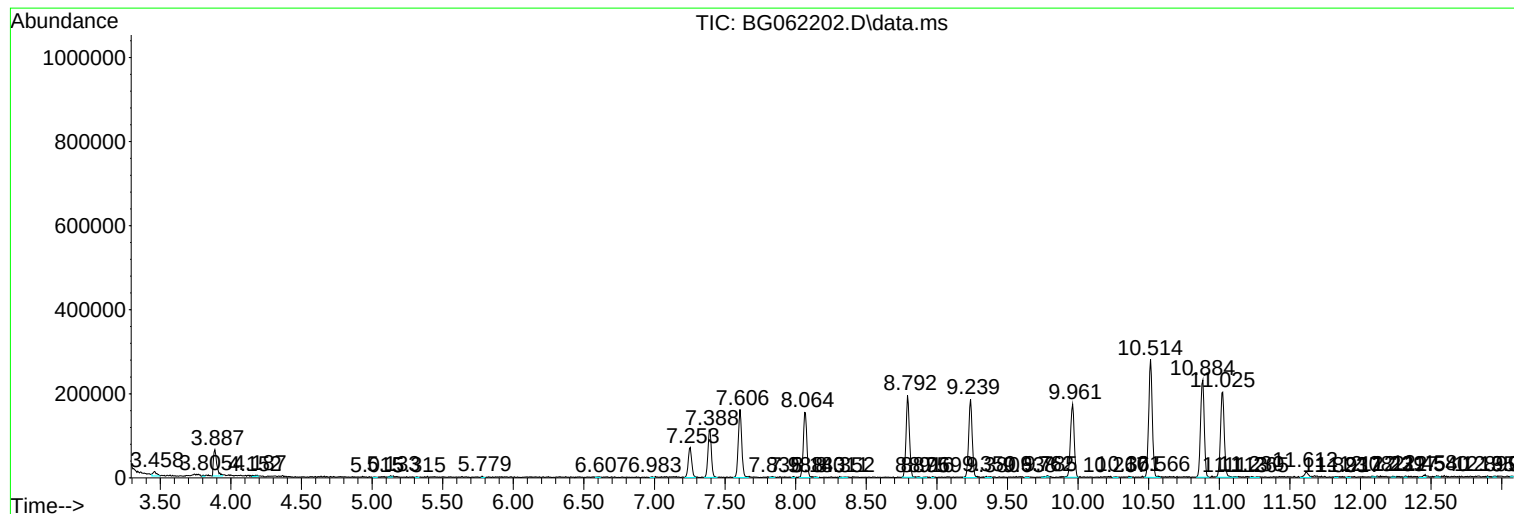

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072324\
Data File : BG062202.D
Acq On : 24 Jul 2024 2:05
Operator : MA/JU
Sample : P3244-08
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YDZF9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072324\
Data File : BG062202.D
Acq On : 24 Jul 2024 2:05
Operator : MA/JU
Sample : P3244-08
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YDZF9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc