


Data Path : Z:\HPCHEM1\BNA_G\Data\BG072415\
Data File : BG018094.D
Acq On : 24 Jul 2015 18:00
Operator : TP/UM
Sample : PB84428BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Jul 25 01:06:23 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG072315.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 24 23:53:51 2015
Response via : Initial Calibration

Instrument :
BNA_G
ClientSampleId :
SBLK88

Manual Integrations
APPROVED
apatel
7/27/2015 3:40:54 PM

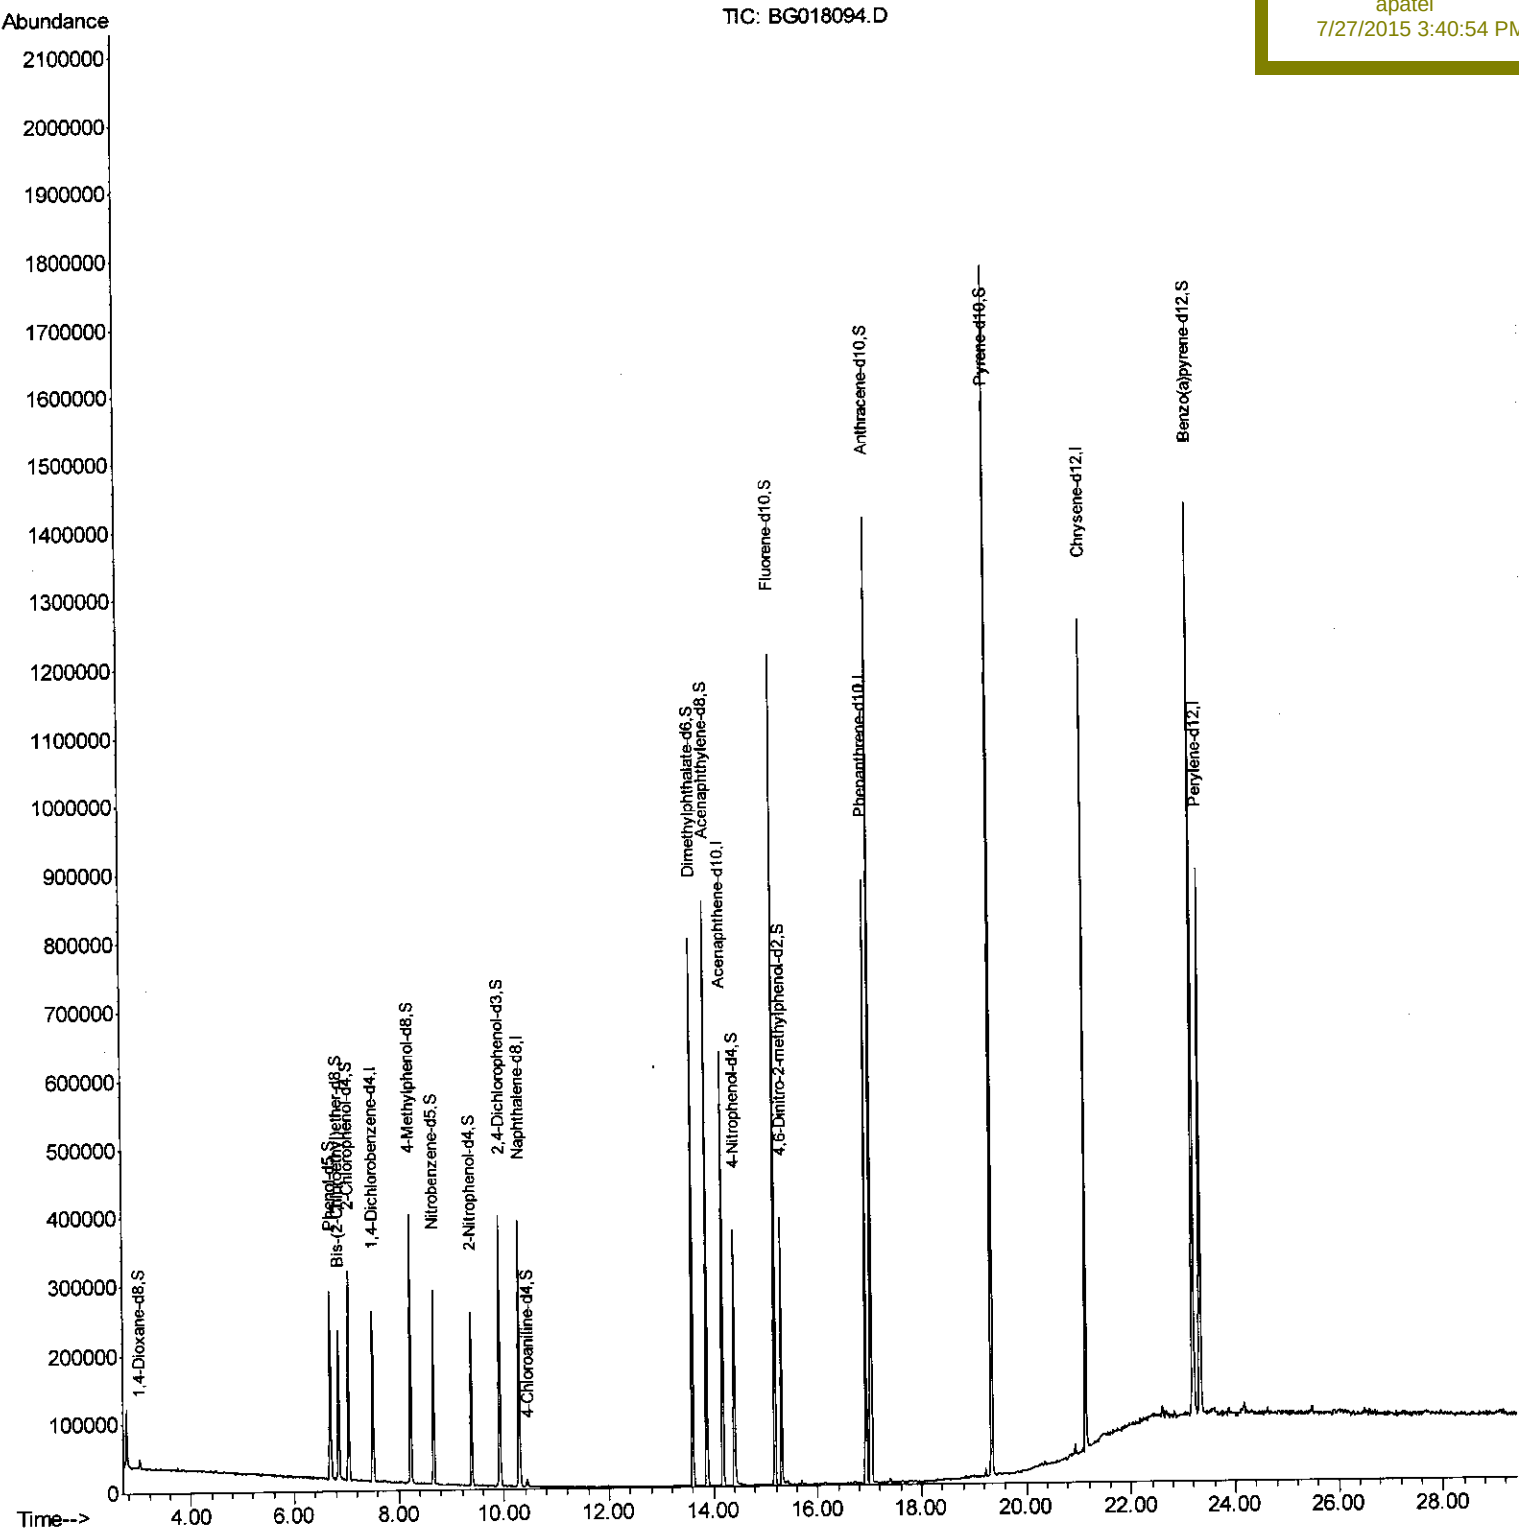

Data Path : Z:\HPCHEM1\BNA_G\Data\BG072415\
Data File : BG018094.D
Acq On : 24 Jul 2015 18:00
Operator : TP/UM
Sample : PB84428BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Jul 25 01:06:23 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG072315.M
Quant Title : SVOA CALIBRATION
Last Update : Fri Jul 24 23:53:51 2015
Response via : Initial Calibration

Instrument :
BNA_G
Client Sample ID :
SBLK88

Manual Integrations
APPROVED

apatel
7/27/2015 3:40:54 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.51	152	71469	20.00	ng/ul	0.00
18) Naphthalene-d8	10.29	136	328206	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.18	164	215032	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.94	188	494693	20.00	ng/ul	0.00
78) Chrysene-d12	21.14	240	539103	20.00	ng/ul	0.00
86) Perylene-d12	23.34	264	528743	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.01	96	7280	6.37	ng/uL	0.00
5) Phenol-d5	6.70	99	161033	29.21	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.85	67	84112	30.90	ng/ul	0.00
9) 2-Chlorophenol-d4	7.04	132	158236	32.37	ng/ul	0.00
13) 4-Methylphenol-d8	8.23	113	142691	29.18	ng/ul	0.00
19) Nitrobenzene-d5	8.66	128	85813	33.08	ng/ul	0.00
22) 2-Nitrophenol-d4	9.38	143	99359	36.27	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.92	165	149948	31.45	ng/ul	0.00
29) 4-Chloroaniline-d4	10.44	131	6484m	1.17	ng/ul	0.00
44) Dimethylphthalate-d6	13.61	166	564761	37.41	ng/ul	0.00
47) Acenaphthylene-d8	13.87	160	635353	34.25	ng/ul	0.00
52) 4-Nitrophenol-d4	14.40	143	118721	37.38	ng/ul	0.00
58) Fluorene-d10	15.19	176	497625	35.66	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.32	200	113045	35.74	ng/ul	0.00
71) Anthracene-d10	17.04	188	768565	35.87	ng/ul	0.00
79) Pyrene-d10	19.35	212	888610	35.98	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.20	264	846484	33.55	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG072415\
Data File : BG018094.D
Acq On : 24 Jul 2015 18:00
Operator : TP/UM
Sample : PB84428BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Jul 25 01:03:43 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG072315.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 24 23:53:51 2015
Response via : Initial Calibration

Instrument :
BNA_G
ClientSampled :
SBLK88

Manual Integrations
APPROVED
apatel
7/27/2015 3:40:54 PM

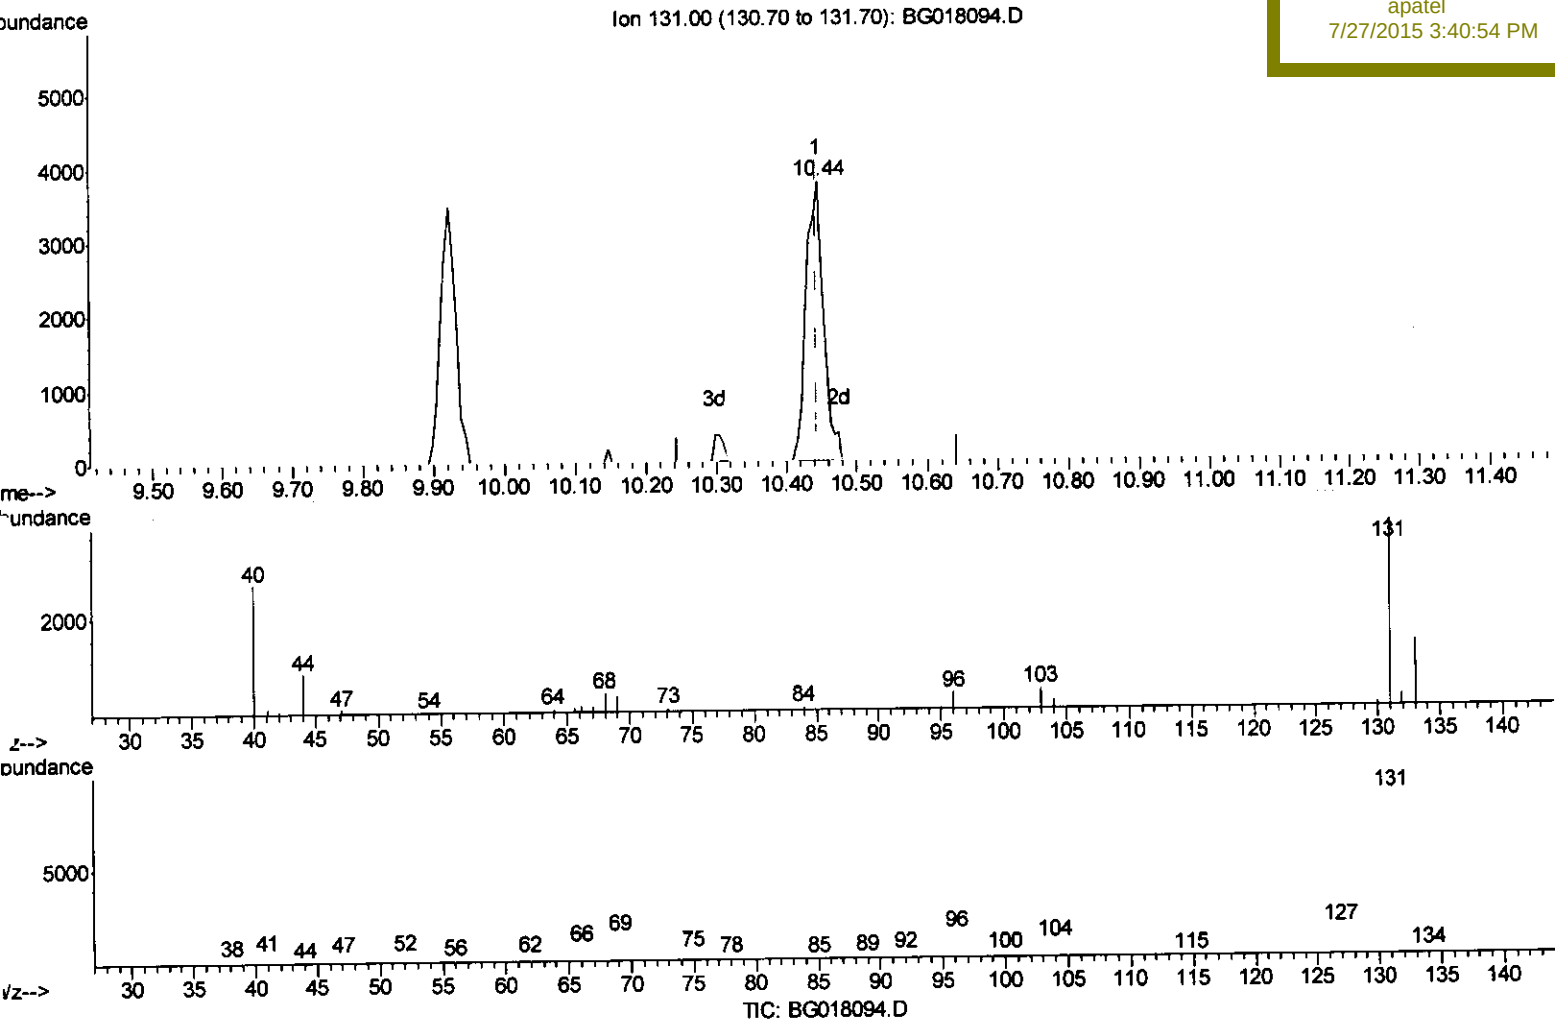

(29) 4-Chloroaniline-d4 (S)
10.445min (+0.001) 1.17ng/ul m
response 6484
T.P
07/27/2015




Ion	Exp%	Act%
131.00	100	100
133.00	32.50	37.82
69.00	15.40	11.71#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG072415\
Data File : BG018094.D
Acq On : 24 Jul 2015 18:00
Operator : TP/UM
Sample : PB84428BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Jul 25 01:03:43 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG072315.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 24 23:53:51 2015
Response via : Initial Calibration

Instrument :
BNA_G
ClientSampleId :
SBLK88

Manual Integrations
APPROVED
apatel
7/27/2015 3:40:54 PM

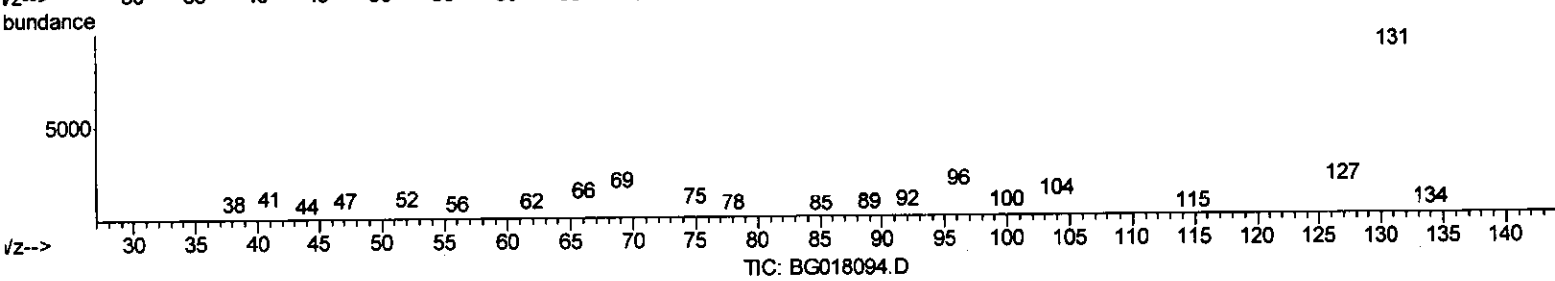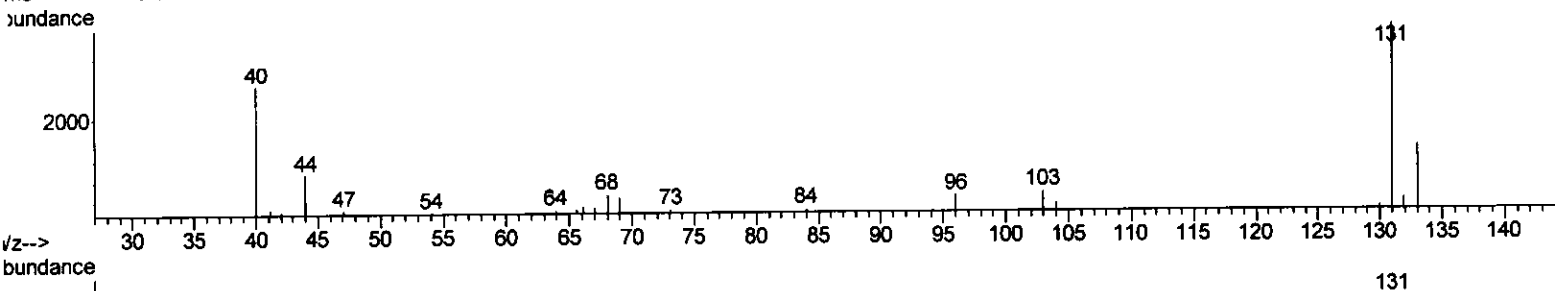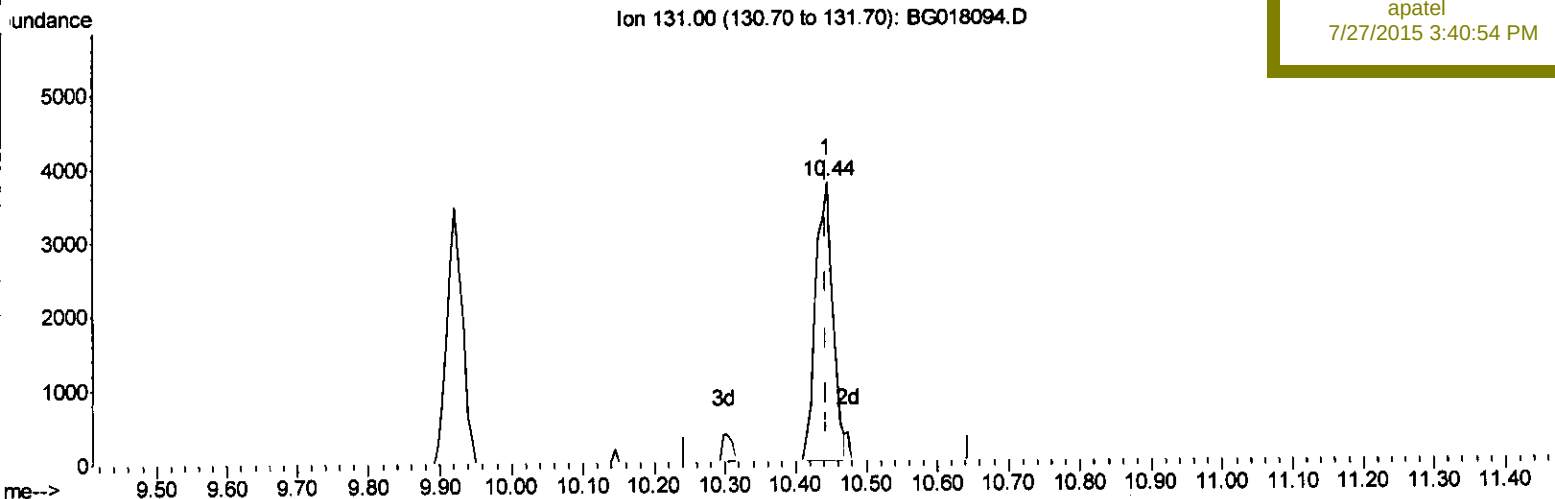

(29) 4-Chloroaniline-d4 (S)
10.445min (+0.001) 1.14ng/ul
response 6351

Ion	Exp%	Act%
131.00	100	100
133.00	32.50	37.82
69.00	15.40	11.71#
0.00	0.00	0.00