


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG072415\
 Data File : BG018089.D
 Acq On : 24 Jul 2015 12:50
 Operator : TP/UM
 Sample : DFTPP18
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP18

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG072315.M
 Title : SVOA CALIBRATION
 Last Update : Fri Jul 24 23:53:51 2015

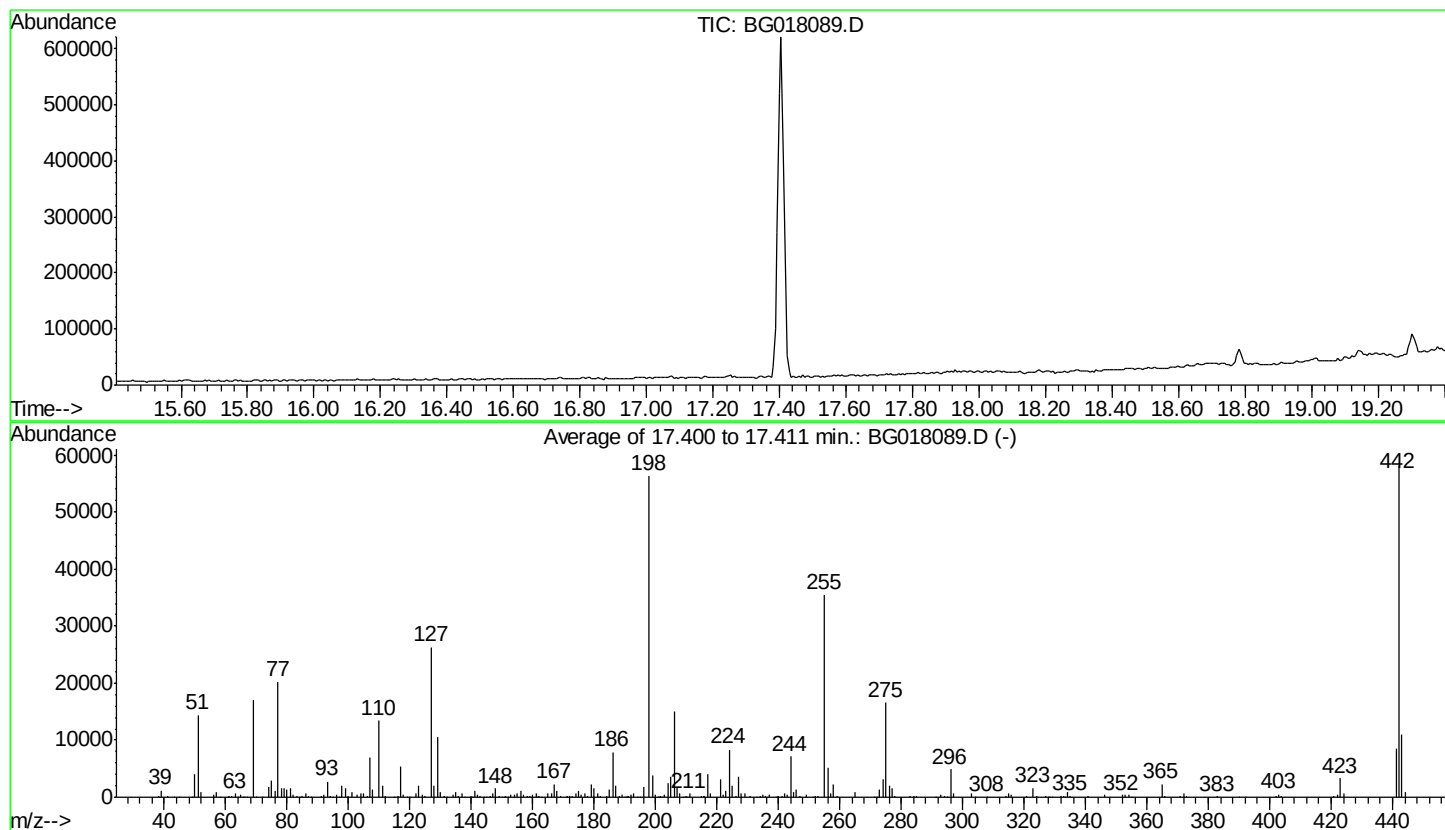

AutoFind: Scans 2504, 2505, 2506; Background Corrected with Scan 2498

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.6	14428	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	30.2	17054	PASS
70	69	0.00	2	0.4	61	PASS
127	198	10	80	46.6	26298	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	56426	PASS
199	198	5	9	7.0	3924	PASS
275	198	10	60	29.4	16572	PASS
365	198	1	100	4.0	2255	PASS
441	442	0.01	24	14.6	8492	PASS
442	198	50	100	103.0	58133	FAIL*
443	442	15	24	19.1	11099	PASS