


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG072418\
 Data File : BG035839.D
 Acq On : 24 Jul 2018 9:16
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 31 12:30:06 2018

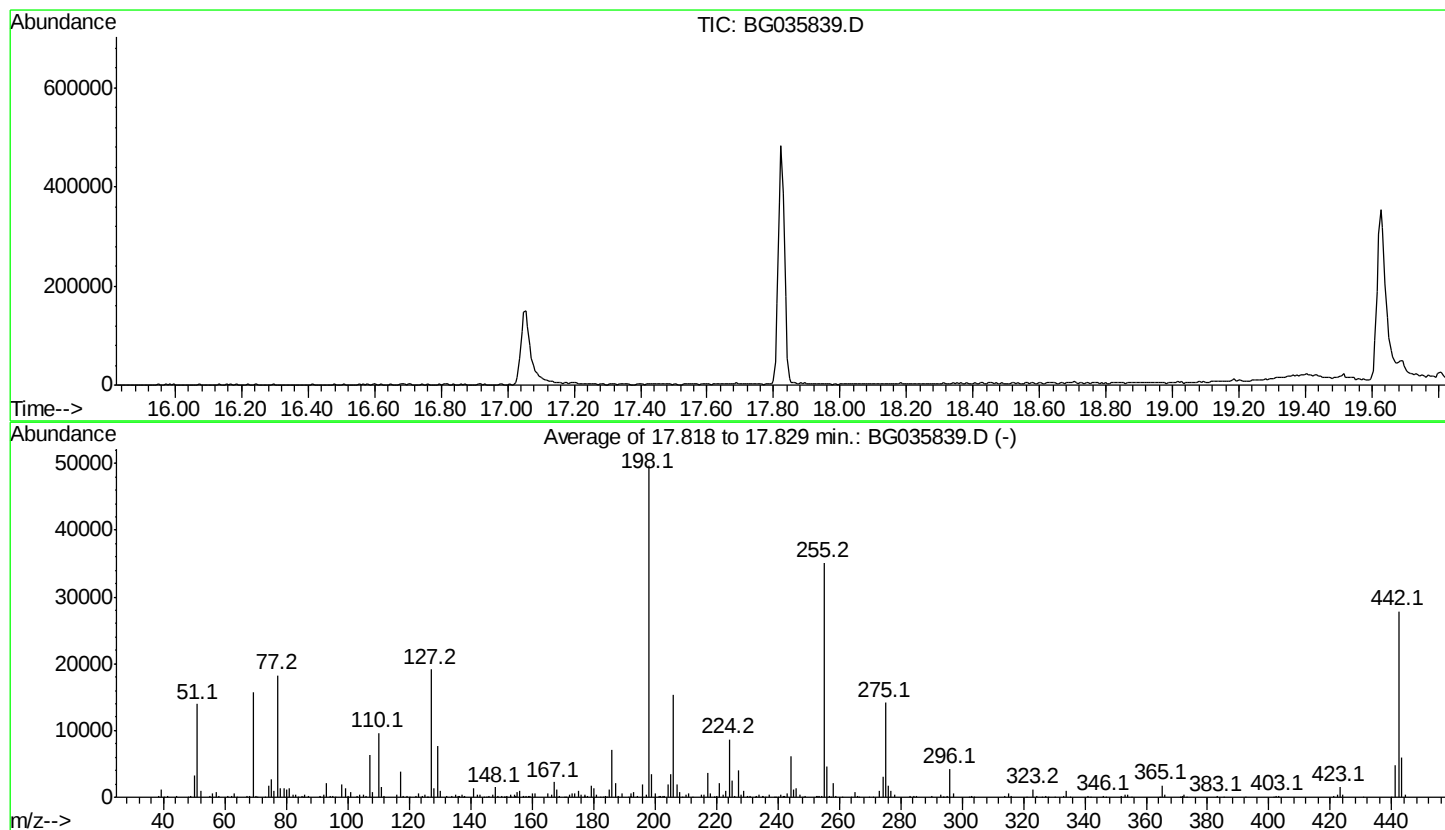

AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.1	13980	PASS
68	69	0.00	2	1.2	184	PASS
69	198	0.00	100	31.8	15788	PASS
70	69	0.00	2	1.0	155	PASS
127	198	10	80	38.4	19082	PASS
197	198	0.00	2	0.7	338	PASS
198	198	100	100	100.0	49664	PASS
199	198	5	9	6.9	3424	PASS
275	198	10	60	28.5	14144	PASS
365	198	1	100	3.5	1749	PASS
441	198	0.01	100	9.6	4778	PASS
442	198	50	100	56.1	27866	PASS
443	442	15	24	21.4	5956	PASS