


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG072418\
 Data File : BG035857.D
 Acq On : 24 Jul 2018 21:54
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 31 12:30:06 2018

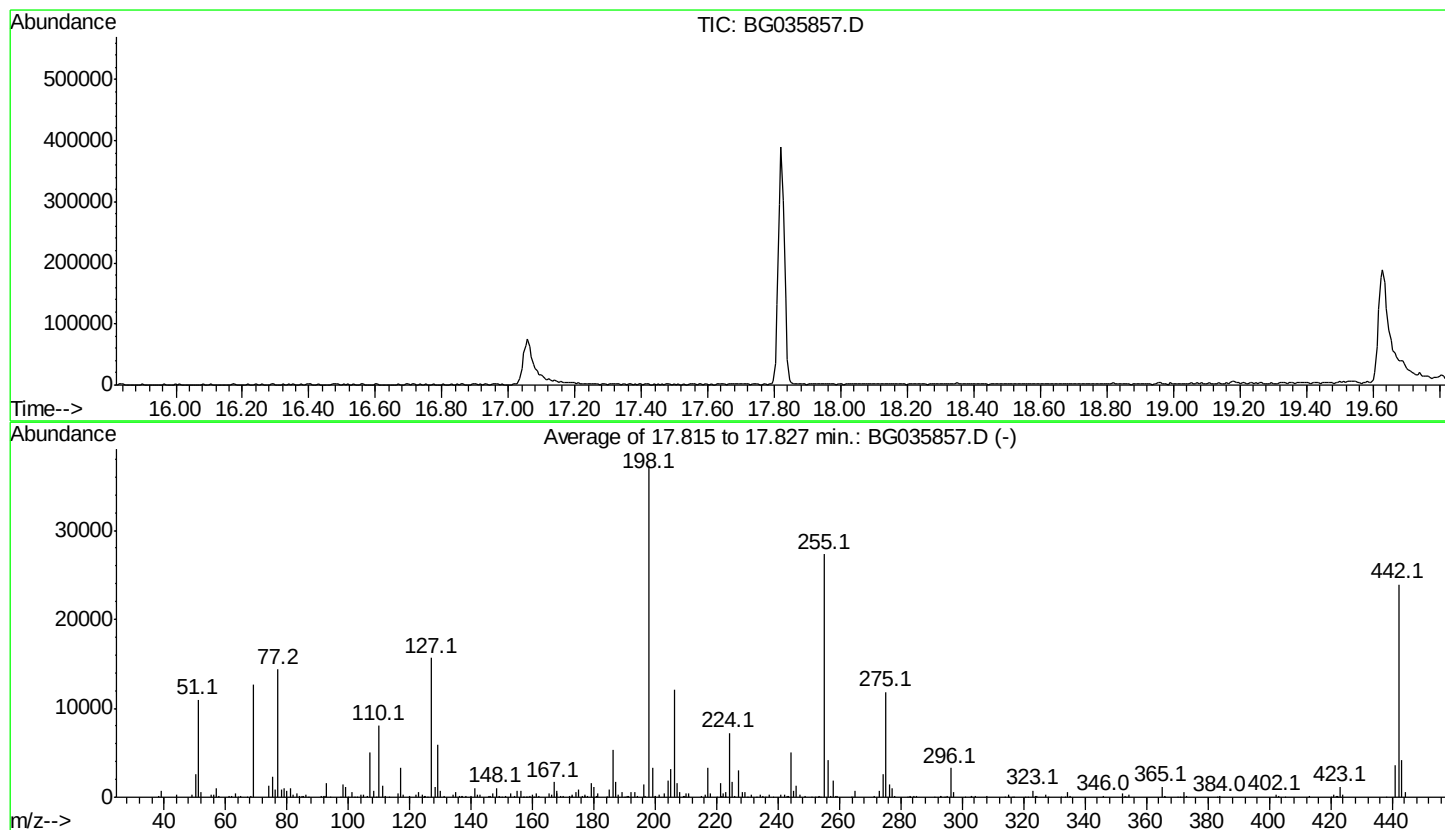

AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2467

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.4	10956	PASS
68	69	0.00	2	1.4	183	PASS
69	198	0.00	100	34.2	12734	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.1	15683	PASS
197	198	0.00	2	0.4	153	PASS
198	198	100	100	100.0	37277	PASS
199	198	5	9	8.7	3256	PASS
275	198	10	60	31.7	11808	PASS
365	198	1	100	3.2	1202	PASS
441	198	0.01	100	9.6	3591	PASS
442	198	50	100	64.3	23957	PASS
443	442	15	24	17.6	4219	PASS