

Data Path : Z:\HPCHEM1\BNA G\DATA\BG072517\
 Data File : BG028023.D
 Acq On : 25 Jul 2017 11:57
 Operator : SJ/JU
 Sample : I4373-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AA2

Quant Time: Jul 26 01:32:59 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG071717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 26 01:32:03 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.36	152	40076	20.00	ng/ul	0.00
18) Naphthalene-d8	11.19	136	169974	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.97	164	121457	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.72	188	336419	20.00	ng/ul	0.00
75) Chrysene-d12	22.05	240	432651	20.00	ng/ul	0.00
83) Perylene-d12	25.57	264	422339	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.86	96	4784	6.58	ng/uL	0.00
5) Phenol-d5	7.51	99	16873	5.12	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.68	67	38762	20.41	ng/ul	0.00
9) 2-Chlorophenol-d4	7.90	132	51399	19.86	ng/ul	0.00
13) 4-Methylphenol-d8	9.06	113	30135	11.05	ng/ul	0.00
19) Nitrobenzene-d5	9.53	128	31664	25.32	ng/ul	0.00
22) 2-Nitrophenol-d4	10.26	143	38560	25.63	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.80	165	71197	24.18	ng/ul	0.00
29) 4-Chloroaniline-d4	11.33	131	3658	1.37	ng/ul	0.00
43) Dimethylphthalate-d6	14.36	166	313481	29.77	ng/ul	0.00
46) Acenaphthylene-d8	14.67	160	313456	26.19	ng/ul	0.00
51) 4-Nitrophenol-d4	15.18	143	6999	4.59	ng/ul	0.02
57) Fluorene-d10	15.96	176	280681	28.28	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.07	200	55731	23.85	ng/ul	0.00
70) Anthracene-d10	17.82	188	467623	28.82	ng/ul	0.00
76) Pyrene-d10	20.09	212	596520	30.69	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.33	264	580624	29.43	ng/ul	0.00


Target Compounds				Ovalue	
44) Dimethylphthalate	14.41	163	20936	2.184	ng/ul# 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG072517\
Data File : BG028023.D
Acq On : 25 Jul 2017 11:57
Operator : SJ/JU
Sample : I4373-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AA2

Quant Time: Jul 26 01:32:59 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG071717.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 26 01:32:03 2017
Response via : Initial Calibration

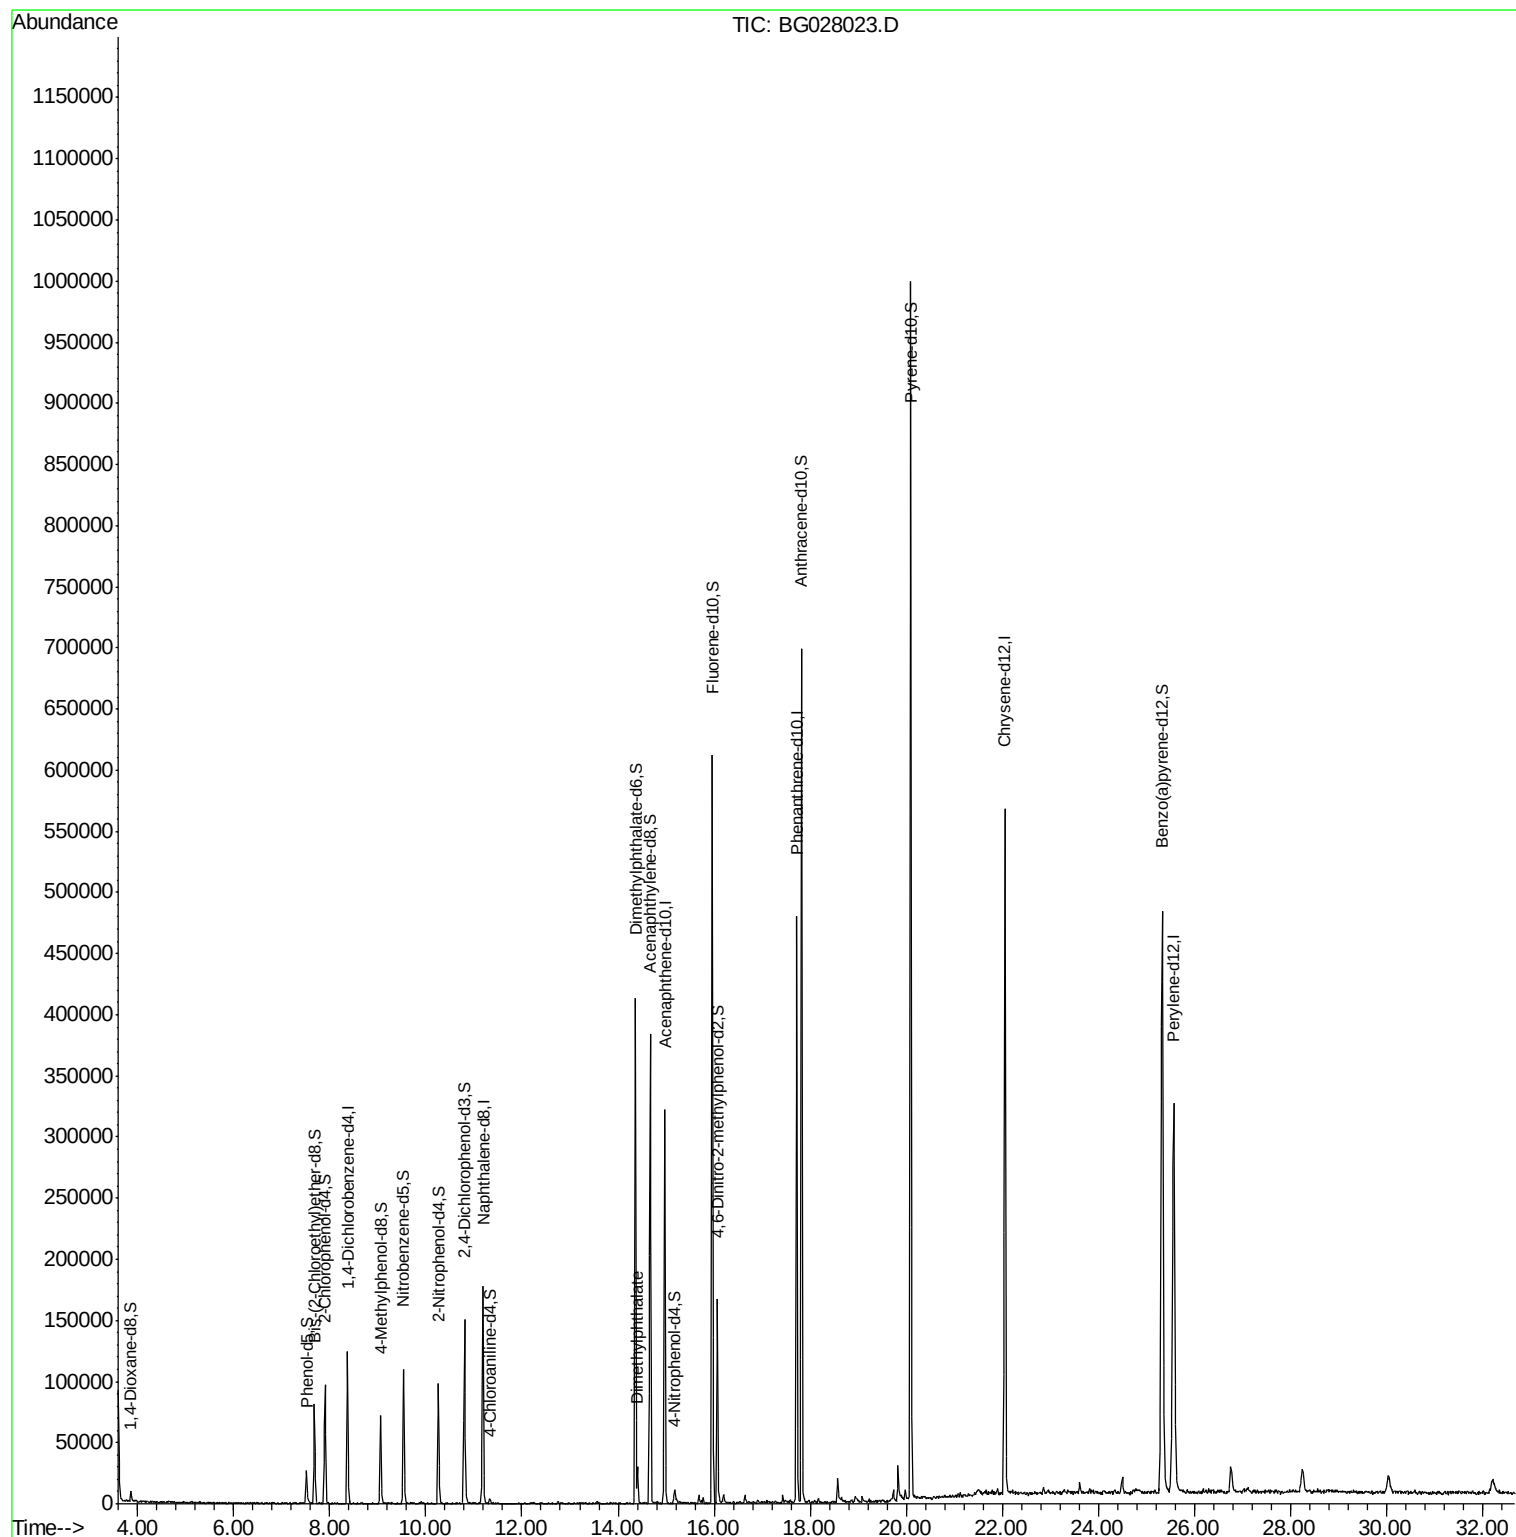

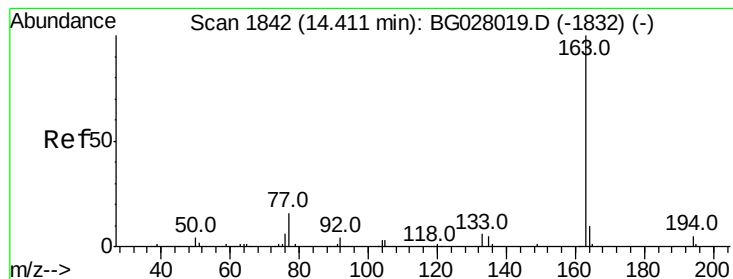

#44

Dimethylphthalate

Concen: 2.184 ng/ul

RT: 14.41 min Scan# 1842

Delta R.T. -0.00 min

Lab File: BG028023.D

Acq: 25 Jul 2017 11:57

Instrument :

BNA_G

ClientSampleId :

C0AA2


Tot Ion:163 Resp: 20936

Ion Ratio Lower Upper

163 100

194 4.8 3.4 5.0

164 14.0 9.0 13.4#

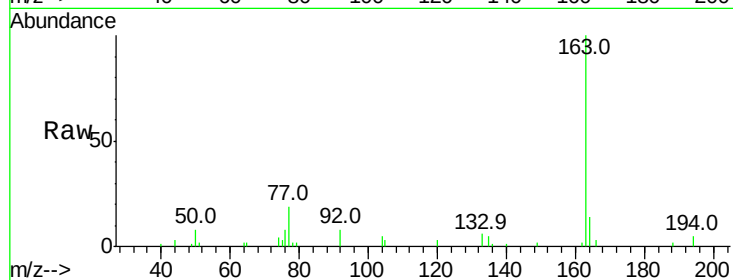

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

