

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072521\
 Data File : BG049461.D
 Acq On : 24 Jul 2021 22:14
 Operator : CG/JU
 Sample : PB137775BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK775

Quant Time: Jul 25 07:22:49 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 24 06:15:51 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.049	152	24383	20.000	ng/ul	0.00
20) Naphthalene-d8	10.868	136	97287	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.698	164	68261	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.442	188	153024	20.000	ng/ul	0.00
79) Chrysene-d12	21.724	240	172519	20.000	ng/ul	0.00
88) Perylene-d12	25.002	264	172326	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.431	96	3250	6.098	ng/uL	0.00
4) Pyridine-d5	3.854	84	50414	32.933	ng/ul	0.00
7) Phenol-d5	7.197	99	67431	31.257	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.367	67	38056	31.147	ng/ul	0.00
11) 2-Chlorophenol-d4	7.579	132	49665	32.117	ng/ul	0.00
15) 4-Methylphenol-d8	8.754	113	51019	31.375	ng/ul	0.00
21) Nitrobenzene-d5	9.212	128	25899	34.625	ng/ul	0.00
24) 2-Nitrophenol-d4	9.940	143	29265	33.389	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.486	165	49769	31.220	ng/ul	0.00
31) 4-Chloroaniline-d4	10.998	131	67281	30.284	ng/ul	0.00
46) Dimethylphthalate-d6	14.093	166	175473	33.558	ng/ul	0.00
49) Acenaphthylene-d8	14.387	160	205225	33.792	ng/ul	0.00
54) 4-Nitrophenol-d4	14.886	143	25049	29.090	ng/ul	0.00
60) Fluorene-d10	15.691	176	146495	32.520	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.803	200	26567	28.017	ng/ul	0.00
73) Anthracene-d10	17.542	188	236481	33.251	ng/ul	0.00
81) Pyrene-d10	19.827	212	288020	32.650	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.773	264	306441	33.834	ng/ul	0.00
Target Compounds						
17) N-Nitroso-di-n-propyla...	8.748	70	1496	1.109	ng/ul#	Qvalue 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072521\
Data File : BG049461.D
Acq On : 24 Jul 2021 22:14
Operator : CG/JU
Sample : PB137775BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK775


Quant Time: Jul 25 07:22:49 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 24 06:15:51 2021
Response via : Initial Calibration

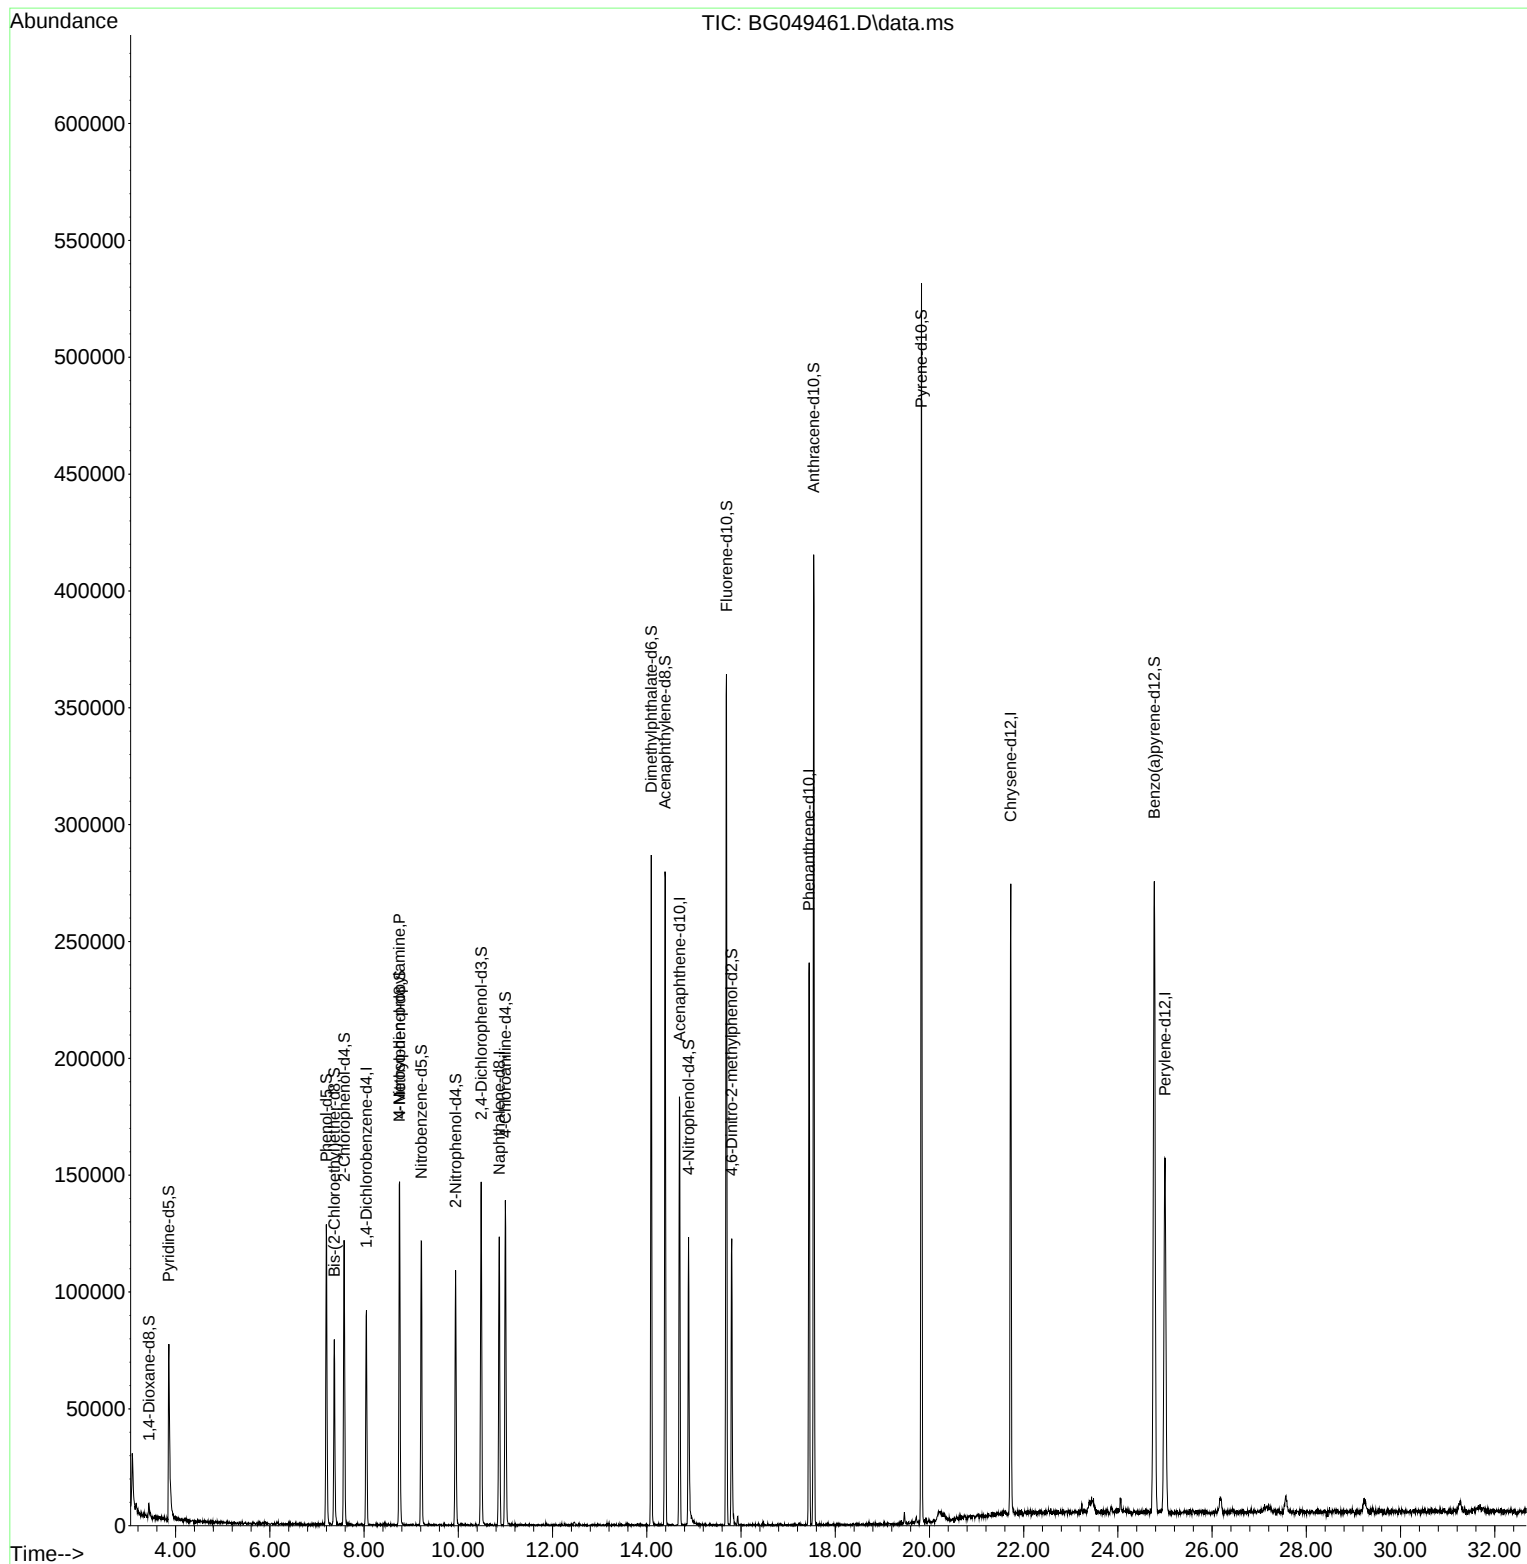

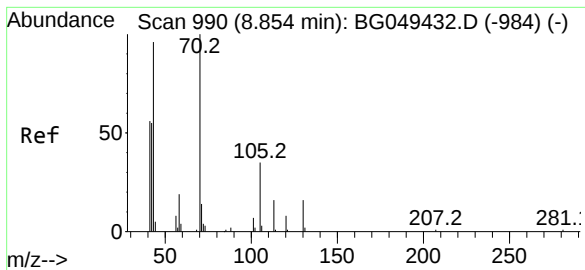

#17
 N-Nitroso-di-n-propylamine
 Concen: 1.109 ng/ul
 RT: 8.748 min Scan# 972
 Delta R.T. -0.106 min
 Lab File: BG049461.D
 Acq: 24 Jul 2021 22:14

Instrument :
 BNA_G
 ClientSampleId :
 SBLK775

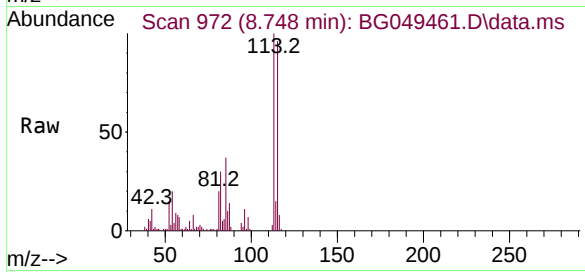

Tgt Ion:	70	Resp:	1496
Ion	Ratio	Lower	Upper
70	100		
42	329.8	44.2	66.4#
101	0.0	5.4	8.0#
130	0.0	12.4	18.6#

