

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072521\
 Data File : BG049463.D
 Acq On : 24 Jul 2021 23:37
 Operator : CG/JU
 Sample : PB137808BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK808

Quant Time: Jul 25 07:23:15 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 24 06:15:51 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.048	152	22792	20.000	ng/ul	0.00
20) Naphthalene-d8	10.867	136	92837	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.698	164	63015	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.447	188	139804	20.000	ng/ul	0.00
79) Chrysene-d12	21.723	240	163025	20.000	ng/ul	0.00
88) Perylene-d12	24.995	264	166212	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.477	96	149	0.299	ng/uL	0.04
4) Pyridine-d5	3.853	84	54915	38.378	ng/ul	0.00
7) Phenol-d5	7.202	99	71012	35.215	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.366	67	44179	38.683	ng/ul	0.00
11) 2-Chlorophenol-d4	7.578	132	53762	37.193	ng/ul	0.00
15) 4-Methylphenol-d8	8.753	113	55034	36.207	ng/ul	0.00
21) Nitrobenzene-d5	9.217	128	28367	39.743	ng/ul	0.00
24) 2-Nitrophenol-d4	9.939	143	31343	37.473	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.486	165	53280	35.025	ng/ul	0.00
31) 4-Chloroaniline-d4	10.997	131	72783	34.330	ng/ul	0.00
46) Dimethylphthalate-d6	14.092	166	186193	38.573	ng/ul	0.00
49) Acenaphthylene-d8	14.392	160	215540	38.445	ng/ul	0.00
54) 4-Nitrophenol-d4	14.885	143	27249	34.279	ng/ul	0.00
60) Fluorene-d10	15.684	176	154219	37.085	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.802	200	28271	32.633	ng/ul	0.00
73) Anthracene-d10	17.541	188	251517	38.709	ng/ul	0.00
81) Pyrene-d10	19.832	212	312508	37.489	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.772	264	339564	38.870	ng/ul	0.00
Target Compounds						
					Qvalue	
17) N-Nitroso-di-n-propyla...	8.747	70	1695	1.344	ng/ul#	1
23) Isophorone	9.939	82	3863	1.082	ng/ul#	70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072521\
Data File : BG049463.D
Acq On : 24 Jul 2021 23:37
Operator : CG/JU
Sample : PB137808BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK808

Quant Time: Jul 25 07:23:15 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 24 06:15:51 2021
Response via : Initial Calibration




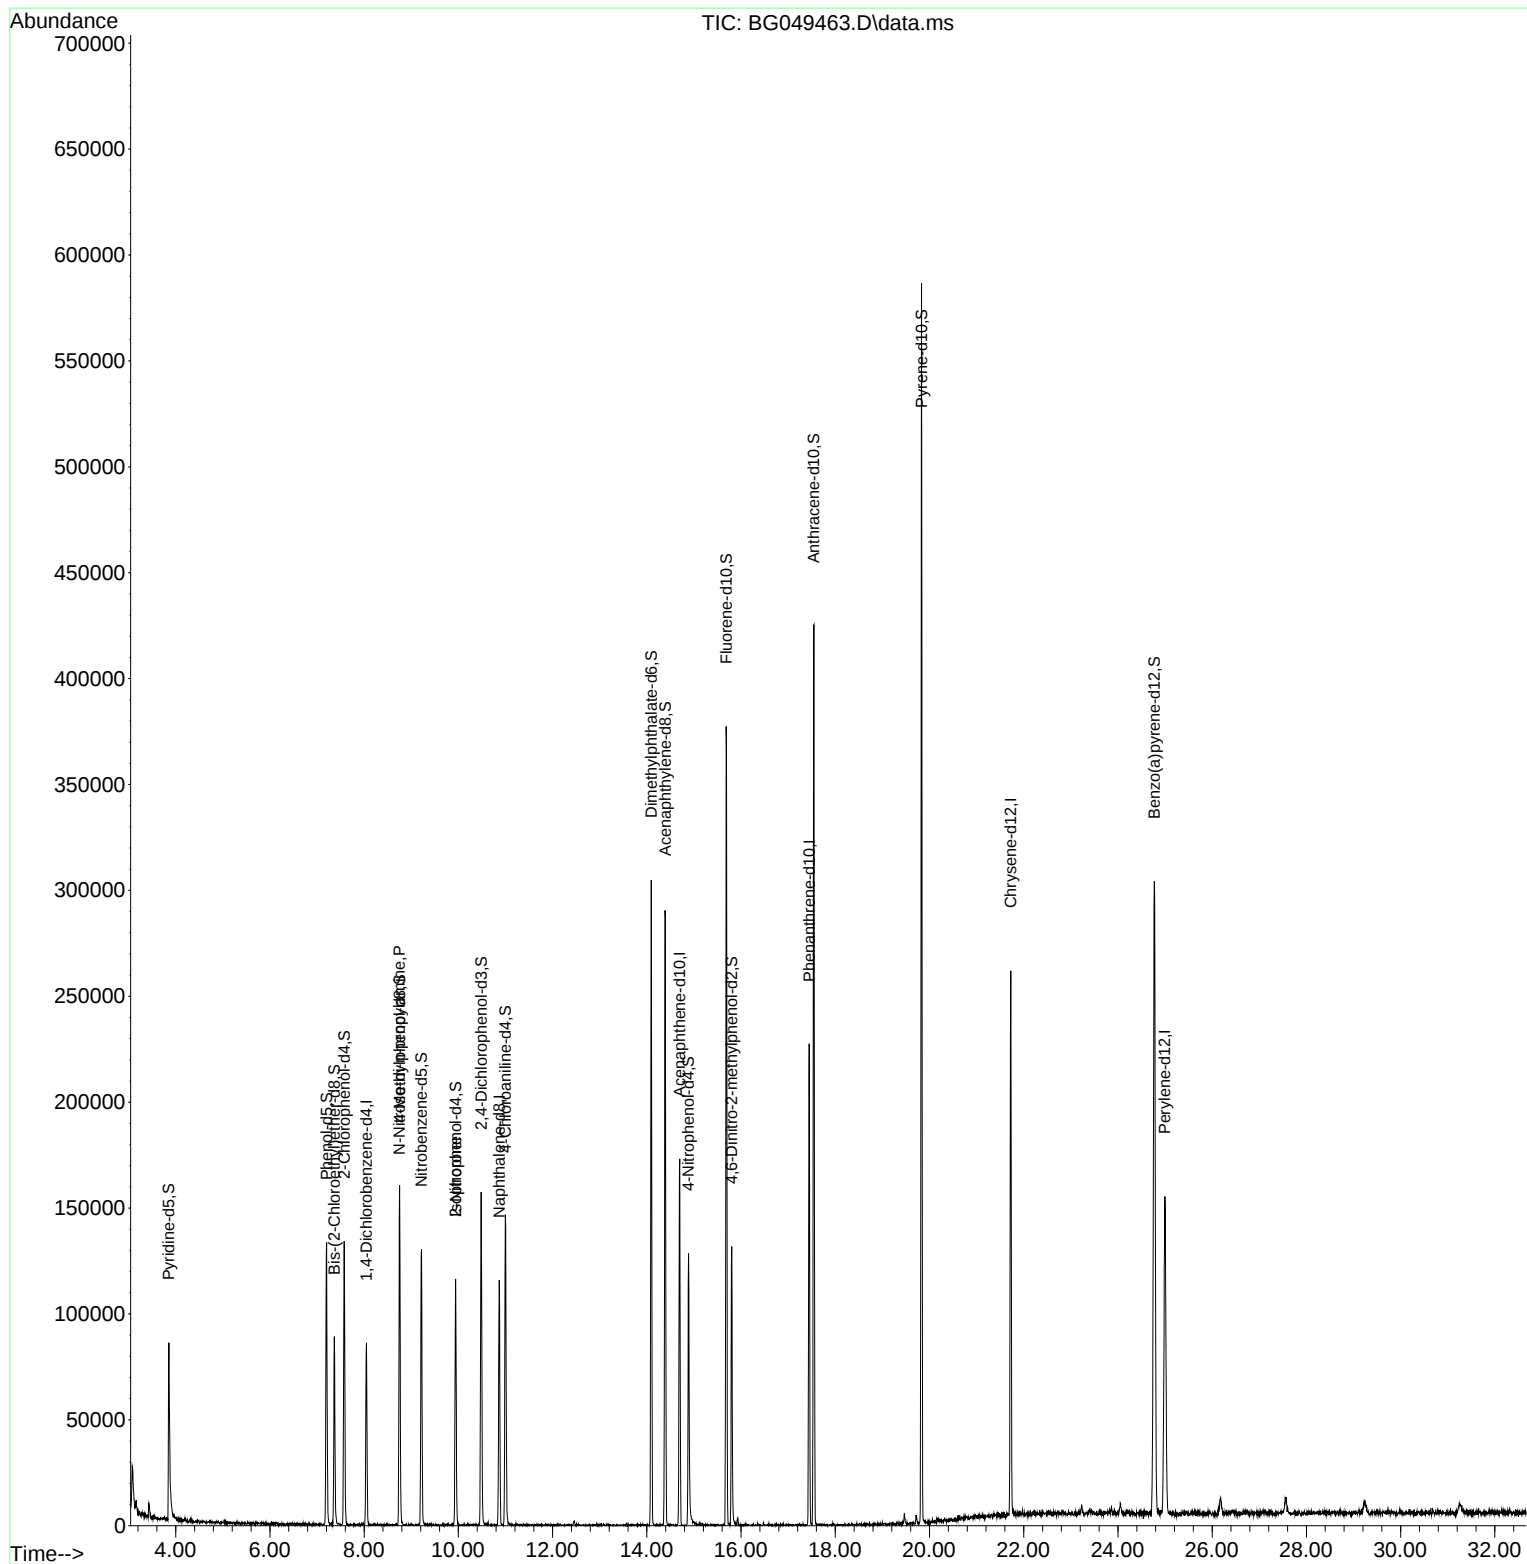


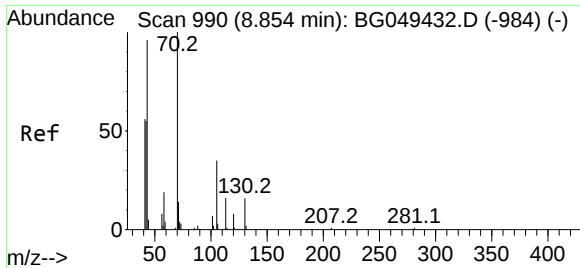

#17
N-Nitroso-di-n-propylamine
Concen: 1.344 ng/ul
RT: 8.747 min Scan# 972
Delta R.T. -0.107 min
Lab File: BG049463.D
Acq: 24 Jul 2021 23:37

Instrument :
BNA_G
ClientSampleId :
SBLK808

Tgt Ion:	70	Resp:	1695
Ion	Ratio	Lower	Upper
70	100		
42	336.3	44.2	66.4#
101	0.0	5.4	8.0#
130	0.0	12.4	18.6#

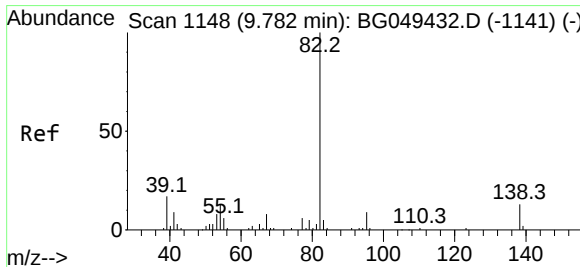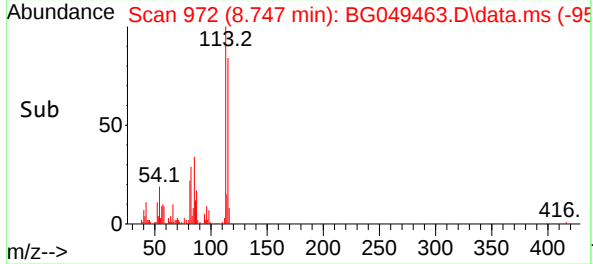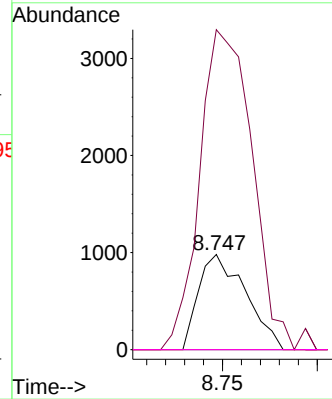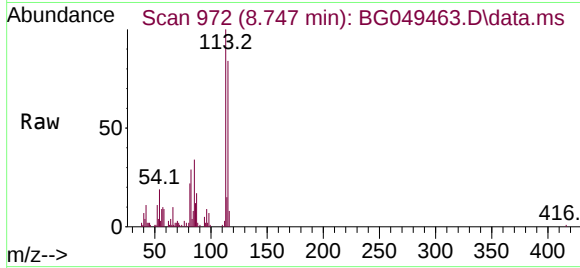

#23
Isophorone
Concen: 1.082 ng/ul
RT: 9.939 min Scan# 1175
Delta R.T. 0.157 min
Lab File: BG049463.D
Acq: 24 Jul 2021 23:37

Tgt Ion:	82	Resp:	3863
Ion	Ratio	Lower	Upper
82	100		
95	0.0	7.4	11.0#
138	0.0	10.7	16.1#

