

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072521\
 Data File : BG049465.D
 Acq On : 25 Jul 2021 1:00
 Operator : CG/JU
 Sample : M3010-06
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGEE4

Quant Time: Jul 25 07:23:42 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 24 06:15:51 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.049	152	22400	20.000	ng/ul	0.00
20) Naphthalene-d8	10.869	136	82771	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.693	164	57672	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.442	188	124418	20.000	ng/ul	0.00
79) Chrysene-d12	21.725	240	140577	20.000	ng/ul	0.00
88) Perylene-d12	24.991	264	138916	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.432	96	3380	6.903	ng/uL	0.00
4) Pyridine-d5	3.855	84	41893	29.790	ng/ul	0.00
7) Phenol-d5	7.197	99	63527	32.054	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.368	67	37229	33.168	ng/ul	0.00
11) 2-Chlorophenol-d4	7.579	132	45884	32.298	ng/ul	0.00
15) 4-Methylphenol-d8	8.754	113	50136	33.562	ng/ul	0.00
21) Nitrobenzene-d5	9.218	128	25318	39.785	ng/ul	0.00
24) 2-Nitrophenol-d4	9.941	143	27495	36.870	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.487	165	46617	34.372	ng/ul	0.00
31) 4-Chloroaniline-d4	10.998	131	61659	32.620	ng/ul	0.00
46) Dimethylphthalate-d6	14.094	166	165338	37.426	ng/ul	0.00
49) Acenaphthylene-d8	14.388	160	195626	38.125	ng/ul	0.00
54) 4-Nitrophenol-d4	14.887	143	22017	30.263	ng/ul	0.00
60) Fluorene-d10	15.686	176	138502	36.391	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.803	200	24233	31.431	ng/ul	0.00
73) Anthracene-d10	17.542	188	222533	38.484	ng/ul	0.00
81) Pyrene-d10	19.827	212	275281	38.296	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.768	264	277904	38.062	ng/ul	0.00


Target Compounds					Qvalue
17) N-Nitroso-di-n-propyla...	8.754	70	1494	1.205 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072521\
Data File : BG049465.D
Acq On : 25 Jul 2021 1:00
Operator : CG/JU
Sample : M3010-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGEE4


Quant Time: Jul 25 07:23:42 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 24 06:15:51 2021
Response via : Initial Calibration

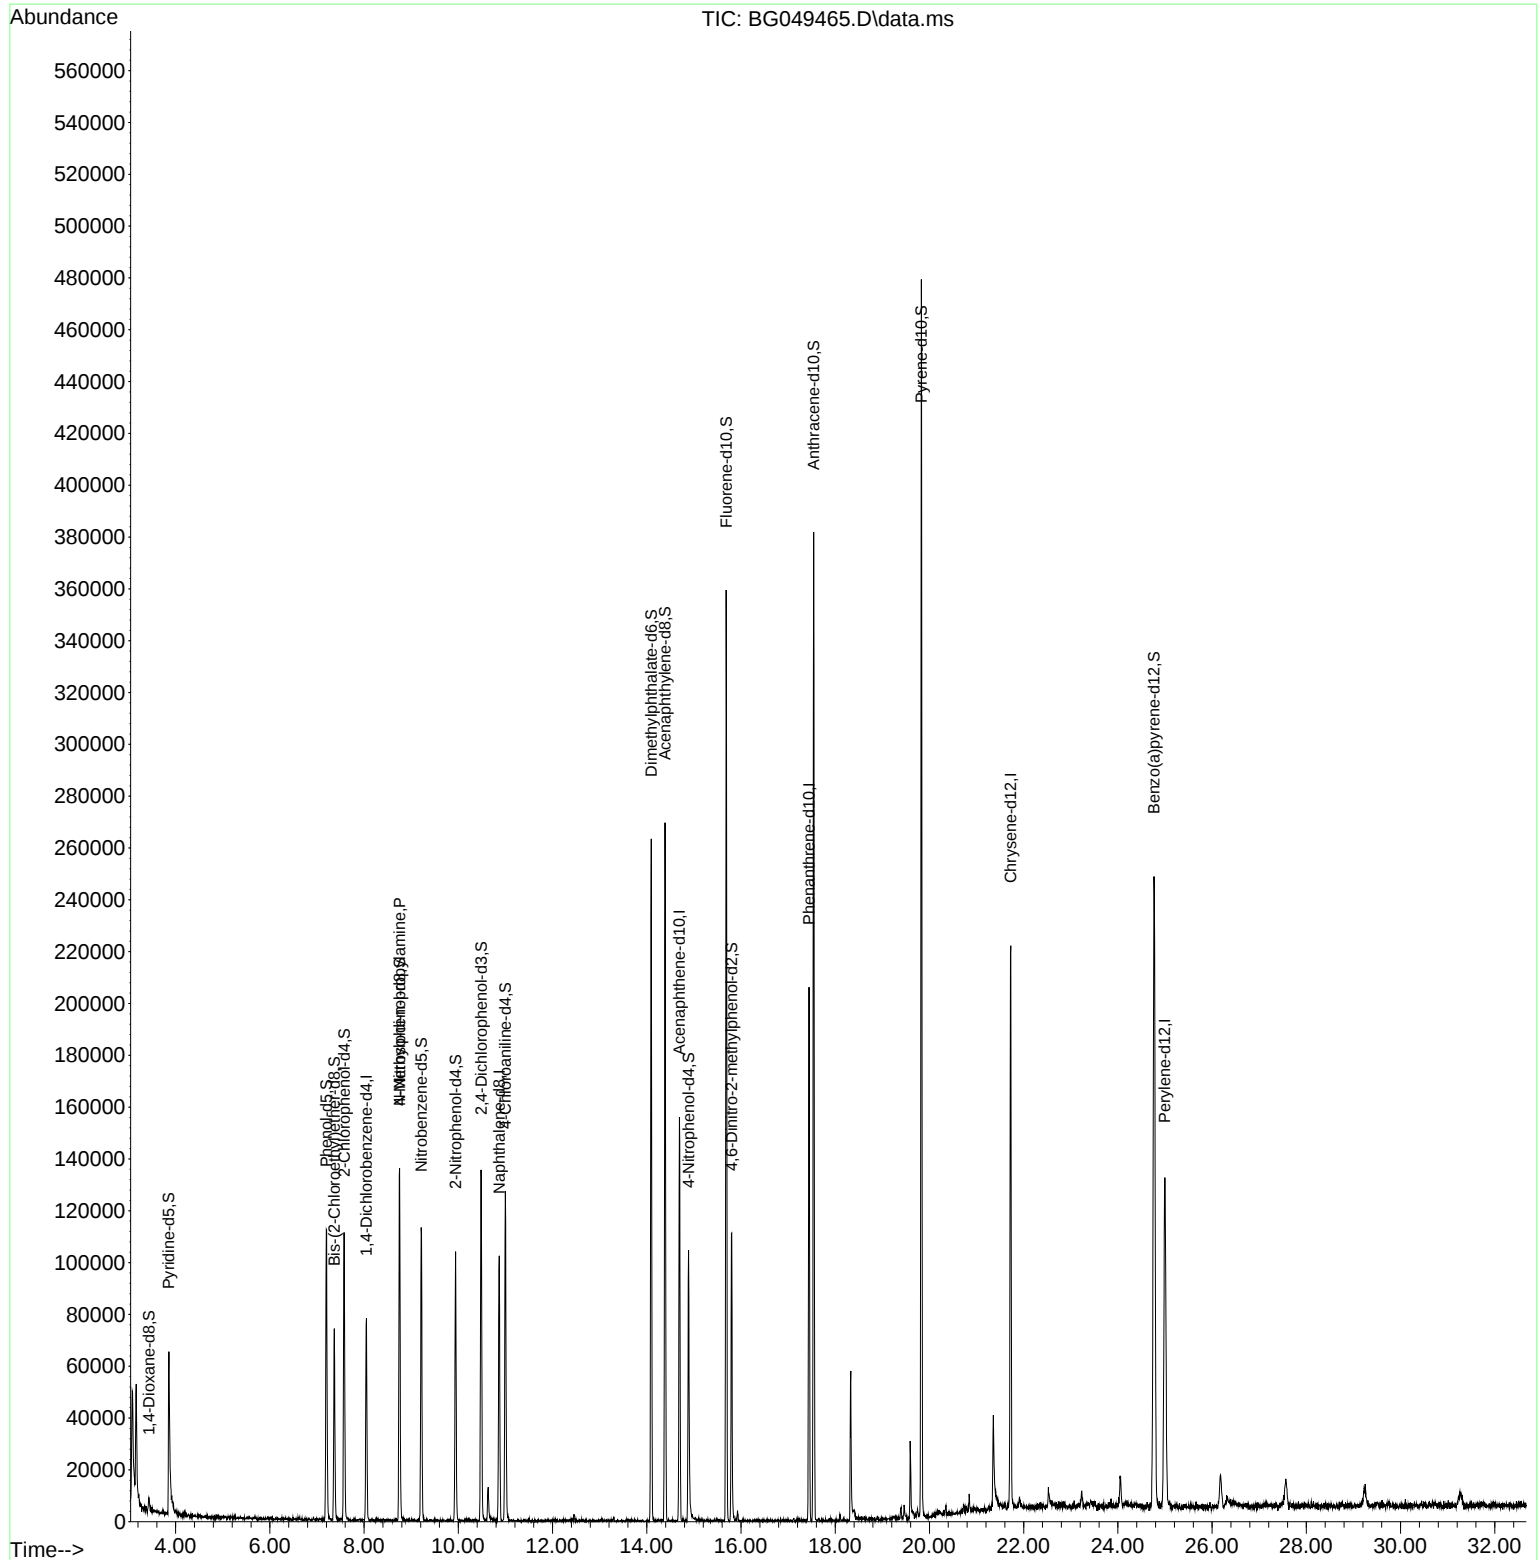

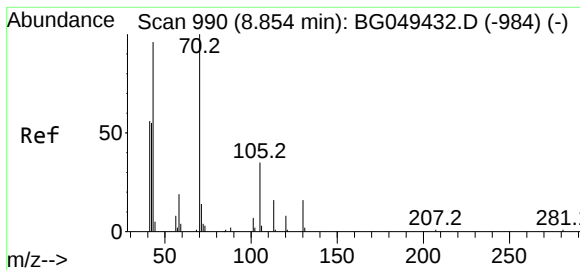

#17
 N-Nitroso-di-n-propylamine
 Concen: 1.205 ng/ul
 RT: 8.754 min Scan# 973
 Delta R.T. -0.100 min
 Lab File: BG049465.D
 Acq: 25 Jul 2021 1:00

Instrument :
 BNA_G
 ClientSampleId :
 BGEE4

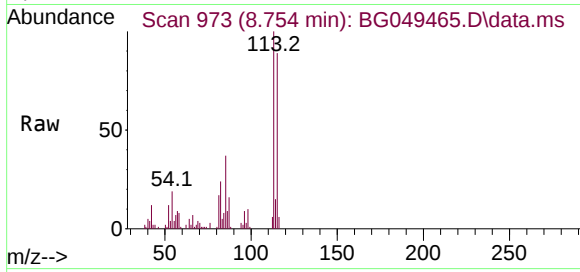

Tgt Ion:	70	Resp:	1494
Ion	Ratio	Lower	Upper
70	100		
42	347.4	44.2	66.4#
101	0.0	5.4	8.0#
130	0.0	12.4	18.6#

