

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072521\
 Data File : BG049468.D
 Acq On : 25 Jul 2021 3:02
 Operator : CG/JU
 Sample : M3010-07
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGEE5

Quant Time: Jul 25 07:24:11 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 24 06:15:51 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.043	152	19365	20.000	ng/ul	0.00
20) Naphthalene-d8	10.869	136	79766	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.693	164	55144	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.448	188	122681	20.000	ng/ul	0.00
79) Chrysene-d12	21.725	240	130739	20.000	ng/ul	# 0.00
88) Perylene-d12	24.997	264	136216	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.432	96	2118	5.004	ng/uL	0.00
4) Pyridine-d5	3.855	84	23370	19.223	ng/ul	0.00
7) Phenol-d5	7.198	99	42860	25.016	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.362	67	24333	25.076	ng/ul	0.00
11) 2-Chlorophenol-d4	7.579	132	29557	24.066	ng/ul	0.00
15) 4-Methylphenol-d8	8.754	113	36508	28.269	ng/ul	0.00
21) Nitrobenzene-d5	9.212	128	16061	26.189	ng/ul	0.00
24) 2-Nitrophenol-d4	9.941	143	19021	26.468	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.481	165	33593	25.702	ng/ul	0.00
31) 4-Chloroaniline-d4	10.998	131	44570	24.468	ng/ul	0.00
46) Dimethylphthalate-d6	14.094	166	128716	30.472	ng/ul	0.00
49) Acenaphthylene-d8	14.388	160	153103	31.206	ng/ul	0.00
54) 4-Nitrophenol-d4	14.887	143	16620	23.892	ng/ul	0.00
60) Fluorene-d10	15.686	176	111098	30.529	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.804	200	18587	24.450	ng/ul	0.00
73) Anthracene-d10	17.542	188	180826	31.714	ng/ul	0.00
81) Pyrene-d10	19.828	212	212724	31.821	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.768	264	221316	30.913	ng/ul	0.00


Target Compounds					Qvalue	
17) N-Nitroso-di-n-propyla...	8.748	70	1085	1.012	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072521\
Data File : BG049468.D
Acq On : 25 Jul 2021 3:02
Operator : CG/JU
Sample : M3010-07
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGEE5


Quant Time: Jul 25 07:24:11 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 24 06:15:51 2021
Response via : Initial Calibration

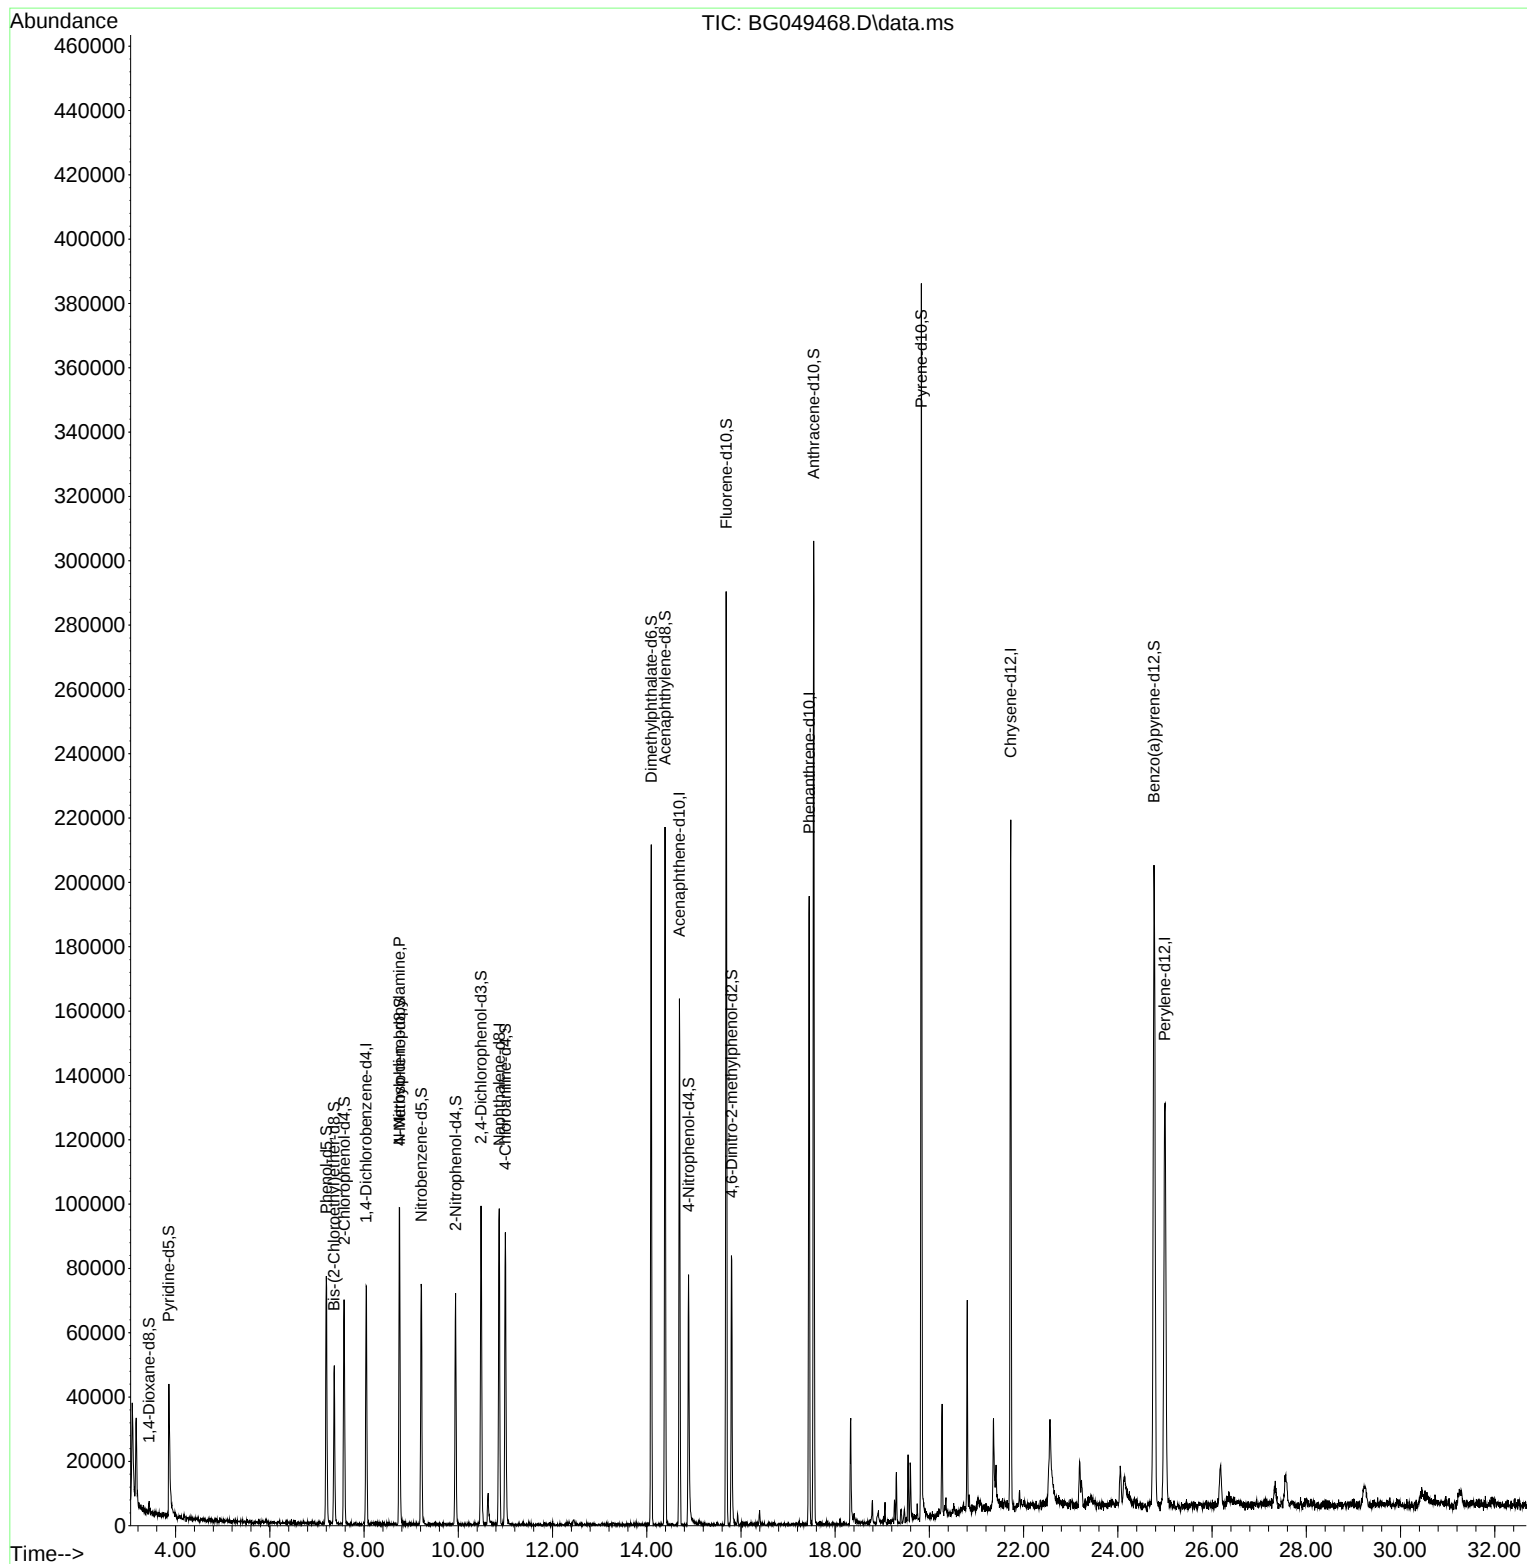

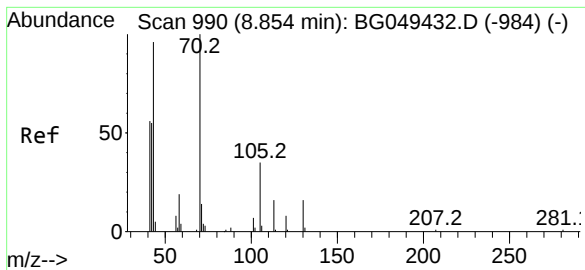

#17
 N-Nitroso-di-n-propylamine
 Concen: 1.012 ng/ul
 RT: 8.748 min Scan# 972
 Delta R.T. -0.106 min
 Lab File: BG049468.D
 Acq: 25 Jul 2021 3:02

Instrument :
 BNA_G
 ClientSampleId :
 BGEE5

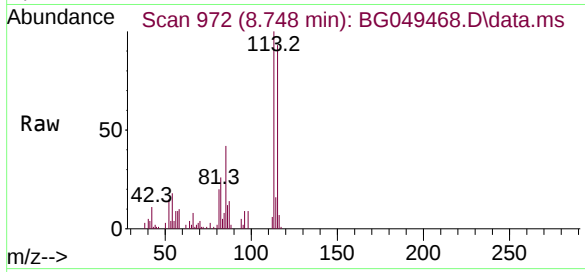

Tgt Ion:	70	Resp:	1085
Ion	Ratio	Lower	Upper
70	100		
42	270.1	44.2	66.4#
101	0.0	5.4	8.0#
130	0.0	12.4	18.6#

