

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072521\
 Data File : BG049450.D
 Acq On : 24 Jul 2021 14:01
 Operator : CG/JU
 Sample : M3087-10
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG049450.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.466	241	243	245	rBV3	2087	1725	0.51%	0.119%
2	4.560	258	259	263	rBV2	1494	1443	0.43%	0.099%
3	4.707	282	284	285	rBV	1277	1182	0.35%	0.081%
4	4.948	323	325	326	rBV	1265	943	0.28%	0.065%
5	5.224	370	372	374	rBV3	799	773	0.23%	0.053%
6	5.652	443	445	447	rBV	1260	943	0.28%	0.065%
7	5.811	470	472	476	rVB	1413	1763	0.52%	0.121%
8	5.870	479	482	483	rVV2	1283	1003	0.30%	0.069%
9	6.034	509	510	513	rBV2	1143	777	0.23%	0.054%
10	6.187	535	536	539	rBV2	1200	1068	0.32%	0.074%
11	6.804	640	641	643	rBV	1188	802	0.24%	0.055%
12	7.145	695	699	701	rVB	936	1146	0.34%	0.079%
13	7.180	703	705	708	rBV	735	838	0.25%	0.058%
14	7.303	725	726	729	rBV	1275	1032	0.31%	0.071%
15	7.509	759	761	764	rBV2	1142	815	0.24%	0.056%
16	7.597	771	776	778	rBV	900	1362	0.40%	0.094%
17	7.908	827	829	833	rVB	1186	1240	0.37%	0.085%
18	8.049	847	853	864	rVB2	65408	114860	34.06%	7.911%
19	8.137	864	868	871	rBV	762	1595	0.47%	0.110%
20	8.437	918	919	922	rBV	959	866	0.26%	0.060%
21	8.866	989	992	993	rVB	1146	856	0.25%	0.059%
22	8.983	1010	1012	1016	rVB	756	1044	0.31%	0.072%
23	9.148	1038	1040	1043	rBV	800	958	0.28%	0.066%
24	9.195	1047	1048	1054	rVB	840	968	0.29%	0.067%
25	9.653	1123	1126	1128	rBV2	987	772	0.23%	0.053%
26	9.835	1154	1157	1159	rBV2	1209	1142	0.34%	0.079%
27	9.941	1173	1175	1178	rBV	759	808	0.24%	0.056%
28	10.869	1326	1333	1345	rBV	80347	147085	43.61%	10.131%
29	11.169	1382	1384	1389	rBB	923	984	0.29%	0.068%
30	11.556	1448	1450	1455	rVB	710	820	0.24%	0.056%
31	12.302	1572	1577	1578	rBB	591	766	0.23%	0.053%
32	12.543	1615	1618	1621	rVB	893	932	0.28%	0.064%
33	12.696	1641	1644	1646	rBV	695	774	0.23%	0.053%
34	12.849	1666	1670	1672	rBV	621	778	0.23%	0.054%
35	13.195	1726	1729	1732	rBB	717	894	0.27%	0.062%
36	14.699	1979	1985	1991	rBV	127530	205120	60.82%	14.128%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072521\
 Data File : BG049450.D
 Acq On : 24 Jul 2021 14:01
 Operator : CG/JU
 Sample : M3087-10
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
 Title : SVOA CALIBRATION

37	14.799	1998	2002	2005	rBB	741	1181	0.35%	0.081%
38	16.226	2241	2245	2248	rBB	882	1058	0.31%	0.073%
39	16.649	2312	2317	2318	rBV	992	983	0.29%	0.068%
40	17.448	2447	2453	2461	rBV	174942	265588	78.75%	18.293%
41	17.525	2464	2466	2468	rBV	845	892	0.26%	0.061%
42	17.595	2476	2478	2481	rVB	724	772	0.23%	0.053%
43	17.660	2486	2489	2491	rBV	721	915	0.27%	0.063%
44	17.795	2510	2512	2514	rBV	992	821	0.24%	0.057%
45	17.877	2524	2526	2529	rBV	900	1153	0.34%	0.079%
46	18.224	2582	2585	2589	rBB	915	908	0.27%	0.063%
47	18.429	2616	2620	2621	rBB	814	796	0.24%	0.055%
48	18.864	2692	2694	2696	rVB	1031	926	0.27%	0.064%
49	18.893	2696	2699	2701	rBV	1357	1313	0.39%	0.090%
50	18.934	2703	2706	2707	rBV2	779	803	0.24%	0.055%
51	19.246	2757	2759	2761	rBV	1280	945	0.28%	0.065%
52	19.346	2773	2776	2779	rBV2	738	942	0.28%	0.065%
53	19.592	2816	2818	2821	rVB2	1113	1146	0.34%	0.079%
54	19.628	2821	2824	2827	rBV2	1324	1424	0.42%	0.098%
55	19.757	2842	2846	2848	rBV2	1081	1379	0.41%	0.095%
56	19.780	2848	2850	2853	rVB2	1393	940	0.28%	0.065%
57	19.822	2856	2857	2859	rBV	1317	771	0.23%	0.053%
58	20.009	2887	2889	2890	rBV	1823	1074	0.32%	0.074%
59	20.027	2890	2892	2895	rVB3	1087	1047	0.31%	0.072%
60	20.280	2933	2935	2936	rBV	1731	1204	0.36%	0.083%
61	20.861	3033	3034	3036	rVB2	2317	1168	0.35%	0.080%
62	21.725	3175	3181	3189	rBV	195655	337245	100.00%	23.229%
63	25.003	3732	3739	3752	rVB3	111425	323561	95.94%	22.286%




Sum of corrected areas: 1451832

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072521\
Data File : BG049450.D
Acq On : 24 Jul 2021 14:01
Operator : CG/JU
Sample : M3087-10
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

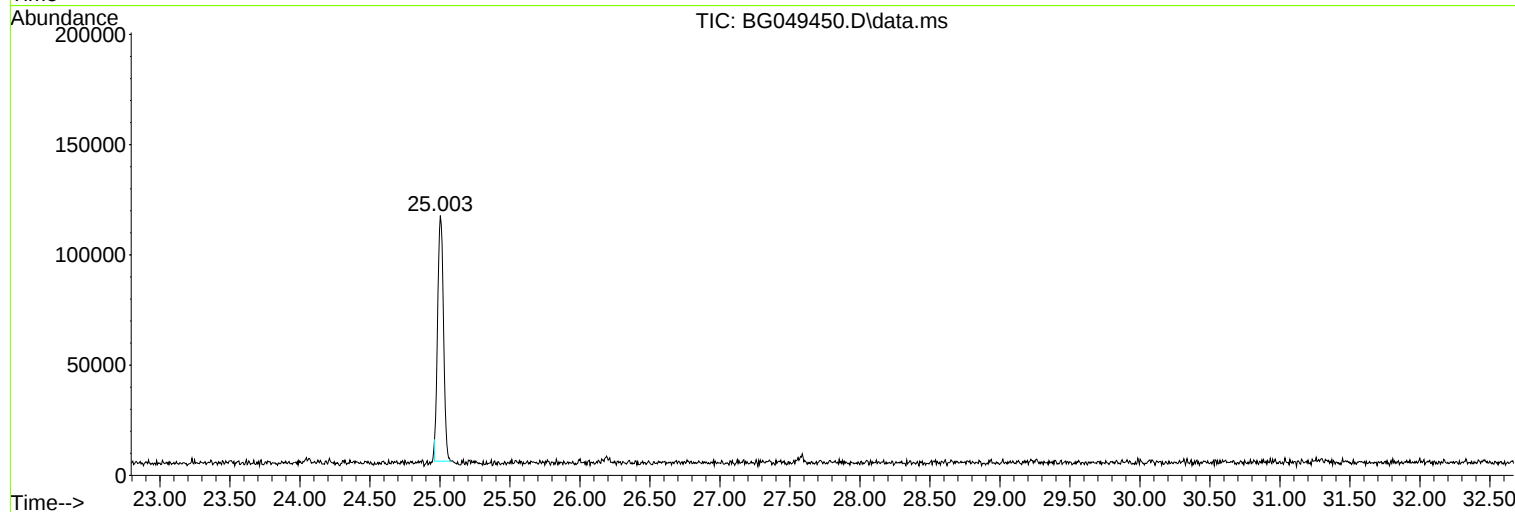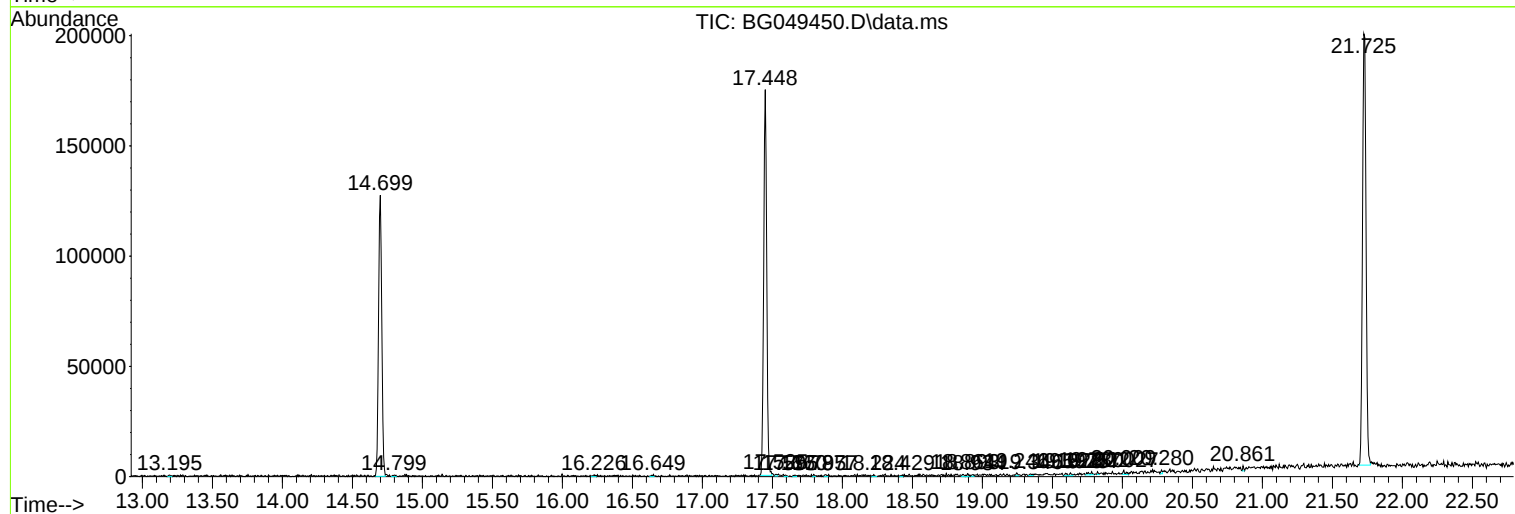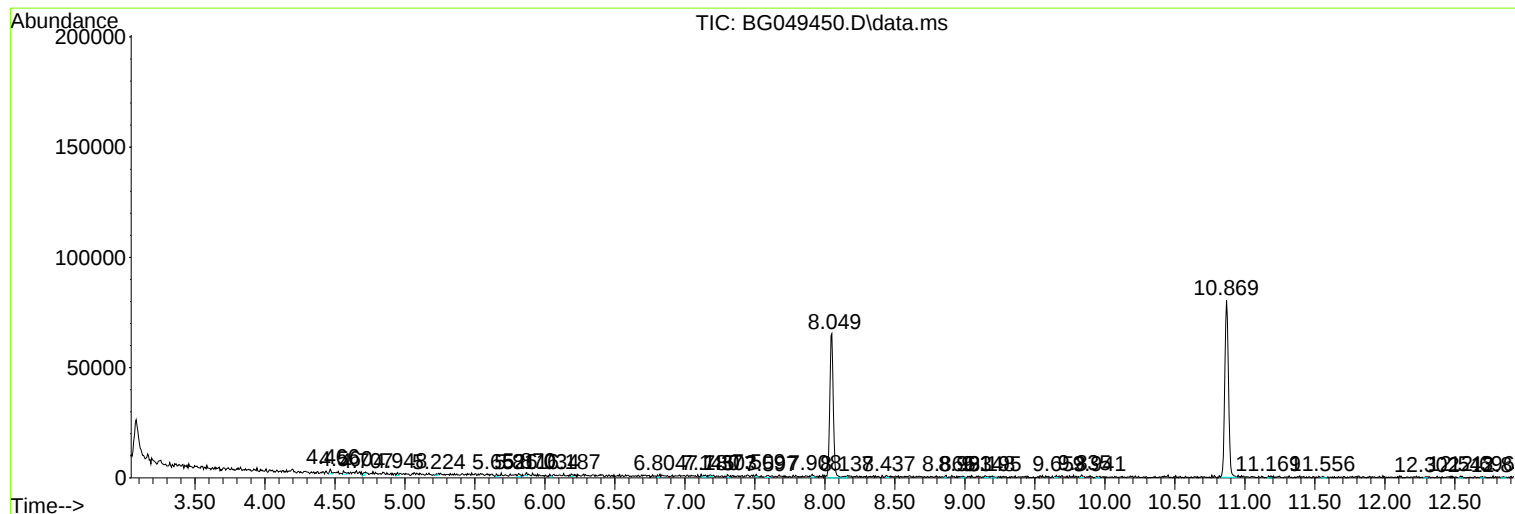

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072521\
Data File : BG049450.D
Acq On : 24 Jul 2021 14:01
Operator : CG/JU
Sample : M3087-10
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072521\
Data File : BG049450.D
Acq On : 24 Jul 2021 14:01
Operator : CG/JU
Sample : M3087-10
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------