
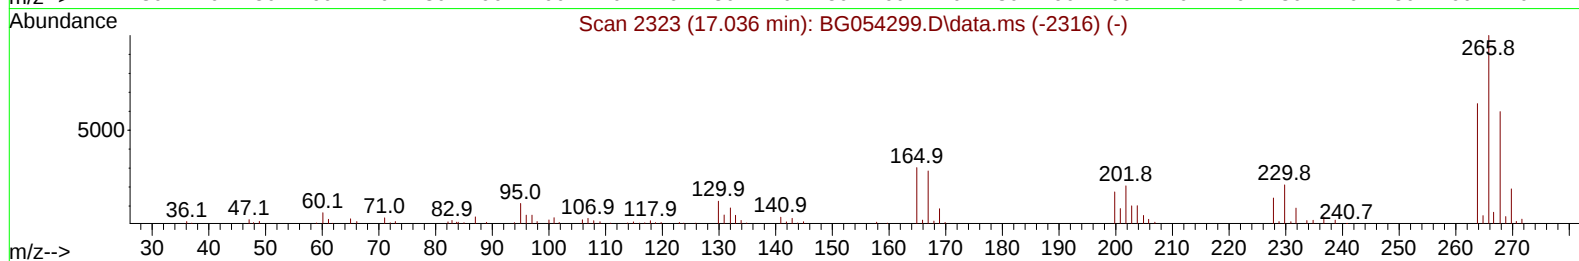
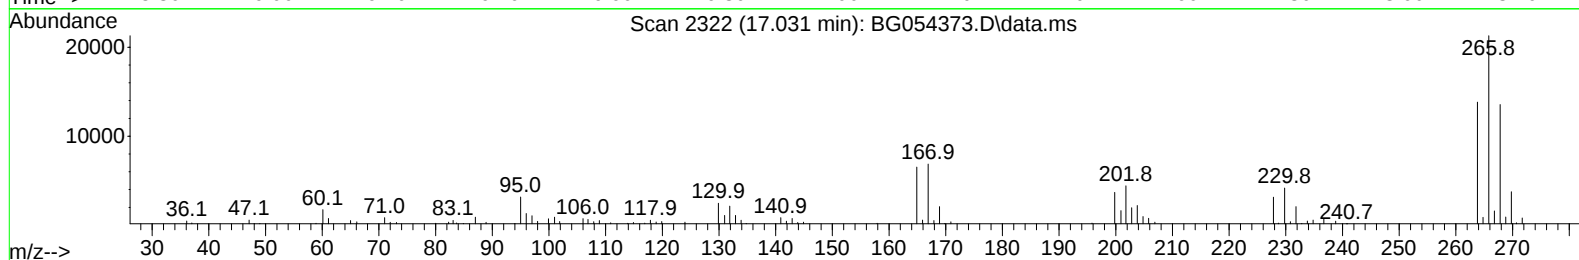


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG072522\  
Data File : BG054373.D  
Acq On : 25 Jul 2022 10:14  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 25 10:52:08 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG071522.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Jul 15 15:54:11 2022  
Response via : Initial Calibration

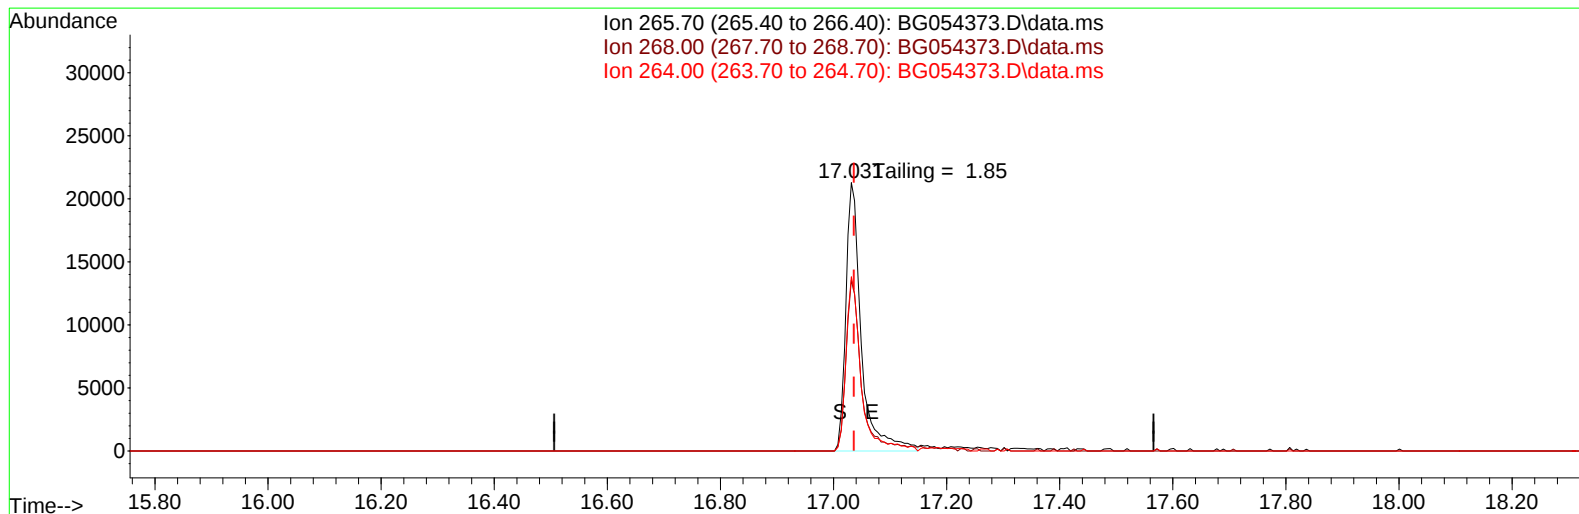

TIC: BG054373.D\data.ms

**(70) Pentachlorophenol (C)**




17.031min (-0.005) 18695.64 ng

response 40592

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 70.20  | 63.67  |
| 264.00 | 66.20  | 64.91  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG072522\  
 Data File : BG054373.D  
 Acq On : 25 Jul 2022 10:14  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 25 10:52:08 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG071522.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jul 15 15:54:11 2022  
 Response via : Initial Calibration

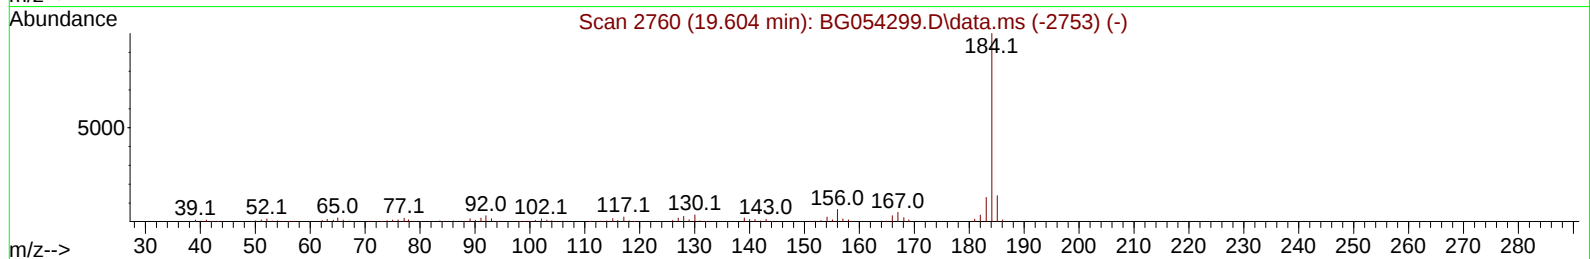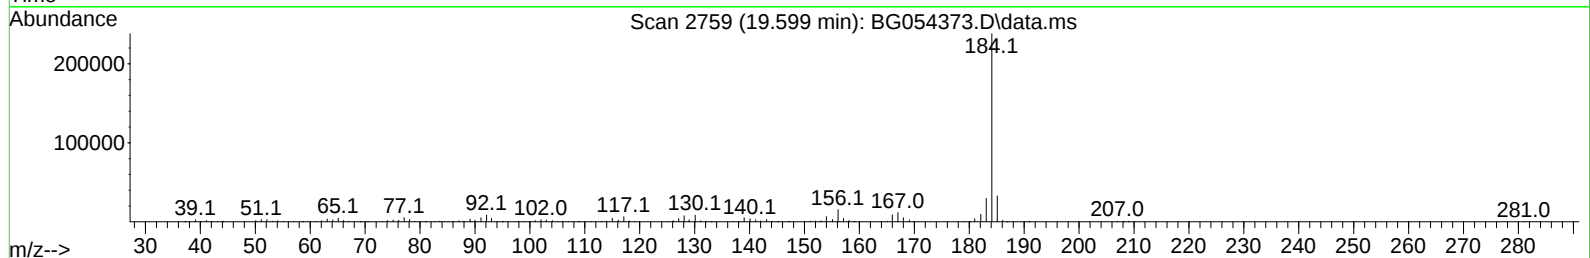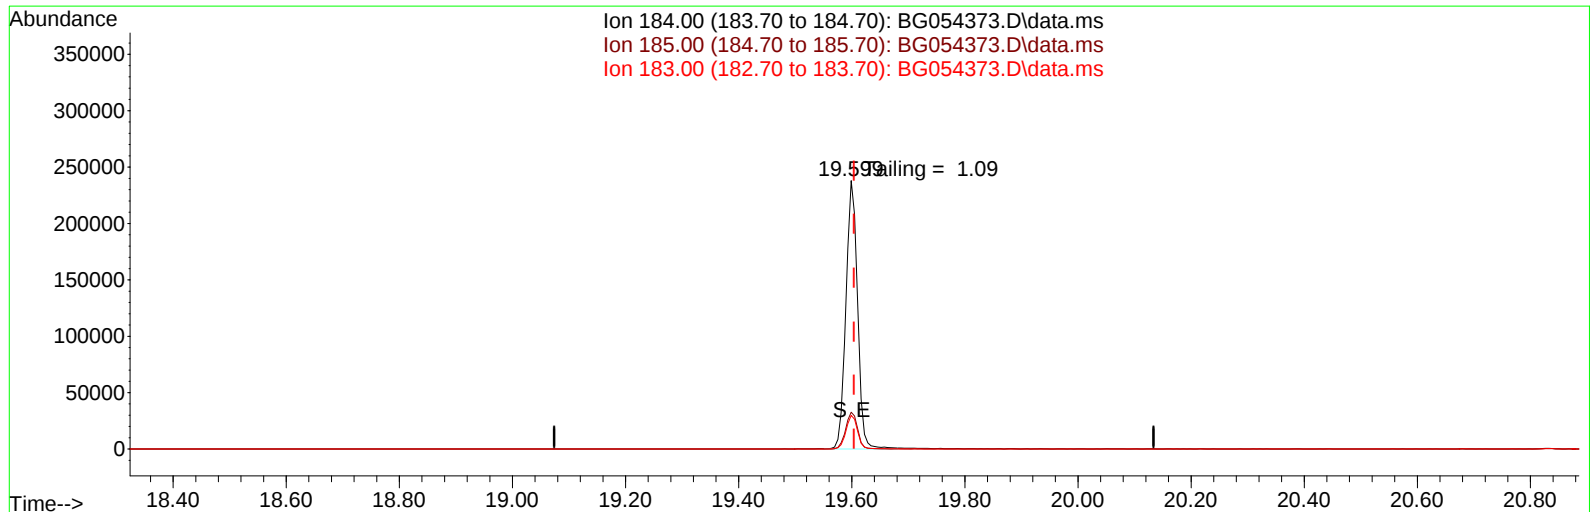

TIC: BG054373.D\data.ms

**(77) Benzidine****19.599min (-0.005) 314810.11 ng****response 342087**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.70  | 13.75  |
| 183.00 | 11.10  | 12.51  |
| 0.00   | 0.00   | 0.00   |