
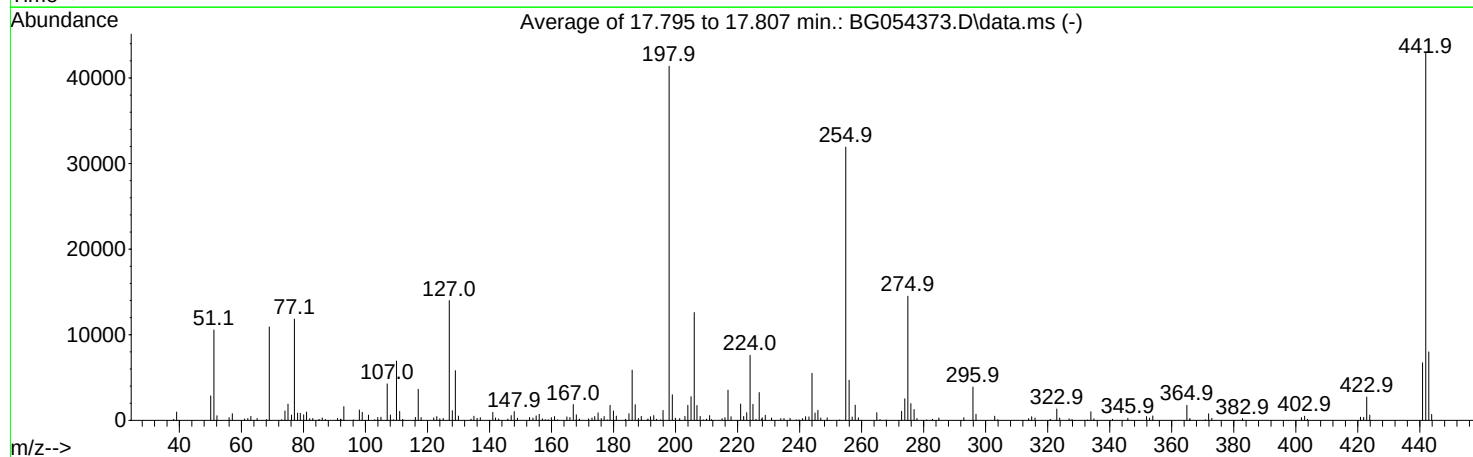


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072522\
 Data File : BG054373.D
 Acq On : 25 Jul 2022 10:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 15 15:54:11 2022

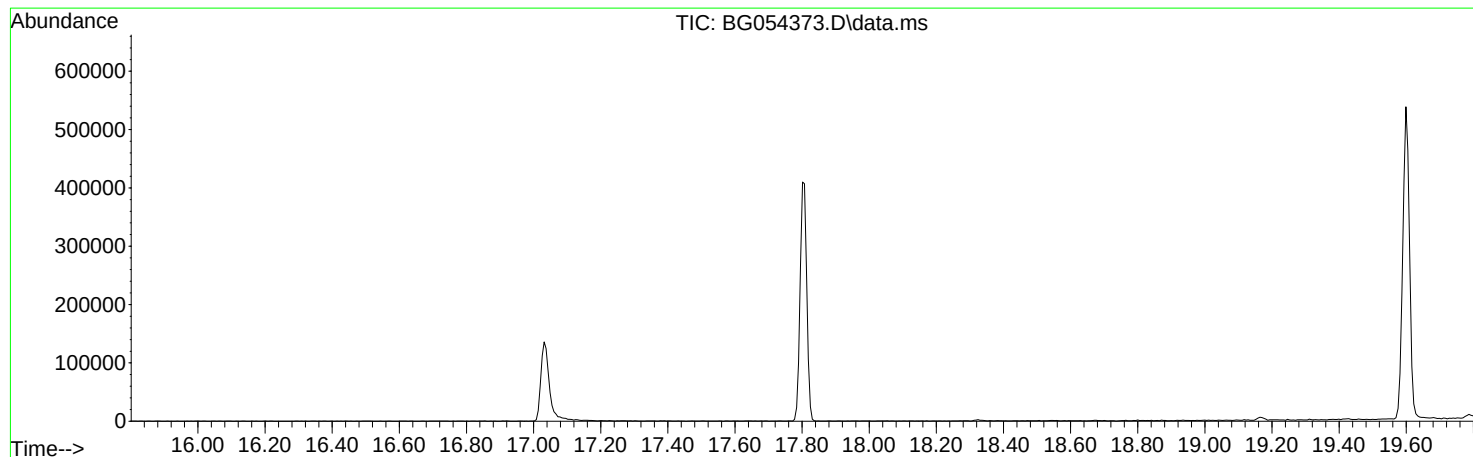




AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2446

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.5	10561	PASS
68	69	0.00	2	0.8	90	PASS
69	198	0.00	100	26.4	10919	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	33.8	13995	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	41363	PASS
199	198	5	9	7.3	3000	PASS
275	198	10	60	35.1	14511	PASS
365	198	1	100	4.3	1758	PASS
441	198	0.01	100	16.3	6739	PASS
442	442	50	100	100.0	42968	PASS
443	442	15	24	18.6	8006	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072522\
Data File : BG054373.D
Acq On : 25 Jul 2022 10:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 25 10:52:08 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 15 15:54:11 2022
Response via : Initial Calibration

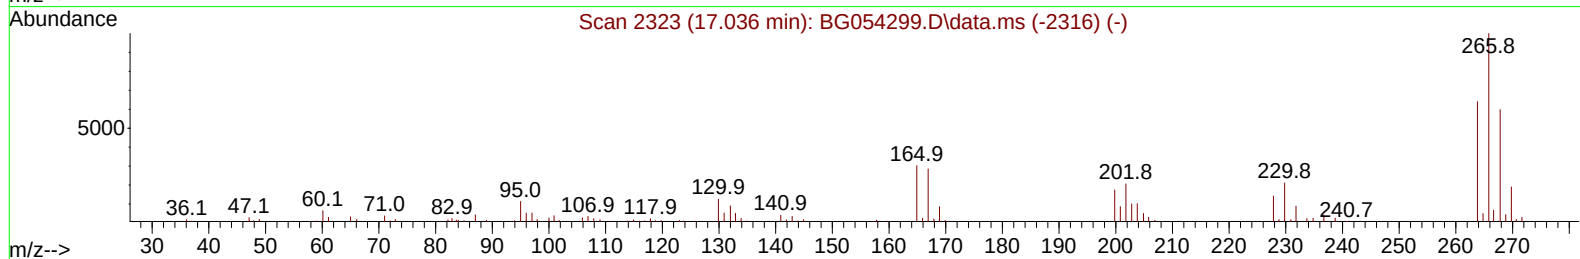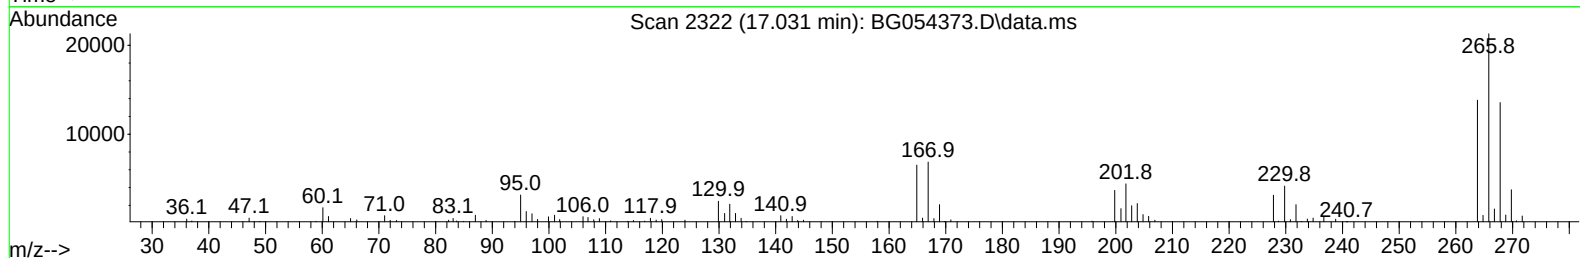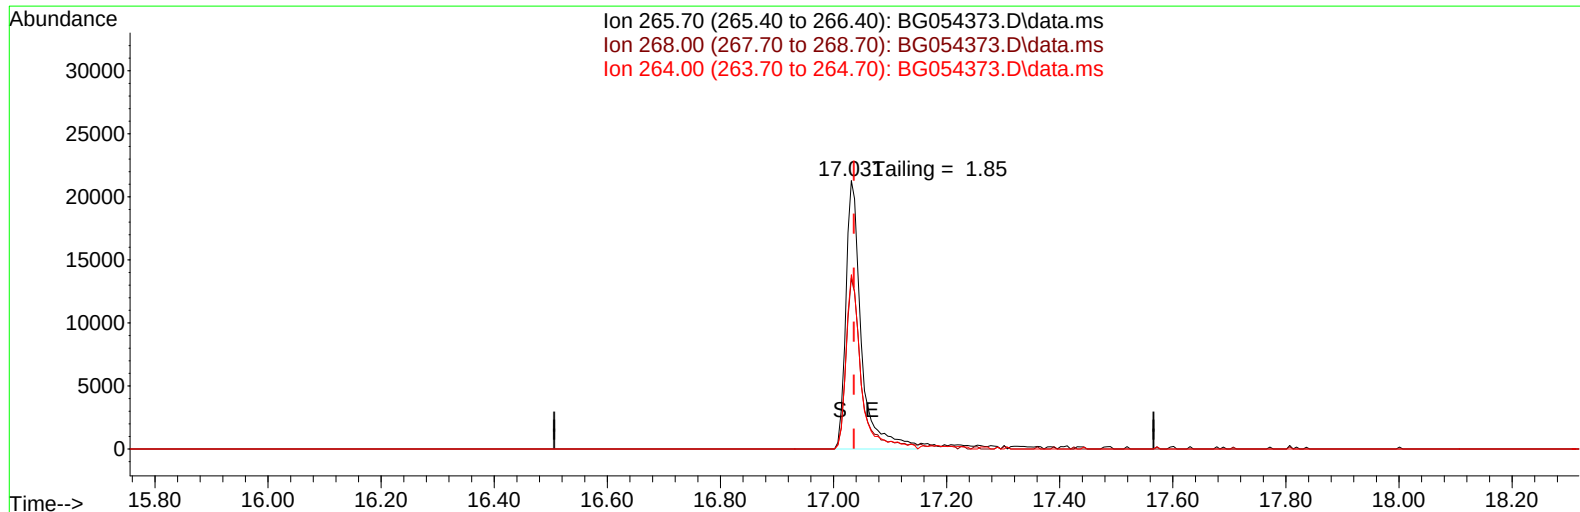

TIC: BG054373.D\data.ms

(70) Pentachlorophenol (C)

17.031min (-0.005) 18695.64 ng




response 40592

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	63.67
264.00	66.20	64.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072522\
 Data File : BG054373.D
 Acq On : 25 Jul 2022 10:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Jul 25 10:52:08 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 15 15:54:11 2022
 Response via : Initial Calibration

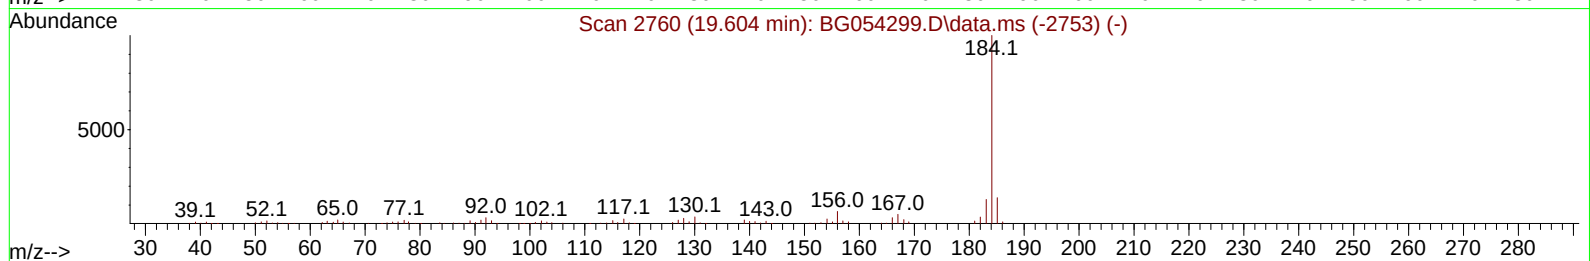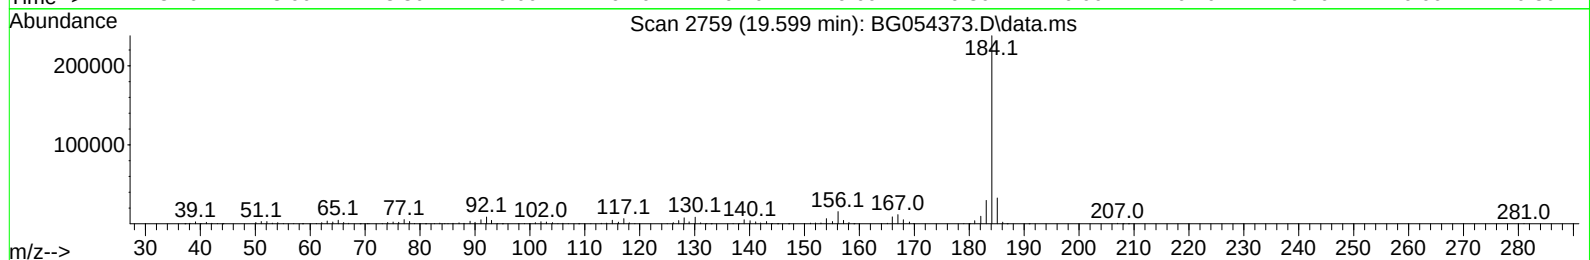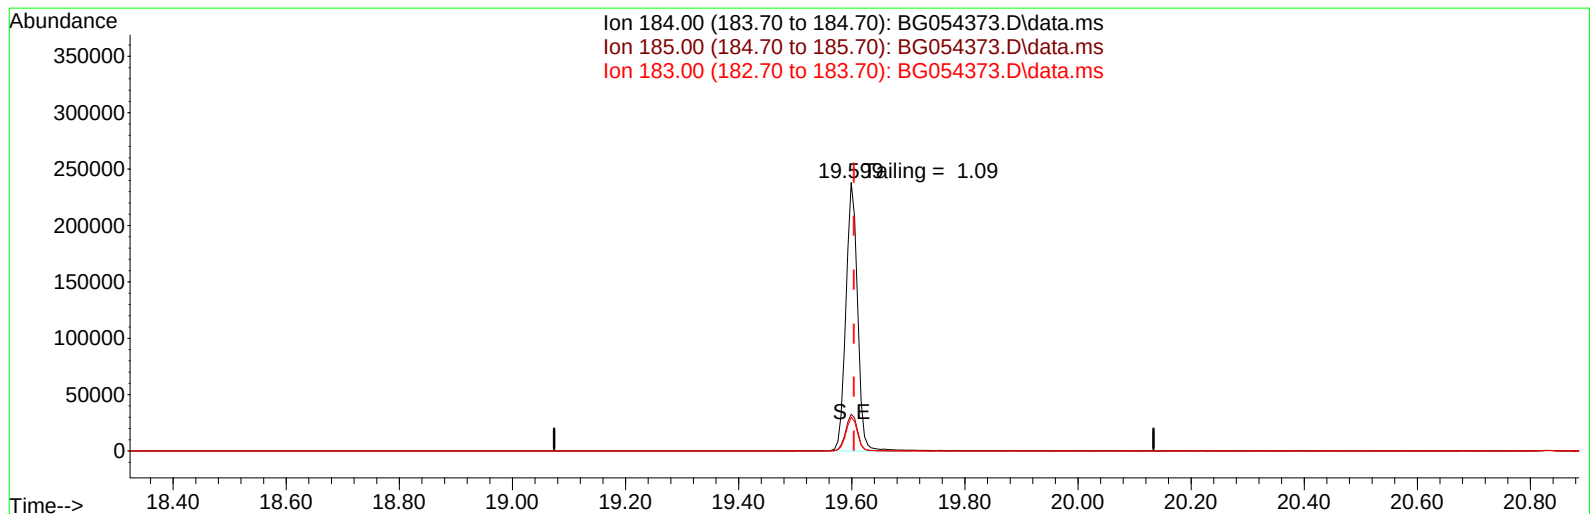

TIC: BG054373.D\data.ms

(77) Benzidine

19.599min (-0.005) 314810.11 ng

response 342087

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.75
183.00	11.10	12.51
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/25/2022	BNA_G	<u>BG054373.D</u>
Compound Name	Response	Retention Time
DDT	181703	20.833
DDD	3421	20.392
DDE	225	19.887
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3646	185349	1.97

Instrument :
BNA_G
ClientSampleId :
DFTPP