


Data Path : Z:\HPCHEM1\BNA G\DATA\BG072616\
 Data File : BG023267.D
 Acq On : 26 Jul 2016 13:13
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG072616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 27 17:30:33 2016

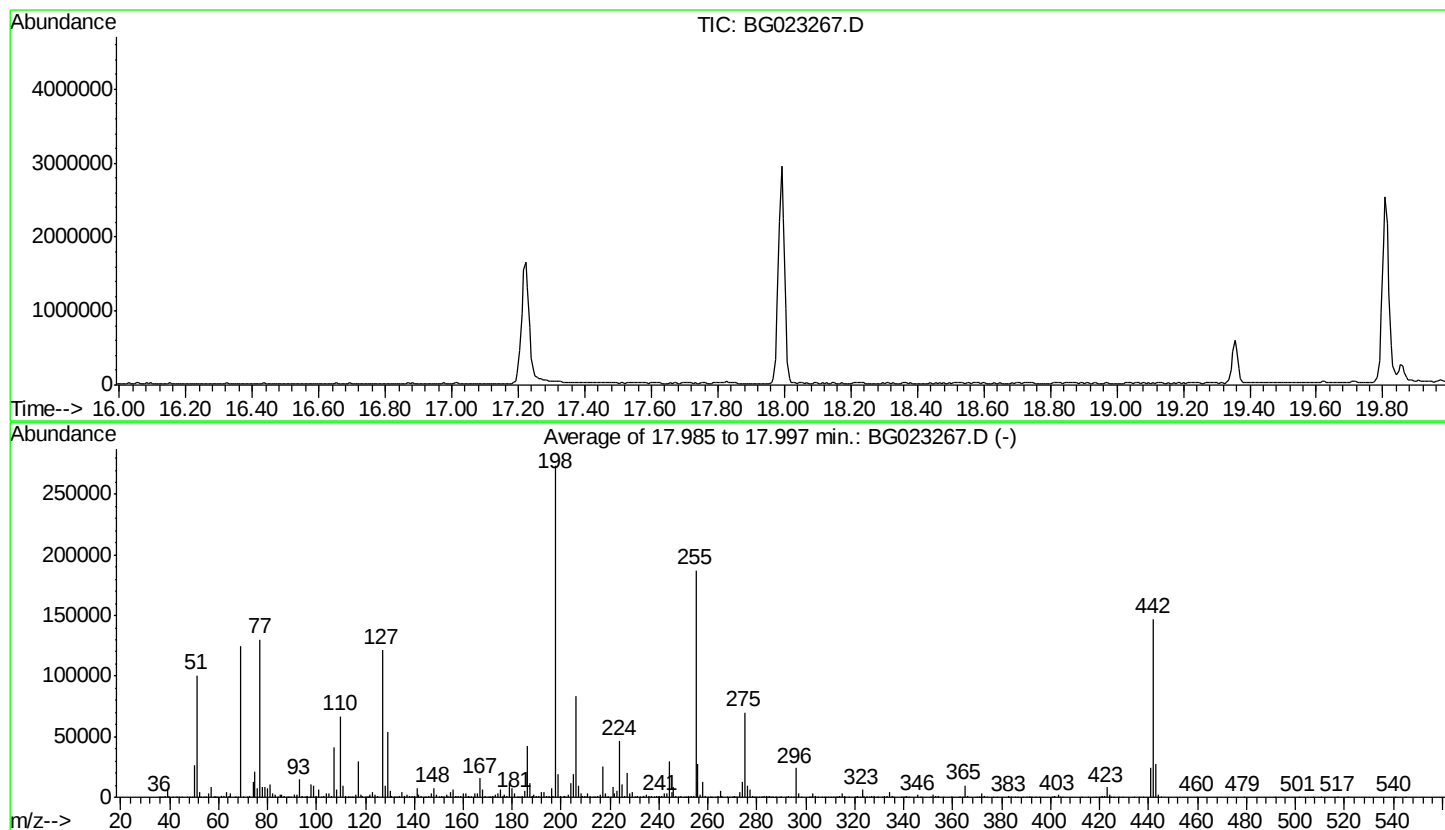

AutoFind: Scans 2578, 2579, 2580; Background Corrected with Scan 2570

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.8	100765	PASS
68	69	0.00	2	0.4	499	PASS
69	198	0.00	100	45.7	125029	PASS
70	69	0.00	2	0.4	456	PASS
127	198	10	80	44.5	121765	PASS
197	198	0.00	2	0.4	1075	PASS
198	198	100	100	100.0	273792	PASS
199	198	5	9	7.1	19376	PASS
275	198	10	60	25.6	69970	PASS
365	198	1	100	3.6	9943	PASS
441	442	0.01	24	16.8	24762	PASS
442	198	50	100	53.7	147008	PASS
443	442	15	24	18.4	27066	PASS