
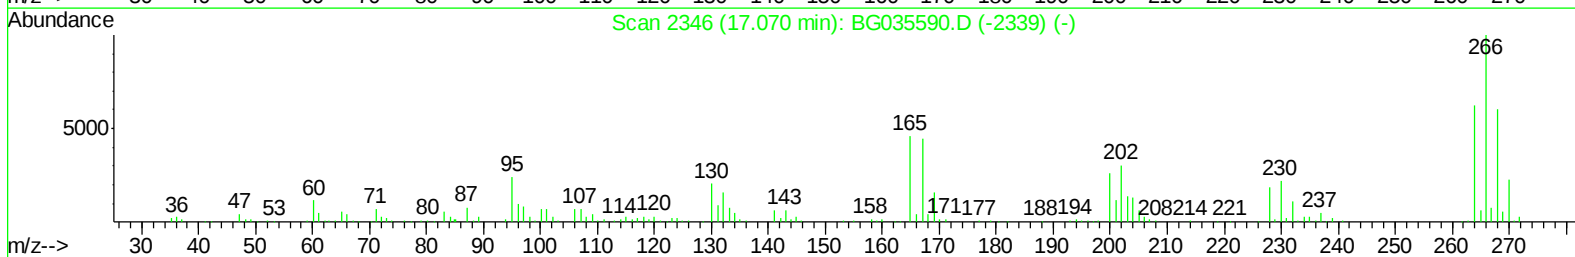
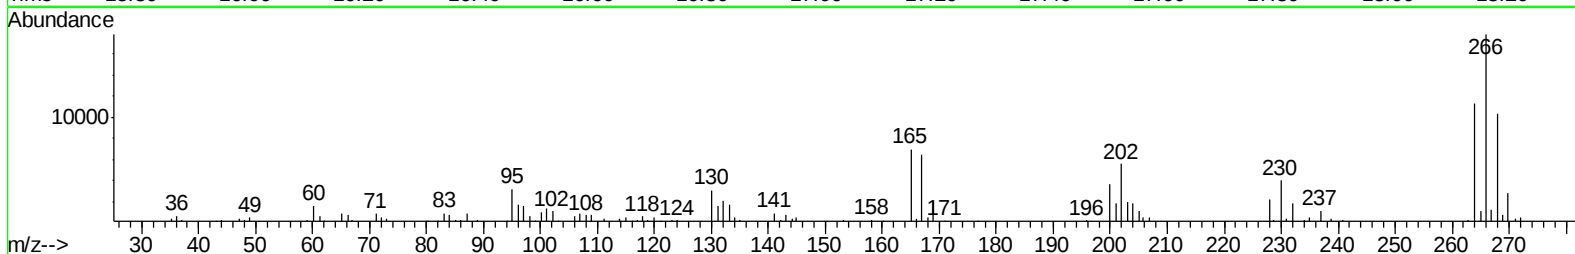


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072618\
Data File : BG035911.D
Acq On : 26 Jul 2018 16:35
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 30 06:04:09 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 25 11:04:14 2018
Response via : Initial Calibration

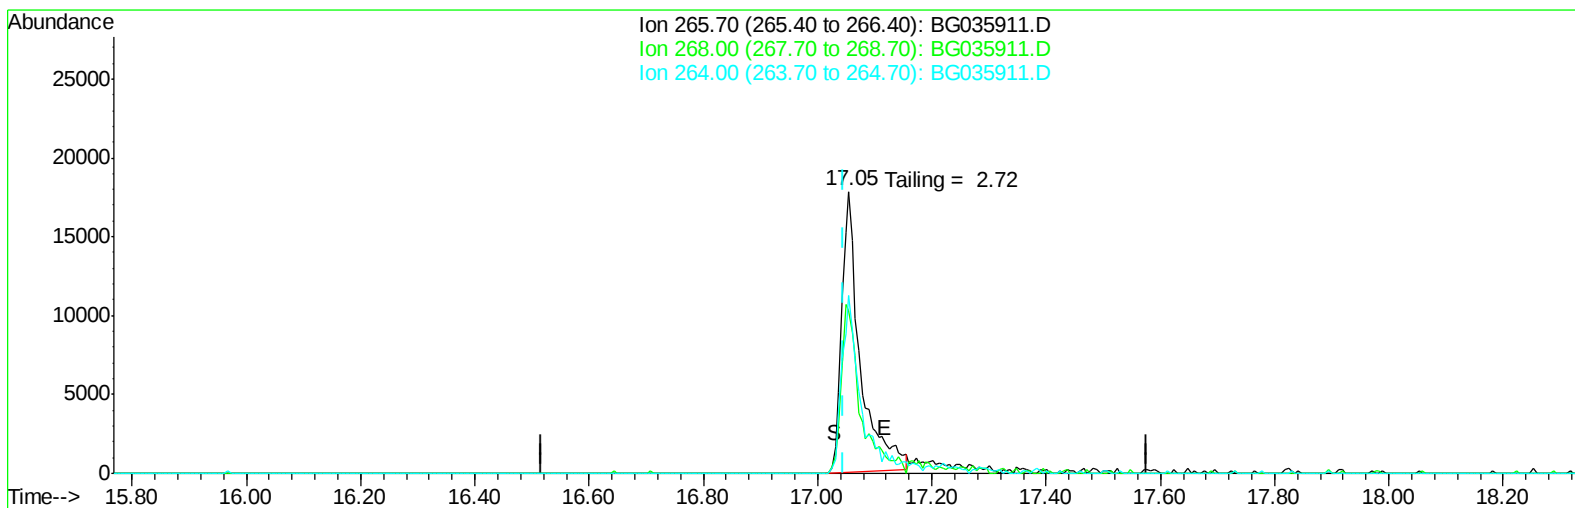

TIC: BG035911.D

(69) Pentachlorophenol (C)




17.054min (+0.007) 77167.43ng

response 40994

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	57.59
264.00	62.00	63.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072618\
Data File : BG035911.D
Acq On : 26 Jul 2018 16:35
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 30 06:04:09 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 25 11:04:14 2018
Response via : Initial Calibration

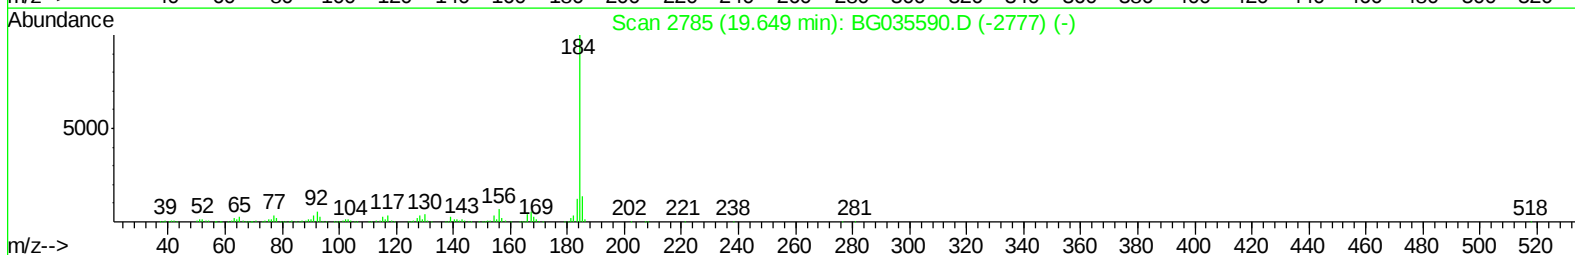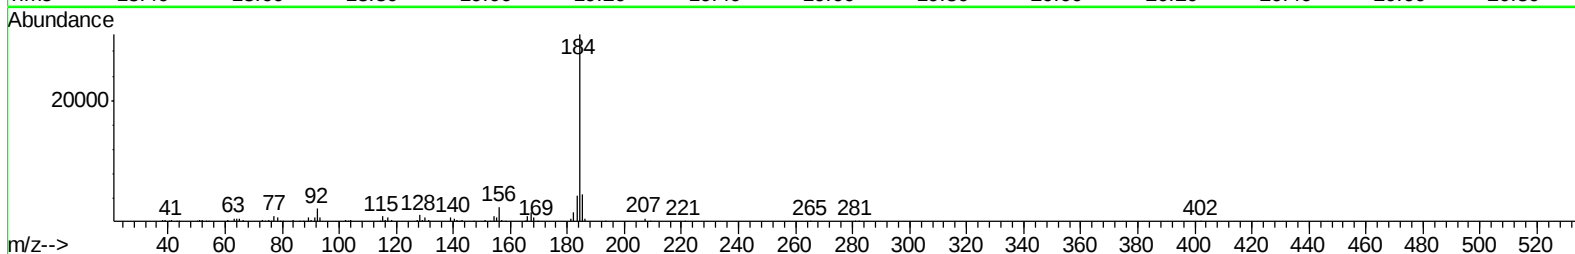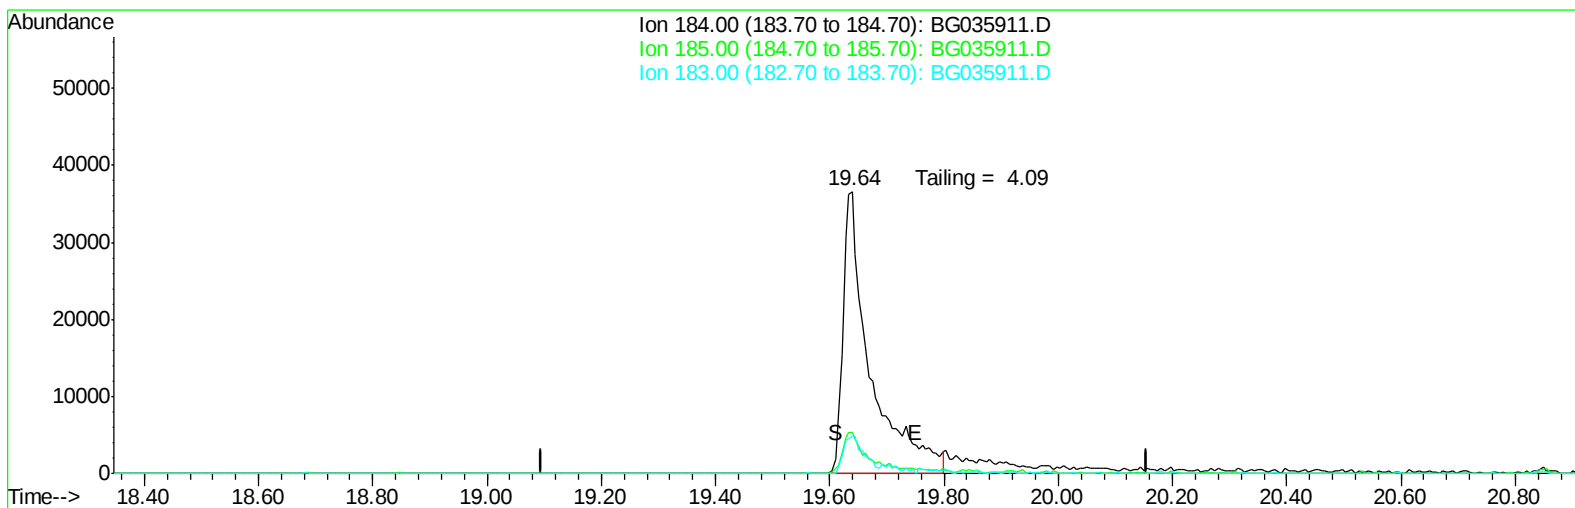

TIC: BG035911.D

(76) Benzidine

19.626min (-19.626) 0.00ng

response 0

Ion	Exp%	Act%
184.00	100	0.00
185.00	13.90	0.00#
183.00	13.30	0.00#
0.00	0.00	0.00