


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG072618\
 Data File : BG035911.D
 Acq On : 26 Jul 2018 16:35
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 31 12:30:06 2018

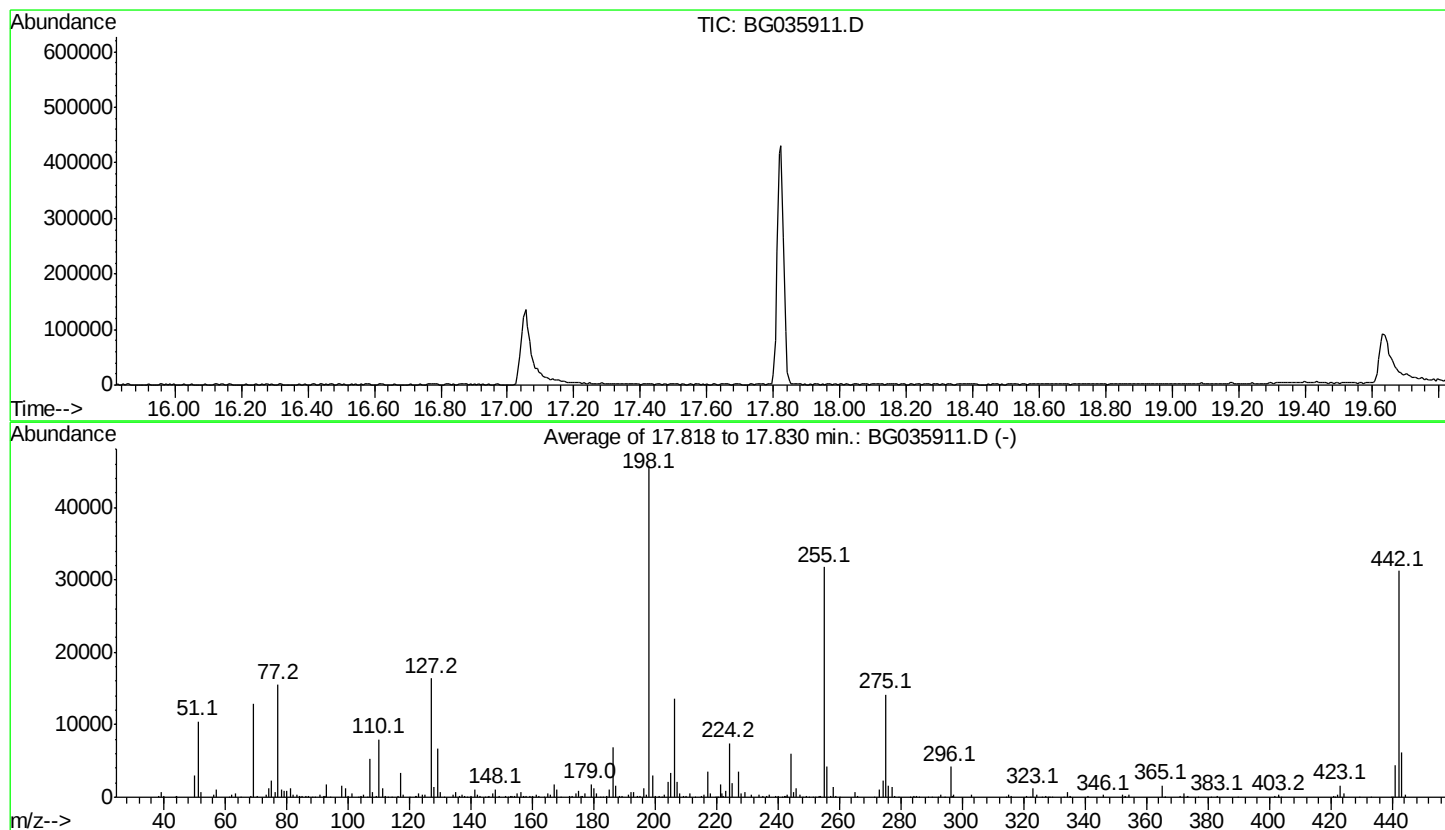

AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.9	10485	PASS
68	69	0.00	2	0.7	94	PASS
69	198	0.00	100	28.4	12981	PASS
70	69	0.00	2	1.4	185	PASS
127	198	10	80	35.8	16384	PASS
197	198	0.00	2	0.7	303	PASS
198	198	100	100	100.0	45760	PASS
199	198	5	9	6.7	3053	PASS
275	198	10	60	30.9	14159	PASS
365	198	1	100	3.6	1666	PASS
441	198	0.01	100	9.7	4455	PASS
442	198	50	100	68.2	31186	PASS
443	442	15	24	20.0	6230	PASS