

Quantitation Report (QT Reviewed)


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072621\  
Data File : BG049523.D  
Acq On    : 28 Jul 2021    2:14  
Operator  : CG/JU  
Sample    : SSTDCCC020EC  
Misc      :  
ALS Vial  : 53    Sample Multiplier: 1
```

Instrument :
BNA_G
LabSampleId :
SSTDCCC020EC

Manual Integrations
APPROVED

mohammad
7/28/2021 11:30:20 AM

Quant Time: Jul 28 06:33:20 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 26 11:36:47 2021
Response via : Initial Calibration

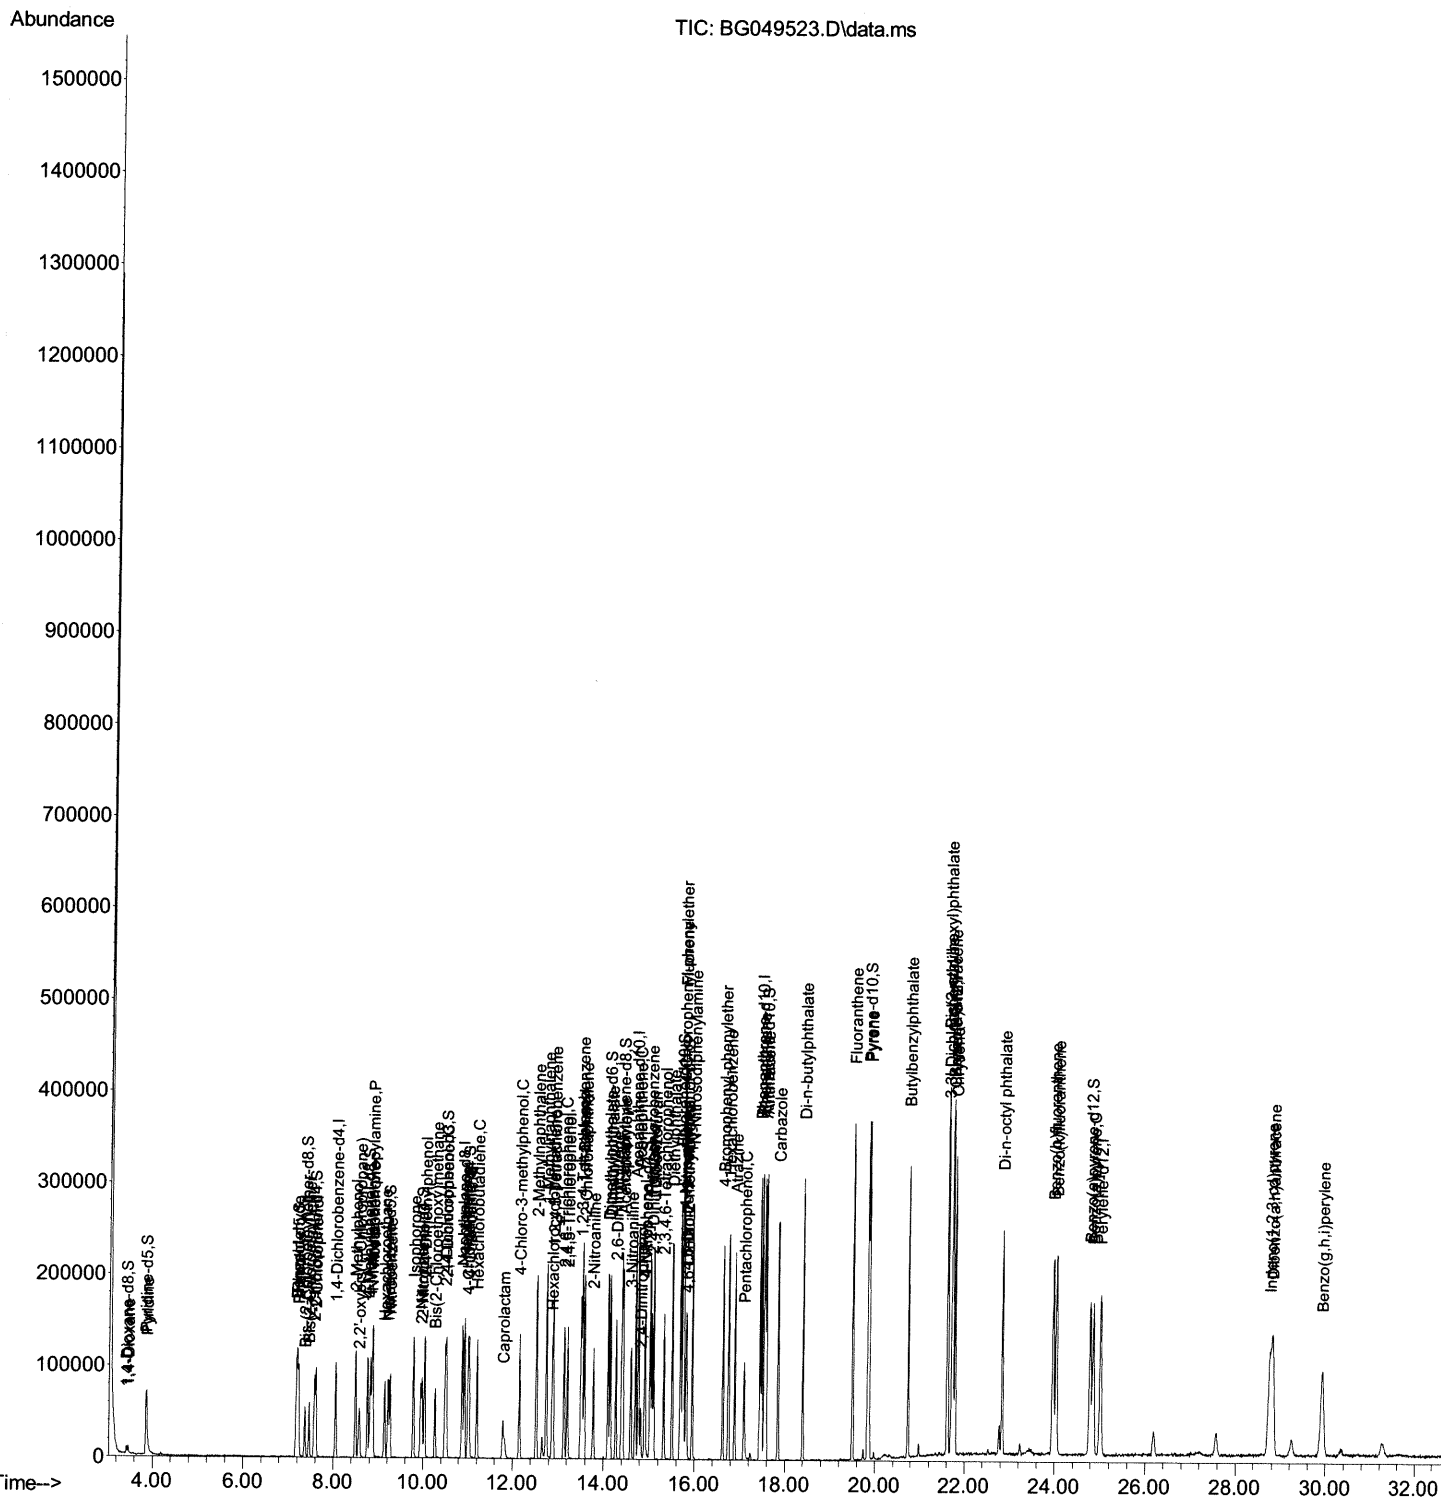

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072621\
 Data File : BG049523.D
 Acq On : 28 Jul 2021 2:14
 Operator : CG/JU
 Sample : SSTDCCC020EC
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020EC

Manual Integrations
 APPROVED

mohammad
 7/28/2021 11:30:20 AM

Quant Time: Jul 28 06:33:20 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 26 11:36:47 2021
 Response via : Initial Calibration

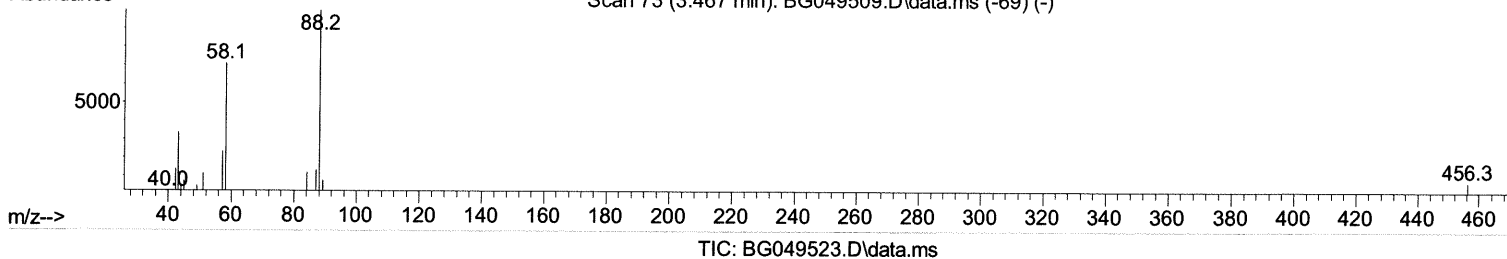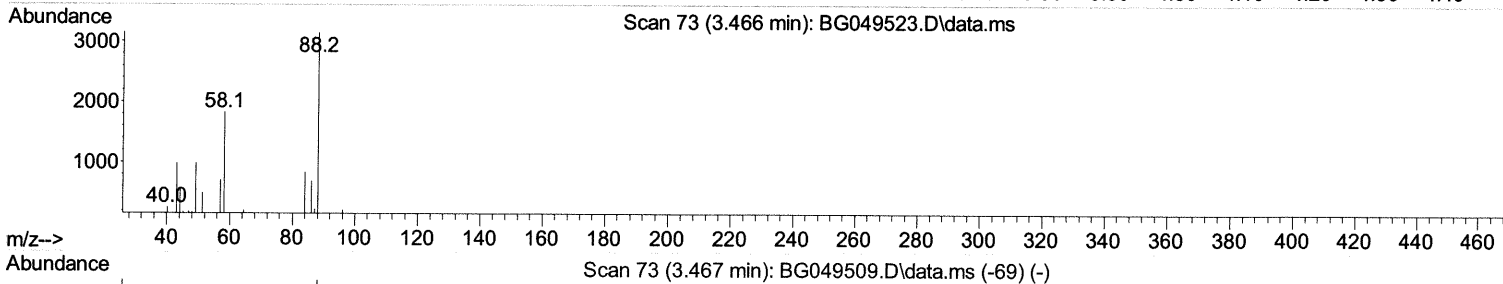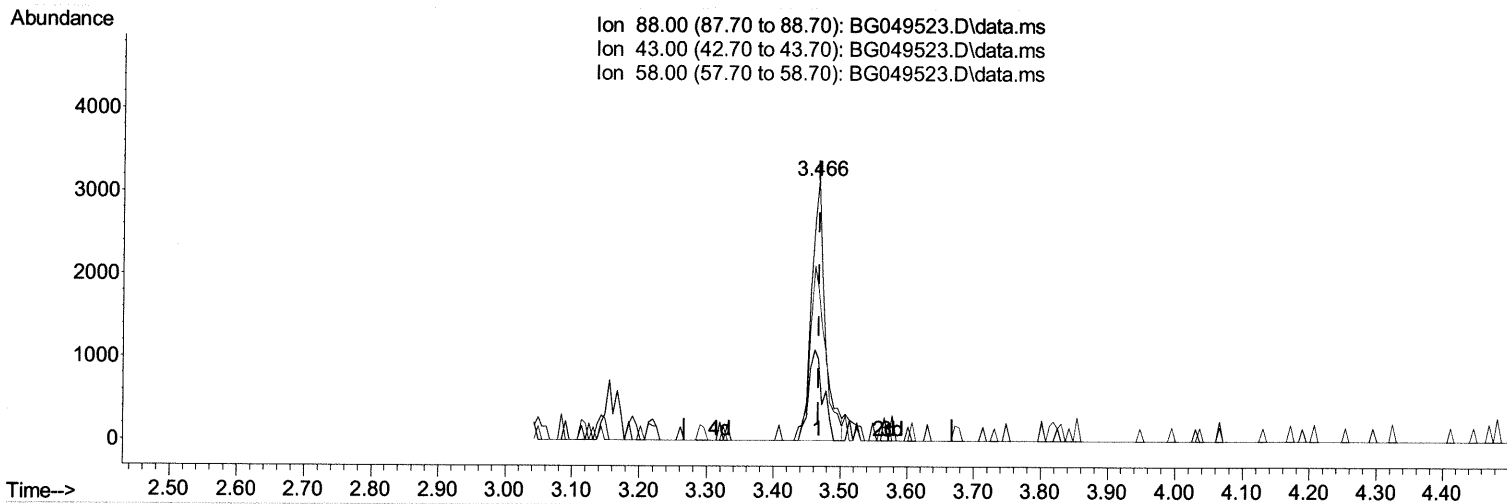

TIC: BG049523.D\data.ms

(2) 1,4-Dioxane

3.466min (-0.001) 5.62 ng/uL

response 4588

Ion	Exp%	Act%
88.00	100.00	100.00
43.00	36.90	31.30
58.00	71.00	58.08
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072621\
 Data File : BG049523.D
 Acq On : 28 Jul 2021 2:14
 Operator : CG/JU
 Sample : SSTDCCC020EC
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020EC

Manual Integrations
 APPROVED

mohammad
 7/28/2021 11:30:20 AM

Quant Time: Jul 28 06:33:20 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 26 11:36:47 2021
 Response via : Initial Calibration

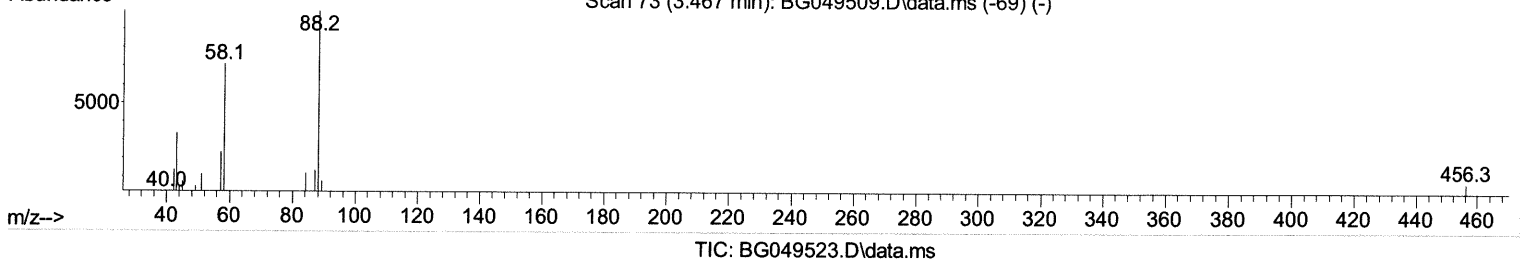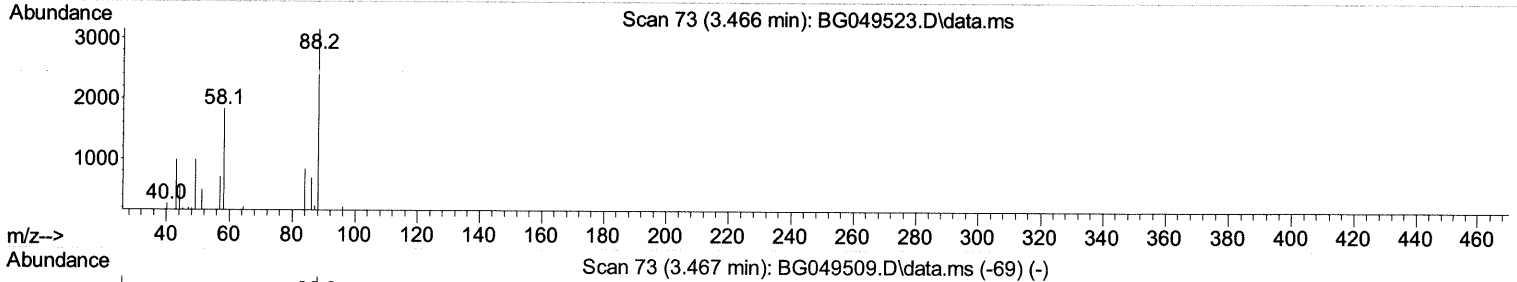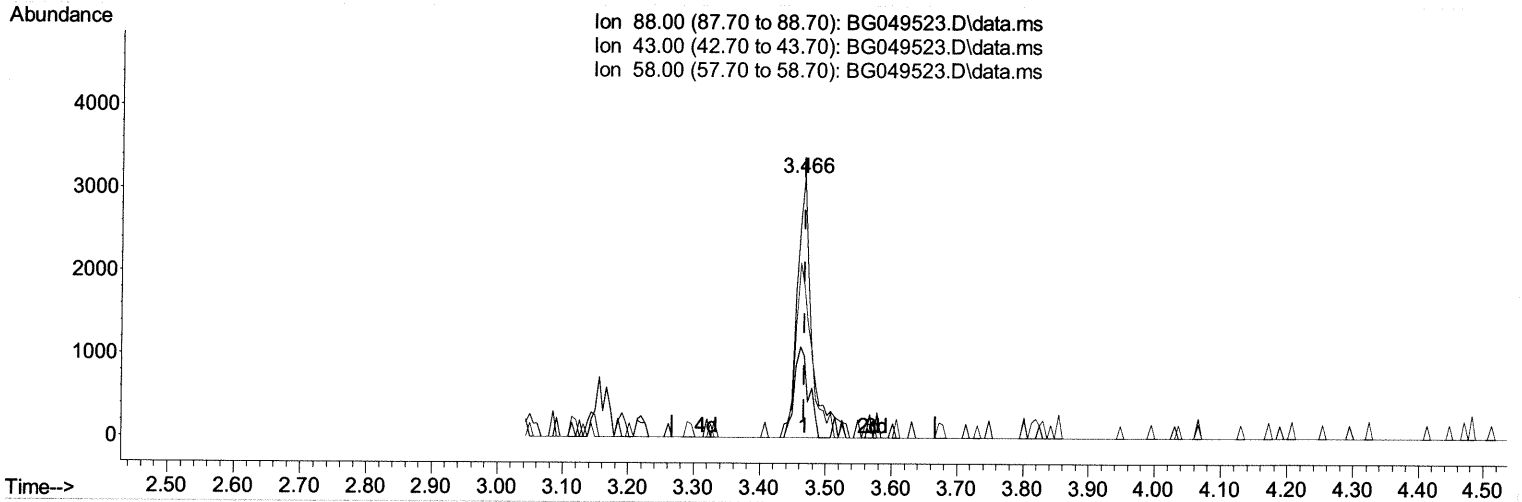

(2) 1,4-Dioxane

3.466min (-0.001) 6.10 ng/uL m 07/29/21ju

response 4984

Ion	Exp%	Act%
88.00	100.00	100.00
43.00	36.90	31.30
58.00	71.00	58.08
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072621\
 Data File : BG049523.D
 Acq On : 28 Jul 2021 2:14
 Operator : CG/JU
 Sample : SSTDCCC020EC
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020EC

Manual Integrations
 APPROVED

mohammad
 7/28/2021 11:30:20 AM

Quant Time: Jul 28 06:33:20 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 26 11:36:47 2021
 Response via : Initial Calibration

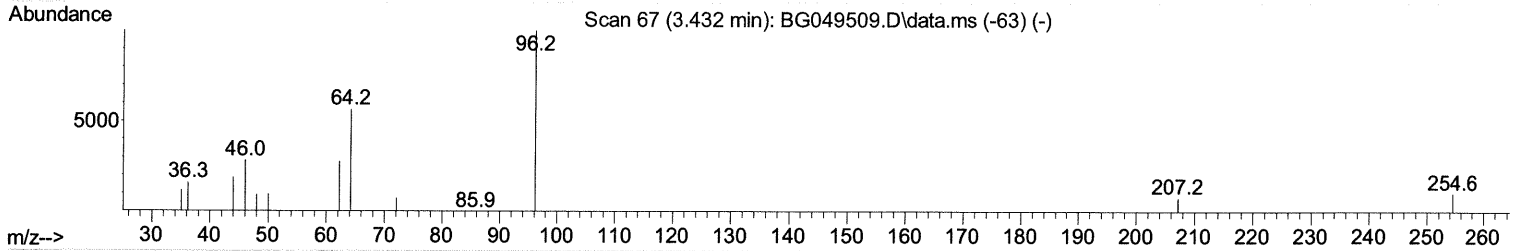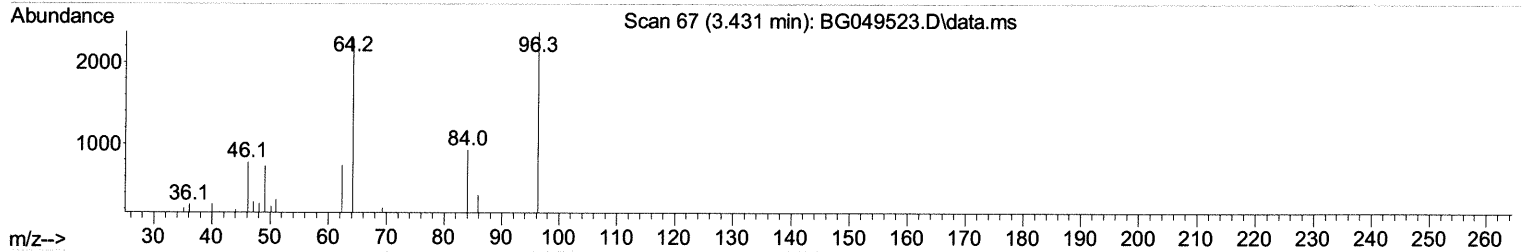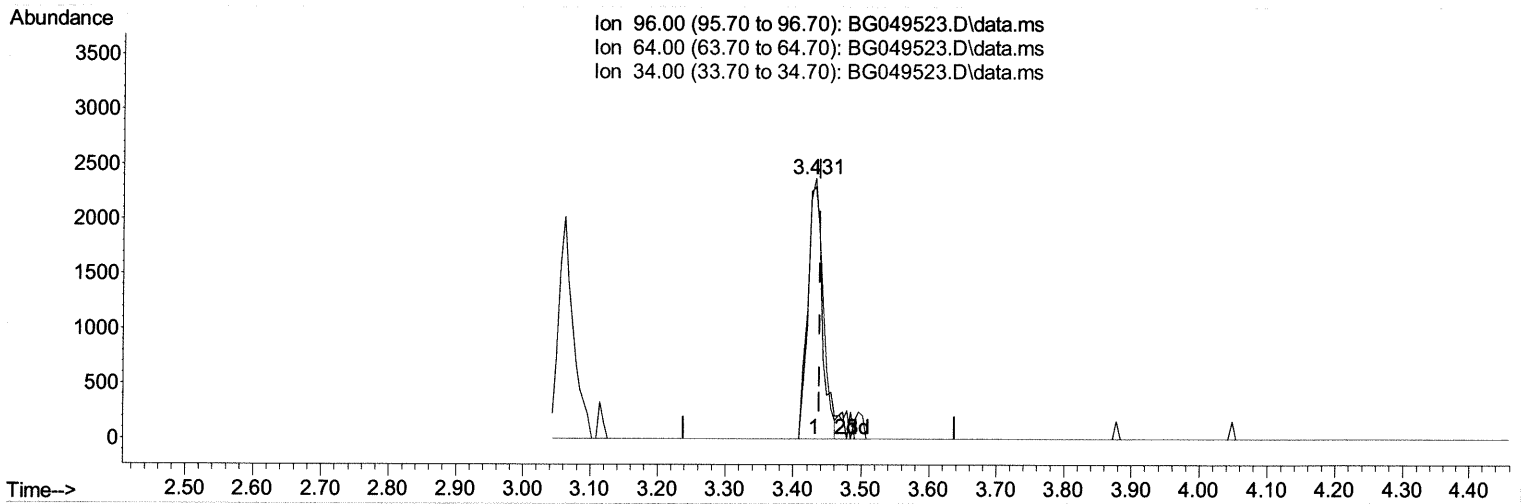

TIC: BG049523.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.431min (-0.007) 6.20 ng/uL

response 3708

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	62.60	96.88#
34.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072621\
 Data File : BG049523.D
 Acq On : 28 Jul 2021 2:14
 Operator : CG/JU
 Sample : SSTDCCC020EC
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020EC

Manual Integrations
 APPROVED

mohammad
 7/28/2021 11:30:20 AM

Quant Time: Jul 28 06:33:20 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 26 11:36:47 2021
 Response via : Initial Calibration

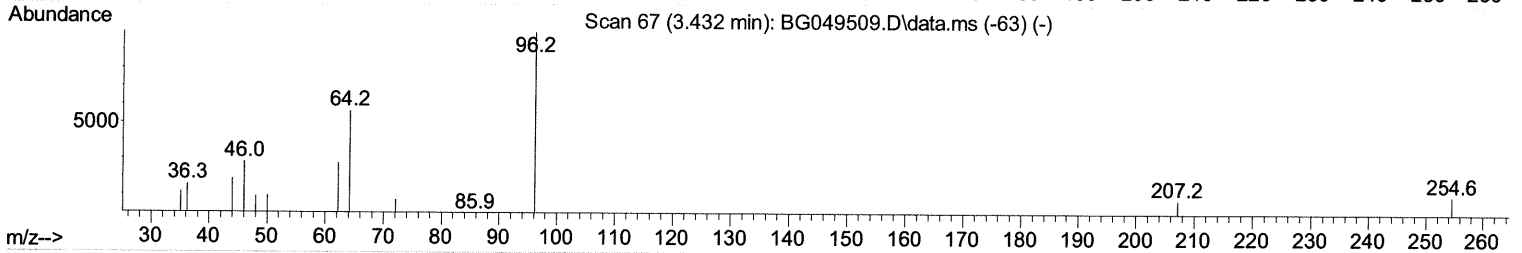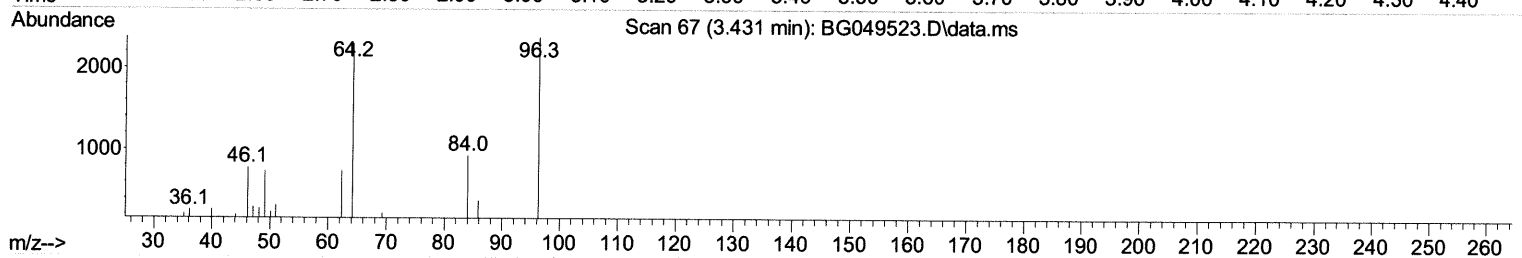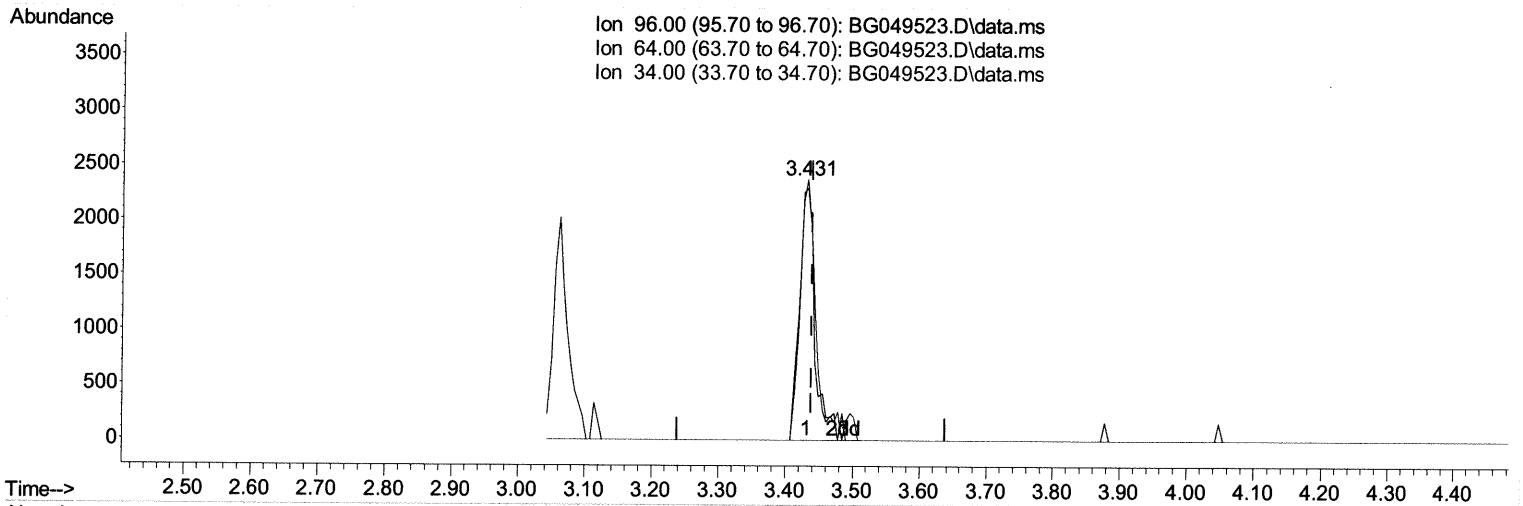

TIC: BG049523.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.431min (-0.007) 6.58 ng/uL m 07/29/21 JU

response 3934

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	62.60	96.88#
34.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072621\
 Data File : BG049523.D
 Acq On : 28 Jul 2021 2:14
 Operator : CG/JU
 Sample : SSTDCCC020EC
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020EC

Manual Integrations
 APPROVED

mohammad
 7/28/2021 11:30:20 AM

Quant Time: Jul 28 06:33:20 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 26 11:36:47 2021
 Response via : Initial Calibration

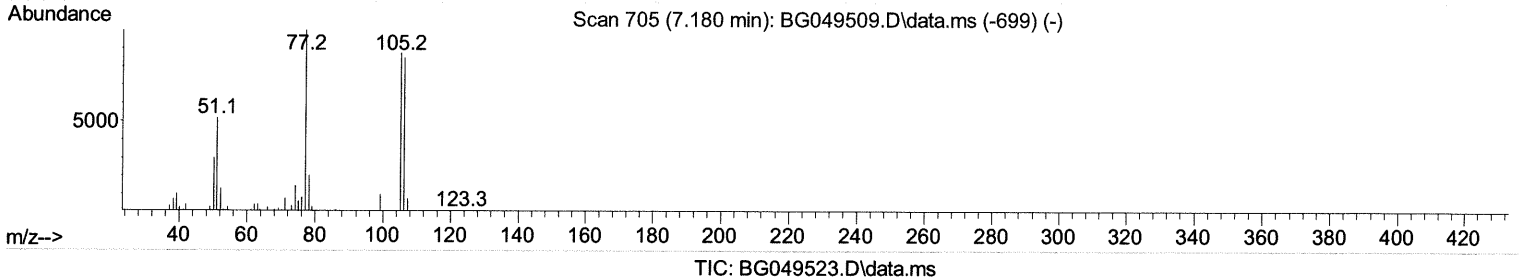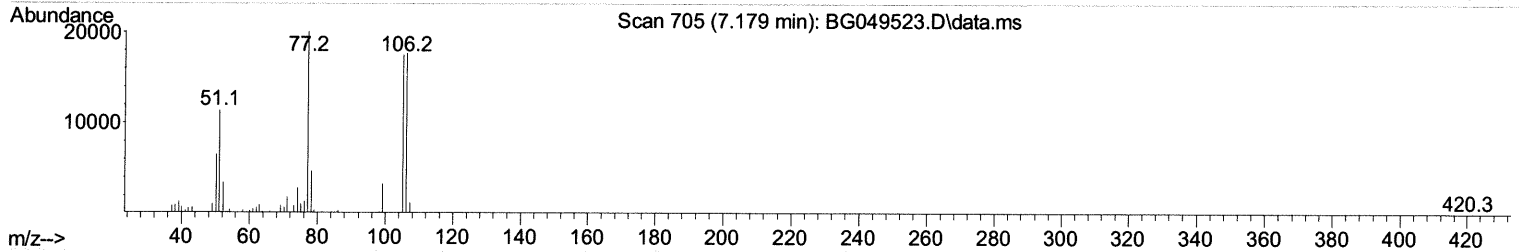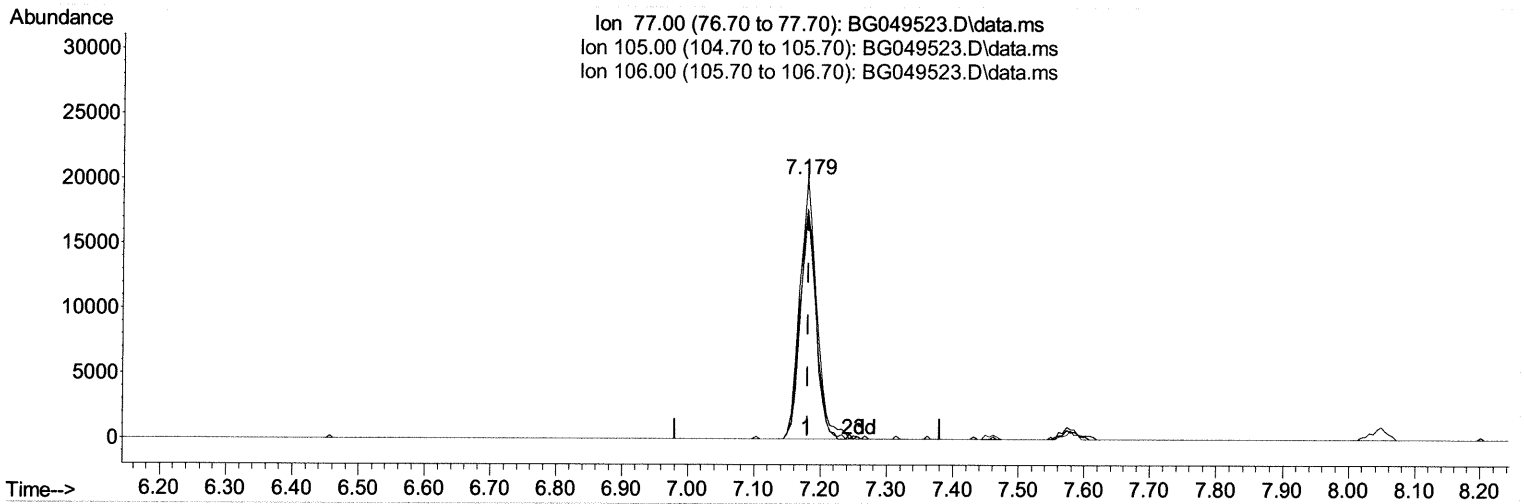

(6) Benzaldehyde

7.179min (-0.001) 24.66 ng/ul

response 35602

Ion	Exp%	Act%
77.00	100.00	100.00
105.00	87.50	87.36
106.00	87.60	88.23
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072621\
 Data File : BG049523.D
 Acq On : 28 Jul 2021 2:14
 Operator : CG/JU
 Sample : SSTDCCC020EC
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020EC

Manual Integrations
 APPROVED

mohammad
 7/28/2021 11:30:20 AM

Quant Time: Jul 28 06:33:20 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 26 11:36:47 2021
 Response via : Initial Calibration

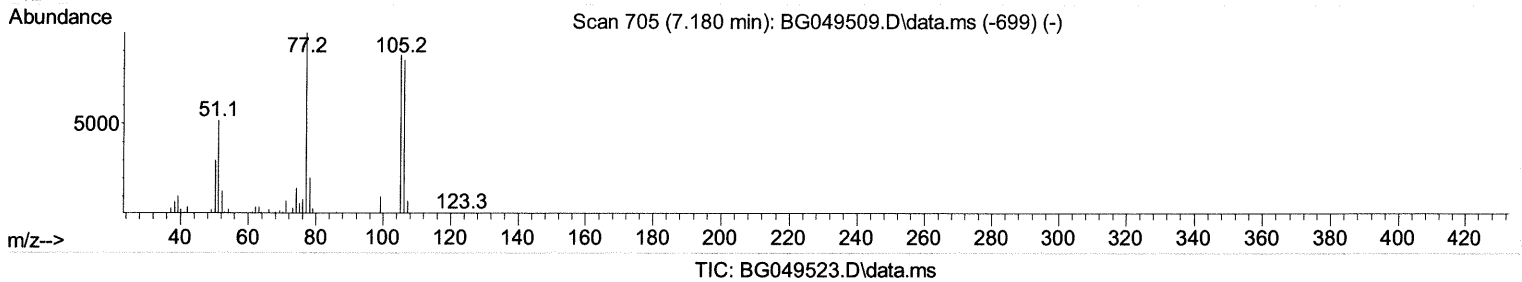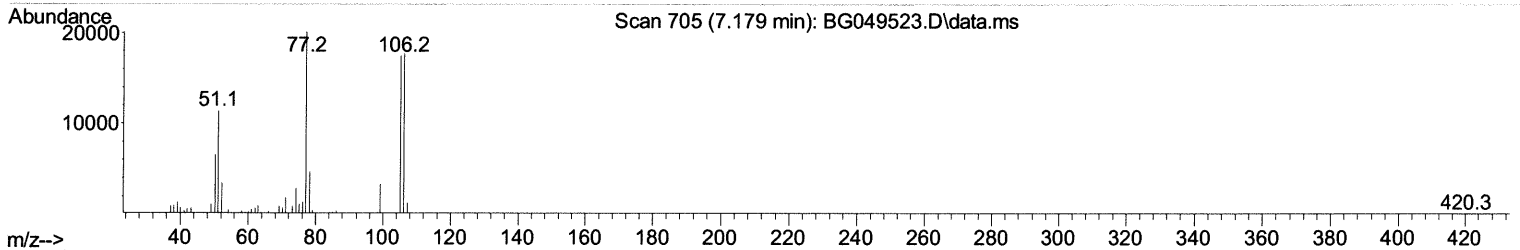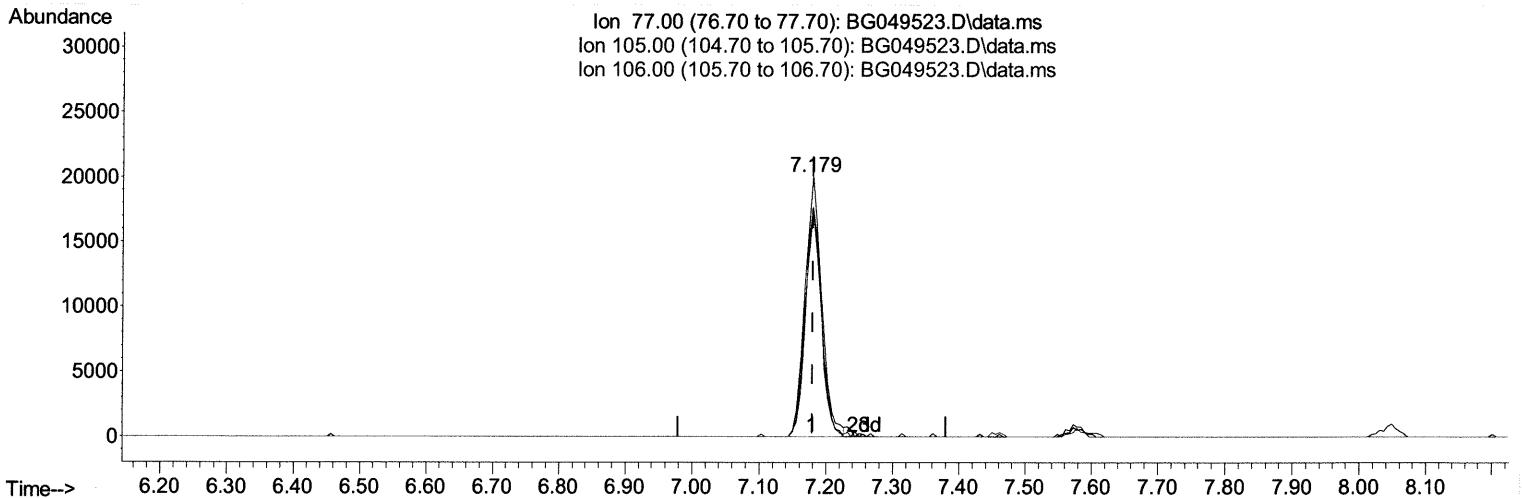

(6) Benzaldehyde

7.179min (-0.001) 24.37 ng/ul m 07/29/21JU

response 35176

Ion	Exp%	Act%
77.00	100.00	100.00
105.00	87.50	87.36
106.00	87.60	88.23
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072621\
 Data File : BG049523.D
 Acq On : 28 Jul 2021 2:14
 Operator : CG/JU
 Sample : SSTDCCC020EC
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020EC

Manual Integrations
 APPROVED

mohammad
 7/28/2021 11:30:20 AM

Quant Time: Jul 28 06:33:20 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 26 11:36:47 2021
 Response via : Initial Calibration

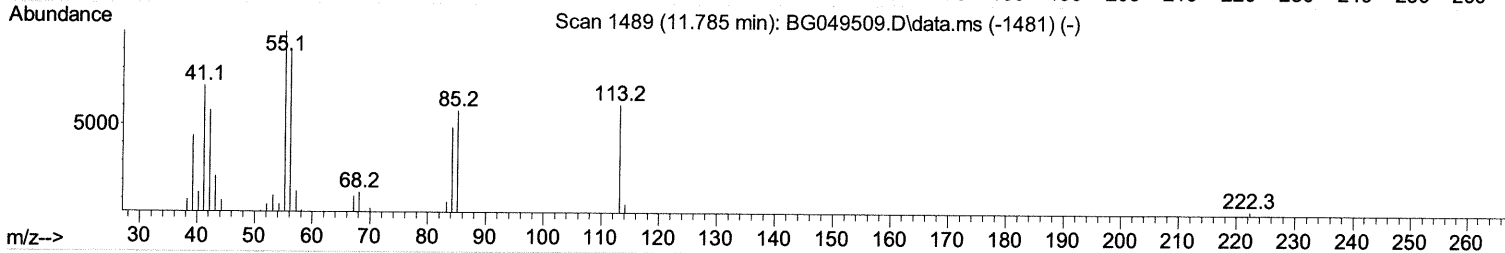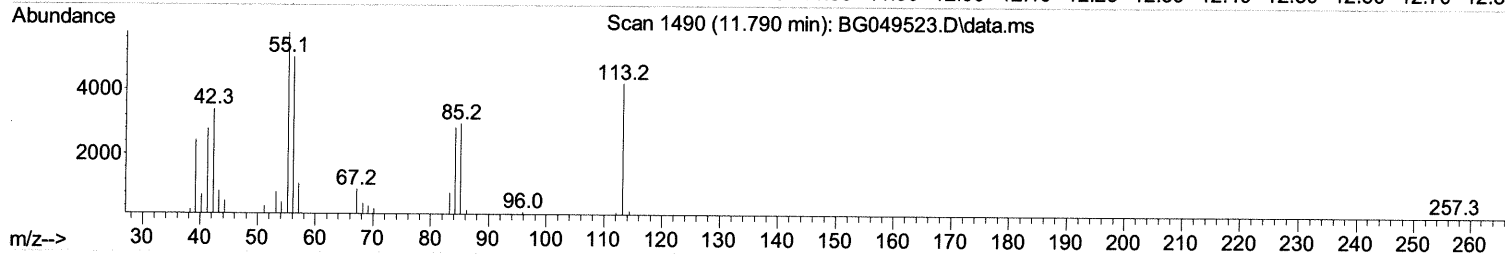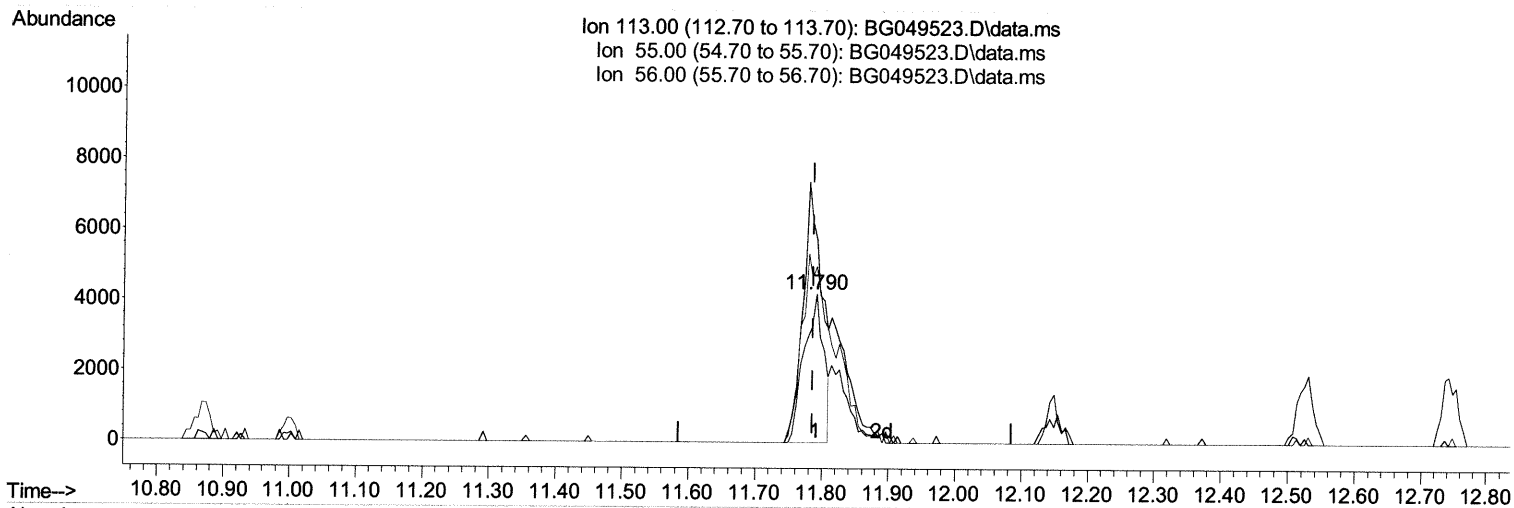

TIC: BG049523.D\data.ms

(34) Caprolactam

11.790min (+ 0.005) 13.30 ng/ul

response 8524

Ion	Exp%	Act%
113.00	100.00	100.00
55.00	145.70	136.54
56.00	118.80	118.41
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072621\
 Data File : BG049523.D
 Acq On : 28 Jul 2021 2:14
 Operator : CG/JU
 Sample : SSTDCCC020EC
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020EC

Manual Integrations
 APPROVED

mohammad
 7/28/2021 11:30:20 AM

Quant Time: Jul 28 06:33:20 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 26 11:36:47 2021
 Response via : Initial Calibration

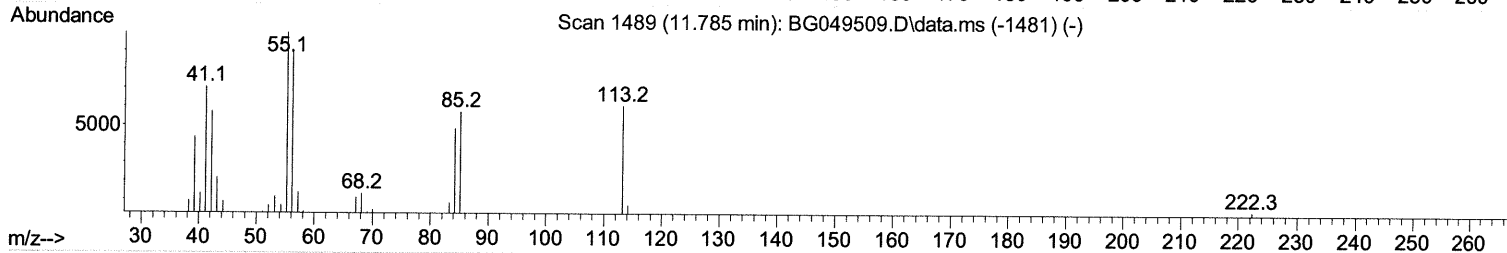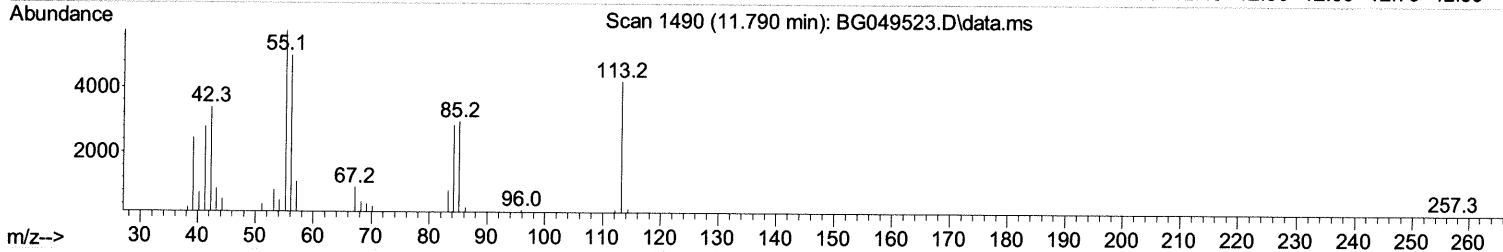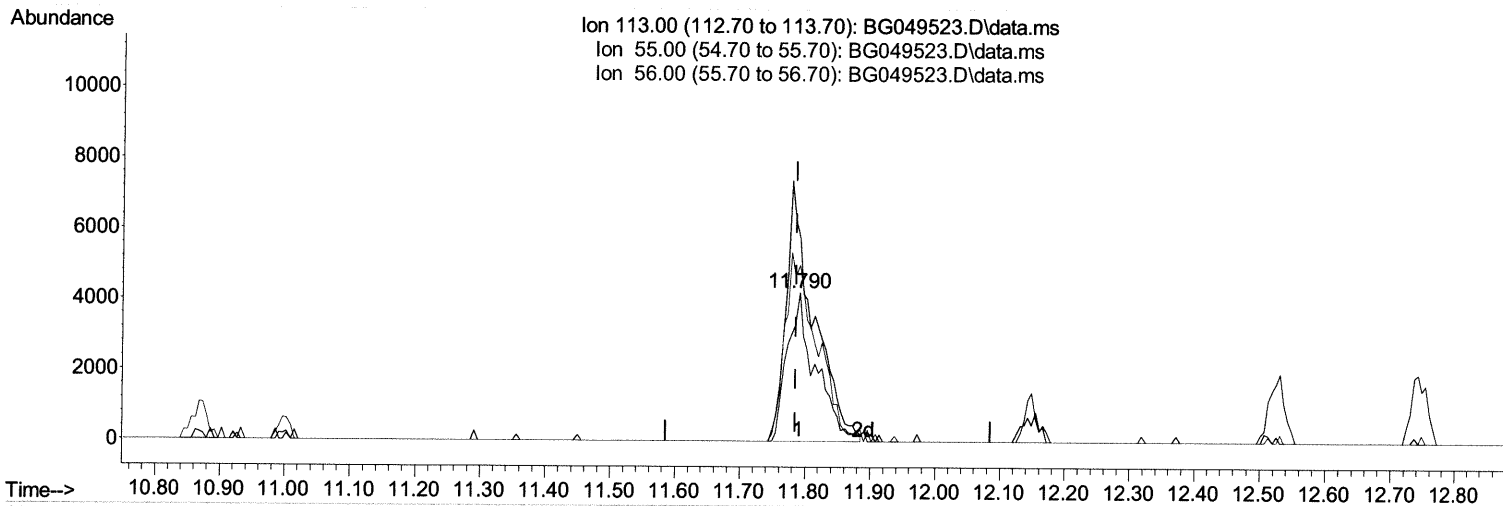

TIC: BG049523.D\data.ms

(34) Caprolactam

11.790min (+ 0.005) 19.90 ng/ul m 07/29/21JU

response 12749

Ion	Exp%	Act%
113.00	100.00	100.00
55.00	145.70	136.54
56.00	118.80	118.41
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072621\
 Data File : BG049523.D
 Acq On : 28 Jul 2021 2:14
 Operator : CG/JU
 Sample : SSTDCCC020EC
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020EC

Manual Integrations
 APPROVED

mohammad
 7/28/2021 11:30:20 AM

Quant Time: Jul 28 06:33:20 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 26 11:36:47 2021
 Response via : Initial Calibration

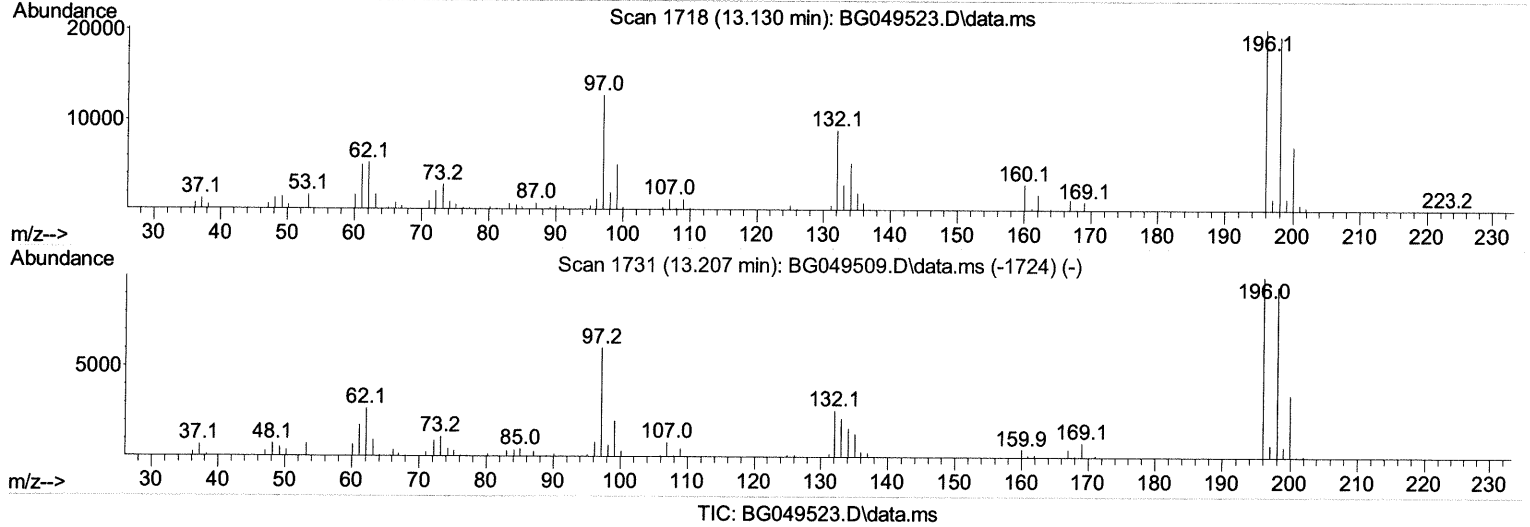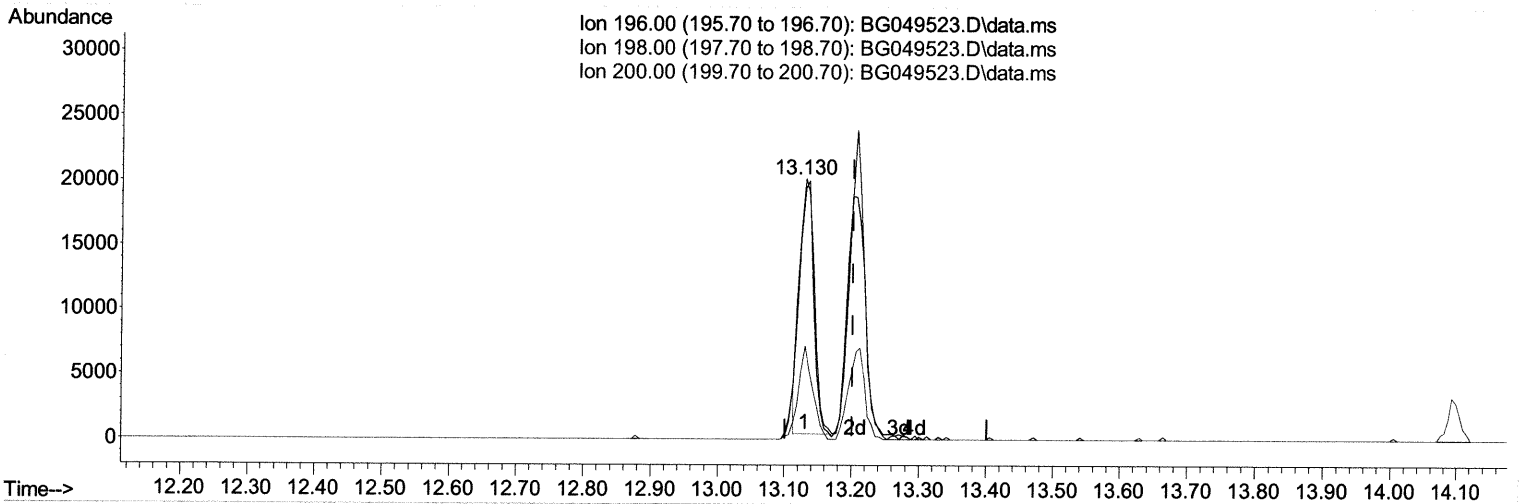

(42) 2,4,5-Trichlorophenol

13.130min (-0.072) 18.68 ng/ul

response 30741

Ion	Exp%	Act%
196.00	100.00	100.00
198.00	101.70	96.31
200.00	33.20	35.82
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072621\
 Data File : BG049523.D
 Acq On : 28 Jul 2021 2:14
 Operator : CG/JU
 Sample : SSTDCCC020EC
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020EC

Manual Integrations
 APPROVED

mohammad
 7/28/2021 11:30:20 AM

Quant Time: Jul 28 06:33:20 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 26 11:36:47 2021
 Response via : Initial Calibration

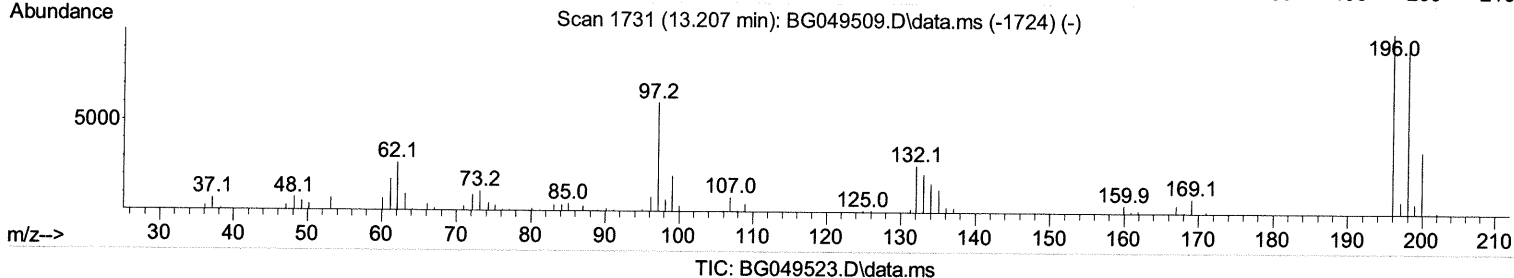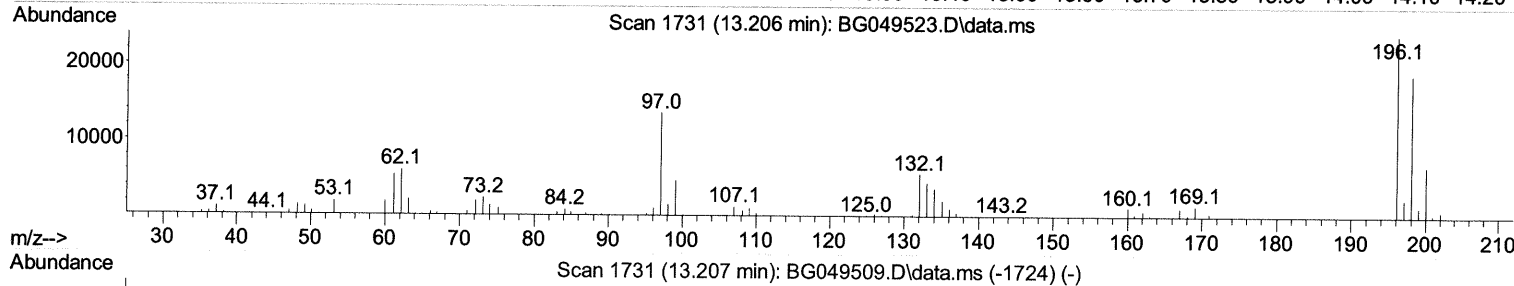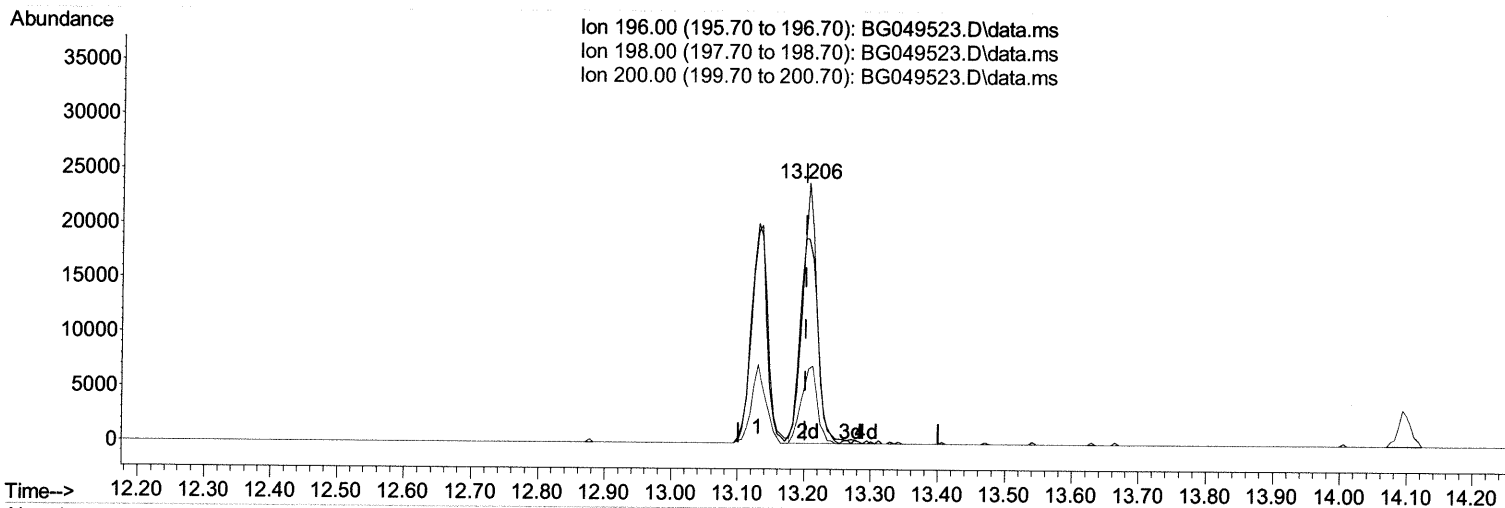

TIC: BG049523.D\data.ms

(42) 2,4,5-Trichlorophenol

13.206min (+ 0.005) 22.83 ng/ul m 07/29/21JU

response 37583

Ion	Exp%	Act%
196.00	100.00	100.00
198.00	101.70	78.49#
200.00	33.20	28.35
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072621\
 Data File : BG049523.D
 Acq On : 28 Jul 2021 2:14
 Operator : CG/JU
 Sample : SSTDCCC020EC
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020EC

Manual Integrations
 APPROVED

mohammad
 7/28/2021 11:30:20 AM

Quant Time: Jul 28 06:33:20 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 26 11:36:47 2021
 Response via : Initial Calibration

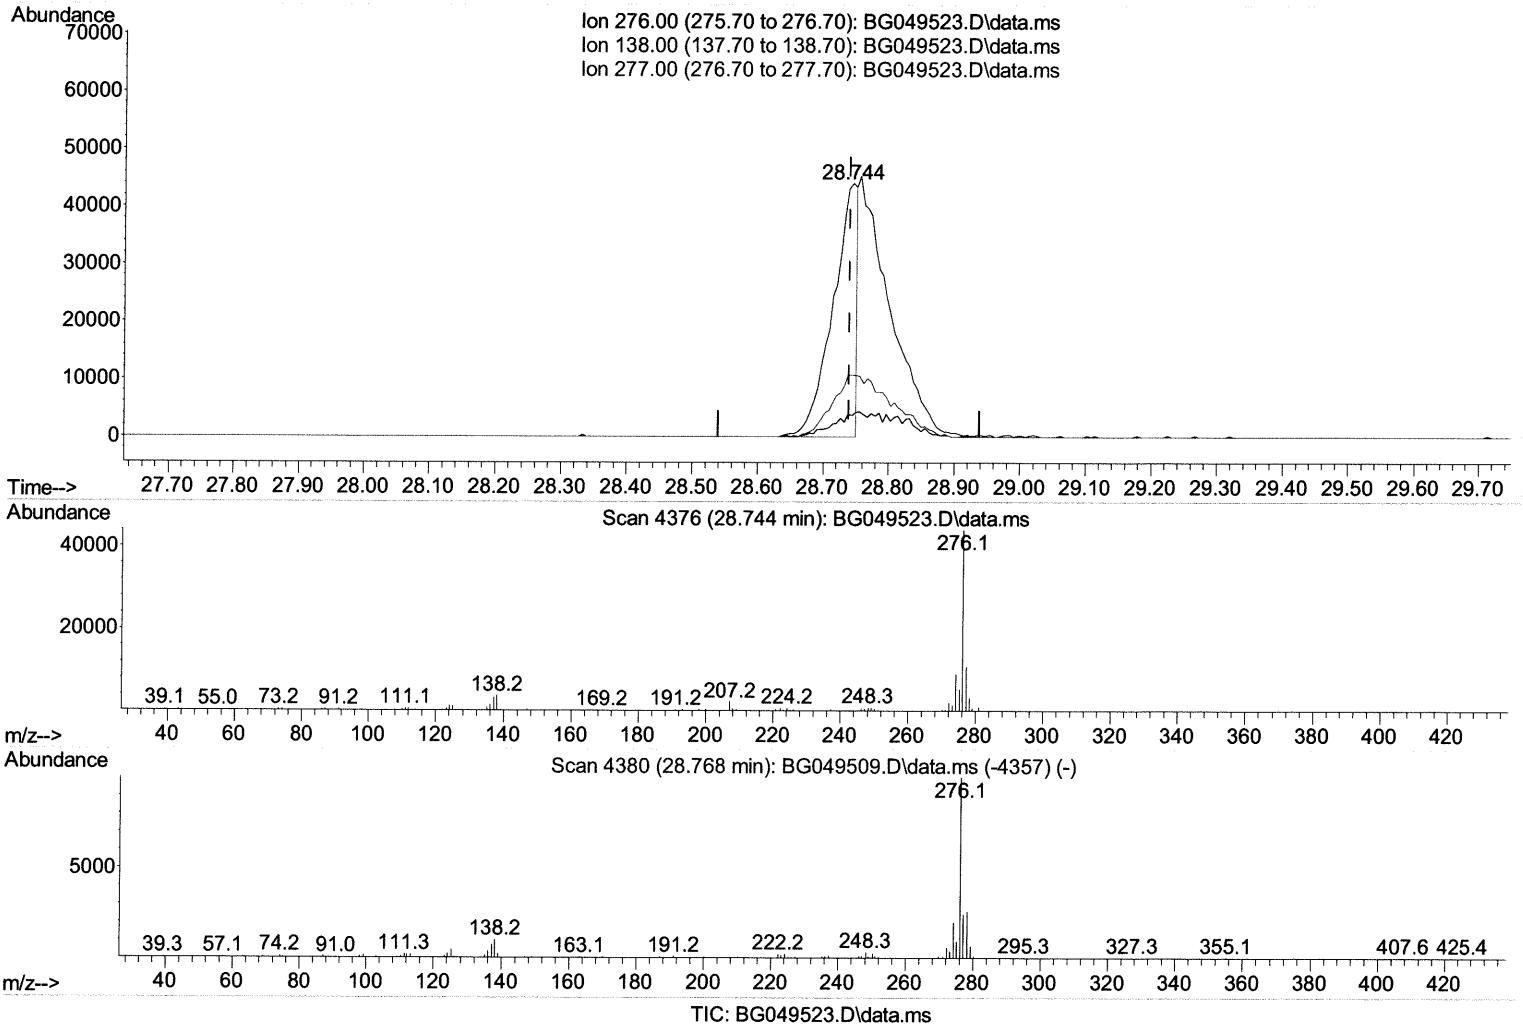

(94) Indeno(1,2,3-cd)pyrene

28.744min (+ 0.005) 9.23 ng/ul

response 114149

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	9.10	8.41
277.00	24.00	24.52
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072621\
 Data File : BG049523.D
 Acq On : 28 Jul 2021 2:14
 Operator : CG/JU
 Sample : SSTDCCC020EC
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020EC

Manual Integrations
 APPROVED

mohammad
 7/28/2021 11:30:20 AM

Quant Time: Jul 28 06:33:20 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 26 11:36:47 2021
 Response via : Initial Calibration

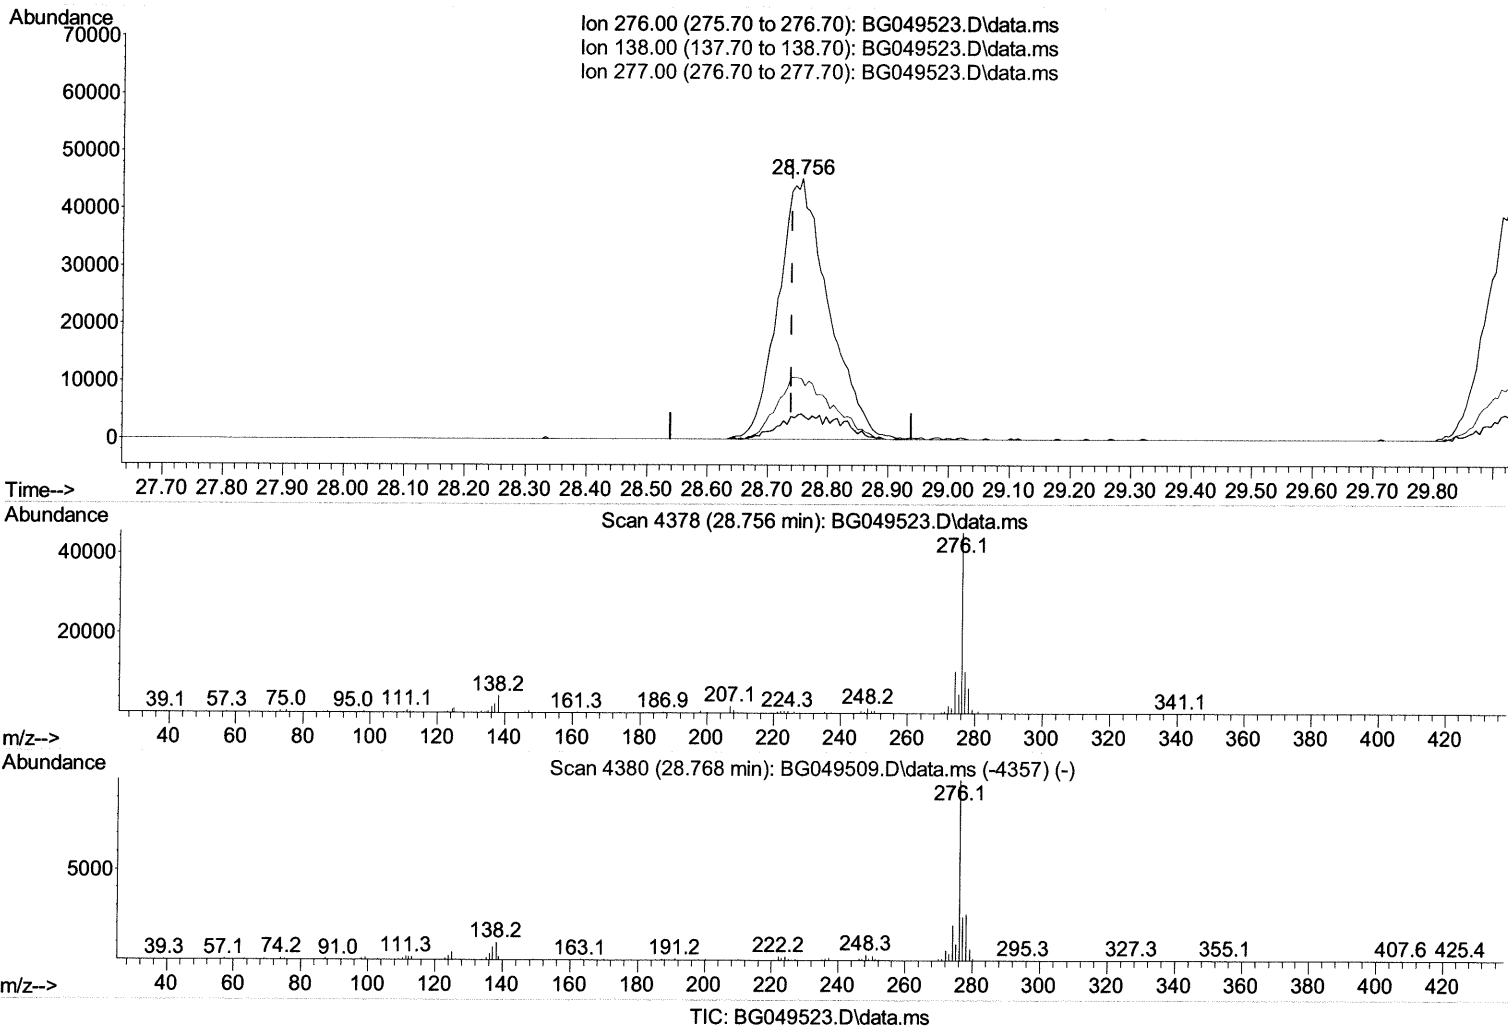

(94) Indeno(1,2,3-cd)pyrene

28.756min (+ 0.017) 21.08 ng/ul m 07/29/21 JU

response 260512

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	9.10	9.66
277.00	24.00	23.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072621\
 Data File : BG049523.D
 Acq On : 28 Jul 2021 2:14
 Operator : CG/JU
 Sample : SSTDCCC020EC
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020EC

Manual Integrations
 APPROVED

mohammad
 7/28/2021 11:30:20 AM

Quant Time: Jul 28 06:33:20 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 26 11:36:47 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.048	152	27343	20.000	ng/ul	0.00
20) Naphthalene-d8	10.868	136	117605	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.698	164	84384	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.447	188	186970	20.000	ng/ul	0.00
79) Chrysene-d12	21.730	240	175931	20.000	ng/ul	# 0.00
88) Perylene-d12	25.002	264	178158	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.431	96	3934m	6.582	ng/ul	0.00 07/24/21 JU
4) Pyridine-d5	3.854	84	32938	19.188	ng/ul	0.00
7) Phenol-d5	7.202	99	48919	20.221	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.367	67	26762	19.532	ng/ul	0.00
11) 2-Chlorophenol-d4	7.573	132	34763	20.047	ng/ul	0.00
15) 4-Methylphenol-d8	8.753	113	37594	20.617	ng/ul	0.00
21) Nitrobenzene-d5	9.211	128	18665	20.643	ng/ul	0.00
24) 2-Nitrophenol-d4	9.946	143	21294	20.097	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.486	165	39570	20.534	ng/ul	0.00
31) 4-Chloroaniline-d4	10.997	131	53238	19.823	ng/ul	0.00
46) Dimethylphthalate-d6	14.099	166	128417	19.867	ng/ul	0.00
49) Acenaphthylene-d8	14.393	160	154676	20.602	ng/ul	0.00
54) 4-Nitrophenol-d4	14.892	143	21396	20.100	ng/ul	0.00
60) Fluorene-d10	15.691	176	113340	20.353	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.808	200	21906	18.907	ng/ul	0.00
73) Anthracene-d10	17.547	188	173598	19.977	ng/ul	0.00
81) Pyrene-d10	19.832	212	194606	21.633	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.779	264	190801	20.376	ng/ul	0.01
Target Compounds						
2) 1,4-Dioxane	3.466	88	4984m	6.101	ng/ul	Qvalue 07/24/21 JU
5) Pyridine	3.872	79	33132	18.044	ng/ul	97
6) Benzaldehyde	7.179	77	35176m	24.368	ng/ul	Qvalue 07/24/21 JU
8) Phenol	7.226	94	47541	20.117	ng/ul	98
10) Bis(2-Chloroethyl)ether	7.461	93	31476	19.333	ng/ul	92
12) 2-Chlorophenol	7.608	128	34575	20.710	ng/ul	98
13) 2-Methylphenol	8.489	108	36197	20.097	ng/ul	87
14) 2,2'-oxybis(1-Chloropr...	8.571	45	36578	19.172	ng/ul#	93
16) Acetophenone	8.871	105	62365	21.250	ng/ul#	91
17) N-Nitroso-di-n-propyla...	8.853	70	31540	20.841	ng/ul#	90
18) 4-Methylphenol	8.818	108	40029	21.125	ng/ul	91
19) Hexachloroethane	9.135	117	16227	21.576	ng/ul#	81
22) Nitrobenzene	9.258	77	53595	19.852	ng/ul	93
23) Isophorone	9.781	82	92092	20.357	ng/ul	96
25) 2-Nitrophenol	9.969	139	21494	21.556	ng/ul#	81
26) 2,4-Dimethylphenol	10.028	107	49392	20.784	ng/ul	90
27) Bis(2-Chloroethoxy)met...	10.263	93	44739	19.829	ng/ul	98
29) 2,4-Dichlorophenol	10.510	162	40245	21.364	ng/ul	95
30) Naphthalene	10.921	128	123129	20.326	ng/ul	98
32) 4-Chloroaniline	11.021	127	50261	19.674	ng/ul#	85
33) Hexachlorobutadiene	11.197	225	29600	20.552	ng/ul	89
34) Caprolactam	11.790	113	12749m	19.899	ng/ul	Qvalue 07/24/21 JU
35) 4-Chloro-3-methylphenol	12.149	107	48854	23.049	ng/ul	99

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072621\
 Data File : BG049523.D
 Acq On : 28 Jul 2021 2:14
 Operator : CG/JU
 Sample : SSTDCCC020EC
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020EC

Manual Integrations
 APPROVED

mohammad
 7/28/2021 11:30:20 AM

Quant Time: Jul 28 06:33:20 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 26 11:36:47 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
36) 2-Methylnaphthalene	12.525	142	93086	20.995	ng/ul	92
37) 1-Methylnaphthalene	12.742	142	92814	20.716	ng/ul#	90
39) 1,2,4,5-Tetrachloroben...	12.895	216	50379	20.087	ng/ul	92
40) Hexachlorocyclopentadiene	12.865	237	24642	16.306	ng/ul#	88
41) 2,4,6-Trichlorophenol	13.130	196	34564	22.426	ng/ul#	79
42) 2,4,5-Trichlorophenol	13.206	196	37583m >	22.833	ng/ul >	07/24/21 JU
43) 1,1'-Biphenyl	13.529	154	119535	19.892	ng/ul	96
44) 2-Chloronaphthalene	13.576	162	96510	20.640	ng/ul	95
45) 2-Nitroaniline	13.776	65	35719	21.525	ng/ul	96
47) Dimethylphthalate	14.146	163	121636	19.350	ng/ul	97
48) 2,6-Dinitrotoluene	14.269	165	27186	21.671	ng/ul#	87
50) Acenaphthylene	14.422	152	145960	20.358	ng/ul	95
51) 3-Nitroaniline	14.598	138	26902	21.501	ng/ul	96
52) Acenaphthene	14.763	153	106301	20.672	ng/ul	96
53) 2,4-Dinitrophenol	14.810	184	11662	18.659	ng/ul	88
55) 4-Nitrophenol	14.910	109	27060	18.747	ng/ul	98
56) Dibenzofuran	15.098	168	145466	20.950	ng/ul	99
57) 2,4-Dinitrotoluene	15.057	165	38854	21.850	ng/ul	92
58) 2,3,4,6-Tetrachlorophenol	15.321	232	31987	21.415	ng/ul	96
59) Diethylphthalate	15.509	149	129263	19.869	ng/ul	98
61) Fluorene	15.744	166	121703	20.647	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.732	204	63004	20.533	ng/ul#	85
63) 4-Nitroaniline	15.761	138	26885	21.669	ng/ul	95
66) 4,6-Dinitro-2-methylph...	15.826	198	20555	19.273	ng/ul	92
67) N-Nitrosodiphenylamine	15.949	169	100980	20.608	ng/ul	95
68) 4-Bromophenyl-phenylether	16.631	248	43044	20.676	ng/ul	92
69) Hexachlorobenzene	16.754	284	47644	20.227	ng/ul	95
70) Atrazine	16.895	200	45146	20.173	ng/ul	97
71) Pentachlorophenol	17.101	266	22041	20.210	ng/ul	93
72) Phenanthrene	17.488	178	193857	19.916	ng/ul	97
74) Anthracene	17.582	178	194190	19.688	ng/ul	98
75) 1,2,3,4-Tetrachloroben...	13.500	216	52199	20.546	ng/ul	97
76) Pentachlorobenzene	15.015	250	56915	21.173	ng/ul	95
77) Carbazole	17.853	167	168066	19.059	ng/ul	99
78) Di-n-butylphthalate	18.399	149	210562	19.202	ng/ul	99
80) Fluoranthene	19.498	202	230664	21.117	ng/ul	98
82) Pyrene	19.862	202	234400	21.614	ng/ul	99
83) Butylbenzylphthalate	20.737	149	89982	21.311	ng/ul	98
84) 3,3'-Dichlorobenzidine	21.618	252	79609	19.693	ng/ul	96
85) Benzo(a)anthracene	21.706	228	218782	20.340	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.606	149	126554	20.197	ng/ul	99
87) Chrysene	21.777	228	205028	19.915	ng/ul	99
89) Di-n-octyl phthalate	22.834	149	212073	20.251	ng/ul	100
90) Benzo(b)fluoranthene	23.962	252	230582	20.649	ng/ul	98
91) Benzo(k)fluoranthene	24.033	252	215967	19.762	ng/ul	99
93) Benzo(a)pyrene	24.849	252	198485	20.489	ng/ul	98
94) Indeno(1,2,3-cd)pyrene	28.756	276	260512m >	21.076	ng/ul >	07/24/21 JU
95) Dibenzo(a,h)anthracene	28.814	278	212987	20.823	ng/ul	96
96) Benzo(g,h,i)perylene	29.930	276	211188	20.550	ng/ul#	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed