

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072621\
 Data File : BG049472.D
 Acq On : 26 Jul 2021 10:14
 Operator : CG/JU
 Sample : PB137826BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK826

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG049472.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.081	3	7	18	rVB5	20305	45085	6.29%	0.611%
2	3.439	64	68	69	rBV3	4796	6265	0.87%	0.085%
3	3.521	80	82	85	rBV3	2344	2120	0.30%	0.029%
4	3.697	109	112	116	rBV3	2595	4244	0.59%	0.057%
5	3.815	128	132	133	rBV3	1281	1160	0.16%	0.016%
6	3.856	136	139	150	rBV	69855	139300	19.43%	1.887%
7	4.115	181	183	187	rVB2	1417	1627	0.23%	0.022%
8	4.197	195	197	202	rVB3	1817	2217	0.31%	0.030%
9	4.490	245	247	252	rBV2	1215	2187	0.30%	0.030%
10	4.614	265	268	269	rBV2	969	1053	0.15%	0.014%
11	5.877	480	483	485	rBV2	1025	1253	0.17%	0.017%
12	6.147	526	529	532	rBV3	1736	2020	0.28%	0.027%
13	6.523	591	593	596	rBV	1144	1626	0.23%	0.022%
14	6.887	652	655	659	rVB	1015	1185	0.17%	0.016%
15	7.063	683	685	689	rBV2	853	1185	0.17%	0.016%
16	7.204	702	709	719	rVB	120053	201453	28.09%	2.729%
17	7.369	730	737	745	rBV2	73230	130258	18.17%	1.765%
18	7.580	766	773	780	rBV	108165	197223	27.50%	2.672%
19	7.633	780	782	785	rVB2	1327	1264	0.18%	0.017%
20	7.962	835	838	840	rBV2	943	1154	0.16%	0.016%
21	8.050	846	853	861	rBV2	81027	137613	19.19%	1.864%
22	8.755	966	973	984	rVB	139668	240702	33.57%	3.261%
23	9.219	1044	1052	1060	rBV2	115930	204400	28.51%	2.769%
24	9.942	1167	1175	1186	rBV	101742	186394	25.99%	2.525%
25	10.488	1261	1268	1282	rVB2	132179	243390	33.94%	3.297%
26	10.870	1324	1333	1340	rBV	100904	189428	26.42%	2.566%
27	11.005	1348	1356	1364	rBV	124151	237610	33.14%	3.219%
28	12.468	1599	1605	1609	rBV3	2146	4026	0.56%	0.055%
29	14.095	1876	1882	1892	rVB	266411	396278	55.26%	5.368%
30	14.395	1926	1933	1941	rBV	257500	415939	58.01%	5.635%
31	14.700	1978	1985	1992	rVB	171823	256479	35.77%	3.474%
32	14.888	2011	2017	2030	rBV	108733	193011	26.92%	2.615%
33	14.970	2030	2031	2034	rVB	2770	1829	0.26%	0.025%
34	15.047	2041	2044	2045	rVB2	1142	1100	0.15%	0.015%
35	15.693	2147	2154	2161	rBV	336682	521286	72.70%	7.062%
36	15.805	2168	2173	2180	rBV	110925	172014	23.99%	2.330%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072621\
 Data File : BG049472.D
 Acq On : 26 Jul 2021 10:14
 Operator : CG/JU
 Sample : PB137826BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK826

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
 Title : SVOA CALIBRATION

37	15.875	2184	2185	2190	rVB	1323	1537	0.21%	0.021%
38	15.928	2190	2194	2198	rBV3	3304	4762	0.66%	0.065%
39	17.238	2412	2417	2421	rVB	1430	1700	0.24%	0.023%
40	17.308	2427	2429	2434	rVB	784	1133	0.16%	0.015%
41	17.449	2445	2453	2460	rBV	209619	317612	44.29%	4.303%
42	17.549	2463	2470	2479	rVV	388493	599622	83.62%	8.123%
43	18.654	2654	2658	2660	rBV	1114	1374	0.19%	0.019%
44	18.783	2677	2680	2682	rVB2	1056	1090	0.15%	0.015%
45	19.247	2755	2759	2763	rBV2	1015	1588	0.22%	0.022%
46	19.406	2781	2786	2790	rVB3	4883	7547	1.05%	0.102%
47	19.464	2790	2796	2801	rBV2	4629	6995	0.98%	0.095%
48	19.834	2853	2859	2866	rVB	510915	717058	100.00%	9.714%
49	19.958	2877	2880	2881	rBV	1172	1234	0.17%	0.017%
50	20.022	2889	2891	2893	rVB2	1550	1149	0.16%	0.016%
51	20.052	2893	2896	2901	rBV3	813	1302	0.18%	0.018%
52	20.099	2901	2904	2907	rBV2	1653	2127	0.30%	0.029%
53	20.163	2914	2915	2918	rBV	1192	1451	0.20%	0.020%
54	20.240	2924	2928	2929	rBV2	1558	1548	0.22%	0.021%
55	20.287	2933	2936	2938	rBV3	1294	1447	0.20%	0.020%
56	20.422	2955	2959	2961	rBV2	2552	3475	0.48%	0.047%
57	20.539	2977	2979	2983	rBV4	1269	1363	0.19%	0.018%
58	20.680	3001	3003	3006	rBV3	1606	2031	0.28%	0.028%
59	20.757	3015	3016	3019	rBV3	2488	1652	0.23%	0.022%
60	20.945	3047	3048	3050	rBV2	1826	1655	0.23%	0.022%
61	21.027	3060	3062	3063	rBV2	1721	1454	0.20%	0.020%
62	21.221	3093	3095	3099	rBV3	1279	1965	0.27%	0.027%
63	21.326	3111	3113	3115	rVB3	1954	1601	0.22%	0.022%
64	21.514	3143	3145	3148	rVB4	1511	1328	0.19%	0.018%
65	21.726	3175	3181	3190	rVB	226517	370995	51.74%	5.026%
66	21.920	3212	3214	3217	rBV3	2014	1790	0.25%	0.024%
67	21.949	3217	3219	3221	rBV3	1646	1459	0.20%	0.020%
68	22.067	3237	3239	3241	rBV3	2237	1458	0.20%	0.020%
69	22.390	3292	3294	3295	rBV2	1902	1193	0.17%	0.016%
70	23.030	3401	3403	3405	rBV2	2236	2814	0.39%	0.038%
71	23.065	3407	3409	3410	rBV2	2498	2147	0.30%	0.029%
72	23.230	3435	3437	3444	rBV5	3378	7327	1.02%	0.099%
73	23.512	3483	3485	3486	rVB2	3120	1629	0.23%	0.022%
74	23.553	3486	3492	3494	rBV5	2881	4360	0.61%	0.059%
75	23.947	3557	3559	3560	rBV2	2502	1916	0.27%	0.026%
76	24.311	3619	3621	3622	rBV	2742	2023	0.28%	0.027%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072621\
 Data File : BG049472.D
 Acq On : 26 Jul 2021 10:14
 Operator : CG/JU
 Sample : PB137826BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK826

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
 Title : SVOA CALIBRATION

77	24.505	3652	3654	3656	rBV3	1609	1470	0.21%	0.020%
78	24.781	3690	3701	3712	rVB2	254180	703070	98.05%	9.524%
79	24.998	3729	3738	3752	rVB3	126852	379457	52.92%	5.140%
80	25.538	3828	3830	3833	rBV3	2004	1899	0.26%	0.026%
81	25.779	3869	3871	3874	rBV4	3053	3298	0.46%	0.045%
82	25.914	3891	3894	3898	rBV5	1942	3293	0.46%	0.045%
83	26.185	3932	3940	3949	rBV9	6876	21980	3.07%	0.298%
84	26.308	3959	3961	3964	rVB4	2284	1687	0.24%	0.023%
85	26.760	4036	4038	4039	rBV2	4101	1798	0.25%	0.024%
86	27.201	4111	4113	4114	rBV2	3429	1717	0.24%	0.023%
87	27.248	4119	4121	4122	rBV2	2133	1566	0.22%	0.021%
88	27.454	4154	4156	4159	rBV3	2563	2893	0.40%	0.039%
89	27.636	4185	4187	4188	rVB2	3438	1883	0.26%	0.026%
90	27.976	4243	4245	4248	rBV2	2042	2177	0.30%	0.029%
91	28.323	4302	4304	4306	rVB3	2604	1539	0.21%	0.021%
92	28.646	4357	4359	4360	rBV2	1875	1636	0.23%	0.022%
93	28.816	4386	4388	4392	rBV5	1951	2698	0.38%	0.037%
94	29.392	4484	4486	4487	rBV2	1890	1252	0.17%	0.017%
95	29.498	4502	4504	4508	rBV4	2126	2148	0.30%	0.029%
96	29.862	4563	4566	4567	rBV3	2044	2253	0.31%	0.031%
97	30.438	4663	4664	4665	rBV	2794	1442	0.20%	0.020%
98	30.561	4683	4685	4692	rBV6	2063	4232	0.59%	0.057%
99	30.667	4702	4703	4706	rBV3	2246	1164	0.16%	0.016%
100	32.382	4993	4995	4998	rBV3	2495	2133	0.30%	0.029%


Sum of corrected areas: 7381974

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072621\
Data File : BG049472.D
Acq On : 26 Jul 2021 10:14
Operator : CG/JU
Sample : PB137826BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK826

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

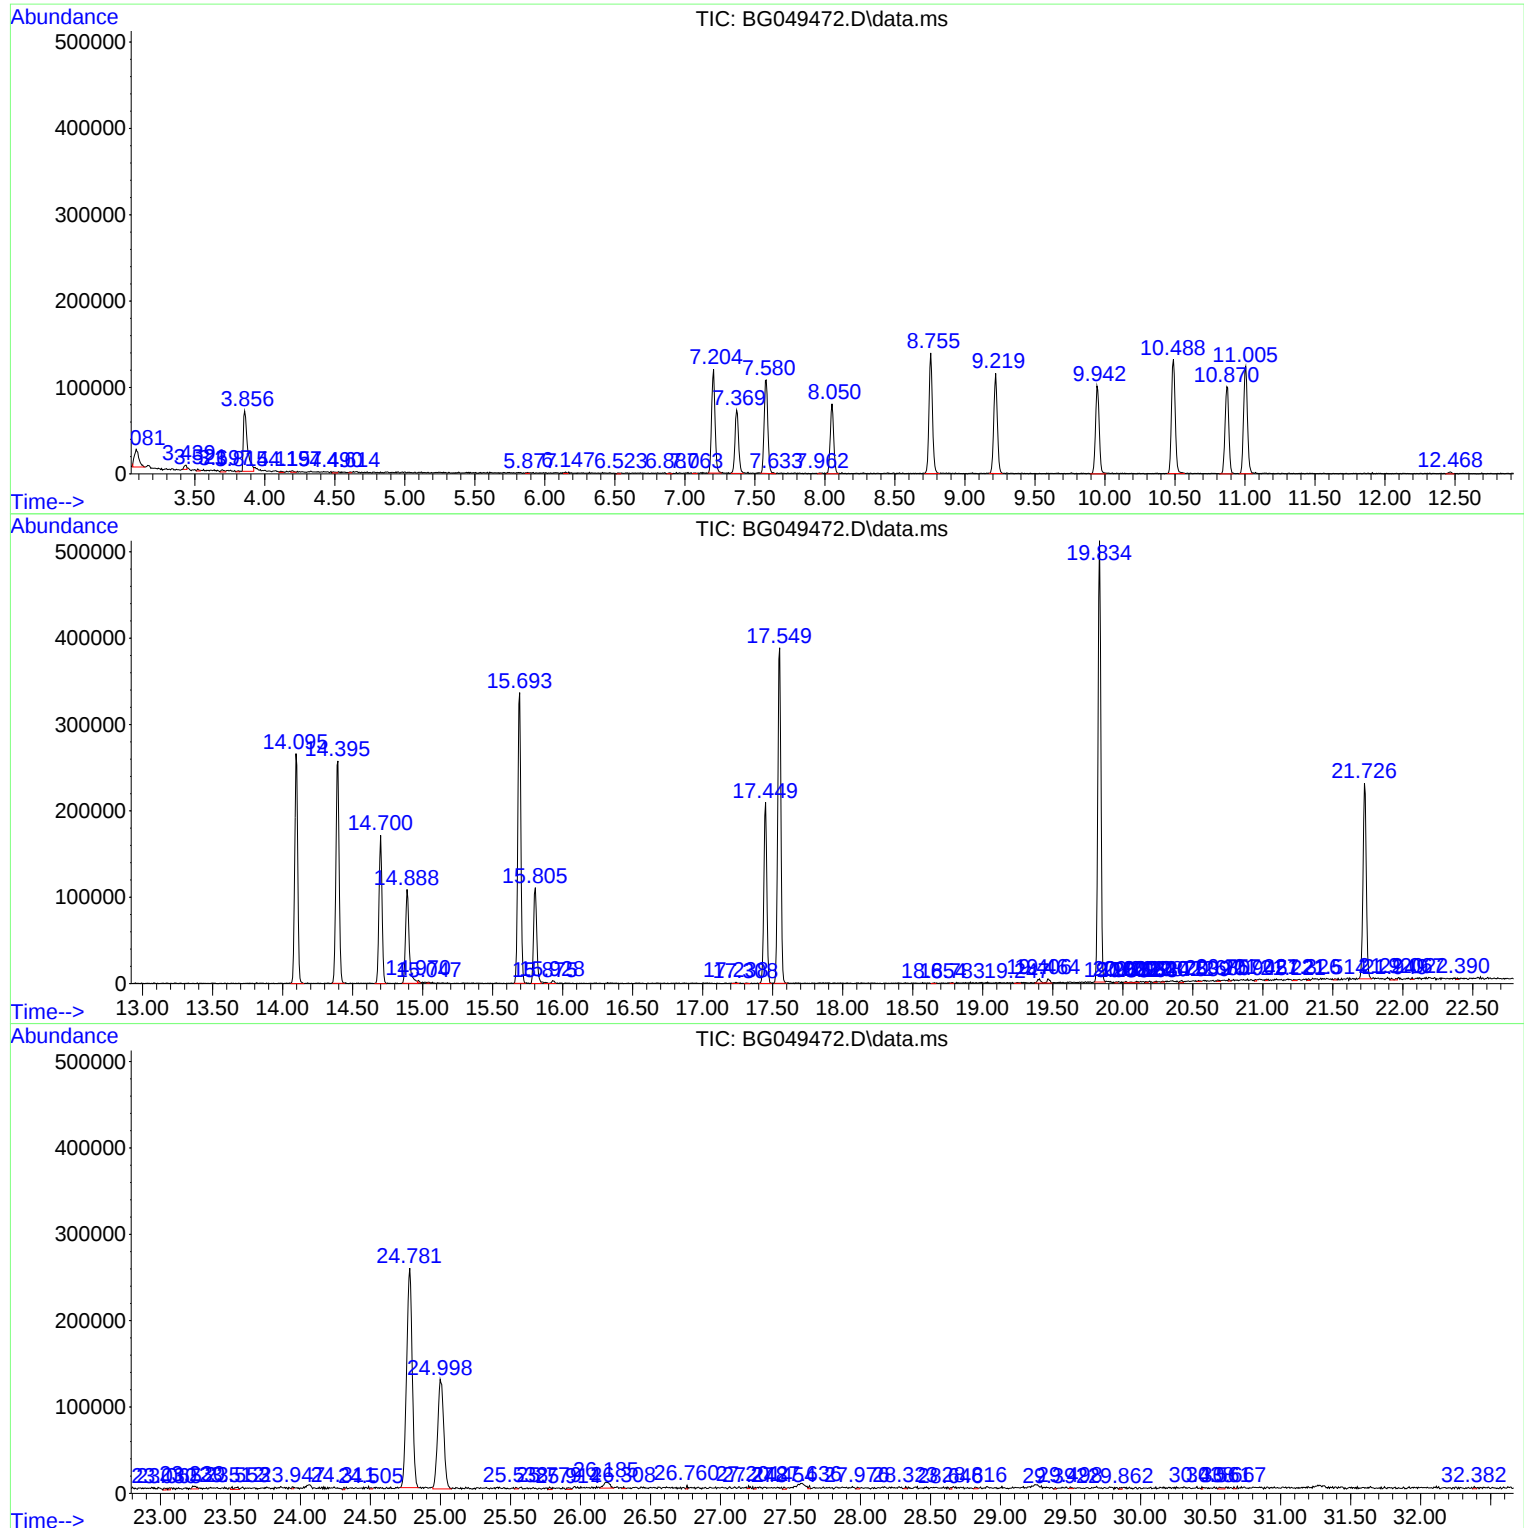

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072621\
Data File : BG049472.D
Acq On : 26 Jul 2021 10:14
Operator : CG/JU
Sample : PB137826BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK826










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Cyclic3.081 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.081	6.55 ng/ul	45085	1,4-Dichlorobenzene-d4	8.050

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclohexane	84	C6H12	000110-82-7	91
2			Cyclohexane	84	C6H12	000110-82-7	86
3			Cyclohexane	84	C6H12	000110-82-7	86
4			1-Pentene, 2-methyl-	84	C6H12	000763-29-1	56
5			2-Acetylpiperidine	127	C7H13NO	097073-22-8	53

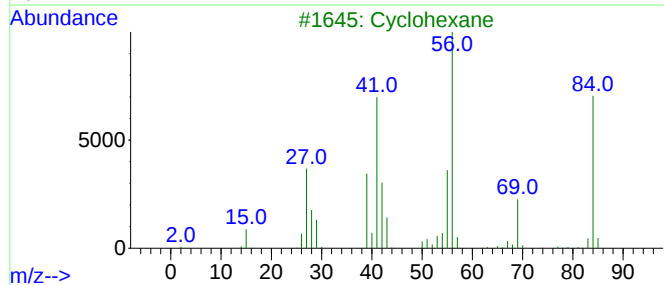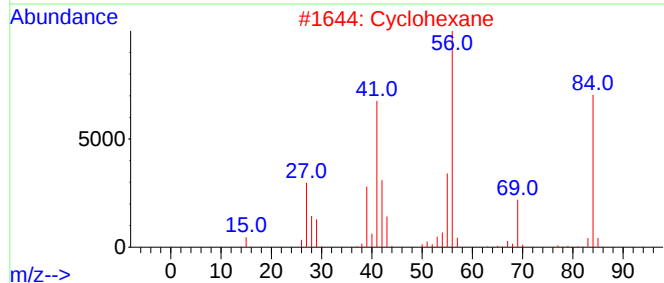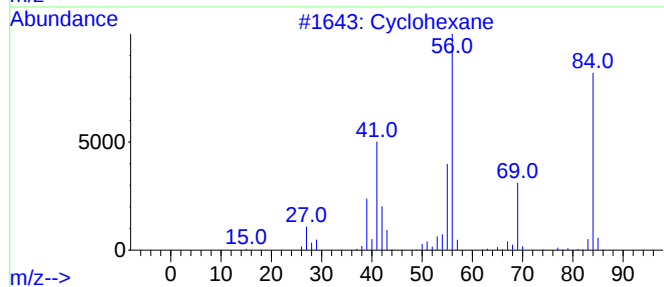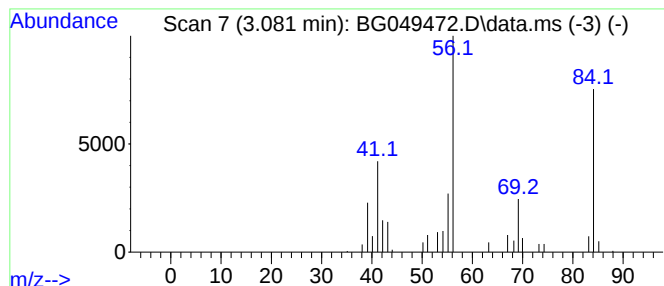

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072621\
Data File : BG049472.D
Acq On : 26 Jul 2021 10:14
Operator : CG/JU
Sample : PB137826BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK826

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: C...	3.081	6.5	ng/ul	45085	1	8.050	137613	20.0