

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072621\
 Data File : BG049484.D
 Acq On : 26 Jul 2021 18:42
 Operator : CG/JU
 Sample : PB137826BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK826

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG049484.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.086	3	8	18	rVB4	20859	54965	5.99%	0.555%
2	3.439	64	68	73	rBV3	8124	14191	1.55%	0.143%
3	3.715	113	115	117	rBV	1548	1611	0.18%	0.016%
4	3.862	137	140	153	rBV	96019	199450	21.73%	2.013%
5	4.061	171	174	175	rBV2	1656	1515	0.17%	0.015%
6	4.202	196	198	202	rVB4	2435	3201	0.35%	0.032%
7	4.290	209	213	214	rBV3	1503	1759	0.19%	0.018%
8	4.937	320	323	329	rVB5	1584	2699	0.29%	0.027%
9	5.113	351	353	356	rVB3	1080	1297	0.14%	0.013%
10	6.452	580	581	586	rBV	1108	1315	0.14%	0.013%
11	6.846	646	648	653	rVB2	1299	1745	0.19%	0.018%
12	7.204	702	709	719	rBV	172476	301649	32.86%	3.044%
13	7.369	731	737	746	rBV	111155	188171	20.50%	1.899%
14	7.580	766	773	781	rBV	162255	288540	31.43%	2.912%
15	8.050	846	853	861	rBV2	99472	168329	18.34%	1.699%
16	8.120	861	865	869	rVB	687	1247	0.14%	0.013%
17	8.150	869	870	875	rBV	1143	1318	0.14%	0.013%
18	8.755	967	973	987	rVB2	211253	364782	39.74%	3.682%
19	9.219	1045	1052	1063	rBV2	169669	300522	32.74%	3.033%
20	9.947	1168	1176	1184	rVB	149162	277007	30.17%	2.796%
21	10.218	1216	1222	1223	rBV2	781	1282	0.14%	0.013%
22	10.488	1261	1268	1281	rBV	201755	371038	40.42%	3.745%
23	10.870	1327	1333	1342	rVB	140332	238357	25.96%	2.406%
24	10.999	1346	1355	1368	rBV	189532	360849	39.31%	3.642%
25	11.299	1401	1406	1411	rBB	1098	1706	0.19%	0.017%
26	12.456	1597	1603	1608	rVB3	2863	5275	0.57%	0.053%
27	14.095	1876	1882	1889	rVB	382704	565419	61.59%	5.707%
28	14.388	1923	1932	1942	rVB	377446	611388	66.60%	6.170%
29	14.700	1976	1985	1993	rVB	207230	325555	35.46%	3.286%
30	14.888	2010	2017	2030	rBV	179835	300266	32.71%	3.030%
31	15.070	2045	2048	2050	rBV	1157	1305	0.14%	0.013%
32	15.693	2145	2154	2162	rVB	479270	758197	82.59%	7.652%
33	15.804	2167	2173	2181	rBV2	165601	251158	27.36%	2.535%
34	15.881	2184	2186	2190	rVB2	1014	1304	0.14%	0.013%
35	15.933	2190	2195	2199	rBV3	4867	6905	0.75%	0.070%
36	17.191	2407	2409	2411	rBV3	1745	1275	0.14%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072621\
 Data File : BG049484.D
 Acq On : 26 Jul 2021 18:42
 Operator : CG/JU
 Sample : PB137826BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK826

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
 Title : SVOA CALIBRATION

37	17.449	2444	2453	2459	rBV	254933	385981	42.05%	3.896%
38	17.549	2463	2470	2477	rVB	542523	829726	90.38%	8.374%
39	17.743	2500	2503	2507	rVB	1183	1672	0.18%	0.017%
40	18.036	2552	2553	2560	rBV	709	1271	0.14%	0.013%

41	18.900	2699	2700	2703	rBV	2001	1669	0.18%	0.017%
42	19.170	2744	2746	2749	rBV	1475	1457	0.16%	0.015%
43	19.235	2752	2757	2760	rVB3	1603	2133	0.23%	0.022%
44	19.399	2780	2785	2792	rBV5	7070	11256	1.23%	0.114%
45	19.464	2792	2796	2802	rVB3	6668	10779	1.17%	0.109%

46	19.570	2811	2814	2815	rBV2	1701	1396	0.15%	0.014%
47	19.646	2823	2827	2829	rVB3	1418	1699	0.19%	0.017%
48	19.705	2834	2837	2839	rBV	2064	1980	0.22%	0.020%
49	19.793	2847	2852	2853	rBV3	2454	3248	0.35%	0.033%
50	19.834	2853	2859	2866	rVV	644363	918007	100.00%	9.265%

51	19.951	2878	2879	2882	rBV	1796	1822	0.20%	0.018%
52	19.975	2882	2883	2886	rVB3	3264	1957	0.21%	0.020%
53	20.004	2886	2888	2889	rBV	1760	1260	0.14%	0.013%
54	20.116	2902	2907	2911	rBV3	3063	5820	0.63%	0.059%
55	20.245	2927	2929	2931	rBV2	2757	2368	0.26%	0.024%

56	20.416	2955	2958	2960	rBV4	1785	2509	0.27%	0.025%
57	20.586	2985	2987	2988	rBV2	3259	2169	0.24%	0.022%
58	20.915	3041	3043	3044	rBV2	3654	2078	0.23%	0.021%
59	21.021	3059	3061	3062	rBV2	4387	1731	0.19%	0.017%
60	21.185	3087	3089	3090	rBV2	3518	2458	0.27%	0.025%

61	21.496	3140	3142	3143	rBV2	3887	1822	0.20%	0.018%
62	21.726	3174	3181	3189	rBV2	240634	402027	43.79%	4.057%
63	22.178	3255	3258	3259	rBV3	3301	3751	0.41%	0.038%
64	24.028	3571	3573	3574	rBV2	4963	4796	0.52%	0.048%
65	24.052	3574	3577	3582	rVB6	7459	11886	1.29%	0.120%

66	24.310	3619	3621	3623	rBV3	3057	2232	0.24%	0.023%
67	24.780	3689	3701	3712	rBV3	303659	865241	94.25%	8.732%
68	25.003	3730	3739	3751	rVB3	133877	401841	43.77%	4.056%
69	27.083	4091	4093	4095	rBV2	3827	3228	0.35%	0.033%
70	28.117	4268	4269	4270	rBV	4469	1718	0.19%	0.017%

71	28.528	4338	4339	4340	rBV	3485	1357	0.15%	0.014%
72	28.728	4371	4373	4375	rBV3	3419	3523	0.38%	0.036%
73	28.781	4380	4382	4383	rBV2	3713	2991	0.33%	0.030%
74	29.756	4547	4548	4550	rBV2	3644	1656	0.18%	0.017%
75	30.490	4671	4673	4676	rBV4	3399	3885	0.42%	0.039%

76	30.537	4679	4681	4685	rBV5	3859	4435	0.48%	0.045%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072621\
Data File : BG049484.D
Acq On : 26 Jul 2021 18:42
Operator : CG/JU
Sample : PB137826BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK826

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
Title : SVOA CALIBRATION

77	30.907	4742	4744	4746	rBV3	4037	2753	0.30%	0.028%
78	31.148	4783	4785	4788	rBV3	3123	2903	0.32%	0.029%
79	31.647	4868	4870	4873	rBV4	2847	3107	0.34%	0.031%
80	31.912	4913	4915	4918	rBV3	4109	3967	0.43%	0.040%
81	31.971	4921	4925	4928	rBV6	4083	6170	0.67%	0.062%




Sum of corrected areas: 9908327

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072621\
Data File : BG049484.D
Acq On : 26 Jul 2021 18:42
Operator : CG/JU
Sample : PB137826BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK826

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

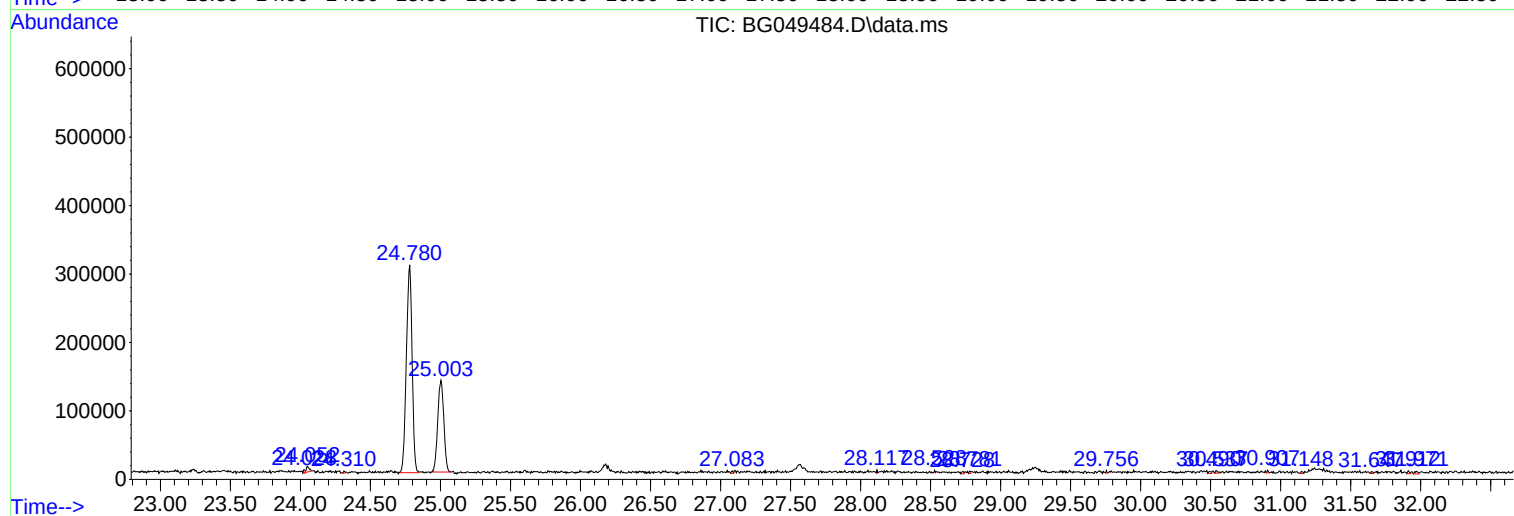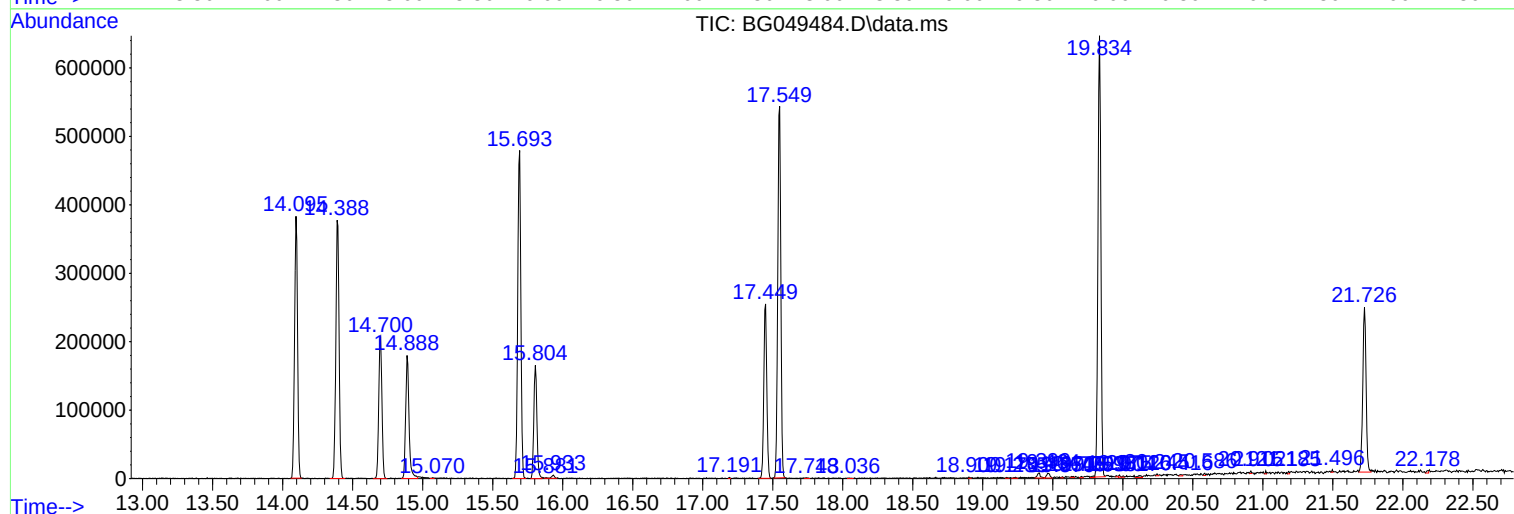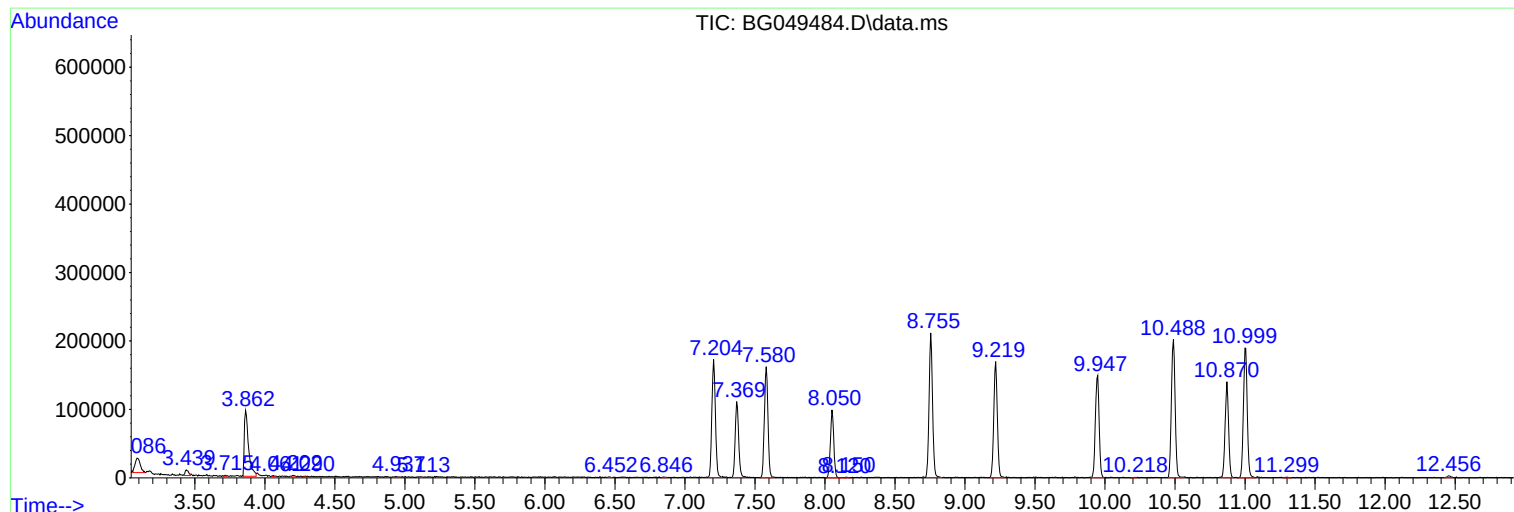

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072621\
Data File : BG049484.D
Acq On : 26 Jul 2021 18:42
Operator : CG/JU
Sample : PB137826BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK826










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Cyclic3.086 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.086	6.53 ng/ul	54965	1,4-Dichlorobenzene-d4	8.050

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclohexane	84	C6H12	000110-82-7	62
2			Cyclohexane	84	C6H12	000110-82-7	62
3			Cyclohexane	84	C6H12	000110-82-7	53
4			1-Hexene	84	C6H12	000592-41-6	53
5			1-Pentene, 2-methyl-	84	C6H12	000763-29-1	53

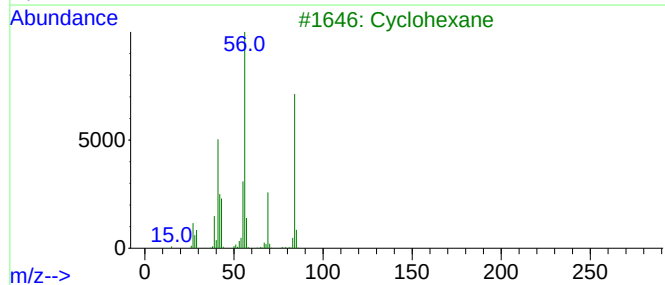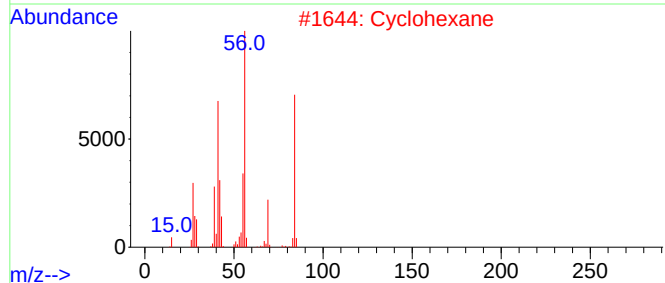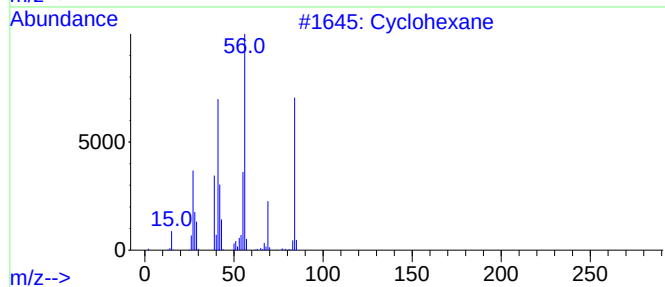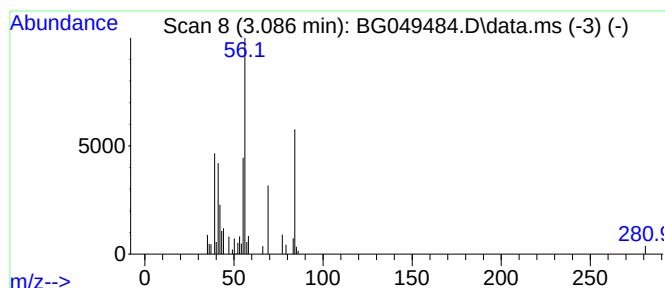

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072621\
Data File : BG049484.D
Acq On : 26 Jul 2021 18:42
Operator : CG/JU
Sample : PB137826BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK826

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: C...	3.086	6.5	ng/ul	54965	1	8.050	168329	20.0