

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072621\
 Data File : BG049510.D
 Acq On : 27 Jul 2021 16:35
 Operator : CG/JU
 Sample : PB137903BL
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK903

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG049510.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.081	3	7	13	rBV3	16719	27005	3.53%	0.326%
2	3.434	63	67	73	rVV4	4346	7734	1.01%	0.093%
3	3.516	77	81	82	rBV2	1246	1621	0.21%	0.020%
4	3.857	135	139	153	rBV	64820	131932	17.26%	1.592%
5	4.103	180	181	186	rVB2	1979	1794	0.23%	0.022%
6	4.144	186	188	189	rBV	1487	1293	0.17%	0.016%
7	4.186	193	195	196	rBV2	2149	2060	0.27%	0.025%
8	4.238	203	204	208	rVB3	1548	1586	0.21%	0.019%
9	4.321	215	218	221	rBV2	1310	1718	0.22%	0.021%
10	4.679	276	279	282	rBV3	1265	1398	0.18%	0.017%
11	4.832	302	305	309	rBV2	1445	2266	0.30%	0.027%
12	4.979	328	330	333	rVB2	1542	1452	0.19%	0.018%
13	5.102	347	351	353	rBV3	1217	1650	0.22%	0.020%
14	5.237	371	374	379	rVB2	1018	1592	0.21%	0.019%
15	5.478	411	415	417	rBV3	1170	1665	0.22%	0.020%
16	6.189	528	536	538	rBV2	1068	1595	0.21%	0.019%
17	6.712	623	625	628	rBV3	1284	1436	0.19%	0.017%
18	7.205	702	709	718	rBV2	117554	219374	28.69%	2.648%
19	7.369	730	737	745	rBV	74977	132511	17.33%	1.599%
20	7.581	765	773	779	rBV	113059	207901	27.19%	2.509%
21	7.792	807	809	812	rBV	911	1163	0.15%	0.014%
22	7.822	812	814	820	rVB	948	1186	0.16%	0.014%
23	8.051	845	853	863	rVB2	83927	154844	20.25%	1.869%
24	8.409	910	914	917	rBV2	1057	1600	0.21%	0.019%
25	8.756	966	973	981	rBV2	146351	269888	35.30%	3.258%
26	9.220	1044	1052	1061	rBV	120899	222445	29.09%	2.685%
27	9.737	1136	1140	1143	rBV	721	1204	0.16%	0.015%
28	9.843	1154	1158	1162	rBV	1172	1612	0.21%	0.019%
29	9.942	1168	1175	1188	rBV	112863	205603	26.89%	2.482%
30	10.489	1262	1268	1278	rBV	148901	273550	35.78%	3.302%
31	10.871	1324	1333	1343	rBV	127249	228230	29.85%	2.755%
32	11.000	1348	1355	1365	rBV	138713	269276	35.22%	3.250%
33	12.104	1539	1543	1546	rBV2	1007	1522	0.20%	0.018%
34	12.457	1598	1603	1609	rVB2	2467	4388	0.57%	0.053%
35	13.197	1726	1729	1732	rBV2	1427	1347	0.18%	0.016%
36	14.096	1875	1882	1891	rBV	292158	435140	56.91%	5.252%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072621\
 Data File : BG049510.D
 Acq On : 27 Jul 2021 16:35
 Operator : CG/JU
 Sample : PB137903BL
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK903

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
 Title : SVOA CALIBRATION

37	14.395	1925	1933	1948	rBV	307247	492427	64.41%	5.944%
38	14.572	1957	1963	1965	rBV	1055	1404	0.18%	0.017%
39	14.701	1978	1985	1994	rVB	206038	334363	43.73%	4.036%
40	14.895	2011	2018	2028	rBV	134765	238442	31.19%	2.878%
41	15.318	2088	2090	2093	rVB	1200	1299	0.17%	0.016%
42	15.688	2147	2153	2161	rBV	392070	615528	80.51%	7.430%
43	15.805	2168	2173	2184	rBV3	129383	200894	26.28%	2.425%
44	15.934	2190	2195	2198	rVB2	4543	5577	0.73%	0.067%
45	17.150	2400	2402	2407	rVB	1056	1316	0.17%	0.016%
46	17.450	2446	2453	2462	rVB	285734	424122	55.47%	5.119%
47	17.550	2462	2470	2477	rBV2	459593	710534	92.93%	8.577%
48	18.008	2546	2548	2551	rBV2	1101	1347	0.18%	0.016%
49	18.090	2560	2562	2565	rBV	1268	1155	0.15%	0.014%
50	18.190	2577	2579	2582	rBV	1461	1636	0.21%	0.020%
51	18.672	2658	2661	2663	rBV	1339	1304	0.17%	0.016%
52	18.742	2669	2673	2674	rVB	877	1164	0.15%	0.014%
53	18.801	2678	2683	2684	rVB	1043	1227	0.16%	0.015%
54	18.966	2708	2711	2712	rBV	1867	1715	0.22%	0.021%
55	19.083	2730	2731	2733	rBV2	1646	1151	0.15%	0.014%
56	19.400	2782	2785	2789	rBV2	5774	6855	0.90%	0.083%
57	19.471	2791	2797	2801	rBV3	5154	9417	1.23%	0.114%
58	19.547	2807	2810	2812	rBV	1443	1480	0.19%	0.018%
59	19.665	2826	2830	2831	rVB2	1554	1313	0.17%	0.016%
60	19.688	2831	2834	2835	rBV	1125	1280	0.17%	0.015%
61	19.747	2841	2844	2845	rBV2	1933	1271	0.17%	0.015%
62	19.835	2852	2859	2868	rBV	539664	764555	100.00%	9.229%
63	20.046	2892	2895	2898	rVB3	3381	3853	0.50%	0.047%
64	20.093	2901	2903	2905	rVV3	2483	2719	0.36%	0.033%
65	20.135	2907	2910	2912	rVB3	2026	2262	0.30%	0.027%
66	20.187	2917	2919	2920	rBV2	2605	1303	0.17%	0.016%
67	20.311	2939	2940	2943	rBV3	2461	1520	0.20%	0.018%
68	20.340	2943	2945	2950	rVB4	2224	1600	0.21%	0.019%
69	20.587	2986	2987	2990	rBV3	2097	1269	0.17%	0.015%
70	20.610	2990	2991	2994	rBV2	2196	1932	0.25%	0.023%
71	20.734	3010	3012	3017	rVB4	5826	5220	0.68%	0.063%
72	20.851	3031	3032	3035	rBV3	2272	2454	0.32%	0.030%
73	21.010	3057	3059	3060	rBV2	2817	2238	0.29%	0.027%
74	21.215	3092	3094	3095	rBV2	2539	1341	0.18%	0.016%
75	21.727	3175	3181	3188	rVB	248642	416032	54.41%	5.022%
76	22.020	3229	3231	3232	rBV2	3435	2056	0.27%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072621\
 Data File : BG049510.D
 Acq On : 27 Jul 2021 16:35
 Operator : CG/JU
 Sample : PB137903BL
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK903

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
 Title : SVOA CALIBRATION

77	23.019	3399	3401	3405	rBV5	3434	4142	0.54%	0.050%
78	23.442	3471	3473	3474	rVB2	3638	2013	0.26%	0.024%
79	23.459	3474	3476	3477	rBV2	3880	2855	0.37%	0.034%
80	23.530	3486	3488	3489	rBV2	3846	2438	0.32%	0.029%
81	24.376	3630	3632	3633	rBV2	4410	3128	0.41%	0.038%
82	24.552	3661	3662	3665	rBV2	2882	2477	0.32%	0.030%
83	24.781	3690	3701	3711	rVB2	259016	710042	92.87%	8.571%
84	25.010	3729	3740	3750	rBV2	144507	415792	54.38%	5.019%
85	25.375	3800	3802	3805	rBV3	3299	5385	0.70%	0.065%
86	25.463	3815	3817	3818	rBV2	3770	2529	0.33%	0.031%
87	25.498	3821	3823	3825	rBV2	3461	2999	0.39%	0.036%
88	25.686	3852	3855	3856	rBV3	4211	4452	0.58%	0.054%
89	26.056	3916	3918	3920	rBV3	3092	2994	0.39%	0.036%
90	27.049	4085	4087	4088	rBV	4069	2494	0.33%	0.030%
91	27.160	4104	4106	4107	rBV2	3154	2348	0.31%	0.028%
92	27.342	4134	4137	4138	rBV2	3965	4346	0.57%	0.052%
93	28.335	4303	4306	4310	rBV5	3752	5568	0.73%	0.067%
94	29.416	4488	4490	4492	rBV3	2928	1923	0.25%	0.023%
95	30.186	4619	4621	4623	rBV4	3128	2634	0.34%	0.032%
96	30.562	4684	4685	4686	rBV	3342	1477	0.19%	0.018%
97	31.143	4782	4784	4786	rBV2	3242	2273	0.30%	0.027%
98	31.648	4868	4870	4873	rBV4	3606	4491	0.59%	0.054%
99	31.690	4875	4877	4878	rBV2	3444	2623	0.34%	0.032%
100	32.130	4951	4952	4953	rBV	4354	2040	0.27%	0.025%




Sum of corrected areas: 8284619

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072621\
Data File : BG049510.D
Acq On : 27 Jul 2021 16:35
Operator : CG/JU
Sample : PB137903BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK903

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

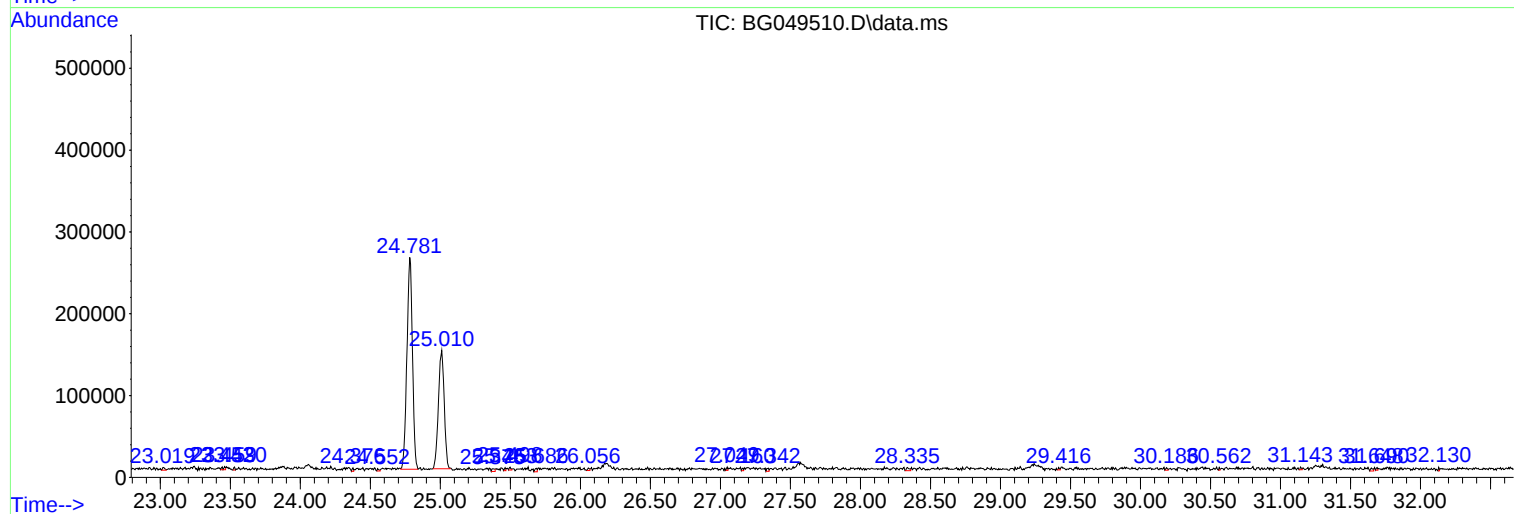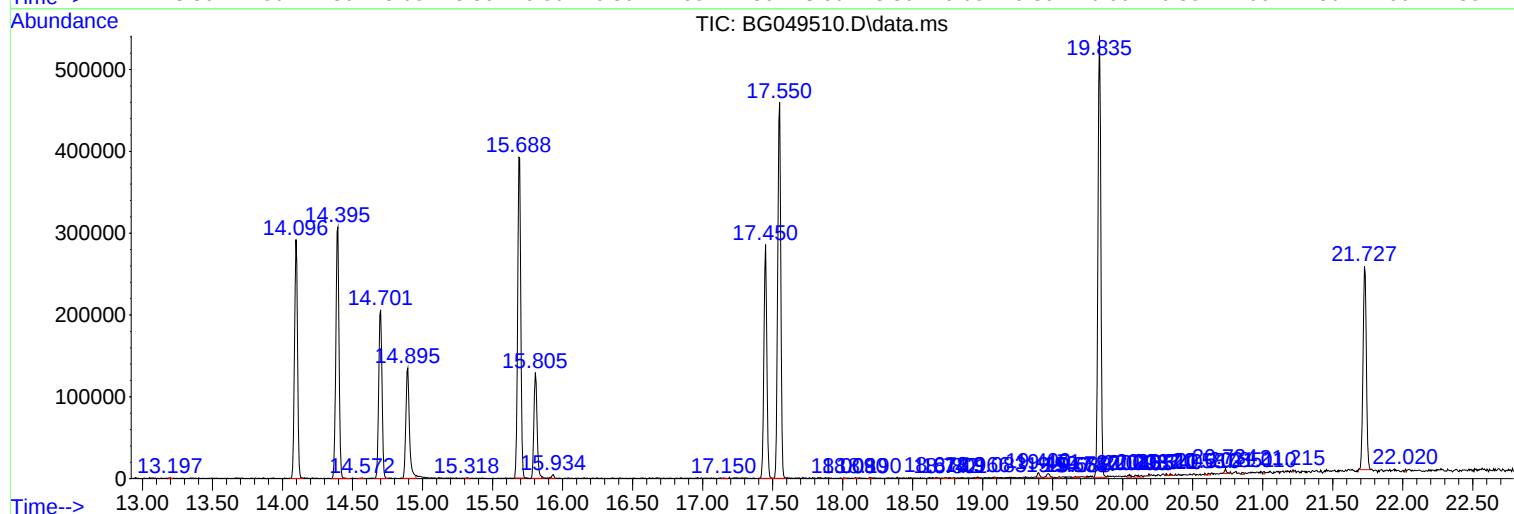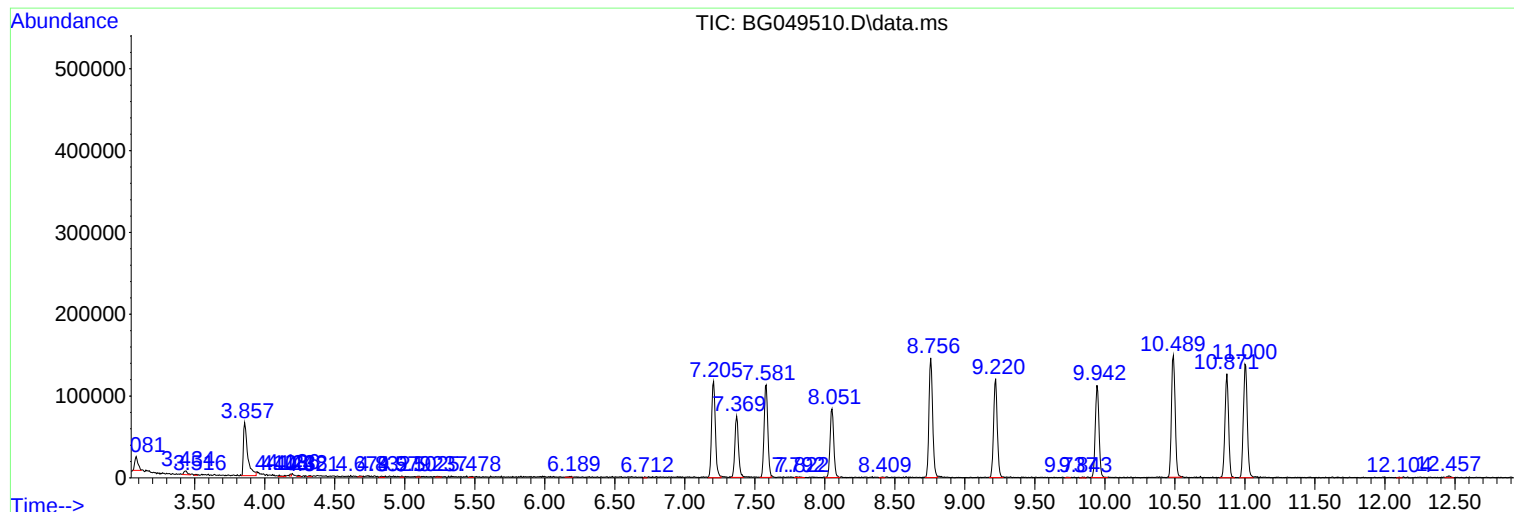

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072621\
Data File : BG049510.D
Acq On : 27 Jul 2021 16:35
Operator : CG/JU
Sample : PB137903BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK903










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.081	3.49 ng/ul	27005	1,4-Dichlorobenzene-d4	8.057

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		1-Pentene, 2-methyl-	84	C6H12	000763-29-1	78
2		2-Amino-oxazole	84	C3H4N2O	004570-45-0	72
3		Cyclohexane	84	C6H12	000110-82-7	68
4		Cyclohexane	84	C6H12	000110-82-7	64
5		Cyclohexane	84	C6H12	000110-82-7	59

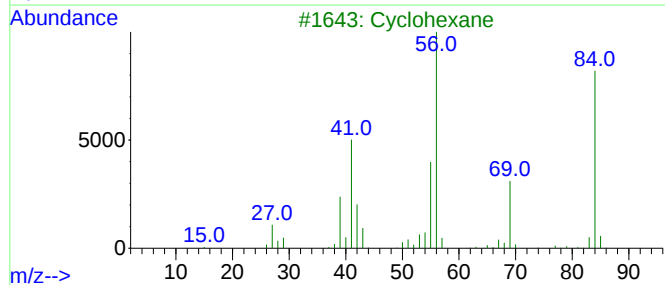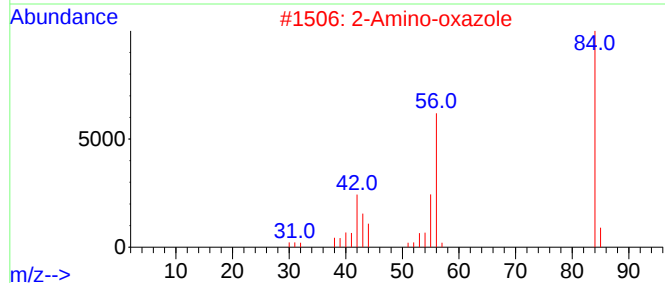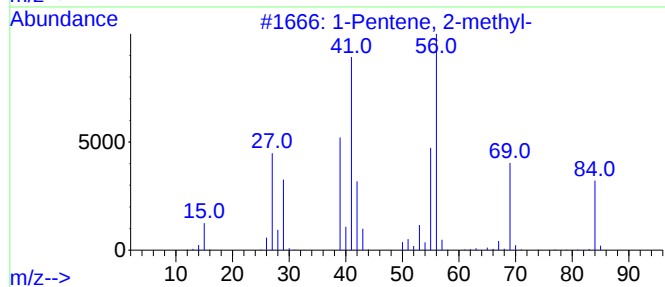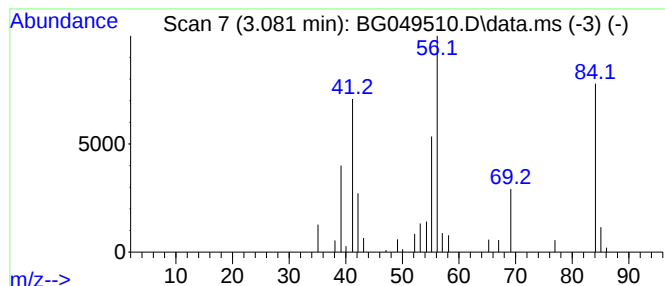

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072621\
Data File : BG049510.D
Acq On : 27 Jul 2021 16:35
Operator : CG/JU
Sample : PB137903BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK903

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	3.081	3.5	ng/u1	27005	1	8.057	154844	20.0