
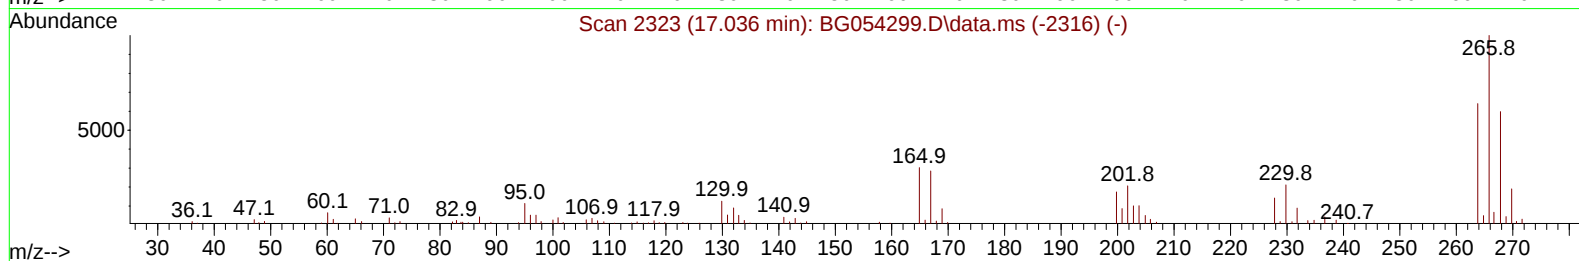
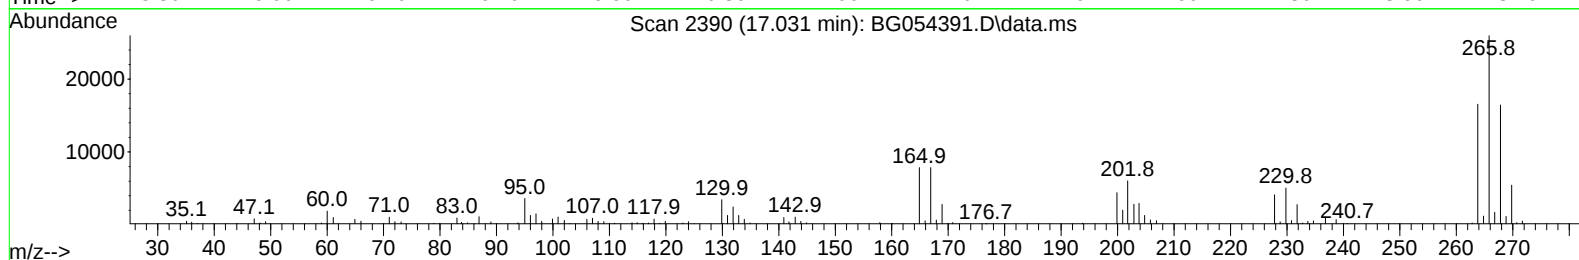


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072622\
Data File : BG054391.D
Acq On : 26 Jul 2022 9:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 27 05:58:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 15 15:54:11 2022
Response via : Initial Calibration

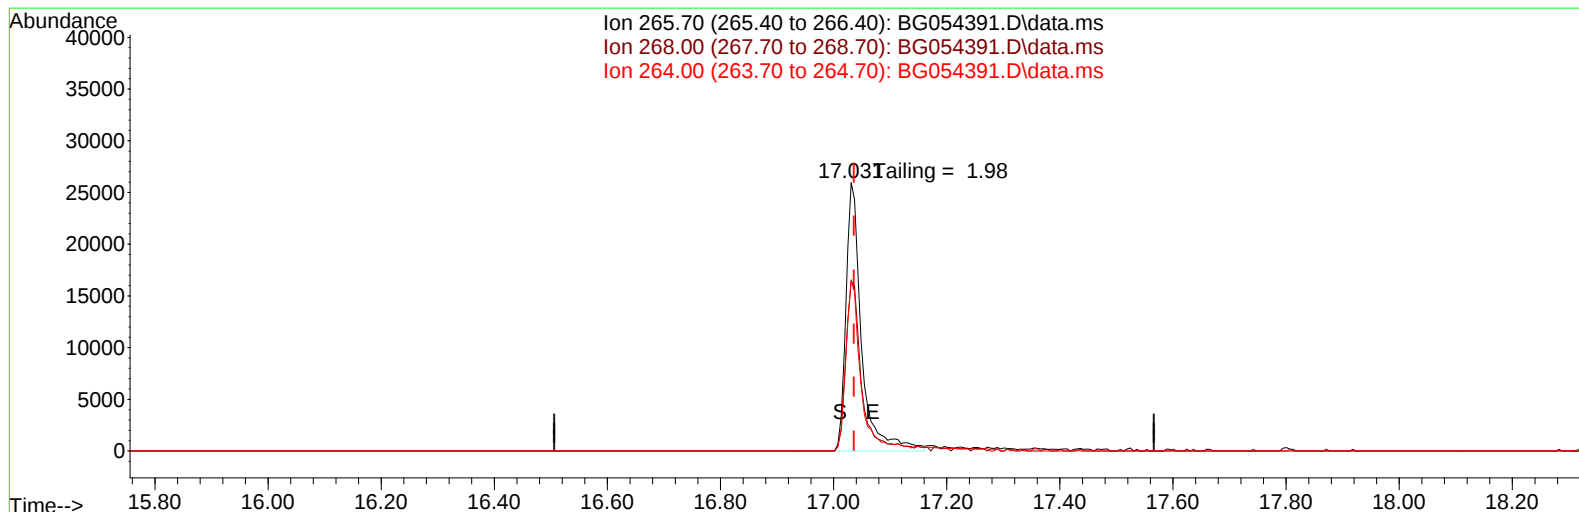

TIC: BG054391.D\data.ms

(70) Pentachlorophenol (C)




17.031min (-0.005) 33749.88 ng

response 50090

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	63.35
264.00	66.20	63.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072622\
 Data File : BG054391.D
 Acq On : 26 Jul 2022 9:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 27 05:58:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 15 15:54:11 2022
 Response via : Initial Calibration

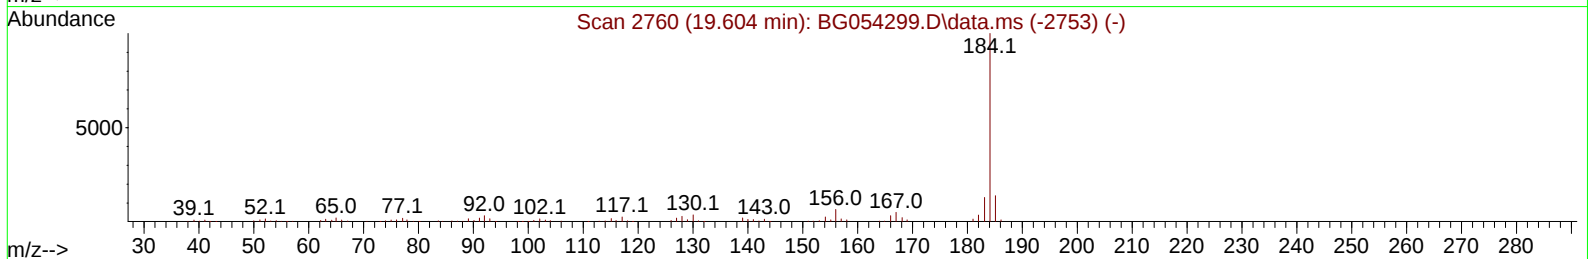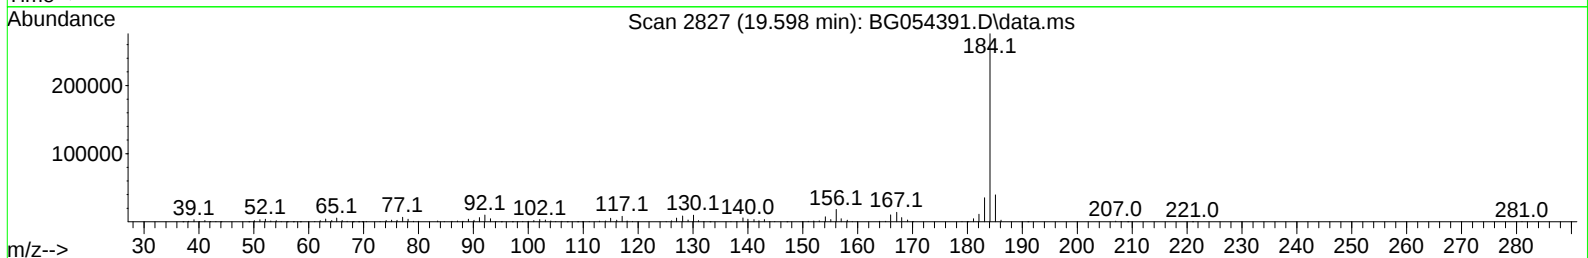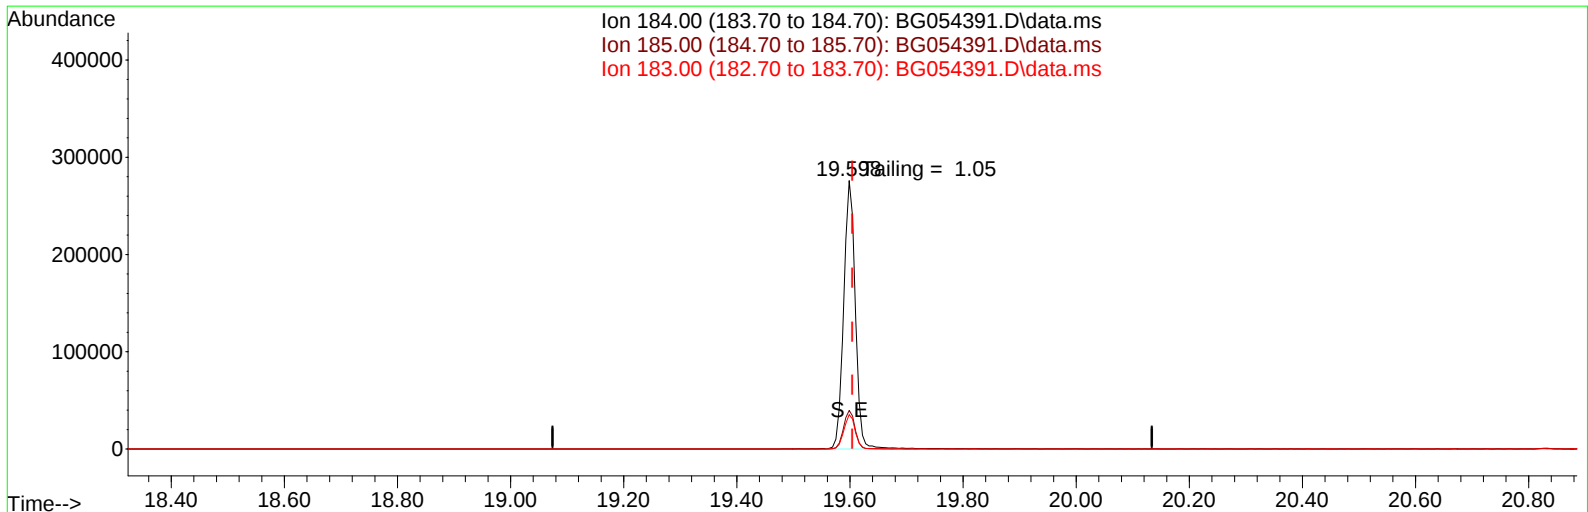

TIC: BG054391.D\data.ms

(77) Benzidine**19.598min (-0.005) 407550.93 ng****response 391196**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.37
183.00	11.10	12.86
0.00	0.00	0.00