

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072622\
 Data File : BG054401.D
 Acq On : 26 Jul 2022 16:55
 Operator : CG/JU
 Sample : N3881-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TP2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG054401.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.026	3	6	15	rVB3	11833	25370	2.13%	0.490%
2	3.108	15	20	34	rVB	77997	141337	11.84%	2.728%
3	5.564	431	438	452	rBV	191931	327841	27.47%	6.328%
4	7.168	703	711	723	rBV	206521	372078	31.18%	7.182%
5	7.984	844	850	858	rBB	53278	95251	7.98%	1.839%
6	9.148	1041	1048	1059	rBB	130217	239512	20.07%	4.623%
7	10.793	1321	1328	1338	rBB	72567	135002	11.31%	2.606%
8	13.243	1738	1745	1754	rBV	424332	676482	56.69%	13.058%
9	14.618	1973	1979	1988	rBB	137395	221399	18.55%	4.274%
10	16.110	2227	2233	2246	rBV	418796	653779	54.79%	12.620%
11	17.368	2440	2447	2457	rVB	186992	292896	24.54%	5.654%
12	18.026	2555	2559	2563	rVB	9860	12010	1.01%	0.232%
13	19.976	2885	2891	2897	rBV	905508	1193343	100.00%	23.035%
14	21.269	3107	3111	3119	rVB5	20349	33839	2.84%	0.653%
15	21.627	3166	3172	3178	rVB2	211664	358828	30.07%	6.926%
16	24.824	3709	3716	3728	rVB2	143854	401549	33.65%	7.751%




Sum of corrected areas: 5180516

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072622\
Data File : BG054401.D
Acq On : 26 Jul 2022 16:55
Operator : CG/JU
Sample : N3881-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

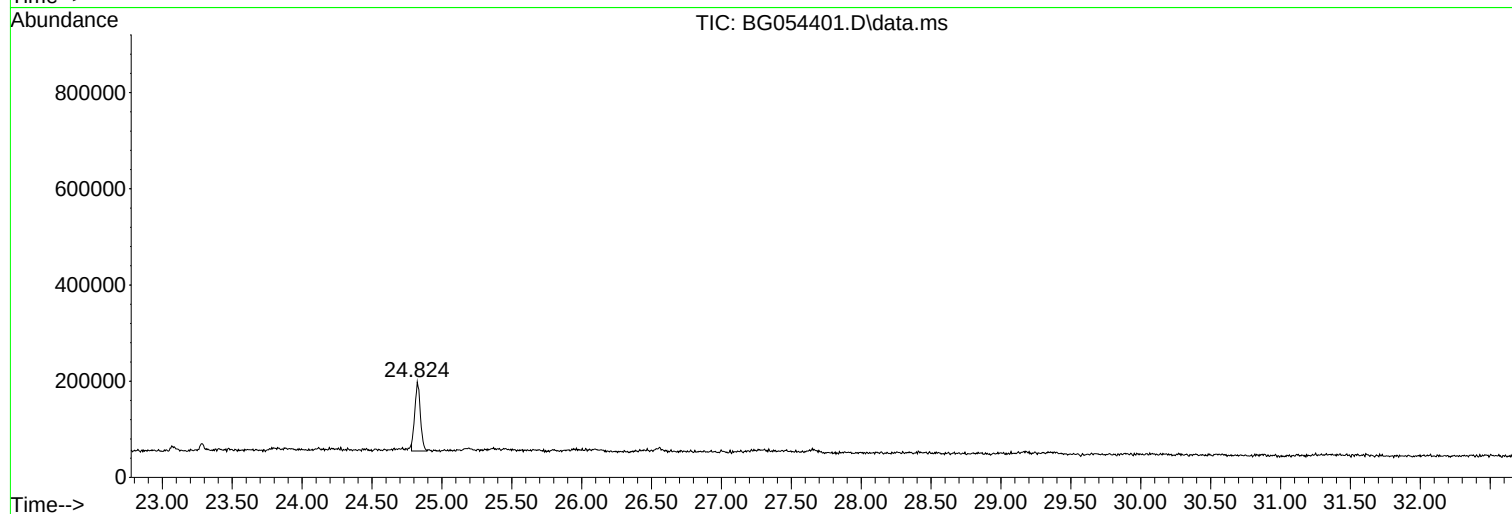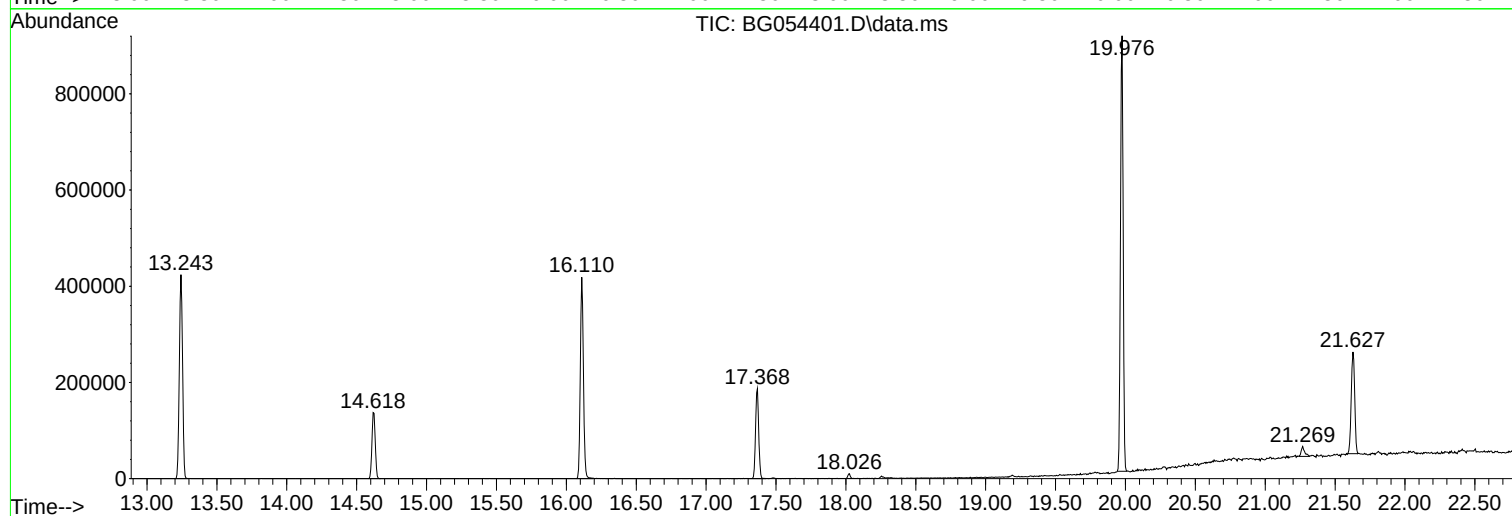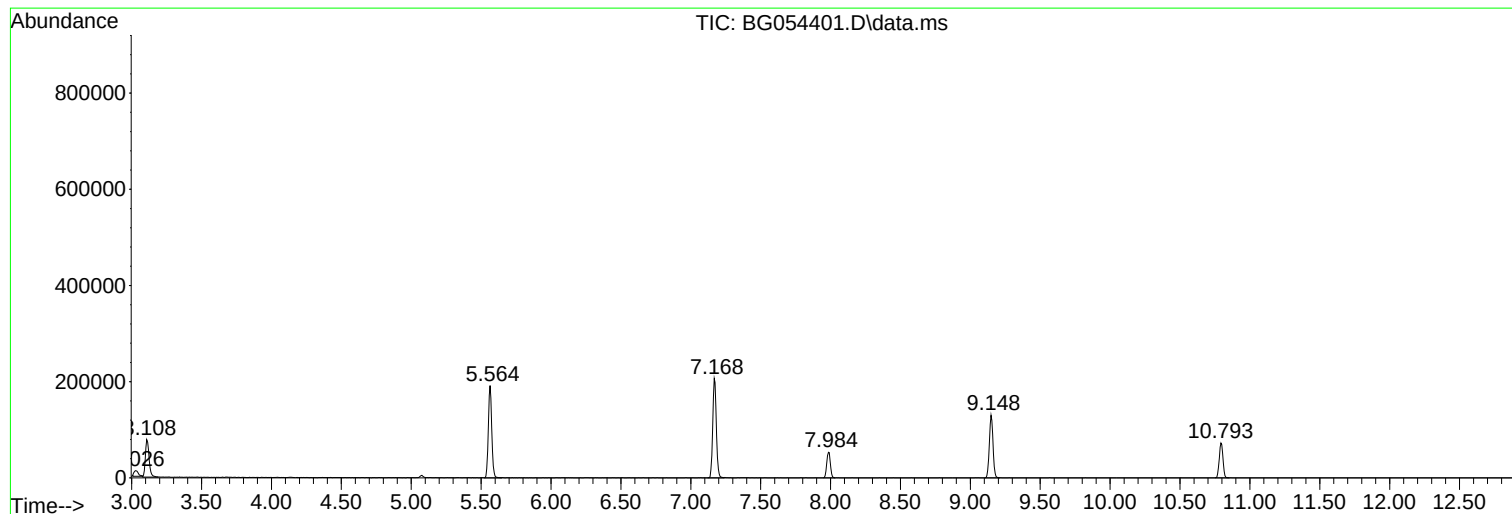

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072622\
Data File : BG054401.D
Acq On : 26 Jul 2022 16:55
Operator : CG/JU
Sample : N3881-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP2










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.108	29.68 ng	141337	1,4-Dichlorobenzene-d4	7.990

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	28
3			Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	12
4			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9
5			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	9

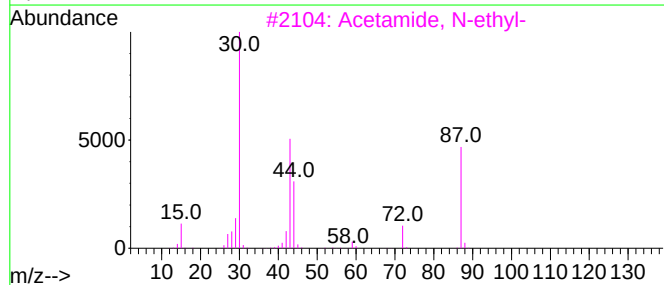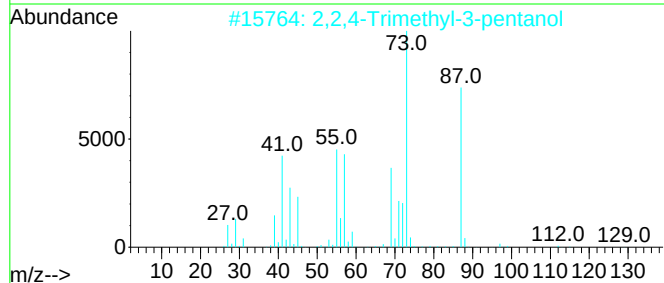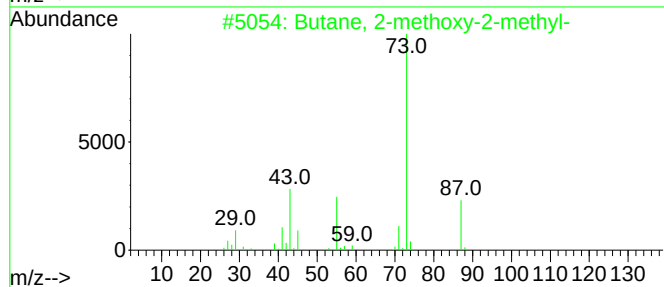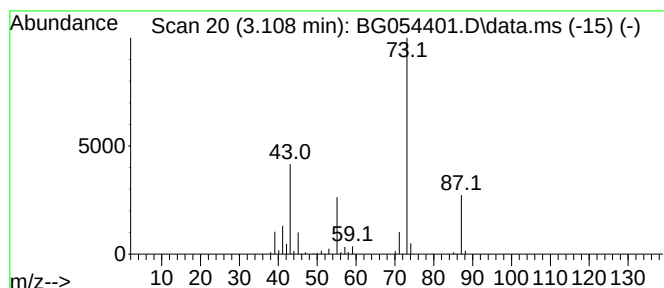

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072622\
Data File : BG054401.D
Acq On : 26 Jul 2022 16:55
Operator : CG/JU
Sample : N3881-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.108	29.7	ng	141337	1	7.990	95251	20.0