


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072622\
 Data File : BG054391.D
 Acq On : 26 Jul 2022 9:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 15 15:54:11 2022

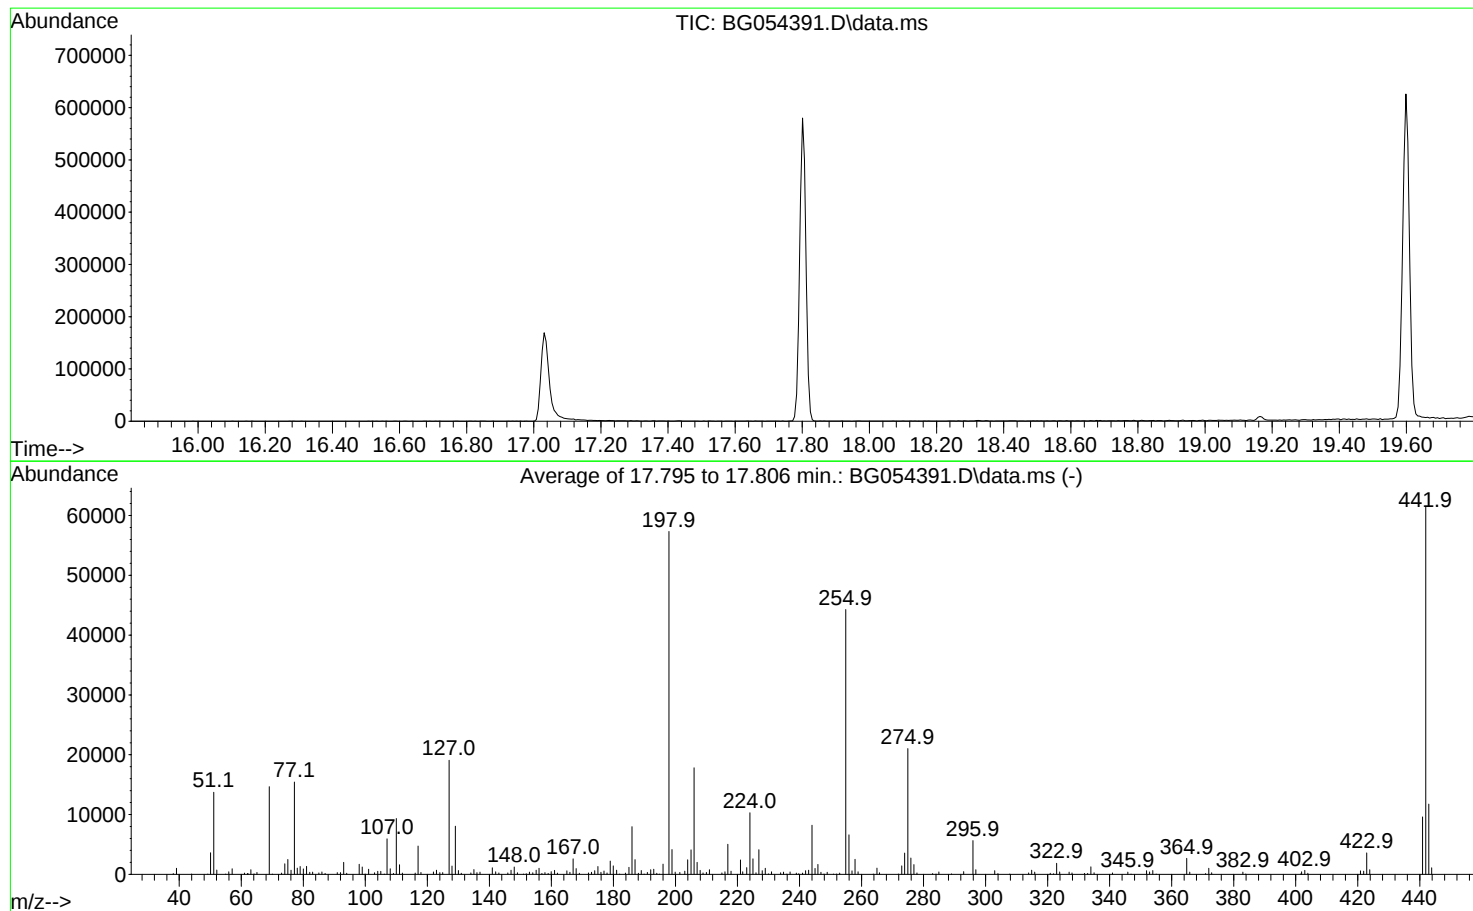




AutoFind: Scans 2520, 2521, 2522; Background Corrected with Scan 2514

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.9	13727	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	25.6	14664	PASS
70	69	0.00	2	0.4	56	PASS
127	198	10	80	33.3	19083	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	57336	PASS
199	198	5	9	7.3	4161	PASS
275	198	10	60	36.7	21037	PASS
365	198	1	100	4.7	2671	PASS
441	198	0.01	100	16.7	9603	PASS
442	442	50	100	100.0	61499	PASS
443	442	15	24	19.1	11737	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072622\
Data File : BG054391.D
Acq On : 26 Jul 2022 9:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 27 05:58:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 15 15:54:11 2022
Response via : Initial Calibration

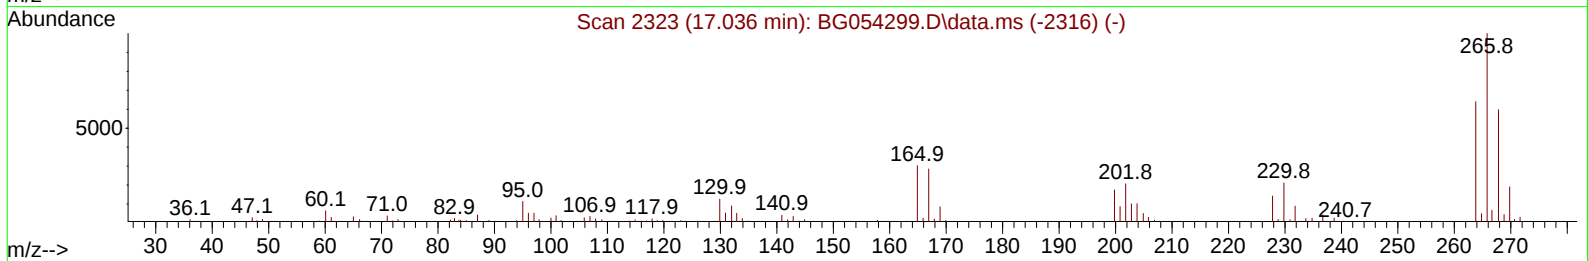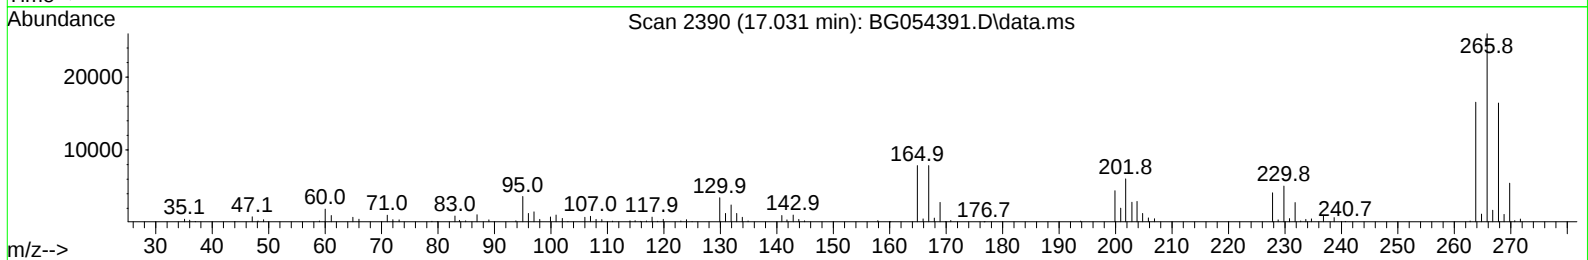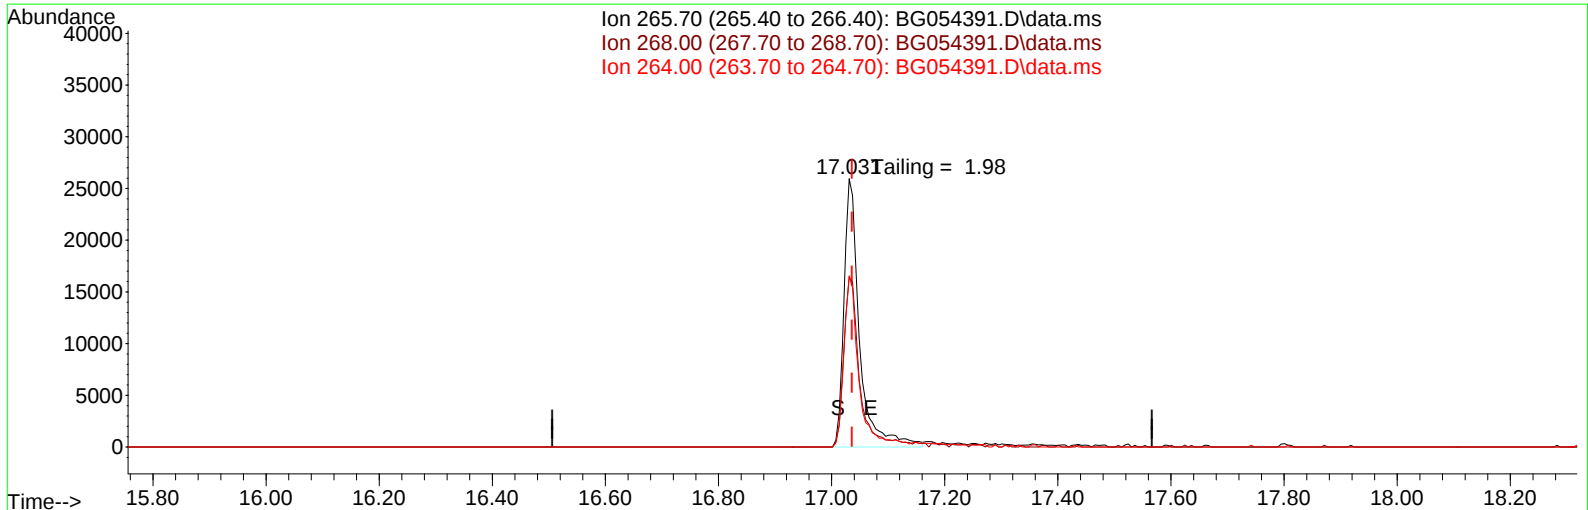

TIC: BG054391.D\data.ms

(70) Pentachlorophenol (C)

17.031min (-0.005) 33749.88 ng




response 50090

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	63.35
264.00	66.20	63.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072622\
 Data File : BG054391.D
 Acq On : 26 Jul 2022 9:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Jul 27 05:58:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 15 15:54:11 2022
 Response via : Initial Calibration

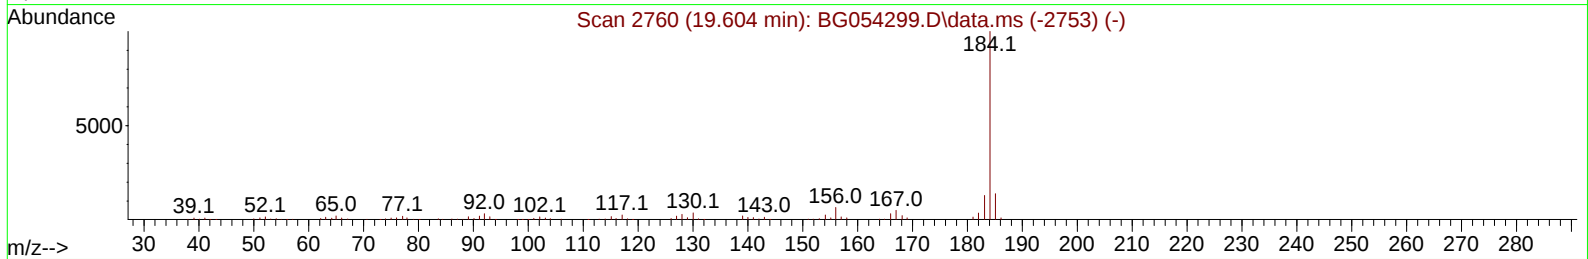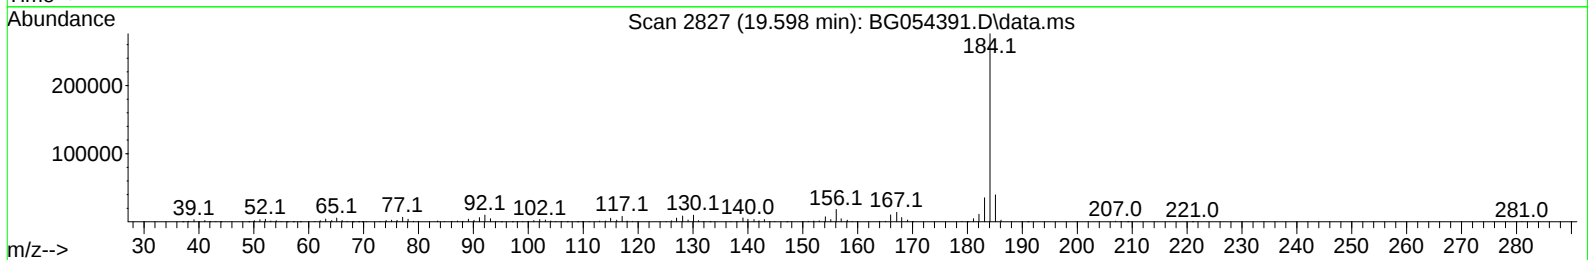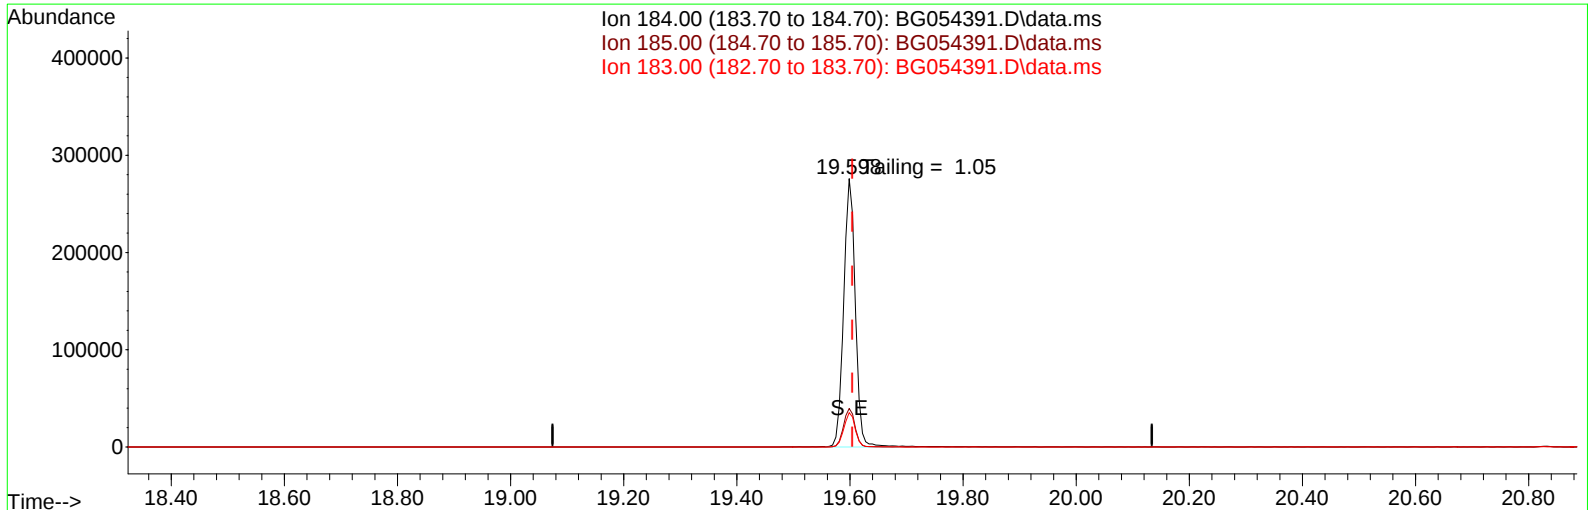

TIC: BG054391.D\data.ms

(77) Benzidine**19.598min (-0.005) 407550.93 ng****response 391196**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.37
183.00	11.10	12.86
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/26/2022	BNA_G	<u>BG054391.D</u>
Compound Name	Response	Retention Time
DDT	217961	20.832
DDD	5222	20.398
DDE	501	19.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5723	223684	2.56

Instrument :
BNA_G
ClientSampleId :
DFTPP