

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG072715\
 Data File : BG018114.D
 Acq On : 27 Jul 2015 15:29
 Operator : TP/UM
 Sample : G3030-17
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C02F2

Quant Time: Jul 28 01:59:28 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG072315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 28 01:54:27 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.51	152	29015	20.00	ng/ul	0.00
18) Naphthalene-d8	10.29	136	137354	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.18	164	89243	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.93	188	203389	20.00	ng/ul	0.00
78) Chrysene-d12	21.14	240	216154	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	219295	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.01	96	3497	7.53	ng/uL	0.00
5) Phenol-d5	6.69	99	76325	34.10	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.85	67	38028	34.42	ng/ul	0.00
9) 2-Chlorophenol-d4	7.04	132	73142	36.85	ng/ul	0.00
13) 4-Methylphenol-d8	8.23	113	70407	35.47	ng/ul	0.00
19) Nitrobenzene-d5	8.66	128	32836	30.24	ng/ul	0.00
22) 2-Nitrophenol-d4	9.38	143	33301	29.05	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.92	165	72580	36.37	ng/ul	0.00
29) 4-Chloroaniline-d4	10.43	131	105956	45.64	ng/ul	0.00
44) Dimethylphthalate-d6	13.60	166	247407	39.49	ng/ul	0.00
47) Acenaphthylene-d8	13.87	160	272689	35.42	ng/ul	0.00
52) 4-Nitrophenol-d4	14.40	143	34024	25.81	ng/ul	0.00
58) Fluorene-d10	15.18	176	204676	35.34	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.31	200	25833	19.87	ng/ul	0.00
71) Anthracene-d10	17.03	188	335605	38.10	ng/ul	0.00
79) Pyrene-d10	19.34	212	330883	33.42	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	348827	33.33	ng/ul	0.00


Target Compounds						Qvalue
45) Dimethylphthalate	13.64	163	131798	20.90	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG072715\
Data File : BG018114.D
Acq On : 27 Jul 2015 15:29
Operator : TP/UM
Sample : G3030-17
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C02F2

Quant Time: Jul 28 01:59:28 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG072315.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 28 01:54:27 2015
Response via : Initial Calibration

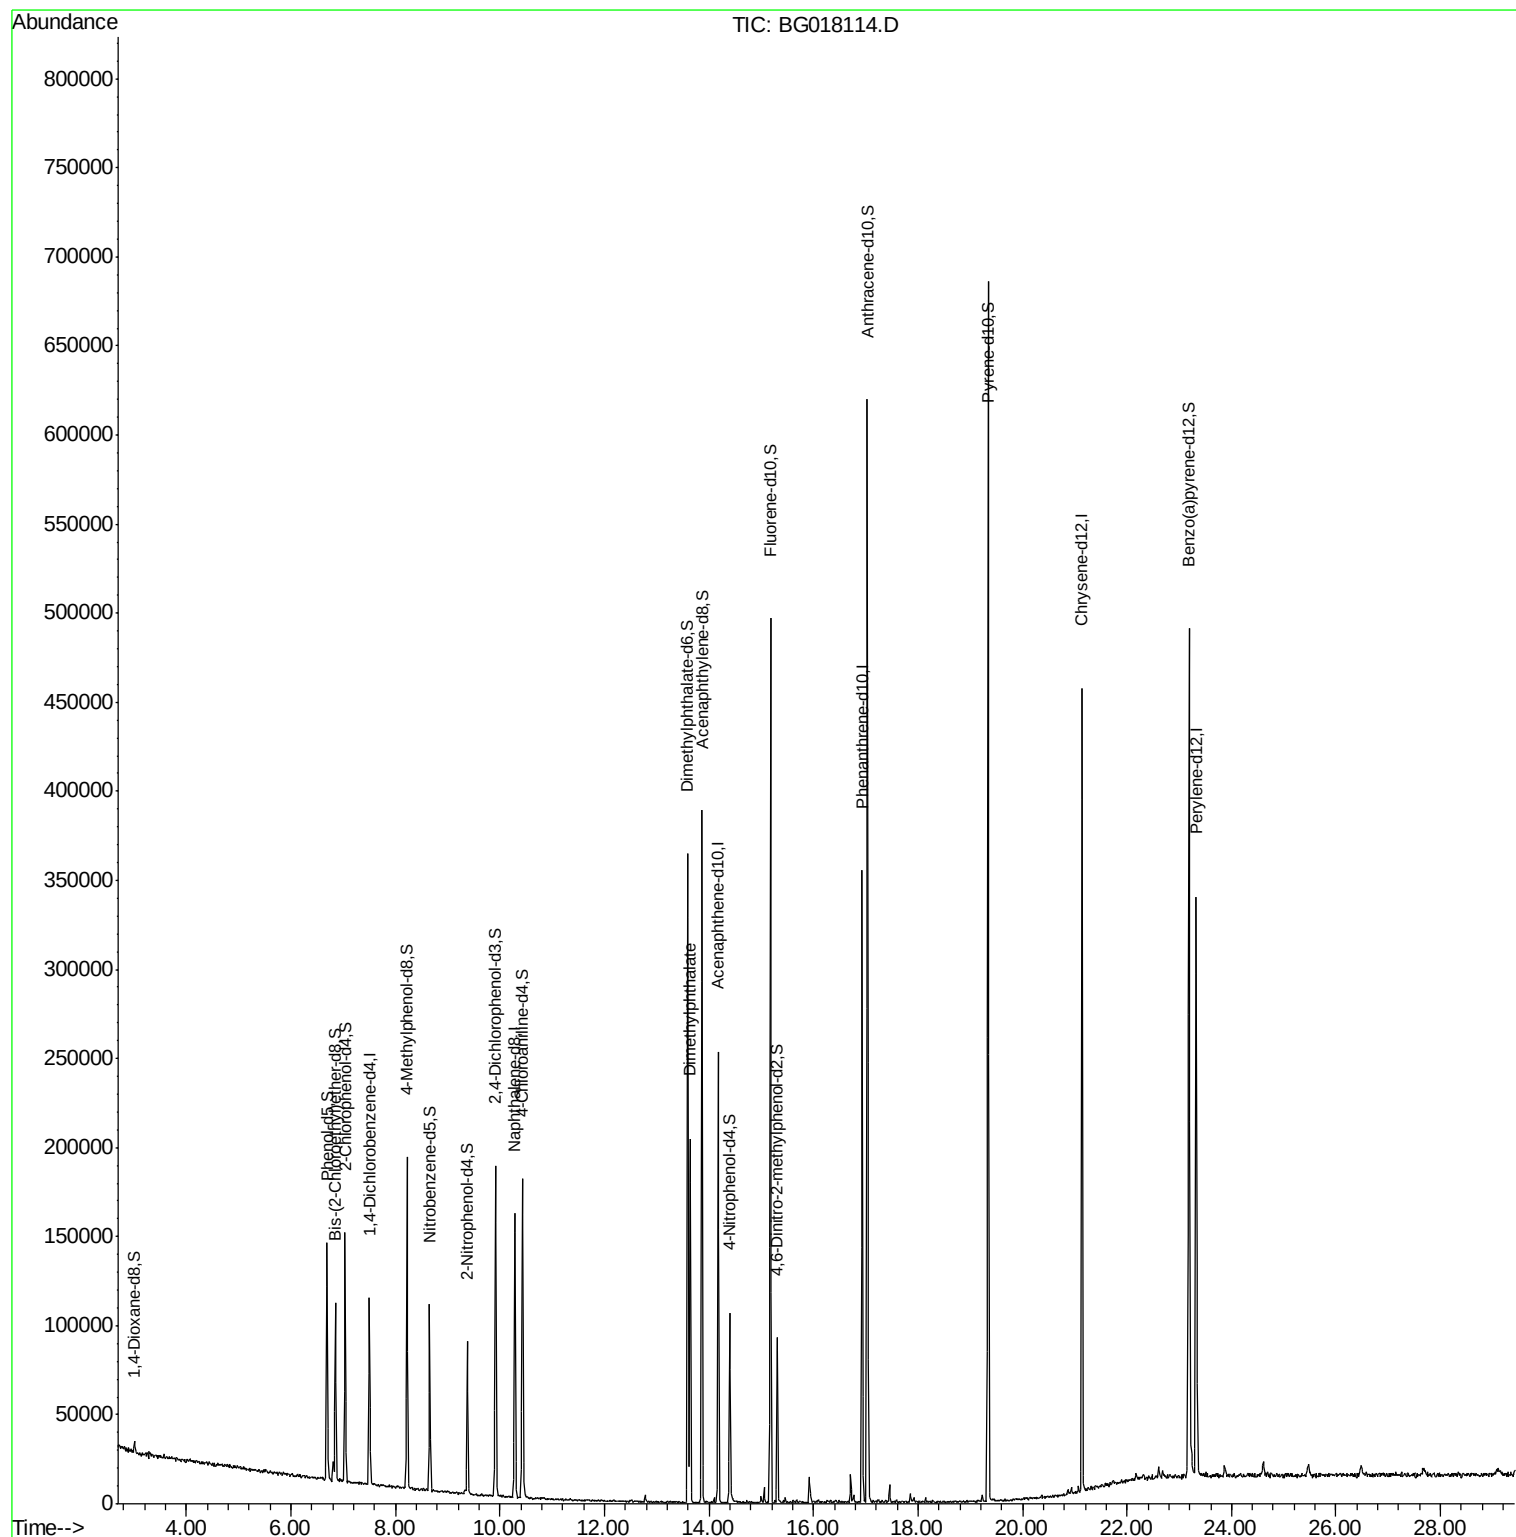

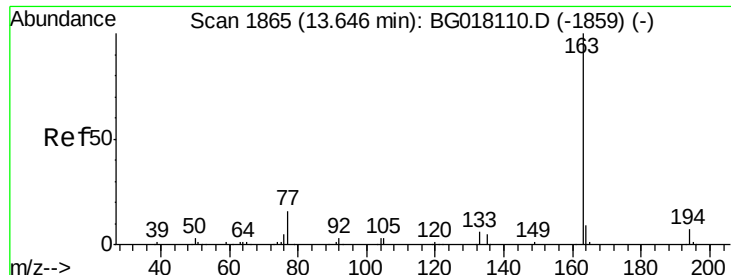

#45

Dimethylphthalate

Concen: 20.90 ng/ul

RT: 13.64 min Scan# 1864

Delta R.T. -0.00 min

Lab File: BG018114.D


Acq: 27 Jul 2015 15:29

Instrument :

BNA_G

ClientSampleId :

C02F2

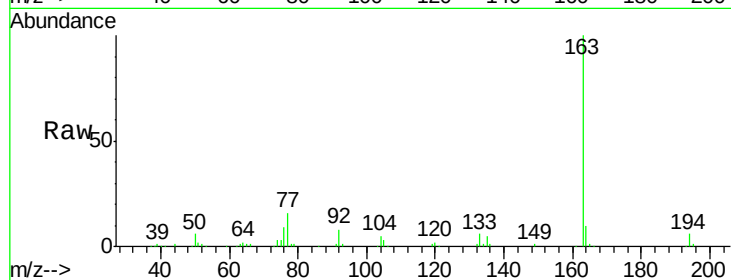


Tgt Ion:163 Resp: 131798

Ion Ratio Lower Upper

163 100

194 6.4 5.4 8.2

164 10.0 8.7 13.1

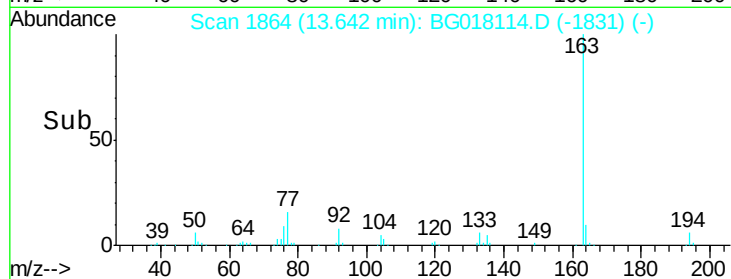

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

