

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG072715\
 Data File : BG018120.D
 Acq On : 27 Jul 2015 19:01
 Operator : TP/UM
 Sample : G2938-08RE
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0207

Quant Time: Jul 28 02:00:16 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG072315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 28 01:54:27 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.51	152	36315	20.00	ng/ul	0.00
18) Naphthalene-d8	10.29	136	170471	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.18	164	113297	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.94	188	265710	20.00	ng/ul	0.00
78) Chrysene-d12	21.14	240	283888	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	279132	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.01	96	813	1.40	ng/uL	0.00
5) Phenol-d5	6.69	99	17553	6.27	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.85	67	37378	27.03	ng/ul	0.00
9) 2-Chlorophenol-d4	7.04	132	57327	23.08	ng/ul	0.00
13) 4-Methylphenol-d8	8.22	113	34652	13.95	ng/ul	0.00
19) Nitrobenzene-d5	8.66	128	39323	29.18	ng/ul	0.00
22) 2-Nitrophenol-d4	9.38	143	39999	28.11	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.92	165	65670	26.51	ng/ul	0.00
29) 4-Chloroaniline-d4	10.43	131	2487	0.86	ng/ul	0.00
44) Dimethylphthalate-d6	13.60	166	243362	30.60	ng/ul	0.00
47) Acenaphthylene-d8	13.87	160	301529	30.85	ng/ul	0.00
52) 4-Nitrophenol-d4	14.40	143	7408	4.43	ng/ul	0.00
58) Fluorene-d10	15.18	176	232680	31.65	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.31	200	40361	23.76	ng/ul	0.00
71) Anthracene-d10	17.04	188	373606	32.46	ng/ul	0.00
79) Pyrene-d10	19.35	212	419497	32.26	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	403999	30.33	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
84) Bis(2-ethylhexyl)phthalate	21.07	149	14274	1.50	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG072715\
Data File : BG018120.D
Acq On : 27 Jul 2015 19:01
Operator : TP/UM
Sample : G2938-08RE
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0207

Quant Time: Jul 28 02:00:16 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG072315.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 28 01:54:27 2015
Response via : Initial Calibration

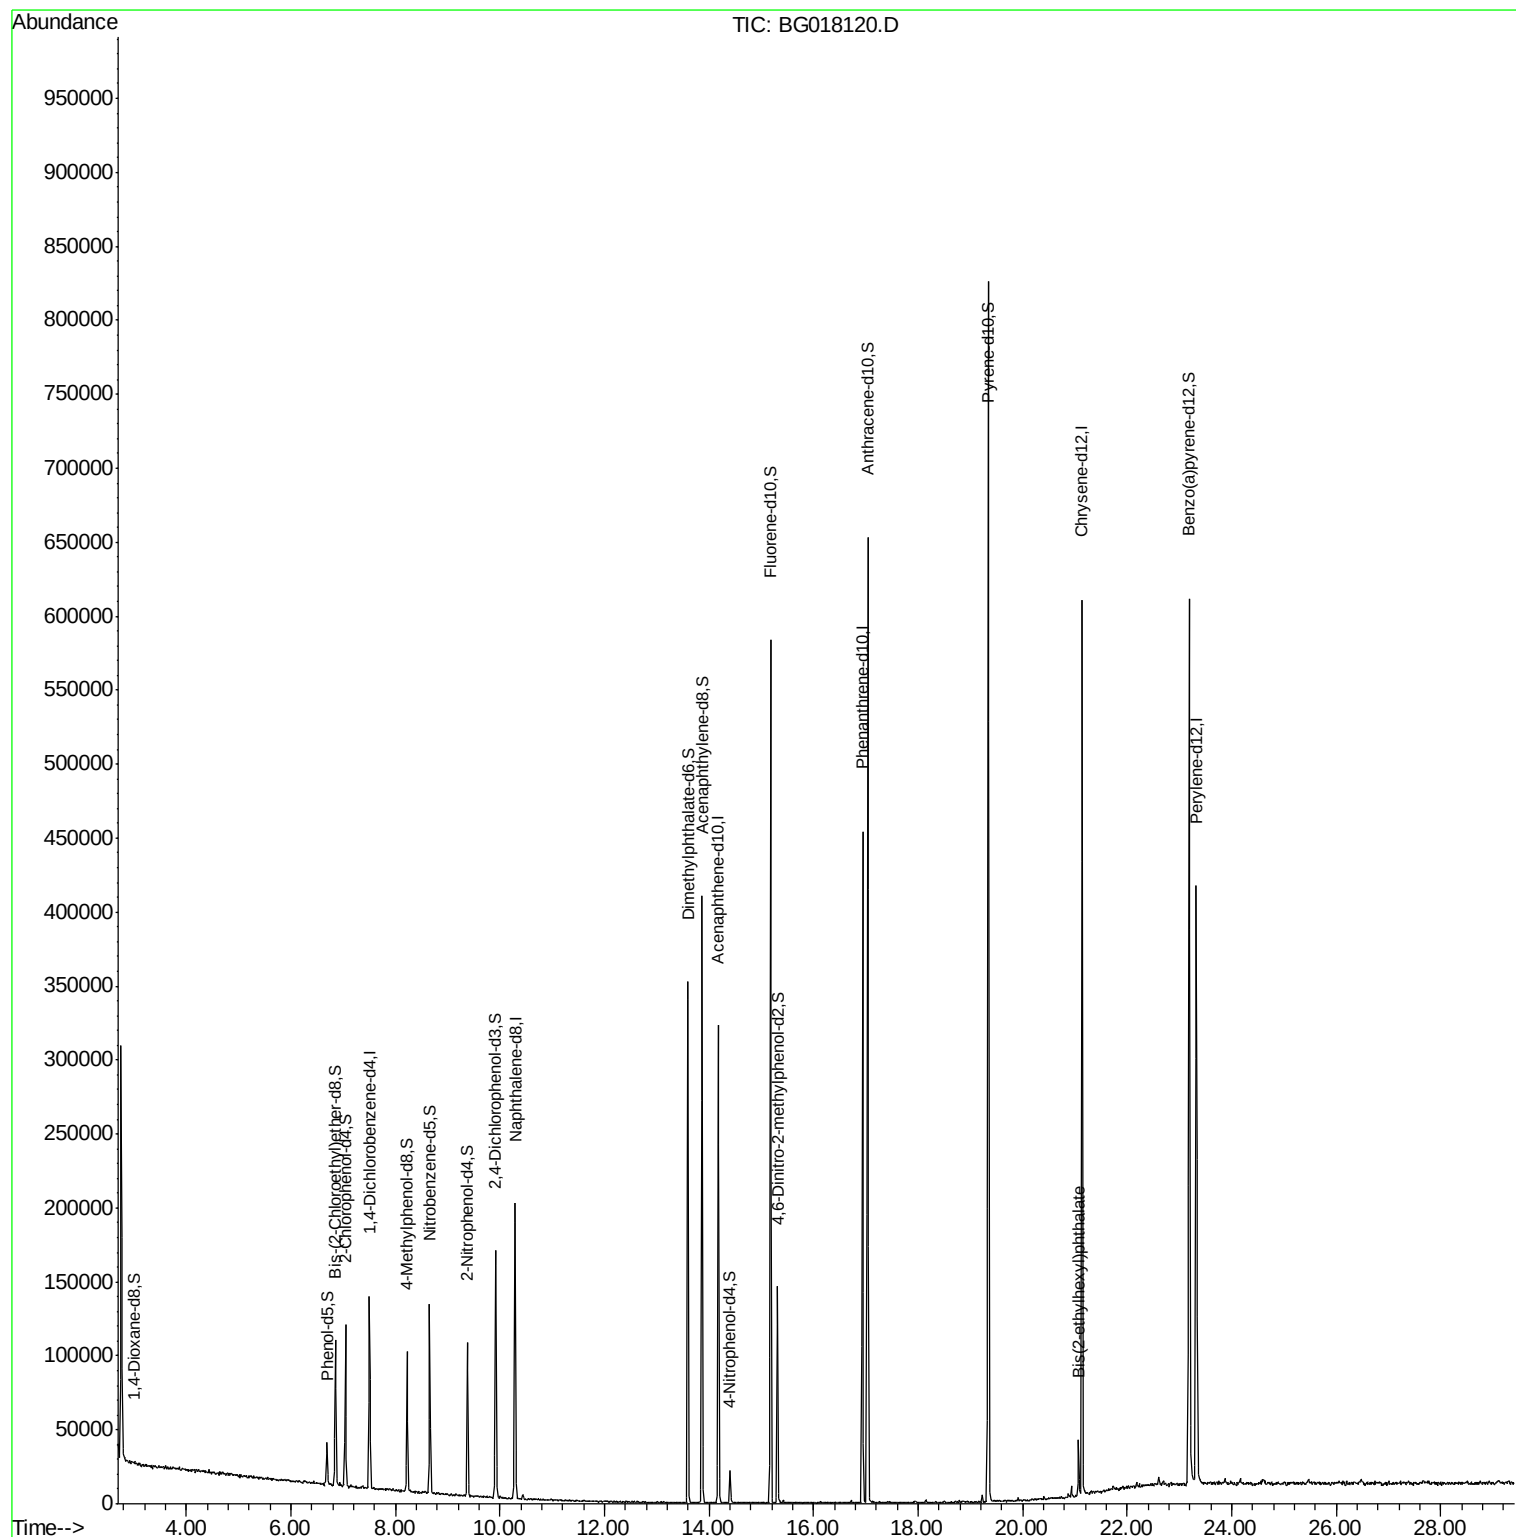

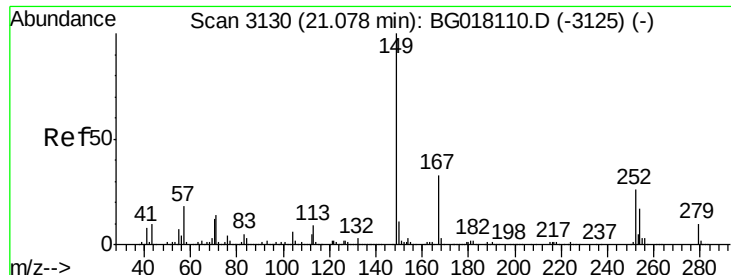

#84

Bis(2-ethylhexyl)phthalate

Concen: 1.50 ng/ul

RT: 21.07 min Scan# 3129

Delta R.T. -0.01 min

Lab File: BG018120.D

Acq: 27 Jul 2015 19:01

Instrument :

BNA_G

ClientSampleId :

C0207


Tgt Ion:149 Resp: 14274

Ion Ratio Lower Upper

149 100

167 30.5 26.2 39.4

279 8.1 7.2 10.8

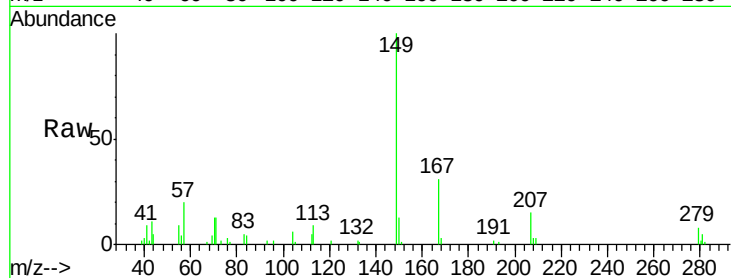

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

