

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG072715\
 Data File : BG018132.D
 Acq On : 28 Jul 2015 2:37
 Operator : TP/UM
 Sample : G3048-08
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C01X1

Quant Time: Jul 28 04:32:04 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG072315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 28 02:39:42 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.51	152	35408	20.00	ng/ul	0.00
18) Naphthalene-d8	10.29	136	163232	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.18	164	105550	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.94	188	240976	20.00	ng/ul	0.00
78) Chrysene-d12	21.14	240	255452	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	254263	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.01	96	3005	5.30	ng/uL	0.00
5) Phenol-d5	6.69	99	80298	29.40	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.85	67	39778	29.50	ng/ul	0.00
9) 2-Chlorophenol-d4	7.04	132	75038	30.98	ng/ul	0.00
13) 4-Methylphenol-d8	8.22	113	73661	30.41	ng/ul	0.00
19) Nitrobenzene-d5	8.66	128	38434	29.79	ng/ul	0.00
22) 2-Nitrophenol-d4	9.38	143	42271	31.03	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.91	165	78037	32.91	ng/ul	0.00
29) 4-Chloroaniline-d4	10.43	131	98469	35.69	ng/ul	0.00
44) Dimethylphthalate-d6	13.60	166	248549	33.54	ng/ul	0.00
47) Acenaphthylene-d8	13.87	160	289339	31.78	ng/ul	0.00
52) 4-Nitrophenol-d4	14.40	143	44646	28.64	ng/ul	0.00
58) Fluorene-d10	15.18	176	219317	32.02	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.31	200	32745	21.25	ng/ul	0.00
71) Anthracene-d10	17.03	188	333580	31.96	ng/ul	0.00
79) Pyrene-d10	19.34	212	367823	31.43	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	389698	32.12	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.65	163	96177	12.90	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG072715\
Data File : BG018132.D
Acq On : 28 Jul 2015 2:37
Operator : TP/UM
Sample : G3048-08
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C01X1

Quant Time: Jul 28 04:32:04 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG072315.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 28 02:39:42 2015
Response via : Initial Calibration

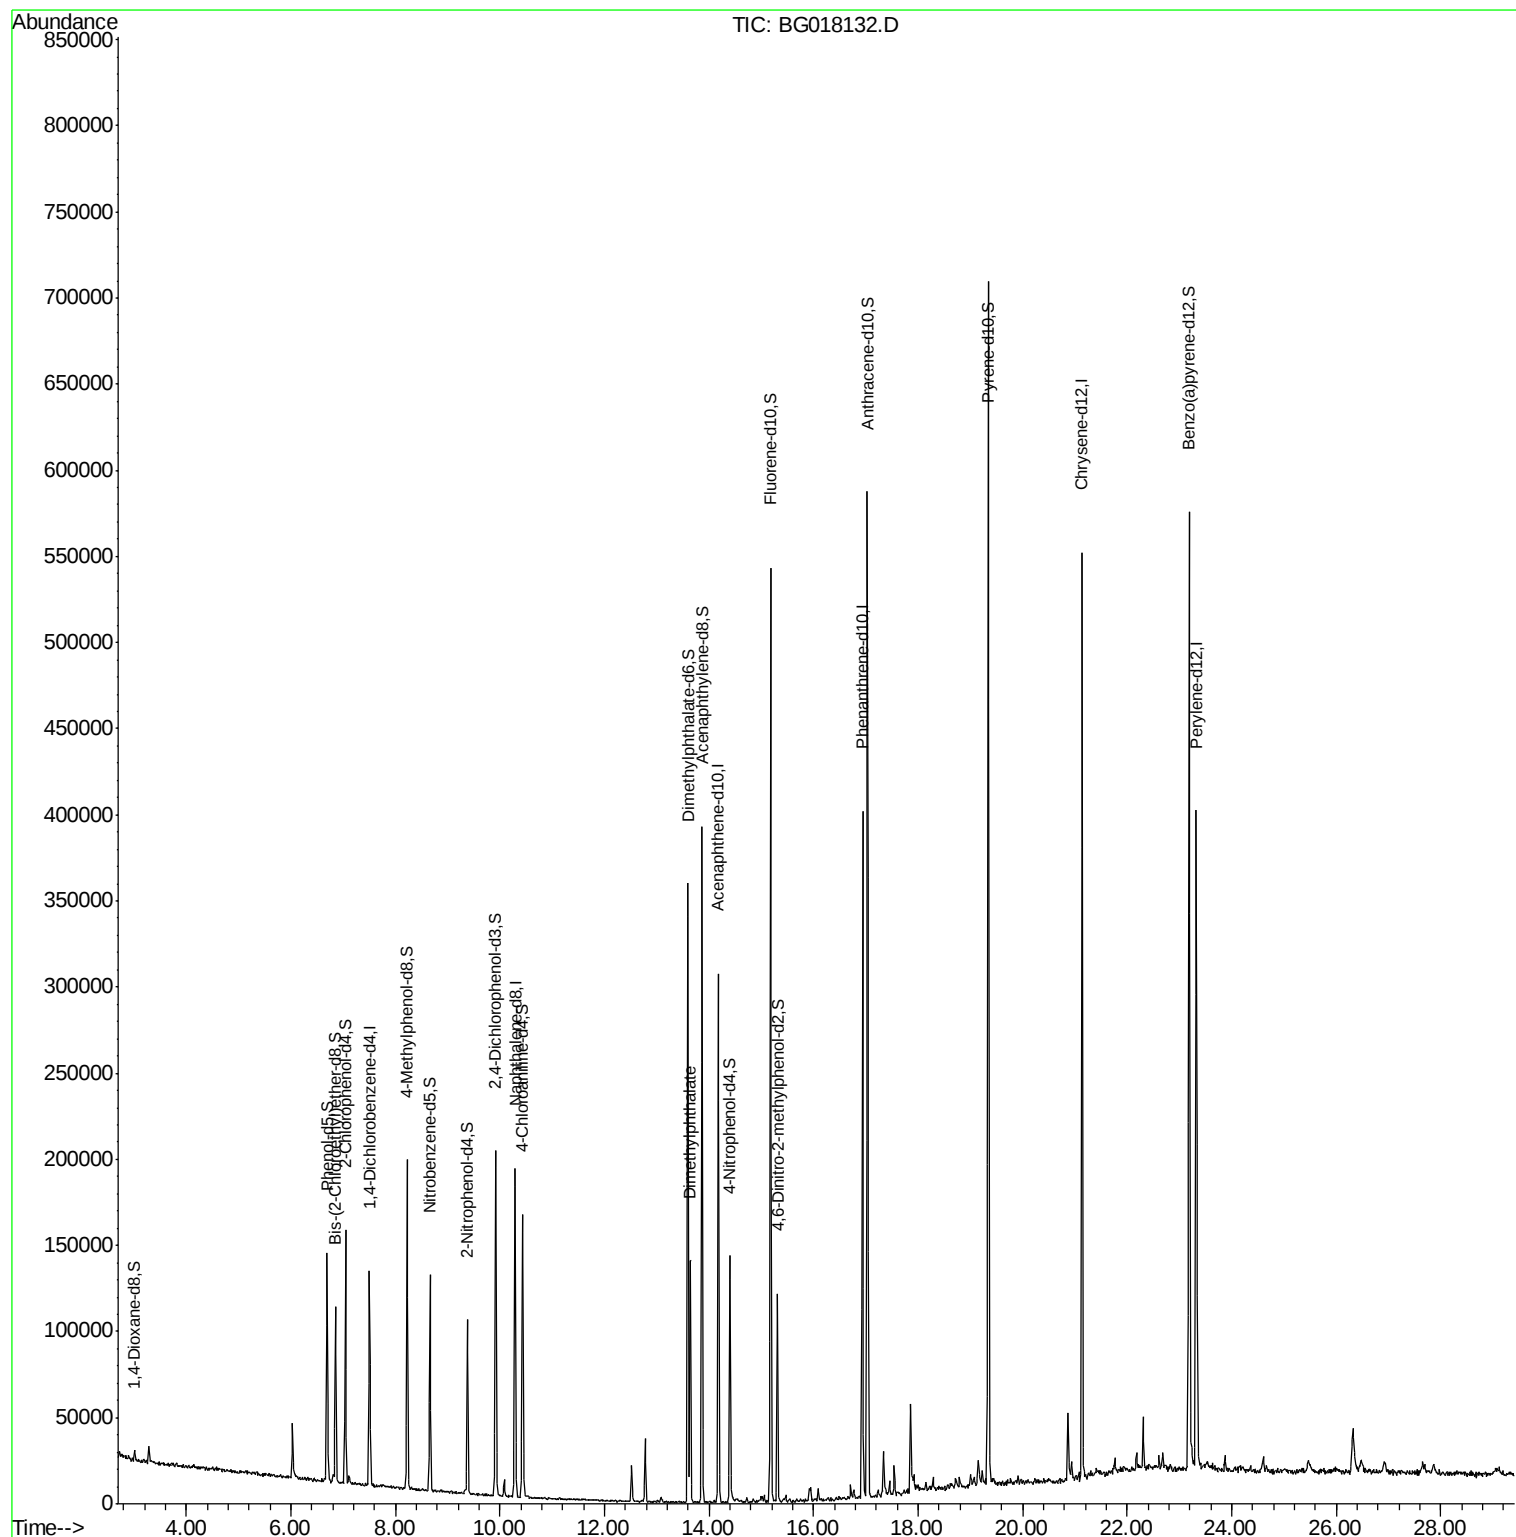

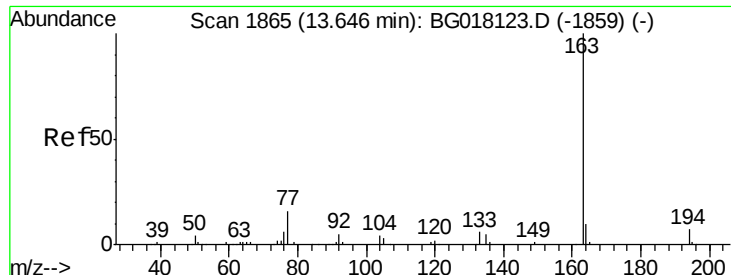

#45

Dimethylphthalate

Concen: 12.90 ng/ul

RT: 13.65 min Scan# 1865

Delta R.T. -0.00 min

Lab File: BG018132.D


Acq: 28 Jul 2015 2:37

Instrument :

BNA_G

ClientSampleId :

C01X1

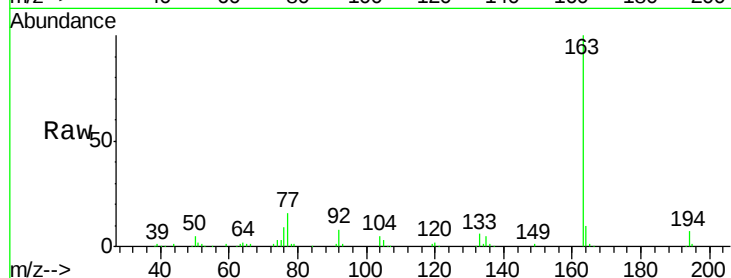

Tgt Ion:	163	Resp:	96177
Ion	Ratio	Lower	Upper
163	100		
194	6.6	5.4	8.2
164	9.7	8.7	13.1

