

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG072715\
 Data File : BG018133.D
 Acq On : 28 Jul 2015 3:12
 Operator : TP/UM
 Sample : G3048-09
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C01X2

Quant Time: Jul 28 04:32:11 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG072315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 28 02:39:42 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.51	152	33069	20.00	ng/ul	0.00
18) Naphthalene-d8	10.29	136	154991	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.18	164	99974	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.93	188	225862	20.00	ng/ul	0.00
78) Chrysene-d12	21.14	240	238290	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	238053	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.01	96	3015	5.70	ng/uL	0.00
5) Phenol-d5	6.69	99	67623	26.51	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.85	67	34790	27.63	ng/ul	0.00
9) 2-Chlorophenol-d4	7.04	132	65009	28.74	ng/ul	0.00
13) 4-Methylphenol-d8	8.22	113	62214	27.50	ng/ul	0.00
19) Nitrobenzene-d5	8.66	128	32866	26.82	ng/ul	0.00
22) 2-Nitrophenol-d4	9.38	143	35335	27.31	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.92	165	66598	29.57	ng/ul	0.00
29) 4-Chloroaniline-d4	10.43	131	90017	34.36	ng/ul	0.00
44) Dimethylphthalate-d6	13.60	166	213348	30.40	ng/ul	0.00
47) Acenaphthylene-d8	13.87	160	246671	28.60	ng/ul	0.00
52) 4-Nitrophenol-d4	14.40	143	34184	23.15	ng/ul	0.00
58) Fluorene-d10	15.18	176	183080	28.22	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.31	200	17997	12.46	ng/ul	0.00
71) Anthracene-d10	17.03	188	286689	29.31	ng/ul	0.00
79) Pyrene-d10	19.34	212	316654	29.01	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	330526	29.10	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.64	163	72665	10.29	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG072715\
Data File : BG018133.D
Acq On : 28 Jul 2015 3:12
Operator : TP/UM
Sample : G3048-09
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C01X2

Quant Time: Jul 28 04:32:11 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG072315.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 28 02:39:42 2015
Response via : Initial Calibration

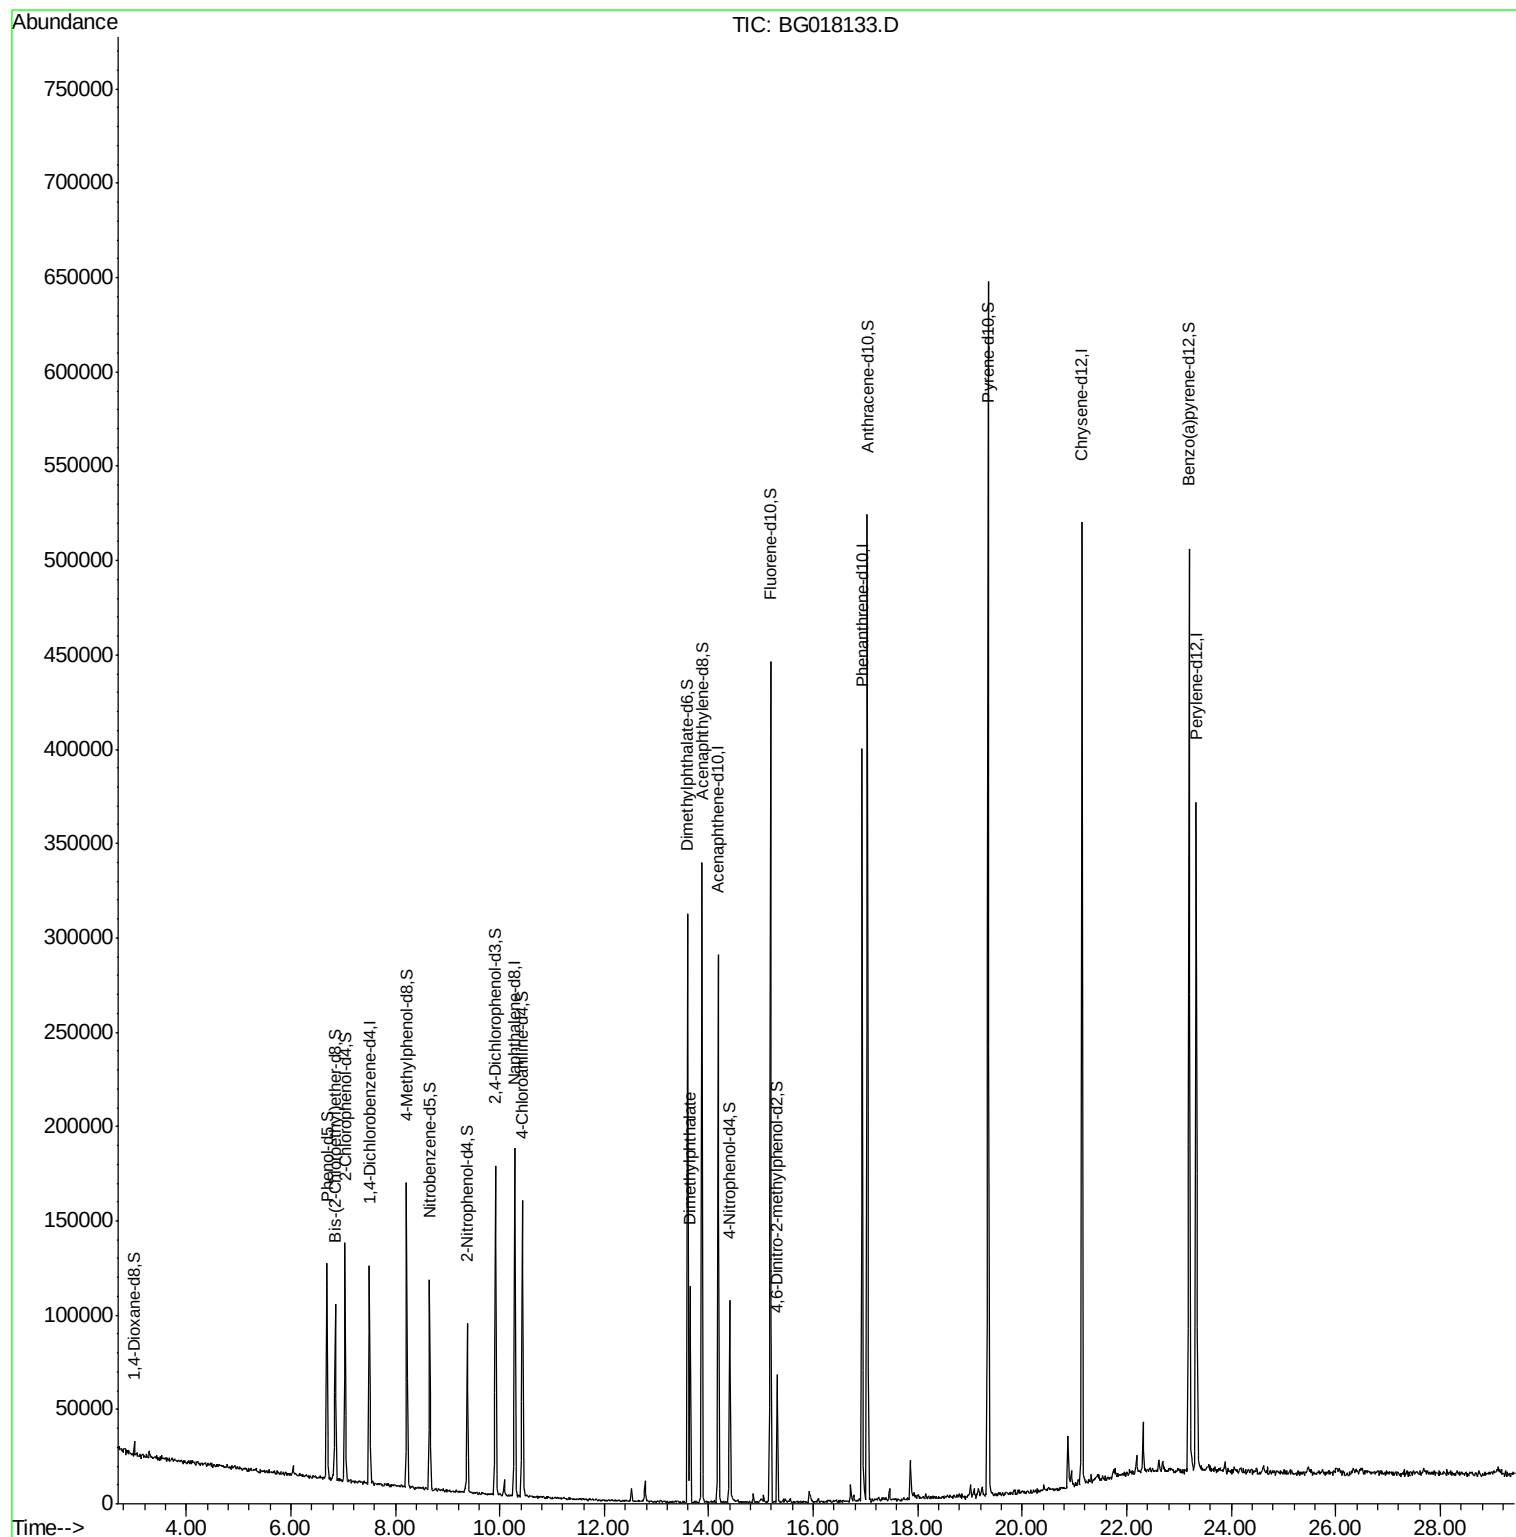

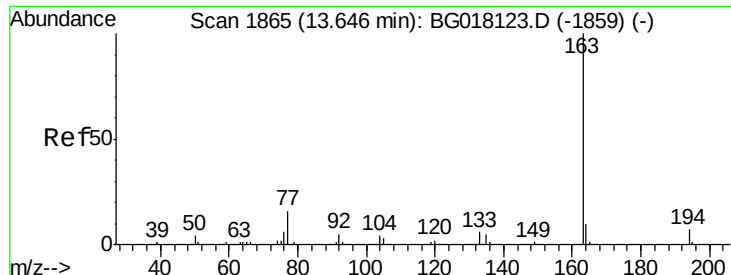

#45

Dimethylphthalate

Concen: 10.29 ng/ul

RT: 13.64 min Scan# 1864

Delta R.T. -0.00 min

Lab File: BG018133.D

Acq: 28 Jul 2015 3:12

Instrument :

BNA_G

ClientSampleId :

C01X2


Tgt Ion:163 Resp: 72665

Ion Ratio Lower Upper

163 100

194 7.3 5.4 8.2

164 10.3 8.7 13.1

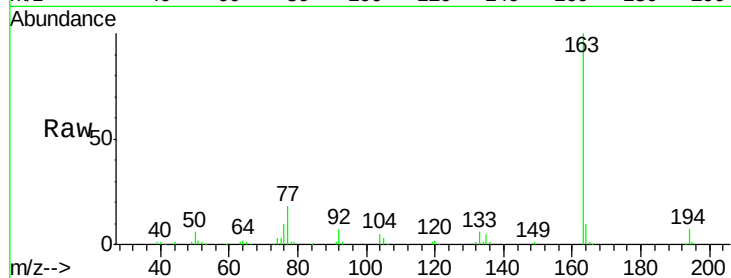

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

