

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG072715\
 Data File : BG018137.D
 Acq On : 28 Jul 2015 5:32
 Operator : TP/UM
 Sample : G3030-07
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C01M9

Quant Time: Jul 28 06:51:32 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG072315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 28 02:39:42 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.51	152	34637	20.00	ng/ul	0.00
18) Naphthalene-d8	10.29	136	156910	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.18	164	100622	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.93	188	220791	20.00	ng/ul	0.00
78) Chrysene-d12	21.14	240	225842	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	232785	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.01	96	1571	2.83	ng/uL	0.00
5) Phenol-d5	6.69	99	38187	14.29	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.85	67	19348	14.67	ng/ul	0.00
9) 2-Chlorophenol-d4	7.04	132	37899	15.99	ng/ul	0.00
13) 4-Methylphenol-d8	8.23	113	31543	13.31	ng/ul	0.00
19) Nitrobenzene-d5	8.66	128	19693	15.88	ng/ul	0.00
22) 2-Nitrophenol-d4	9.38	143	19422	14.83	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.92	165	35603	15.62	ng/ul	0.00
29) 4-Chloroaniline-d4	10.43	131	29036	10.95	ng/ul	0.00
44) Dimethylphthalate-d6	13.60	166	115175	16.30	ng/ul	0.00
47) Acenaphthylene-d8	13.87	160	117558	13.54	ng/ul	0.00
52) 4-Nitrophenol-d4	14.40	143	11693	7.87	ng/ul	0.00
58) Fluorene-d10	15.18	176	86807	13.29	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.31	200	6579	4.66	ng/ul	0.00
71) Anthracene-d10	17.03	188	124028	12.97	ng/ul	0.00
79) Pyrene-d10	19.34	212	128565	12.43	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	126409	11.38	ng/ul	0.00

Target Compounds


						Qvalue
45) Dimethylphthalate	13.64	163	64211	9.03	ng/ul	98
70) Phenanthrene	16.97	178	30229	2.72	ng/ul	96
77) Fluoranthene	19.01	202	34835	2.95	ng/ul#	95
80) Pyrene	19.37	202	40979	3.17	ng/ul	96
83) Benzo(a)anthracene	21.13	228	19164	1.60	ng/ul	98
85) Chrysene	21.13	228	19827	1.76	ng/ul	95
88) Benzo(b)fluoranthene	22.68	252	18902	1.48	ng/ul#	91
89) Benzo(k)fluoranthene	22.68	252	18902	1.53	ng/ul#	90
91) Benzo(a)pyrene	23.24	252	14783	1.20	ng/ul#	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG072715\
Data File : BG018137.D
Acq On : 28 Jul 2015 5:32
Operator : TP/UM
Sample : G3030-07
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C01M9

Quant Time: Jul 28 06:51:32 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG072315.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 28 02:39:42 2015
Response via : Initial Calibration

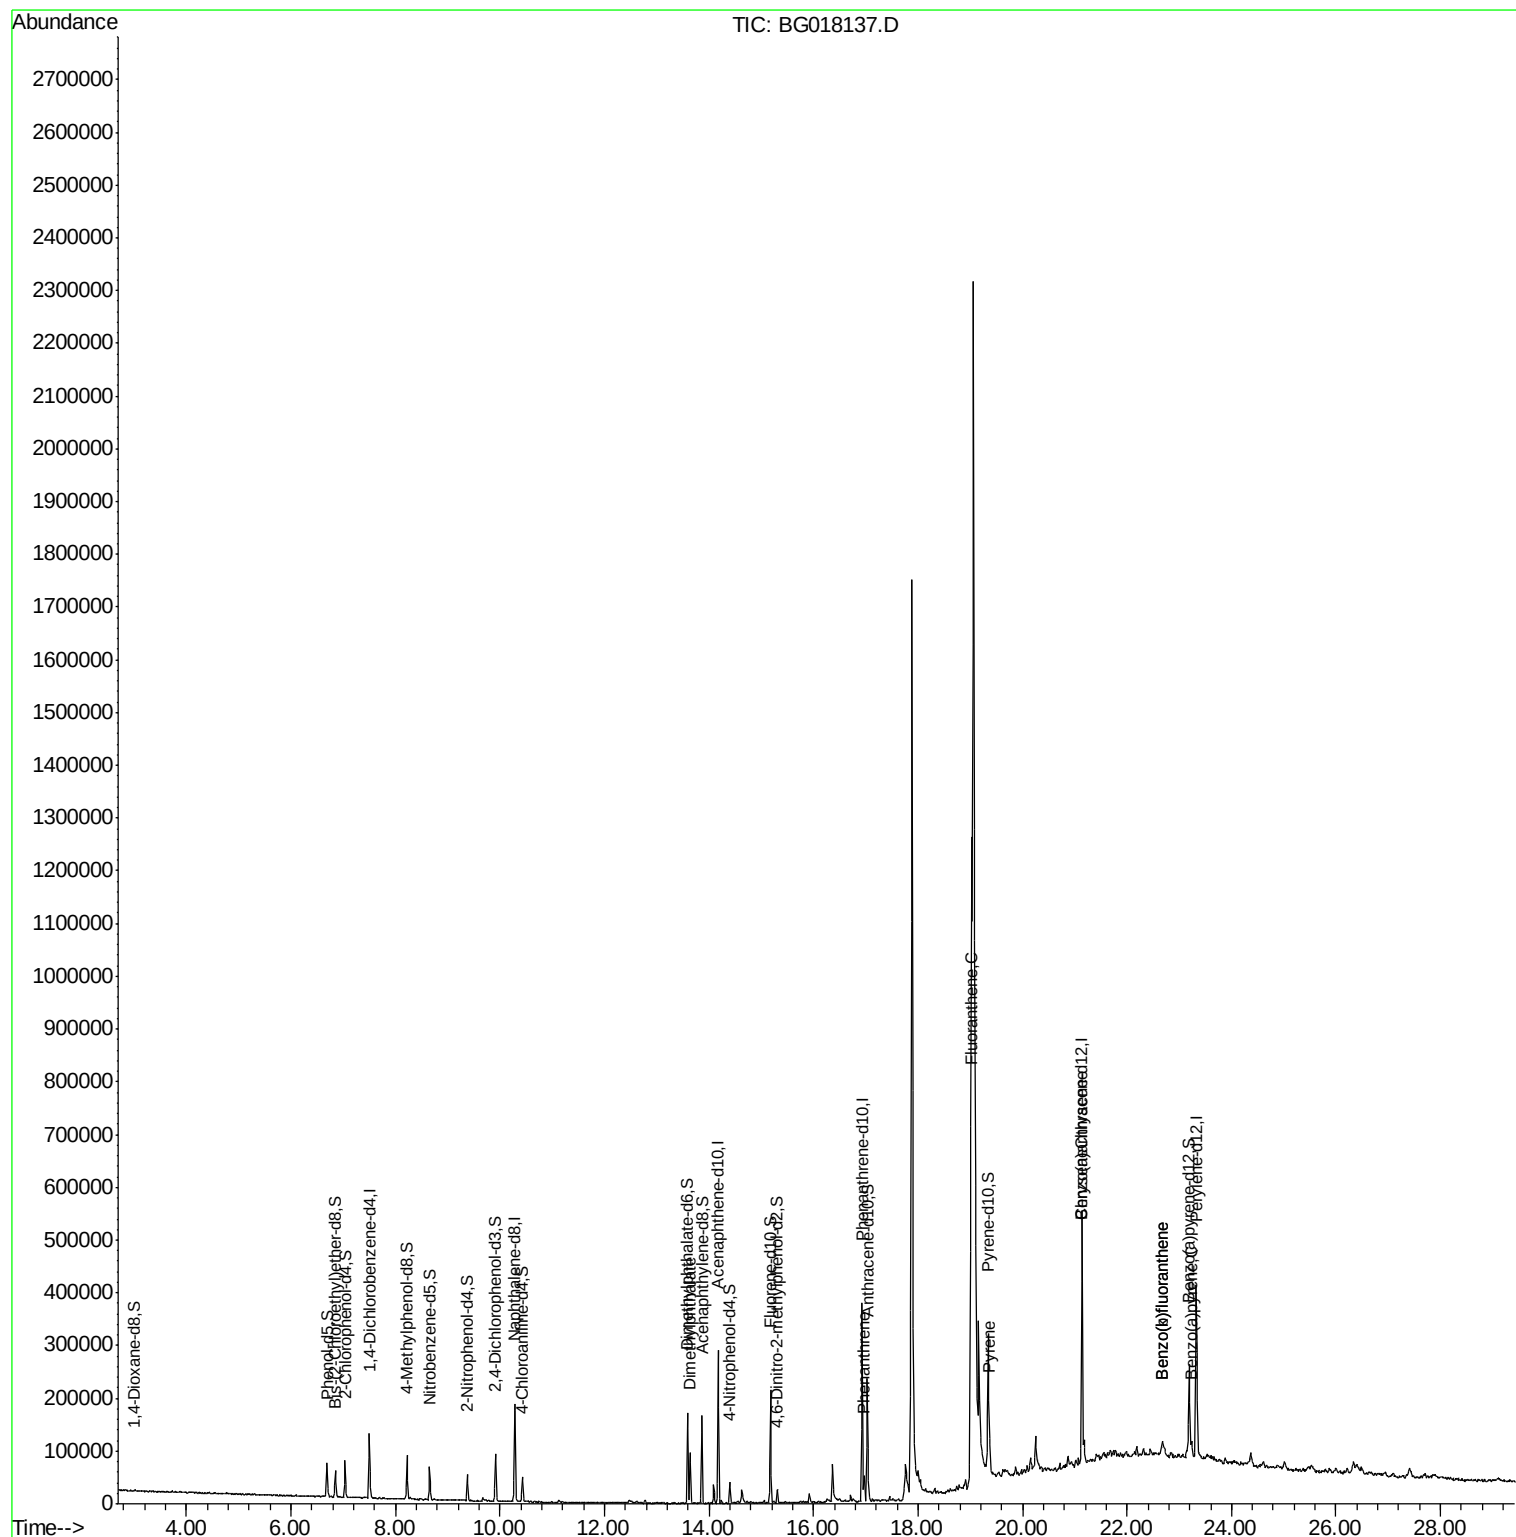

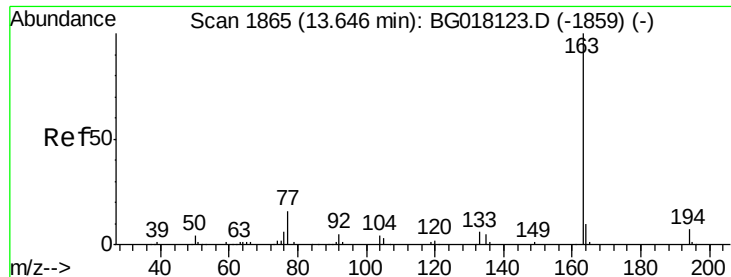

#45

Dimethylphthalate

Concen: 9.03 ng/ul

RT: 13.64 min Scan# 1864

Delta R.T. -0.00 min

Lab File: BG018137.D

Acq: 28 Jul 2015 5:32

Instrument :


BNA_G

ClientSampleId :

C01M9

Tgt Ion:163 Resp: 64211




Ion	Ratio	Lower	Upper
163	100		
194	6.8	5.4	8.2
164	9.8	8.7	13.1

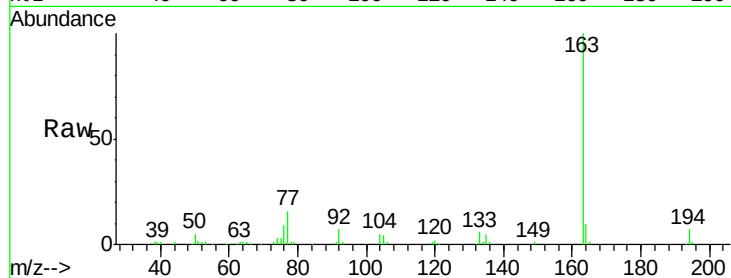

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

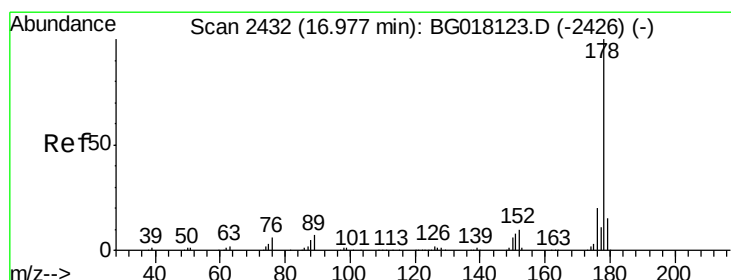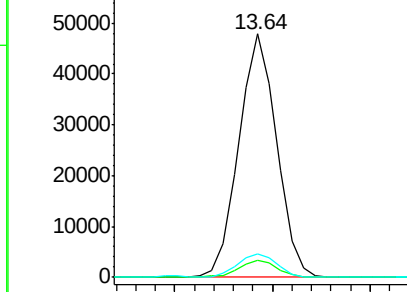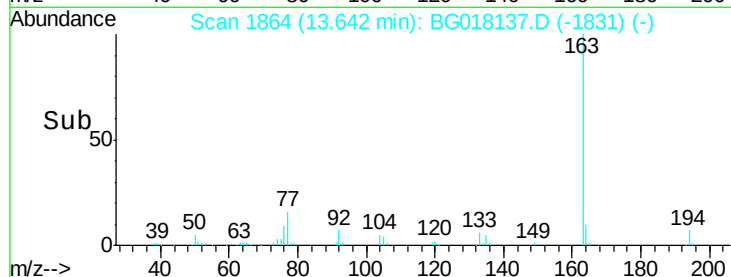

#70

Phenanthrene

Concen: 2.72 ng/ul

RT: 16.97 min Scan# 2431


Delta R.T. -0.00 min

Lab File: BG018137.D

Acq: 28 Jul 2015 5:32

Tgt Ion:178 Resp: 30229



Ion	Ratio	Lower	Upper
178	100		
179	13.8	13.0	19.6
176	18.4	15.8	23.8

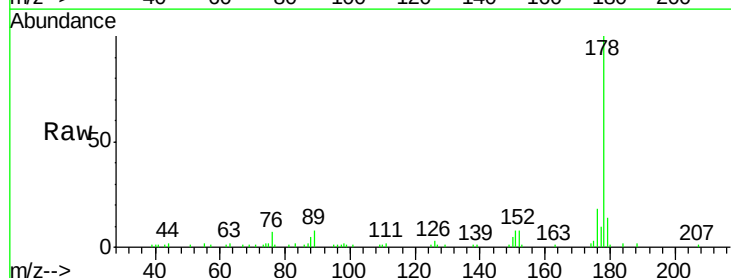


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

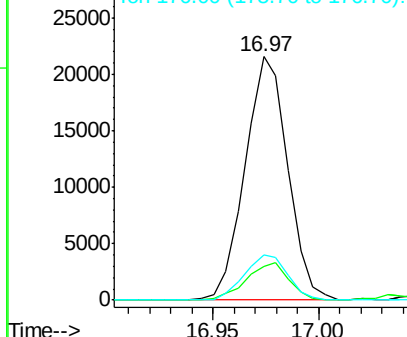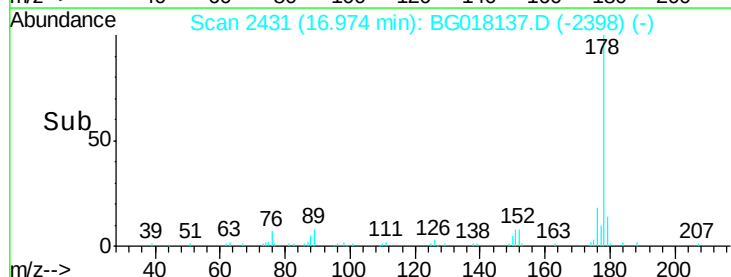

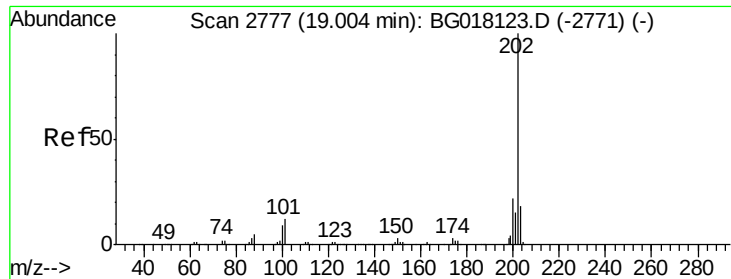

#77

Fluoranthene

Concen: 2.95 ng/ul

RT: 19.01 min Scan# 2777

Delta R.T. 0.00 min

Lab File: BG018137.D

Acq: 28 Jul 2015 5:32

Instrument :

BNA_G

ClientSampled :

C01M9


Tgt Ion:202 Resp: 34835

Ion Ratio Lower Upper

202 100

101 13.7 9.1 13.7#




100 8.1 7.5 11.3

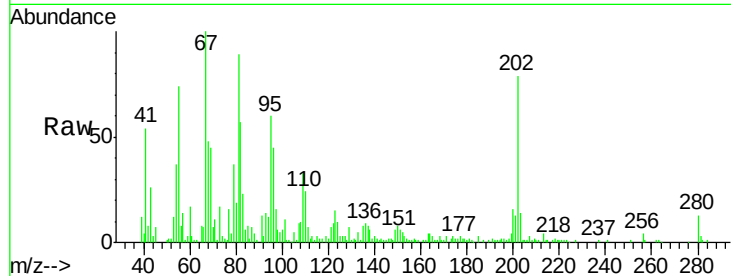

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

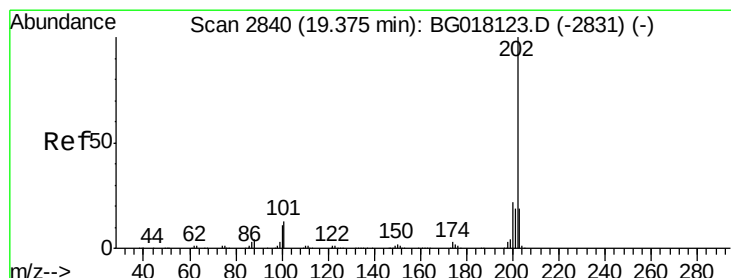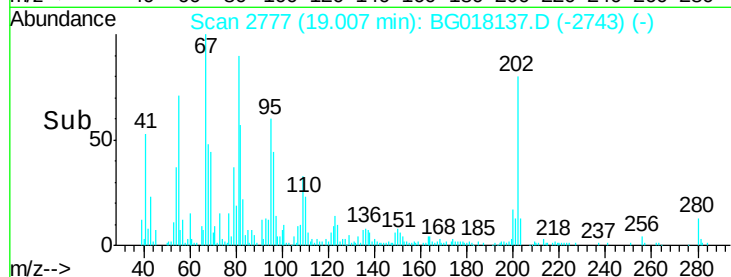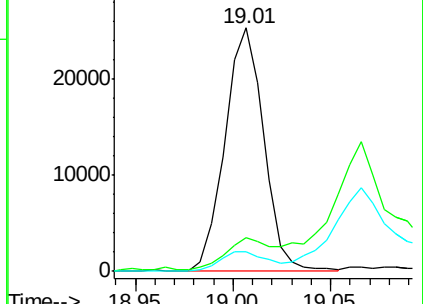

#80

Pyrene

Concen: 3.17 ng/ul

RT: 19.37 min Scan# 2839

Delta R.T. -0.00 min

Lab File: BG018137.D

Acq: 28 Jul 2015 5:32


Tgt Ion:202 Resp: 40979

Ion Ratio Lower Upper

202 100

101 11.6 10.9 16.3



100 9.3 8.5 12.7

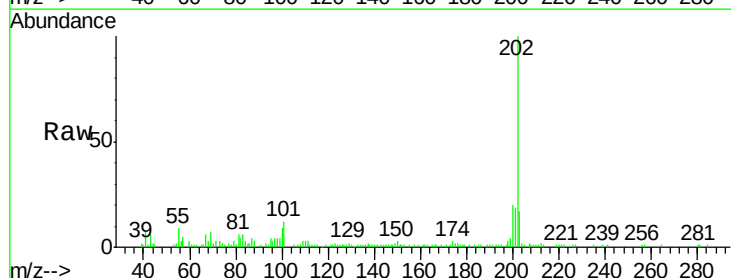


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

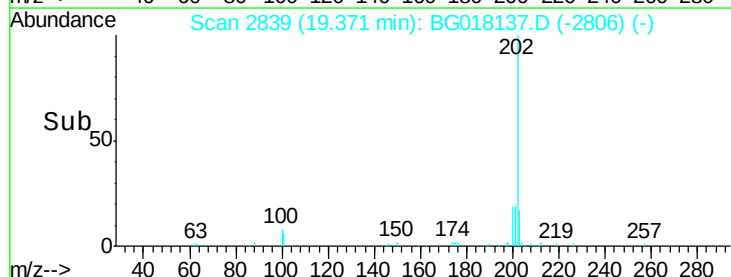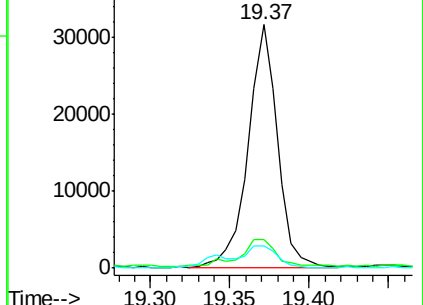

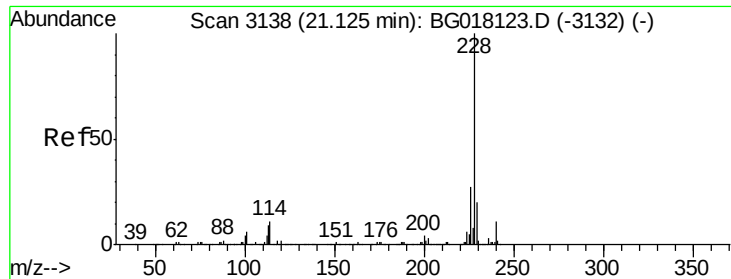

#83

Benzo(a)anthracene

Concen: 1.60 ng/ul

RT: 21.13 min Scan# 3138

Delta R.T. 0.00 min

Lab File: BG018137.D

Acq: 28 Jul 2015 5:32

Instrument :

BNA_G

ClientSampleId :

C01M9


Tgt Ion:228 Resp: 19164

Ion Ratio Lower Upper

228 100

229 21.9 16.6 24.8




226 25.8 21.1 31.7

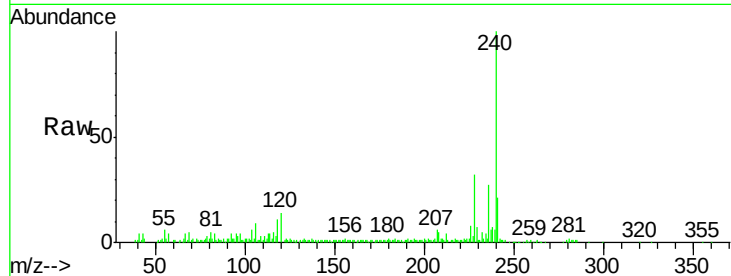

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

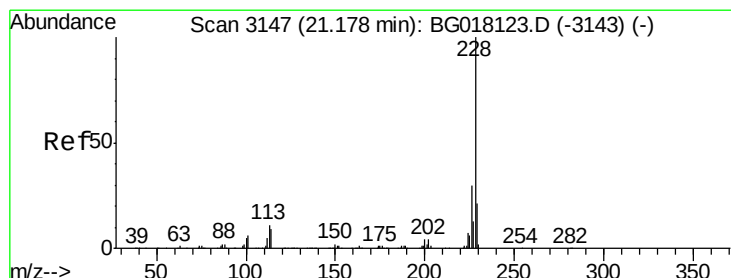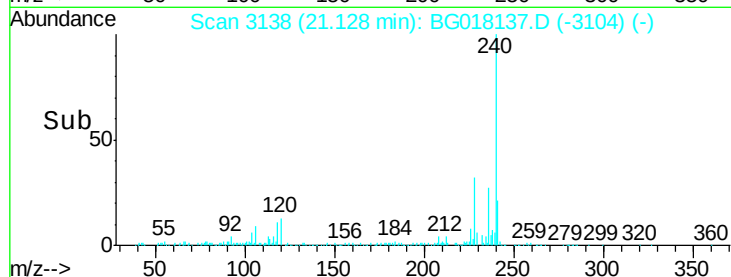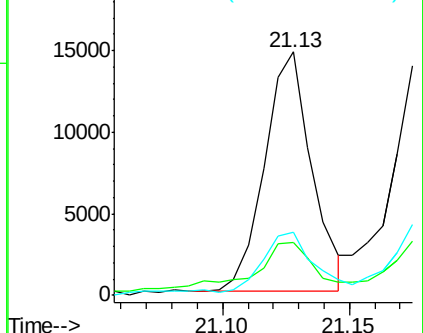

#85

Chrysene

Concen: 1.76 ng/ul

RT: 21.13 min Scan# 3138

Delta R.T. -0.05 min

Lab File: BG018137.D

Acq: 28 Jul 2015 5:32


Tgt Ion:228 Resp: 19827

Ion Ratio Lower Upper

228 100

226 25.8 22.9 34.3



229 21.9 15.6 23.4

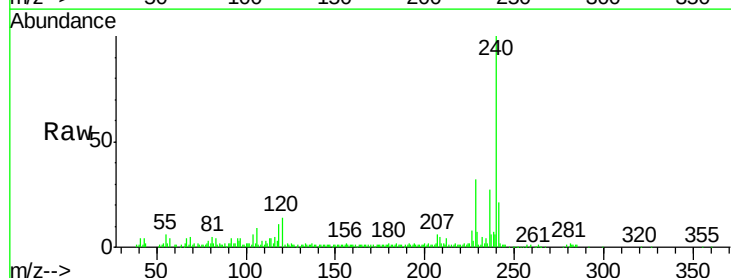


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

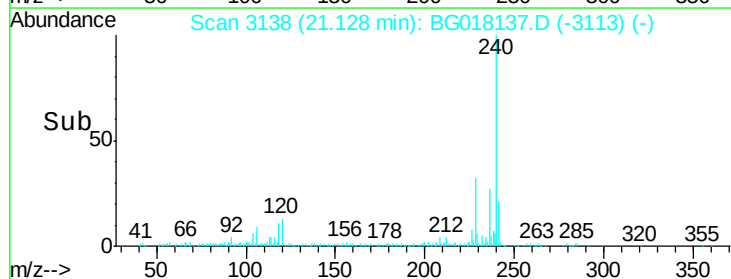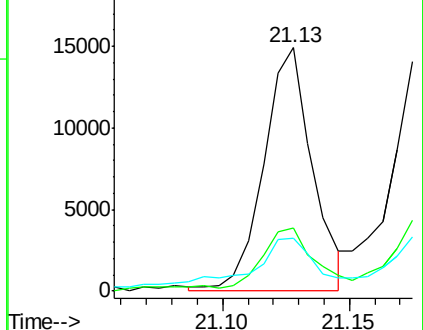

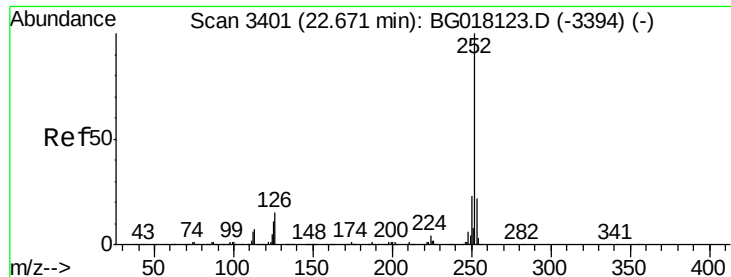

#88

Benzo(b)fluoranthene

Concen: 1.48 ng/ul

RT: 22.68 min Scan# 3402

Delta R.T. 0.01 min

Lab File: BG018137.D

Acq: 28 Jul 2015 5:32

Instrument :

BNA_G

ClientSampleId :

C01M9





Tgt Ion:252 Resp: 18902

Ion Ratio Lower Upper

252 100

253 26.1 18.5 27.7

125 16.9 9.1 13.7#

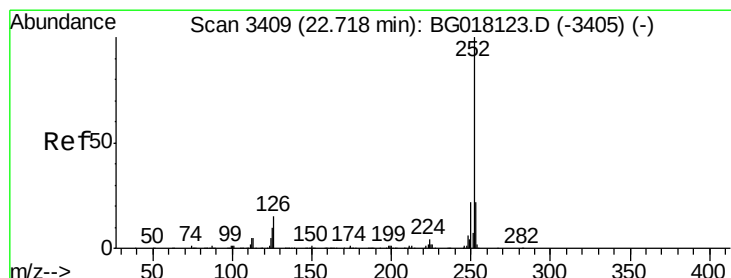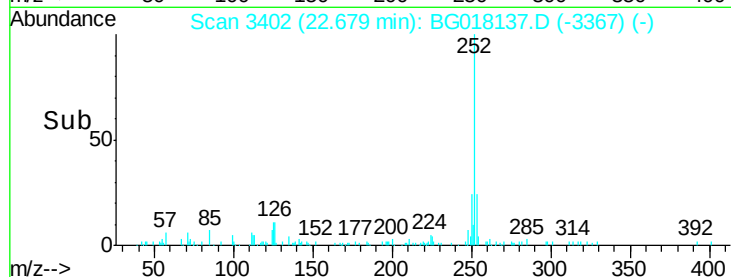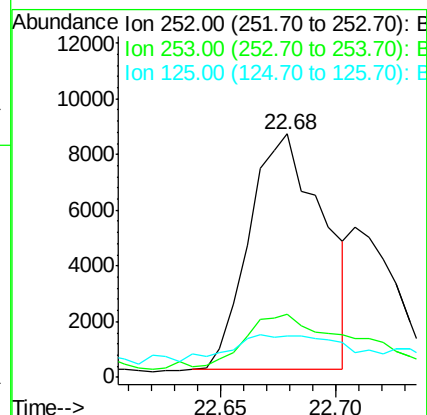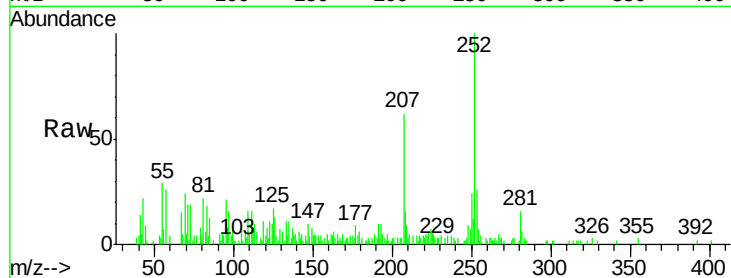

#89

Benzo(k)fluoranthene

Concen: 1.53 ng/ul

RT: 22.68 min Scan# 3402

Delta R.T. -0.04 min

Lab File: BG018137.D

Acq: 28 Jul 2015 5:32




Tgt Ion:252 Resp: 18902


Ion Ratio Lower Upper

252 100

253 26.1 17.8 26.8

125 16.9 9.3 13.9#

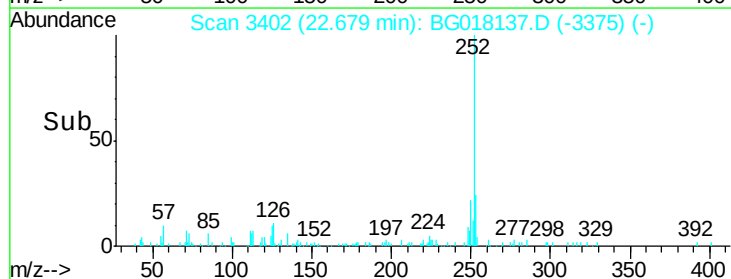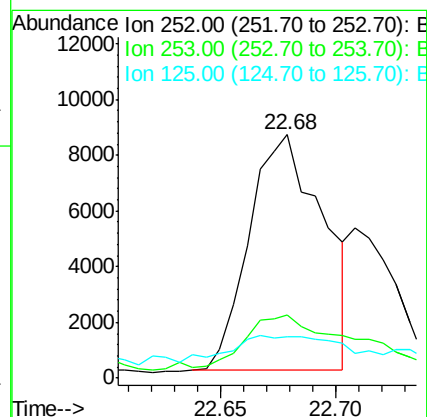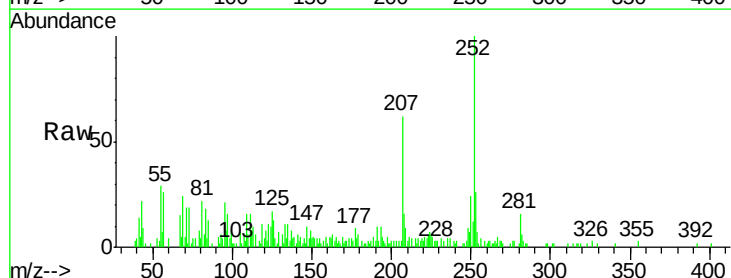

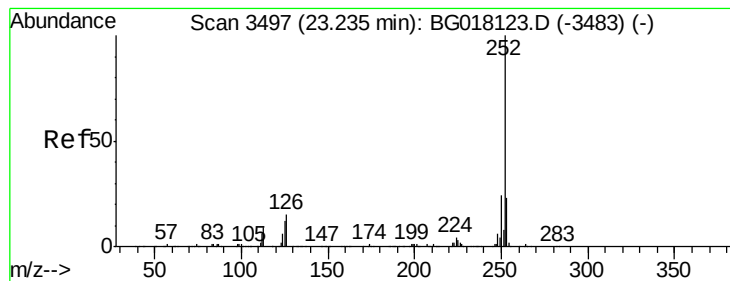

#91

Benzo(a)pyrene

Concen: 1.20 ng/ul

RT: 23.24 min Scan# 3497

Delta R.T. 0.00 min

Lab File: BG018137.D

Acq: 28 Jul 2015 5:32

Instrument :

BNA_G

ClientSampleId :

C01M9


Tgt Ion:252 Resp: 14783

Ion Ratio Lower Upper

252 100

253 24.2 18.0 27.0

125 19.5 10.2 15.2#

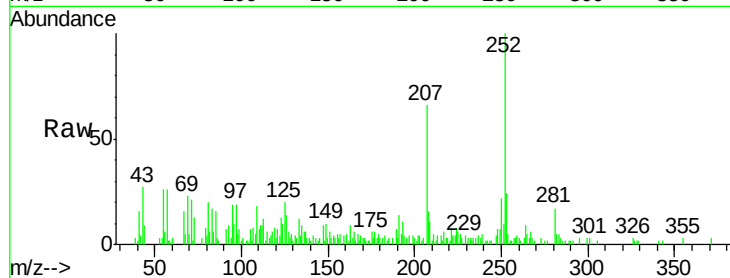

Abundance

Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

