

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG072715\
 Data File : BG018163.D
 Acq On : 29 Jul 2015 1:03
 Operator : TP/UM
 Sample : G3035-13DL 5X
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C02J6DL

Quant Time: Jul 29 02:07:23 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG072315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 29 01:59:28 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.51	152	38075	20.00	ng/ul	0.00
18) Naphthalene-d8	10.30	136	173189	20.00	ng/ul	0.01
36) Acenaphthene-d10	14.19	164	111073	20.00	ng/ul	0.01
62) Phenanthrene-d10	16.94	188	218045	20.00	ng/ul	0.01
78) Chrysene-d12	21.16	240	225507	20.00	ng/ul	0.01
86) Perylene-d12	23.35	264	240392	20.00	ng/ul	0.02

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.02	96	373	0.61	ng/uL	0.01
5) Phenol-d5	6.71	99	11323	3.86	ng/ul	0.02
7) Bis-(2-Chloroethyl)ether-d	6.86	67	5999	4.14	ng/ul	0.00
9) 2-Chlorophenol-d4	7.05	132	11020	4.23	ng/ul	0.01
13) 4-Methylphenol-d8	8.24	113	10109	3.88	ng/ul	0.01
19) Nitrobenzene-d5	8.67	128	6228	4.55	ng/ul	0.00
22) 2-Nitrophenol-d4	9.39	143	6371	4.41	ng/ul	0.01
26) 2,4-Dichlorophenol-d3	9.93	165	12156	4.83	ng/ul	0.02
29) 4-Chloroaniline-d4	10.45	131	10900	3.72	ng/ul	0.01
44) Dimethylphthalate-d6	13.60	166	34164	4.38	ng/ul	0.00
47) Acenaphthylene-d8	13.88	160	45330	4.73	ng/ul	0.01
52) 4-Nitrophenol-d4	14.42	143	4535	2.76	ng/ul	0.02
58) Fluorene-d10	15.19	176	32603	4.52	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	0.00	200	0	0.00	ng/ul	
71) Anthracene-d10	17.04	188	44800	4.74	ng/ul	0.01
79) Pyrene-d10	19.35	212	45300	4.39	ng/ul	0.01
90) Benzo(a)pyrene-d12	23.21	264	44795	3.90	ng/ul	0.01

Target Compounds

						Qvalue
14) Acetophenone	8.34	105	3782	1.03	ng/ul	95
28) Naphthalene	10.35	128	10952	1.35	ng/ul	97
34) 2-Methylnaphthalene	11.97	142	8894	1.45	ng/ul	87
35) 1-Methylnaphthalene	12.20	142	6972	1.17	ng/ul#	93
45) Dimethylphthalate	13.65	163	10185	1.30	ng/ul	97
50) Acenaphthene	14.25	153	29837	4.53	ng/ul	95
54) Dibenzofuran	14.59	168	28346	3.03	ng/ul	95
59) Fluorene	15.25	166	33428	4.15	ng/ul	95
70) Phenanthrene	16.99	178	412969	37.69	ng/ul	99
72) Anthracene	17.08	178	103999	9.35	ng/ul	99
75) Carbazole	17.36	167	37545	3.90	ng/ul	99
77) Fluoranthene	19.02	202	444975	38.13	ng/ul#	95
80) Pyrene	19.39	202	487638	37.76	ng/ul	94
83) Benzo(a)anthracene	21.14	228	243487	20.41	ng/ul	99
85) Chrysene	21.19	228	221775	19.75	ng/ul	96
88) Benzo(b)fluoranthene	22.70	252	243964	18.52	ng/ul	99
89) Benzo(k)fluoranthene	22.70	252	243964	19.14	ng/ul	99
91) Benzo(a)pyrene	23.25	252	194364	15.24	ng/ul	97
92) Indeno(1,2,3-cd)pyrene	25.57	276	93536	6.36	ng/ul#	93
93) Dibenzo(a,h)anthracene	25.58	278	28912	2.30	ng/ul#	88
94) Benzo(g,h,i)perylene	26.26	276	80836	6.65	ng/ul#	92

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG072715\
Data File : BG018163.D
Acq On : 29 Jul 2015 1:03
Operator : TP/UM
Sample : G3035-13DL 5X
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C02J6DL

Quant Time: Jul 29 02:07:23 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG072315.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 29 01:59:28 2015
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)


(#) = qualifier out of range (m) = manual integration (+) = signals summed						

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG072715\
Data File : BG018163.D
Acq On : 29 Jul 2015 1:03
Operator : TP/UM
Sample : G3035-13DL 5X
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C02J6DL

Quant Time: Jul 29 02:07:23 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG072315.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 29 01:59:28 2015
Response via : Initial Calibration

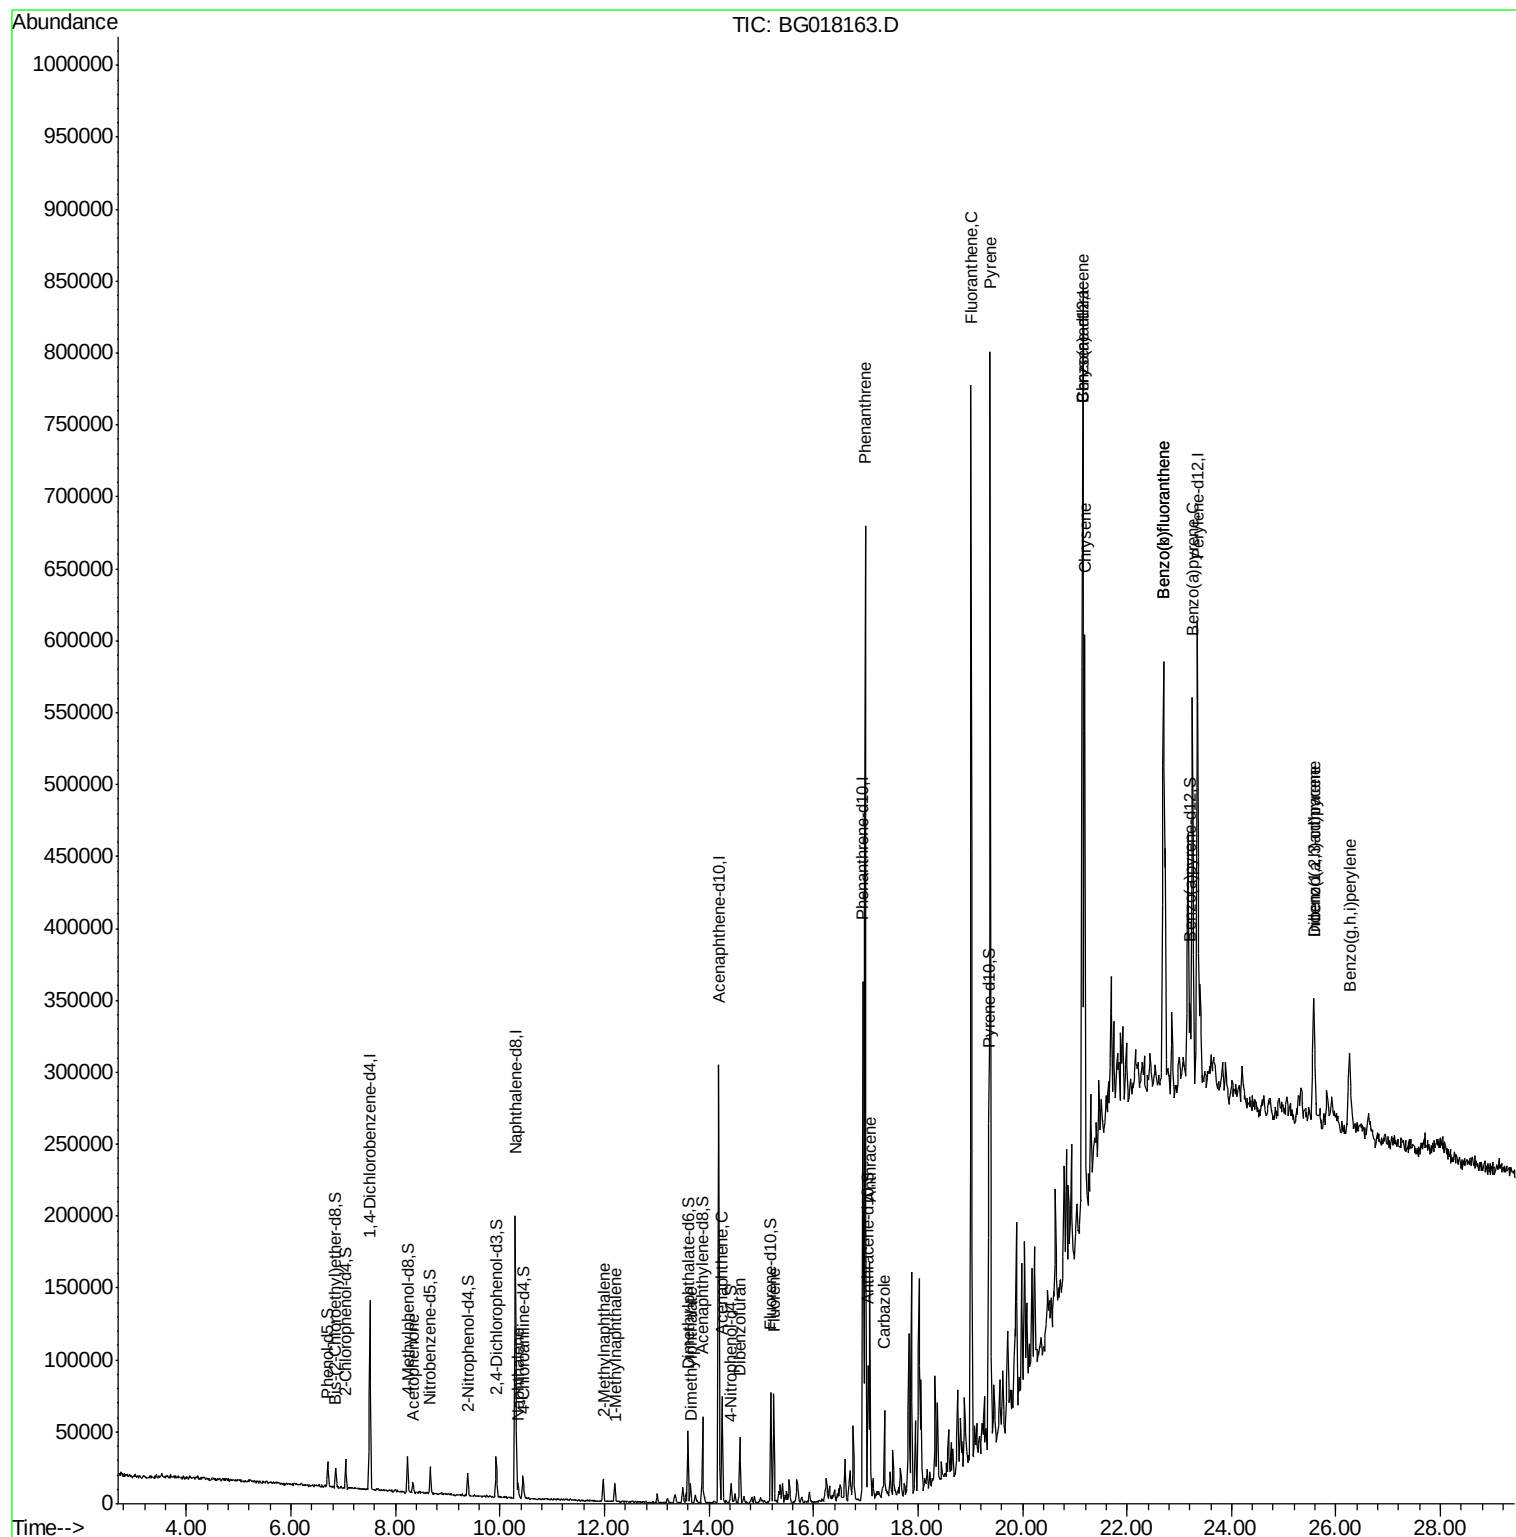

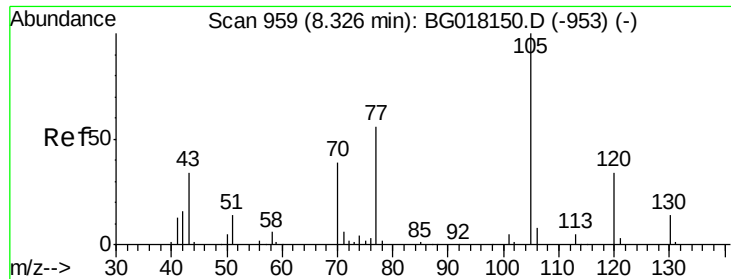

#14

Acetophenone

Concen: 1.03 ng/ul

RT: 8.34 min Scan# 961

Delta R.T. 0.01 min

Lab File: BG018163.D

Acq: 29 Jul 2015 1:03

Instrument :

BNA_G

ClientSampleId :

C02J6DL


Tgt Ion:105 Resp: 3782

Ion Ratio Lower Upper

105 100

77 72.6 61.7 92.5




51 24.6 18.1 27.1

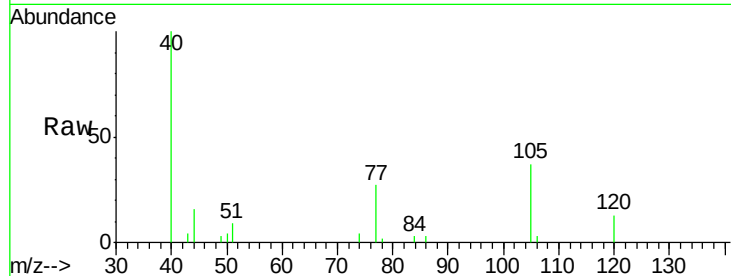

Abundance Ion 105.00 (104.70 to 105.70): E

Ion 77.00 (76.70 to 77.70): BGC

Ion 51.00 (50.70 to 51.70): BGC

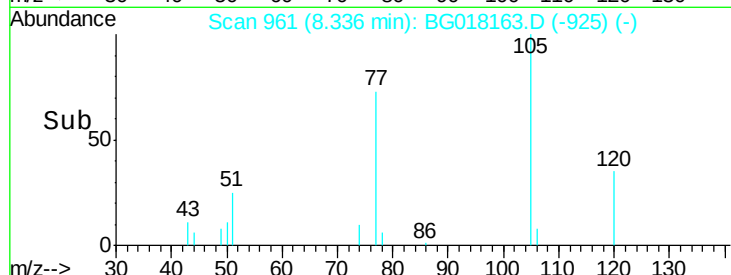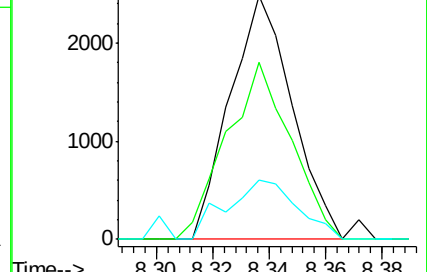

#28

Naphthalene

Concen: 1.35 ng/ul

RT: 10.35 min Scan# 1303

Delta R.T. 0.00 min

Lab File: BG018163.D

Acq: 29 Jul 2015 1:03


Tgt Ion:128 Resp: 10952

Ion Ratio Lower Upper

128 100

129 11.1 9.5 14.3



127 11.2 10.1 15.1




Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

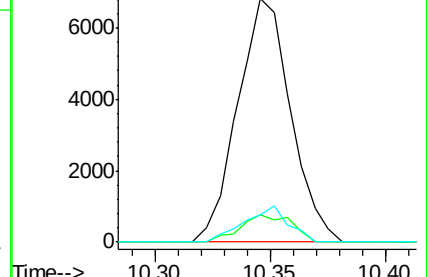

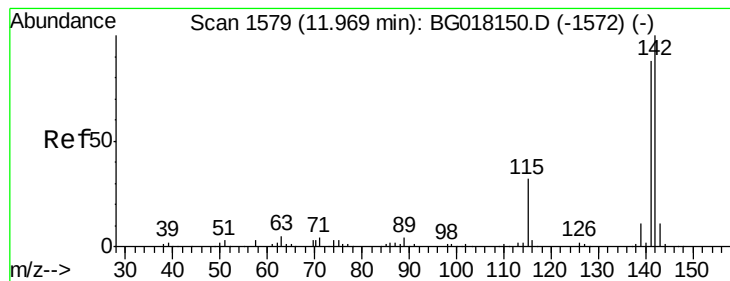

#34

2-Methylnaphthalene

Concen: 1.45 ng/ul

RT: 11.97 min Scan# 1580

Delta R.T. 0.00 min

Lab File: BG018163.D

Acq: 29 Jul 2015 1:03

Instrument :

BNA_G

ClientSampleId :


C02J6DL

Tgt Ion:142 Resp: 8894

Ion Ratio Lower Upper

142 100

141 74.7 69.4 104.0

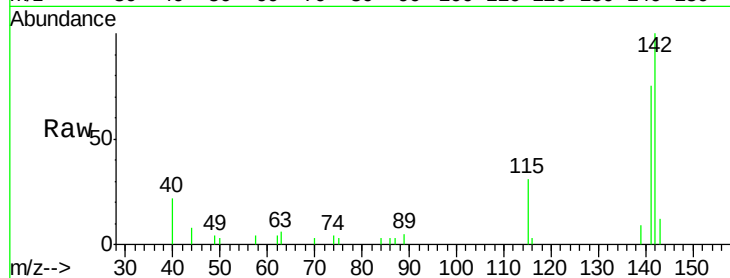

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

11.97

6000

5000

4000



3000

2000

1000

0

Time-->

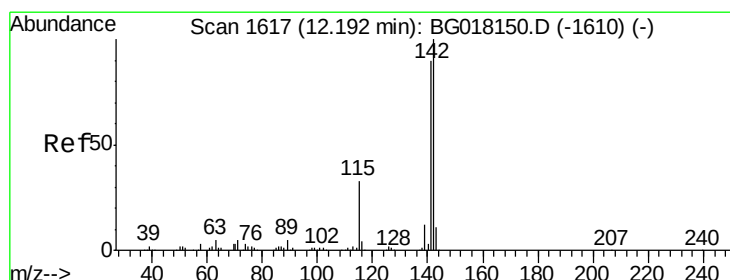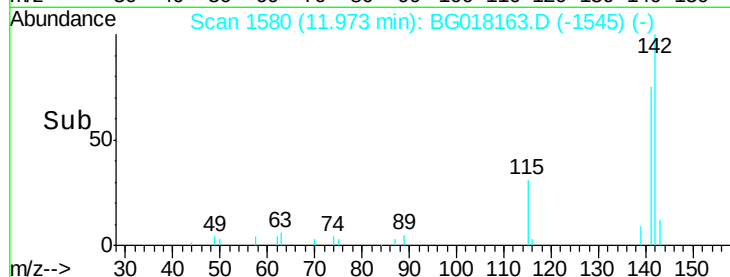

#35

1-Methylnaphthalene

Concen: 1.17 ng/ul

RT: 12.20 min Scan# 1619

Delta R.T. 0.01 min

Lab File: BG018163.D

Acq: 29 Jul 2015 1:03


Tgt Ion:142 Resp: 6972

Ion Ratio Lower Upper

142 100

141 82.9 71.8 107.6

116 0.0 3.2 4.8#

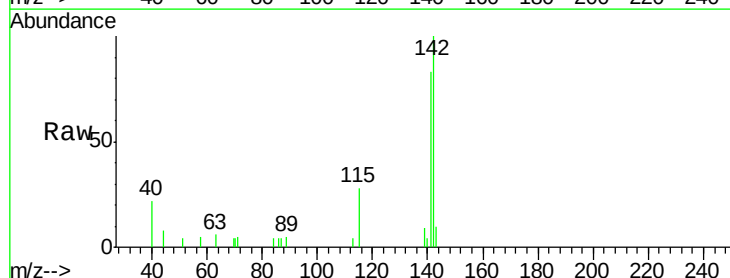

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 116.00 (115.70 to 116.70): E

12.20

6000

5000

4000


3000


2000

1000

0

Time-->

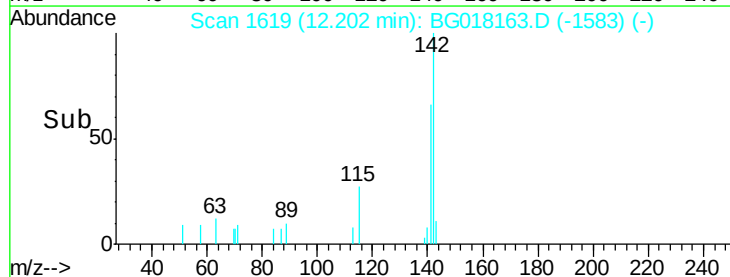

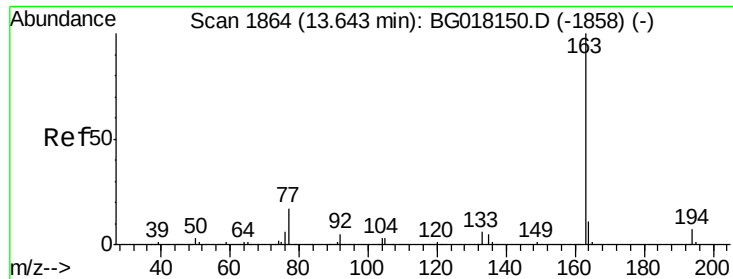

#45

Dimethylphthalate

Concen: 1.30 ng/ul

RT: 13.65 min Scan# 1865

Delta R.T. 0.00 min

Lab File: BG018163.D

Acq: 29 Jul 2015 1:03





Instrument :

BNA_G

ClientSampleId :

C02J6DL

Tgt Ion:	163	Resp:	10185
Ion	Ratio	Lower	Upper
163	100		
194	6.8	5.4	8.2
164	12.9	8.7	13.1

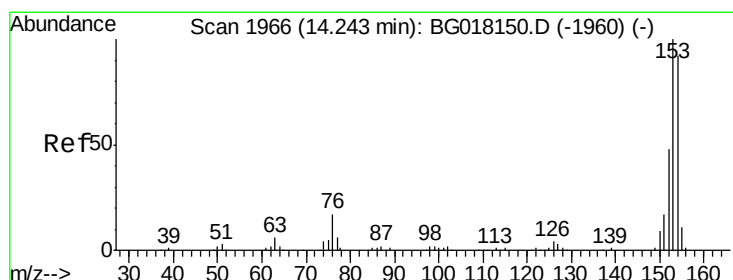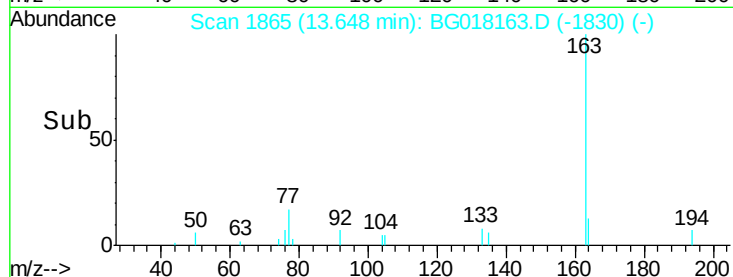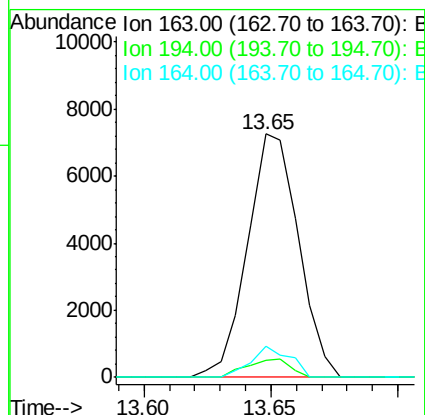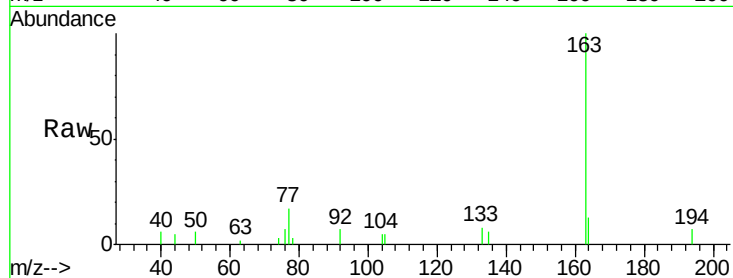

#50

Acenaphthene

Concen: 4.53 ng/ul




RT: 14.25 min Scan# 1968


Delta R.T. 0.01 min

Lab File: BG018163.D

Acq: 29 Jul 2015 1:03

Tgt Ion:	153	Resp:	29837
Ion	Ratio	Lower	Upper
153	100		
152	46.6	38.9	58.3
154	85.2	72.6	108.8

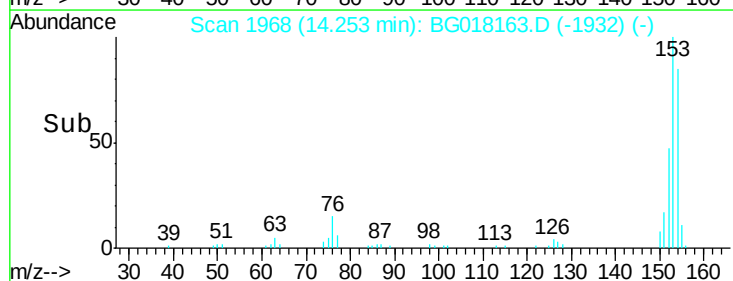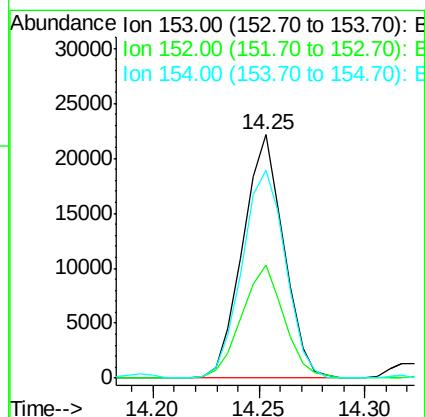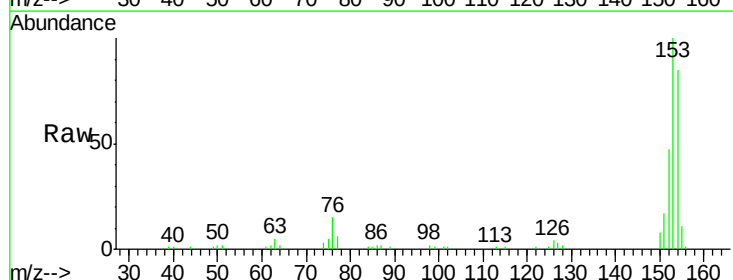

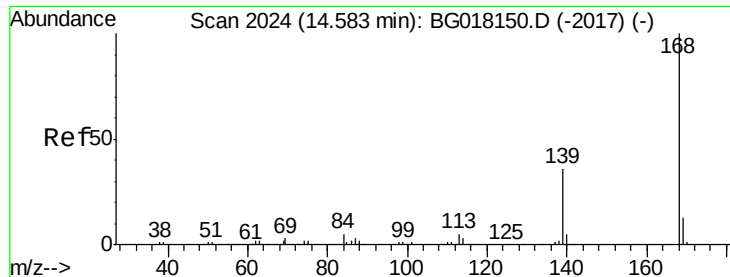

#54

Diben-zofuran

Concen: 3.03 ng/ul

RT: 14.59 min Scan# 2025

Delta R.T. 0.00 min

Lab File: BG018163.D

Acq: 29 Jul 2015 1:03

Instrument :

BNA_G

ClientSampleId :


C02J6DL

Tgt Ion:168 Resp: 28346

Ion Ratio Lower Upper

168 100

139 41.0 30.6 46.0

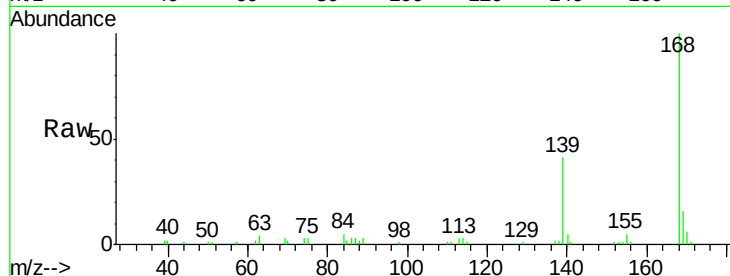

Abundance Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E

14.59

20000



15000

10000

5000

0

Time-->

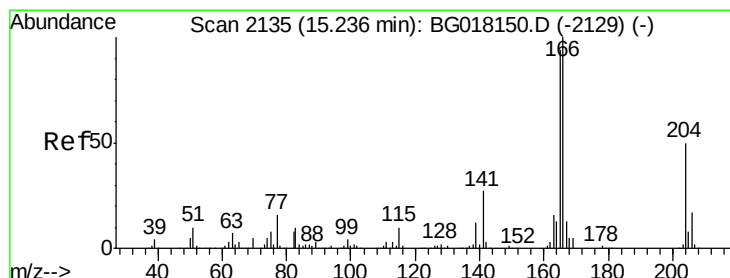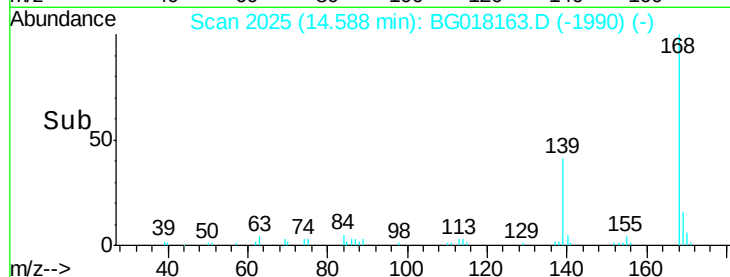

#59

Fluorene

Concen: 4.15 ng/ul

RT: 15.25 min Scan# 2137

Delta R.T. 0.01 min

Lab File: BG018163.D

Acq: 29 Jul 2015 1:03


Tgt Ion:166 Resp: 33428

Ion Ratio Lower Upper

166 100

165 96.6 73.6 110.4

167 14.8 10.8 16.2

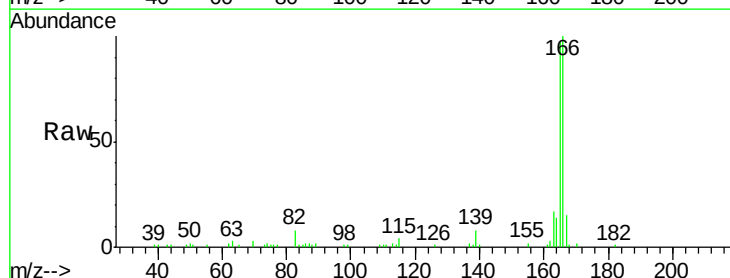

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

15.25

30000

25000

20000


15000


10000

5000

0

Time-->




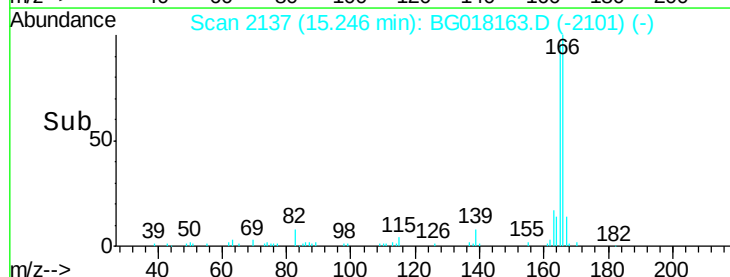


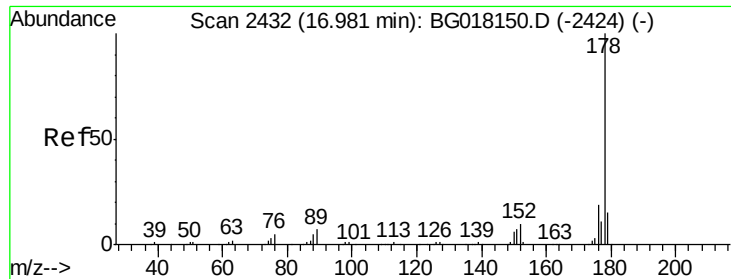

#70
Phenanthrene
Concen: 37.69 ng/ul
RT: 16.99 min Scan# 2434
Delta R.T. 0.01 min
Lab File: BG018163.D
Acq: 29 Jul 2015 1:03




Instrument :
BNA_G
ClientSampleId :
C02J6DL


Tgt Ion:178 Resp: 412969
Ion Ratio Lower Upper
178 100
179 16.0 13.0 19.6
176 19.3 15.8 23.8

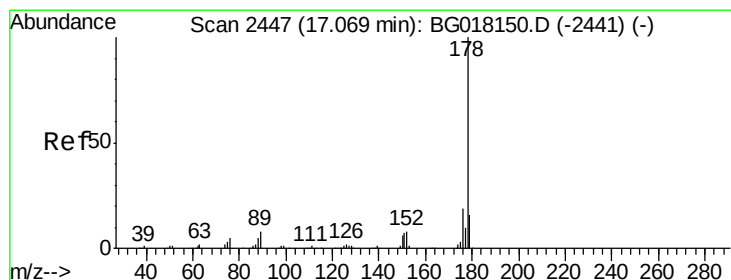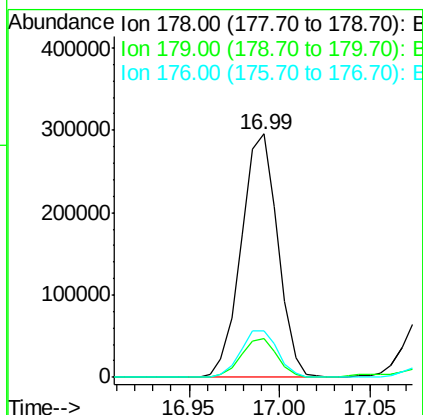

#72
Anthracene
Concen: 9.35 ng/ul
RT: 17.08 min Scan# 2449
Delta R.T. 0.01 min
Lab File: BG018163.D
Acq: 29 Jul 2015 1:03

Tgt Ion:178 Resp: 103999
Ion Ratio Lower Upper
178 100
179 15.1 12.4 18.6
176 20.0 15.8 23.8

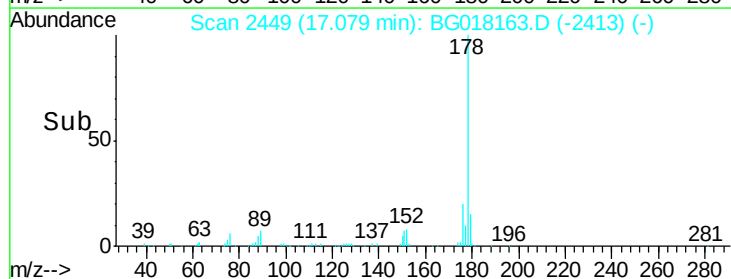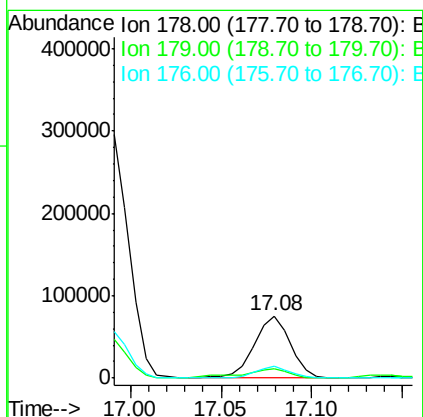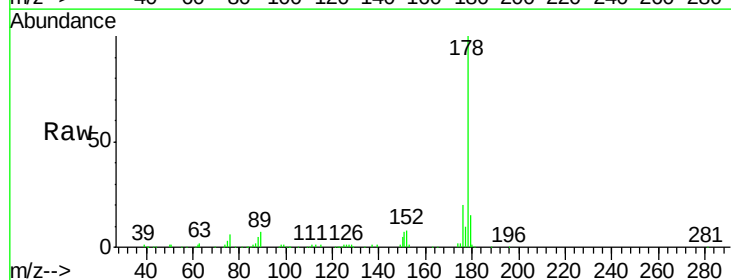


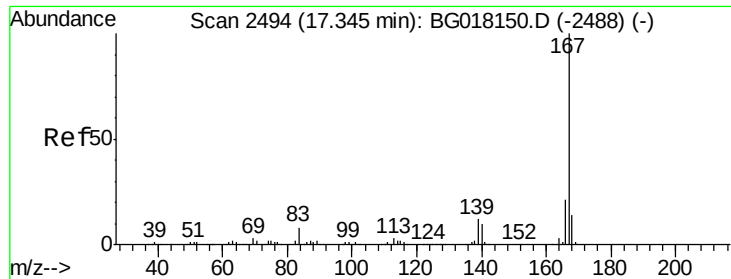




#75
 Carbazole
 Concen: 3.90 ng/ul
 RT: 17.36 min Scan# 2496
 Delta R.T. 0.01 min
 Lab File: BG018163.D
 Acq: 29 Jul 2015 1:03

Instrument :
 BNA_G
 ClientSampleId :
 C02J6DL

Tgt Ion:167 Resp: 37545
 Ion Ratio Lower Upper
 167 100
 166 21.4 17.4 26.2
 139 13.6 10.6 15.8

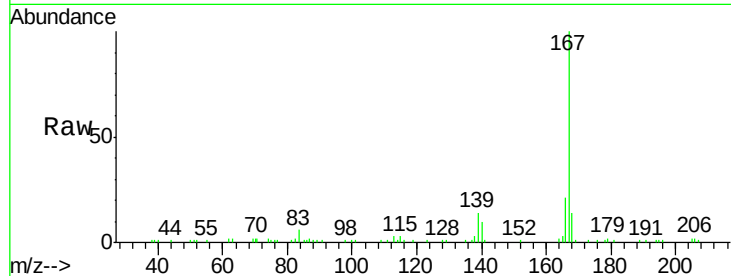


Abundance Ion 167.00 (166.70 to 167.70): E
 Ion 166.00 (165.70 to 166.70): E
 Ion 139.00 (138.70 to 139.70): E

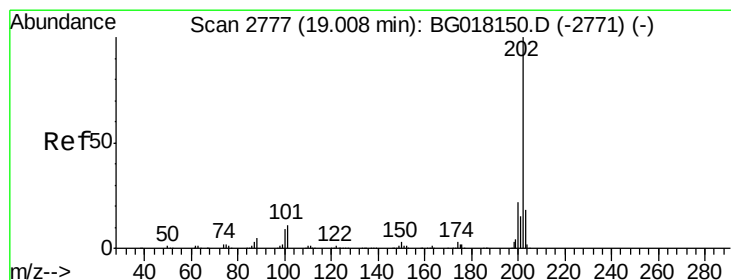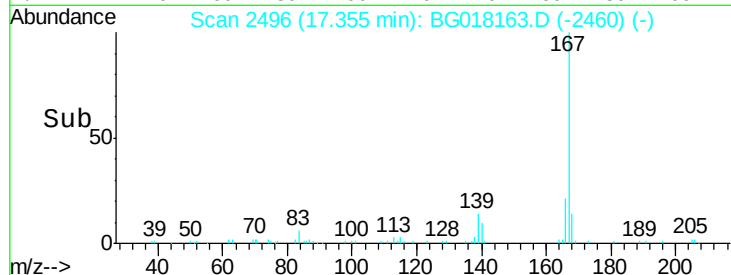
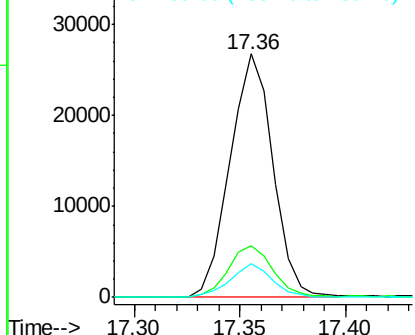



#77
 Fluoranthene
 Concen: 38.13 ng/ul
 RT: 19.02 min Scan# 2780
 Delta R.T. 0.02 min
 Lab File: BG018163.D
 Acq: 29 Jul 2015 1:03

Tgt Ion:202 Resp: 444975
 Ion Ratio Lower Upper
 202 100
 101 9.7 9.1 13.7
 100 7.0 7.5 11.3#



Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 100.00 (99.70 to 100.70): B

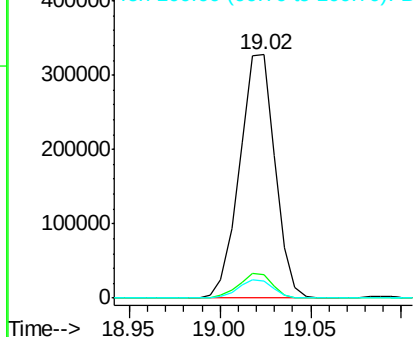



#80

Pyrene

Concen: 37.76 ng/ul

RT: 19.39 min Scan# 2842

Delta R.T. 0.02 min

Lab File: BG018163.D

Acq: 29 Jul 2015 1:03

Instrument :

BNA_G

ClientSampleId :

C02J6DL


Tgt Ion:202 Resp: 487638

Ion Ratio Lower Upper

202 100

101 11.0 10.9 16.3




100 8.8 8.5 12.7

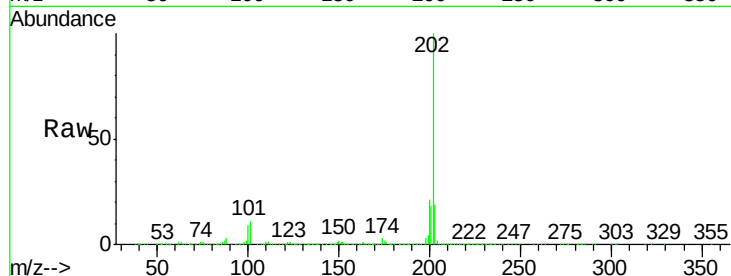

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

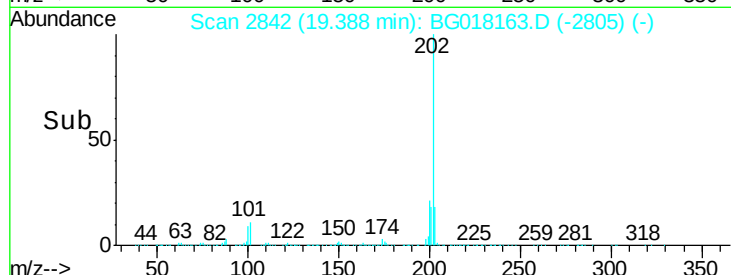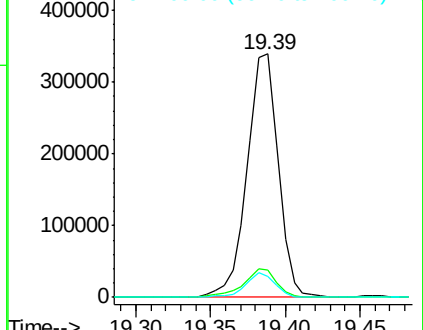

#83

Benzo(a)anthracene

Concen: 20.41 ng/ul

RT: 21.14 min Scan# 3140

Delta R.T. 0.01 min

Lab File: BG018163.D

Acq: 29 Jul 2015 1:03


Tgt Ion:228 Resp: 243487

Ion Ratio Lower Upper

228 100

229 21.6 16.6 24.8



226 27.0 21.1 31.7




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

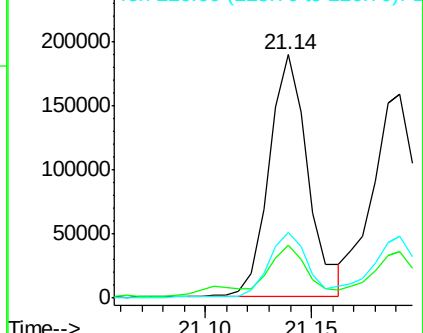

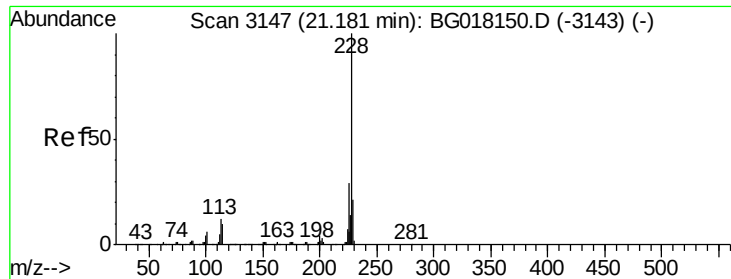

#85

Chrysene

Concen: 19.75 ng/ul

RT: 21.19 min Scan# 3149

Delta R.T. 0.01 min

Lab File: BG018163.D

Acq: 29 Jul 2015 1:03

Instrument :

BNA_G

ClientSampleId :

C02J6DL


Tgt Ion:228 Resp: 221775

Ion Ratio Lower Upper

228 100

226 30.0 22.9 34.3




229 22.5 15.6 23.4



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

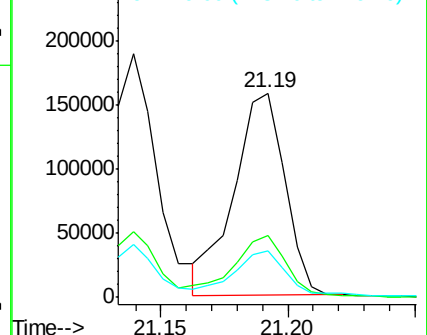

#88

Benzo(b)fluoranthene

Concen: 18.52 ng/ul

RT: 22.70 min Scan# 3405

Delta R.T. 0.02 min

Lab File: BG018163.D

Acq: 29 Jul 2015 1:03


Tgt Ion:252 Resp: 243964

Ion Ratio Lower Upper

252 100

253 22.7 18.5 27.7



125 11.1 9.1 13.7




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

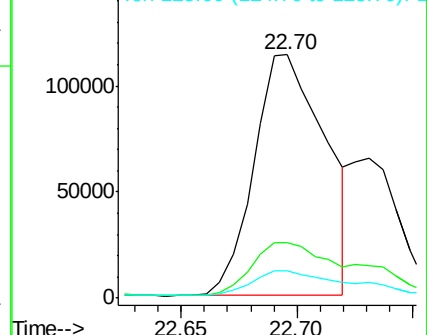



#89

Benzo(k)fluoranthene

Concen: 19.14 ng/ul

RT: 22.70 min Scan# 3405

Delta R.T. -0.02 min

Lab File: BG018163.D

Acq: 29 Jul 2015 1:03

Instrument :

BNA_G

ClientSampleId :

C02J6DL


Tgt Ion:252 Resp: 243964

Ion Ratio Lower Upper

252 100

253 22.7 17.8 26.8




125 11.1 9.3 13.9



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

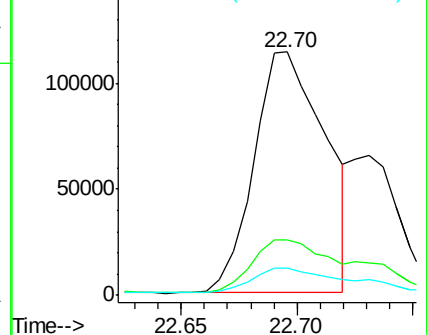

#91

Benzo(a)pyrene

Concen: 15.24 ng/ul

RT: 23.25 min Scan# 3500

Delta R.T. 0.02 min

Lab File: BG018163.D

Acq: 29 Jul 2015 1:03


Tgt Ion:252 Resp: 194364

Ion Ratio Lower Upper

252 100

253 23.7 18.0 27.0



125 11.1 10.2 15.2




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

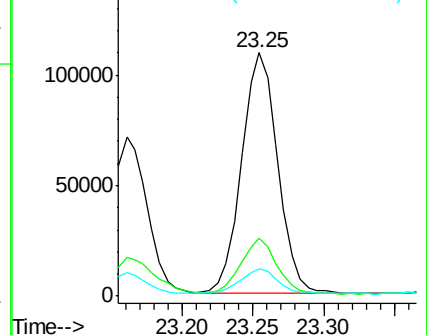

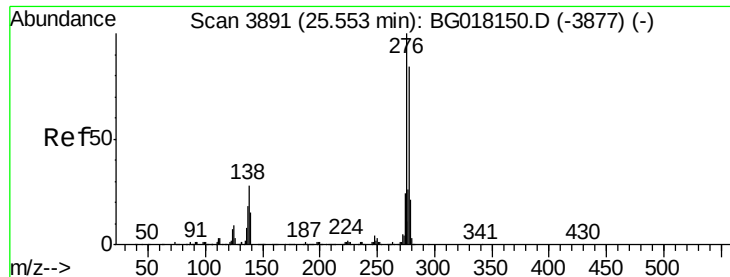

#92

Indeno(1,2,3-cd)pyrene

Concen: 6.36 ng/ul

RT: 25.57 min Scan# 3894

Delta R.T. 0.02 min

Lab File: BG018163.D

Acq: 29 Jul 2015 1:03

Instrument :

BNA_G

ClientSampleId :

C02J6DL


Tgt Ion:276 Resp: 93536

Ion Ratio Lower Upper

276 100

138 22.2 22.6 33.8#




277 25.6 19.8 29.8

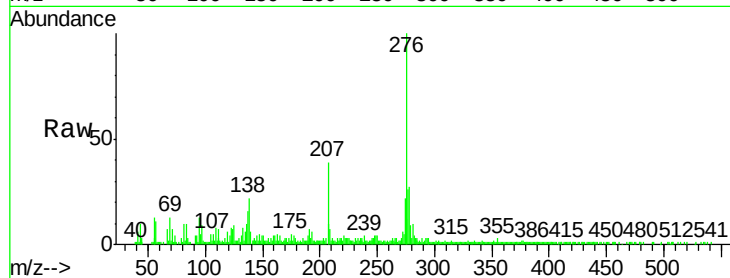

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

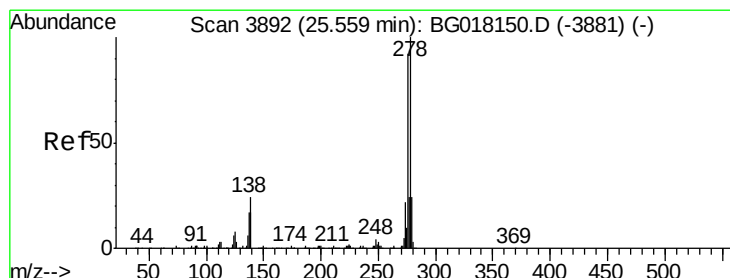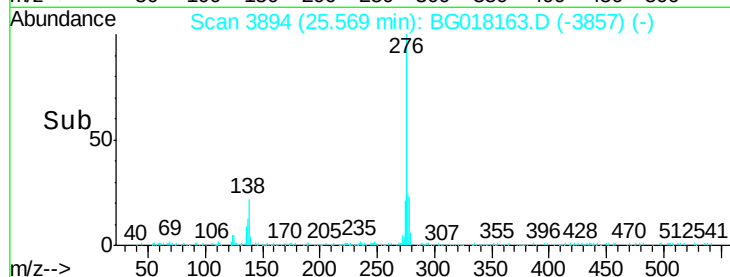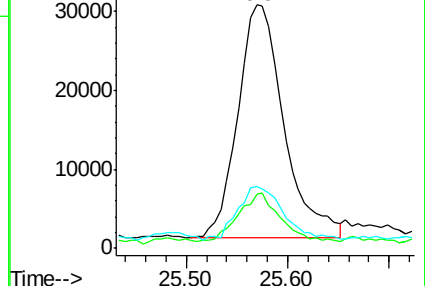

#93

Dibenzo(a,h)anthracene

Concen: 2.30 ng/ul

RT: 25.58 min Scan# 3895

Delta R.T. 0.02 min

Lab File: BG018163.D

Acq: 29 Jul 2015 1:03


Tgt Ion:278 Resp: 28912

Ion Ratio Lower Upper

278 100

139 21.5 13.7 20.5#



279 29.3 18.1 27.1#

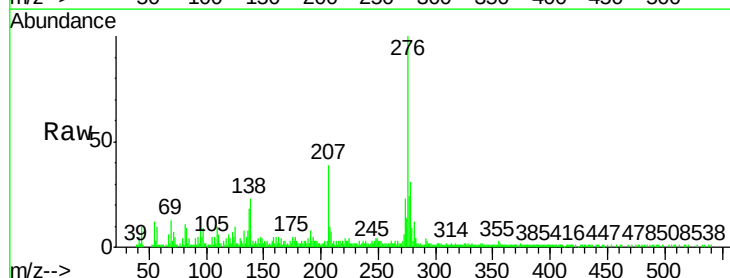


Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

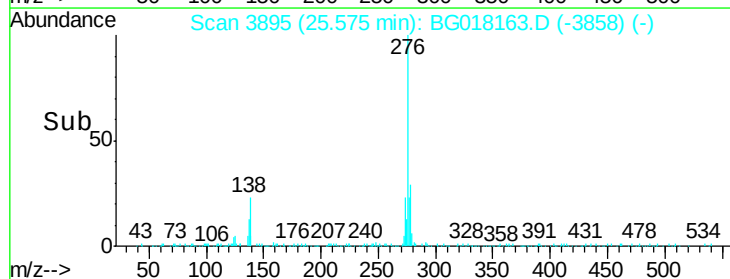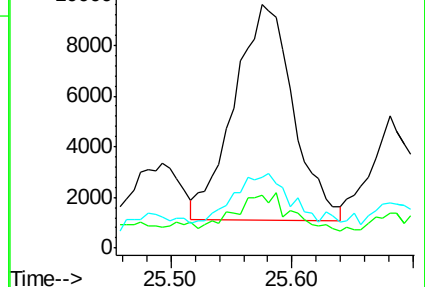

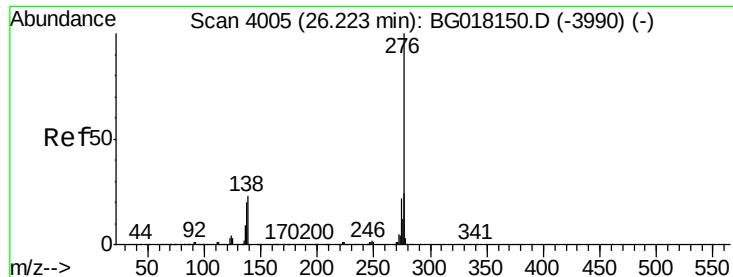

#94

Benzo(g,h,i)perylene

Concen: 6.65 ng/ul

RT: 26.26 min Scan# 4011

Delta R.T. 0.03 min

Lab File: BG018163.D

Acq: 29 Jul 2015 1:03

Instrument :

BNA_G

ClientSampleId :

C02J6DL


Tgt Ion: 276 Resp: 80836

Ion Ratio Lower Upper

276 100

138 18.3 18.8 28.2#

277 26.9 19.3 28.9

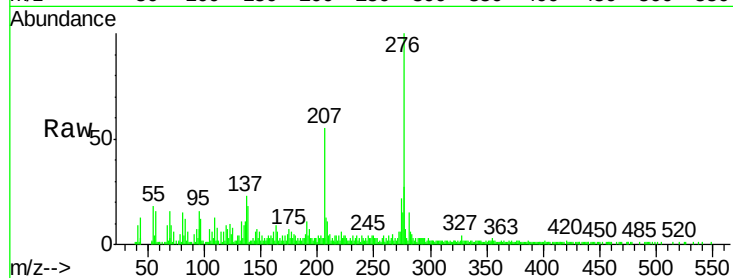

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

