

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG072715\
 Data File : BG018144.D
 Acq On : 28 Jul 2015 12:44
 Operator : TP/UM
 Sample : G3048-06
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C01T3

Quant Time: Jul 28 14:36:49 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG072315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 28 01:54:27 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.51	152	38377	20.00	ng/ul	0.00
18) Naphthalene-d8	10.29	136	181537	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.18	164	113467	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.94	188	241258	20.00	ng/ul	0.00
78) Chrysene-d12	21.14	240	246675	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	242713	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.01	96	2366	3.85	ng/uL	0.00
5) Phenol-d5	6.70	99	67392	22.76	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.85	67	33571	22.97	ng/ul	0.00
9) 2-Chlorophenol-d4	7.04	132	65958	25.12	ng/ul	0.00
13) 4-Methylphenol-d8	8.22	113	62320	23.74	ng/ul	0.00
19) Nitrobenzene-d5	8.66	128	34170	23.81	ng/ul	0.00
22) 2-Nitrophenol-d4	9.38	143	35426	23.38	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.91	165	65177	24.71	ng/ul	0.00
29) 4-Chloroaniline-d4	10.43	131	84172	27.43	ng/ul	0.00
44) Dimethylphthalate-d6	13.60	166	194146	24.37	ng/ul	0.00
47) Acenaphthylene-d8	13.87	160	212950	21.76	ng/ul	0.00
52) 4-Nitrophenol-d4	14.40	143	28985	17.29	ng/ul	0.00
58) Fluorene-d10	15.18	176	141590	19.23	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.31	200	11380	7.38	ng/ul	0.00
71) Anthracene-d10	17.03	188	196056	18.76	ng/ul	0.00
79) Pyrene-d10	19.34	212	189369	16.76	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	151701	13.10	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.65	163	65978	8.23	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG072715\
Data File : BG018144.D
Acq On : 28 Jul 2015 12:44
Operator : TP/UM
Sample : G3048-06
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C01T3

Quant Time: Jul 28 14:36:49 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG072315.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 28 01:54:27 2015
Response via : Initial Calibration

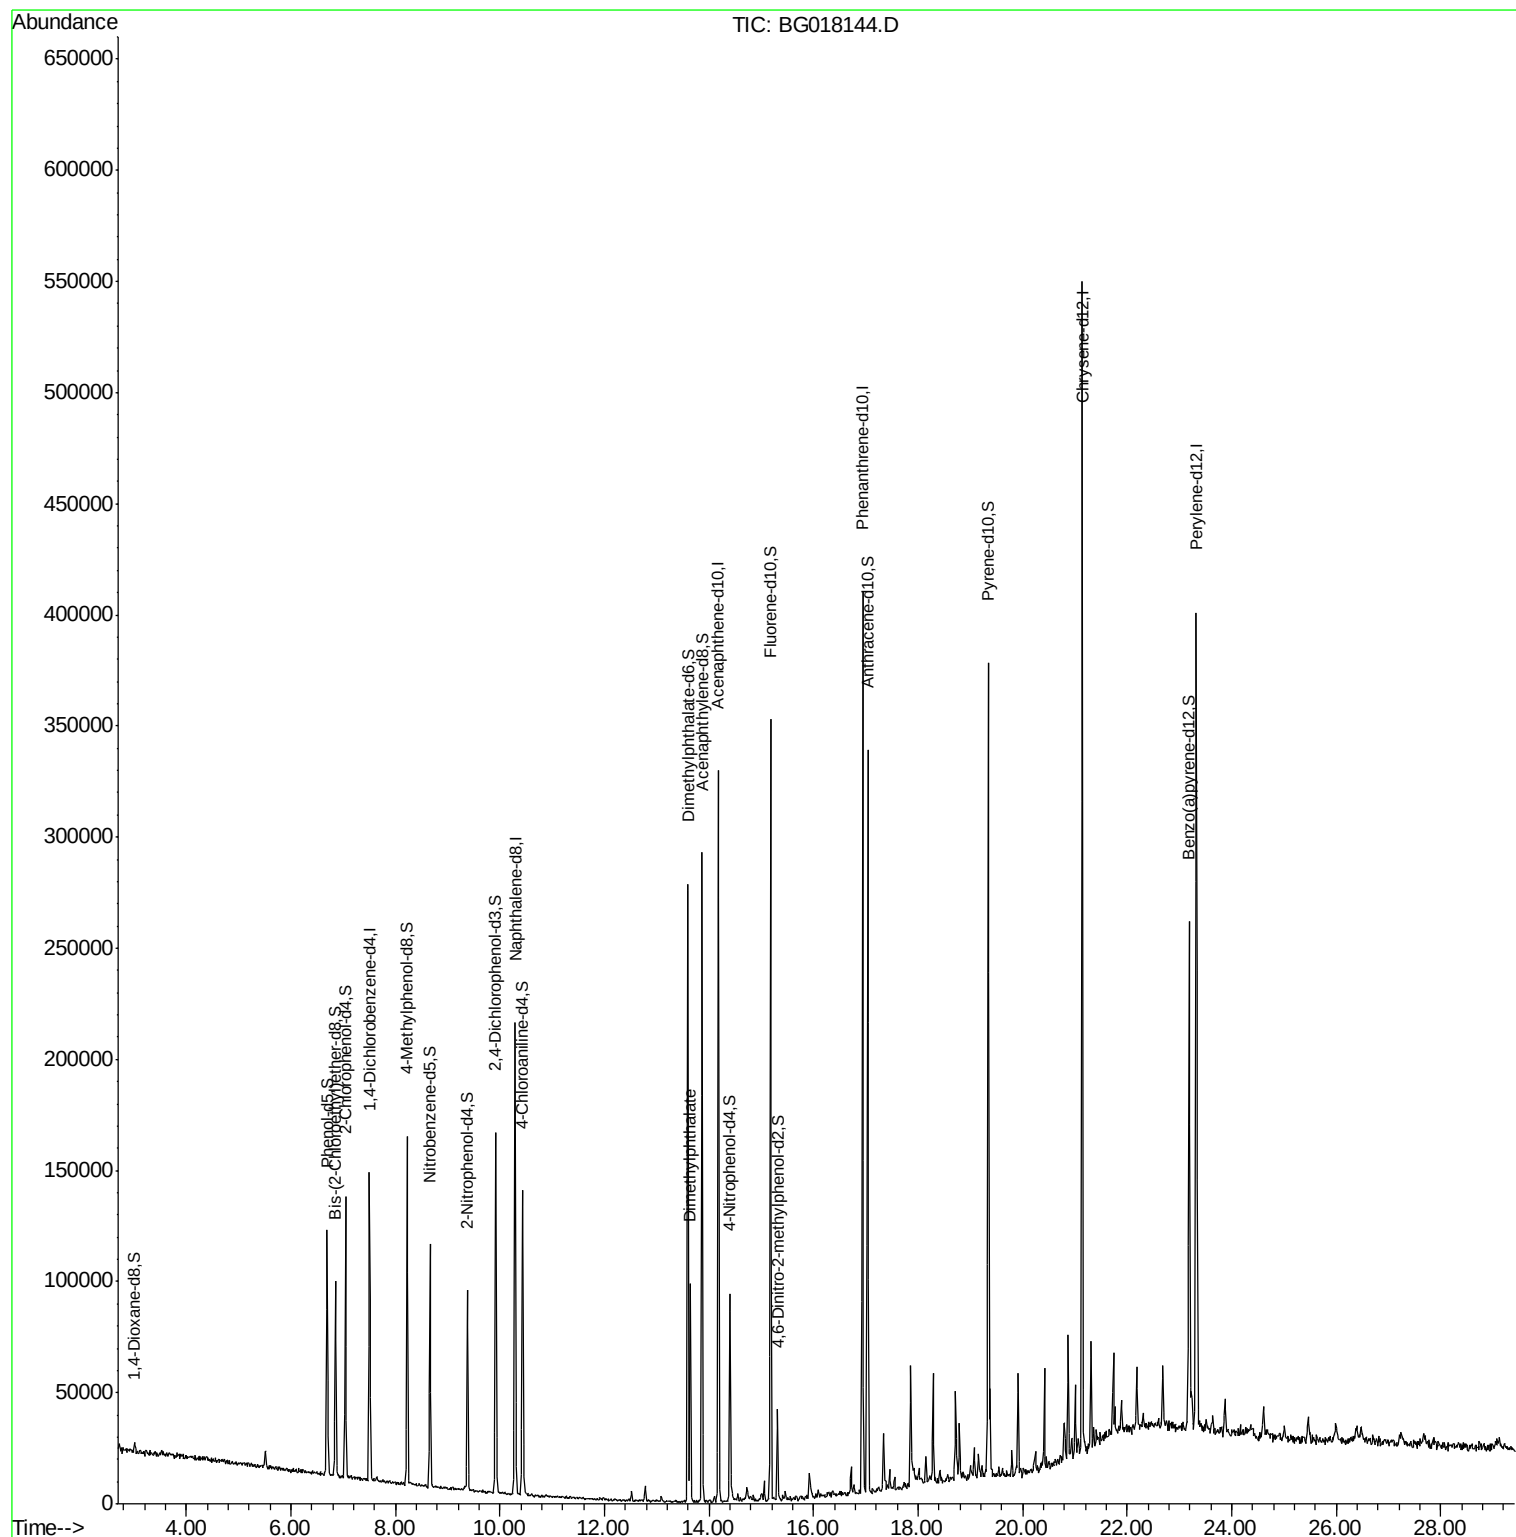

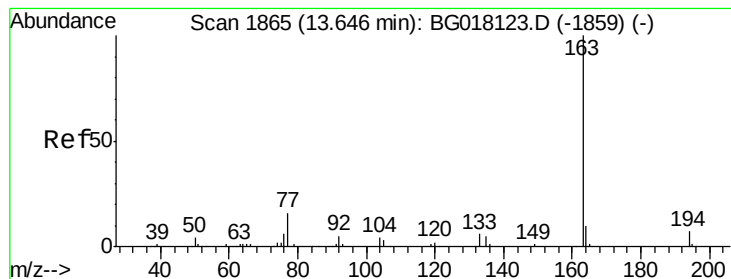

#45
 Dimethylphthalate
 Concen: 8.23 ng/ul
 RT: 13.65 min Scan# 1865
 Delta R.T. 0.00 min
 Lab File: BG018144.D
 Acq: 28 Jul 2015 12:44

Instrument :
 BNA_G
 ClientSampleId :
 C01T3

Tgt Ion:163 Resp: 65978
 Ion Ratio Lower Upper
 163 100
 194 6.7 5.4 8.2
 164 9.5 8.7 13.1

