

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG072715\
 Data File : BG018147.D
 Acq On : 28 Jul 2015 14:29
 Operator : TP/UM
 Sample : G2936-02
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C01T2

Quant Time: Jul 28 15:28:57 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG072315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 28 01:54:27 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.50	152	67732	20.00	ng/ul	0.00
18) Naphthalene-d8	10.29	136	317170	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.18	164	197330	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.93	188	424001	20.00	ng/ul	0.00
78) Chrysene-d12	21.14	240	446396	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	446559	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.01	96	1547	1.43	ng/uL	0.00
5) Phenol-d5	6.69	99	36999	7.08	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.85	67	73578	28.53	ng/ul	0.00
9) 2-Chlorophenol-d4	7.04	132	119677	25.83	ng/ul	0.00
13) 4-Methylphenol-d8	8.22	113	74519	16.08	ng/ul	0.00
19) Nitrobenzene-d5	8.66	128	79110	31.55	ng/ul	0.00
22) 2-Nitrophenol-d4	9.38	143	87796	33.16	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.92	165	139263	30.22	ng/ul	0.00
29) 4-Chloroaniline-d4	10.44	131	3730	0.70	ng/ul	0.00
44) Dimethylphthalate-d6	13.60	166	427016	30.82	ng/ul	0.00
47) Acenaphthylene-d8	13.87	160	571155	33.55	ng/ul	0.00
52) 4-Nitrophenol-d4	14.40	143	17495	6.00	ng/ul	0.00
58) Fluorene-d10	15.18	176	418636	32.69	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.31	200	71860	26.51	ng/ul	0.00
71) Anthracene-d10	17.03	188	613400	33.40	ng/ul	0.00
79) Pyrene-d10	19.34	212	653216	31.94	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	659983	30.97	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) 1,4-Dioxane	3.05	88	14212	12.22	ng/uL	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG072715\
Data File : BG018147.D
Acq On : 28 Jul 2015 14:29
Operator : TP/UM
Sample : G2936-02
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C01T2

Quant Time: Jul 28 15:28:57 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG072315.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 28 01:54:27 2015
Response via : Initial Calibration

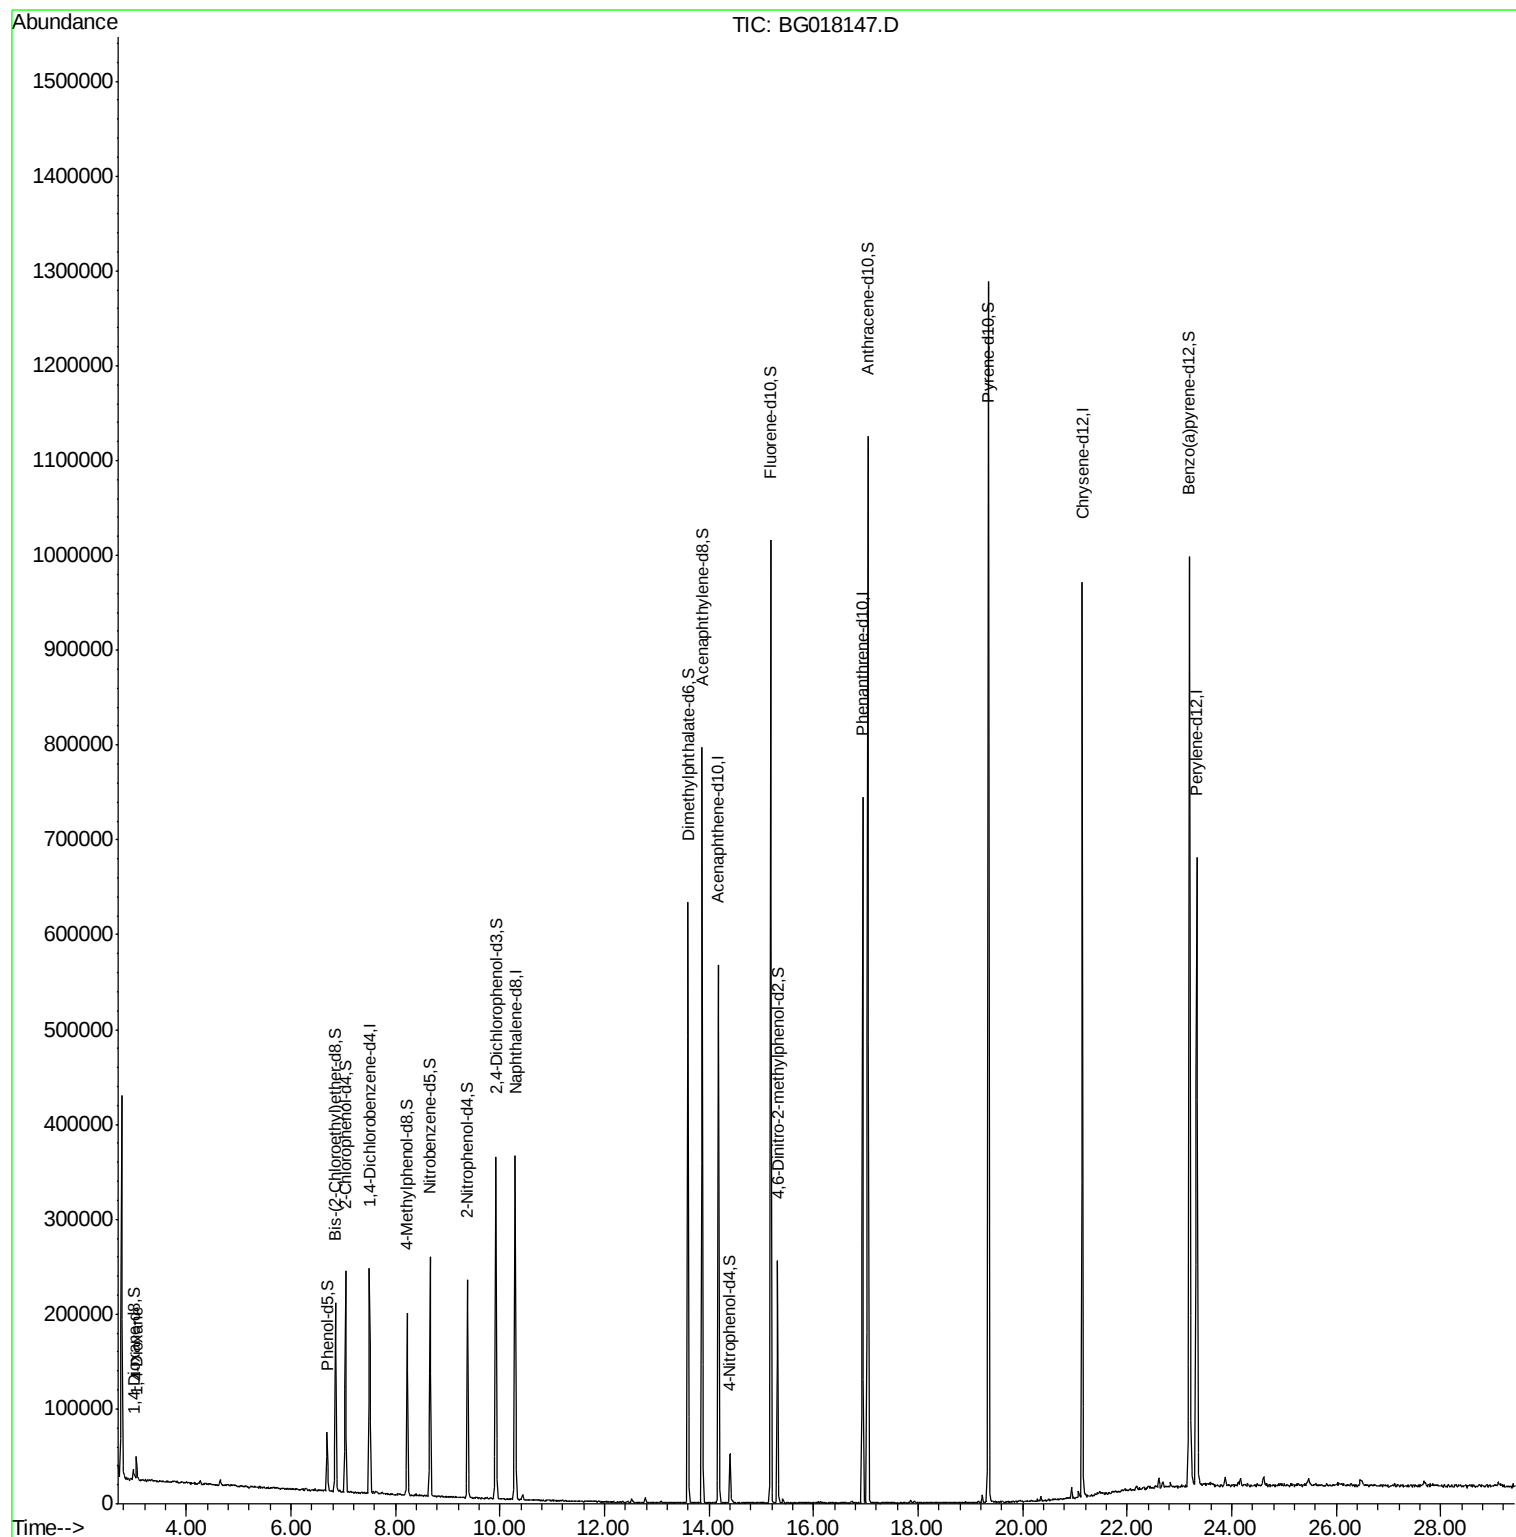

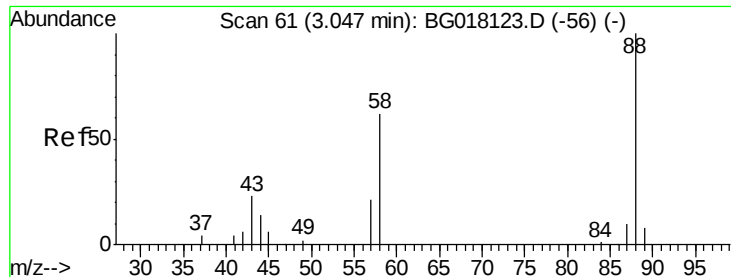

#2
 1,4-Dioxane
 Concen: 12.22 ng/uL
 RT: 3.05 min Scan# 61
 Delta R.T. 0.00 min
 Lab File: BG018147.D
 Acq: 28 Jul 2015 14:29

Instrument :
 BNA_G
 ClientSampleId :
 C01T2

Tgt Ion: 88 Resp: 14212
 Ion Ratio Lower Upper
 88 100
 43 23.3 22.6 33.8
 58 54.5 48.6 73.0

