
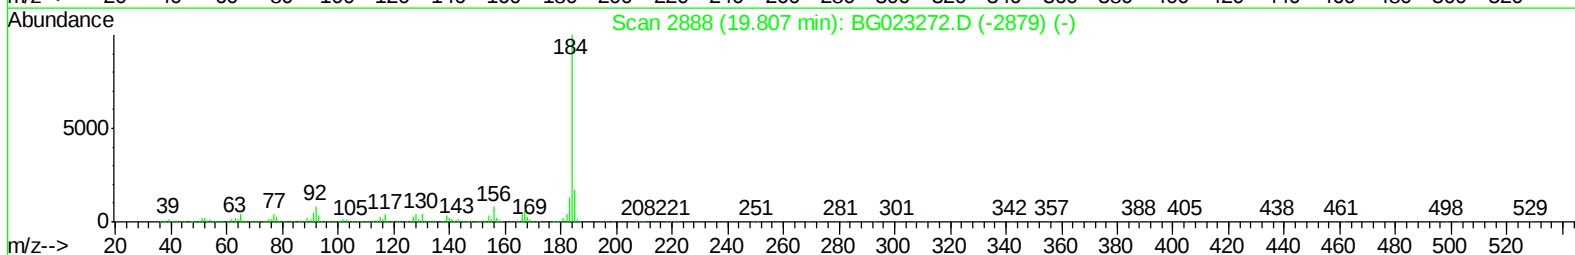
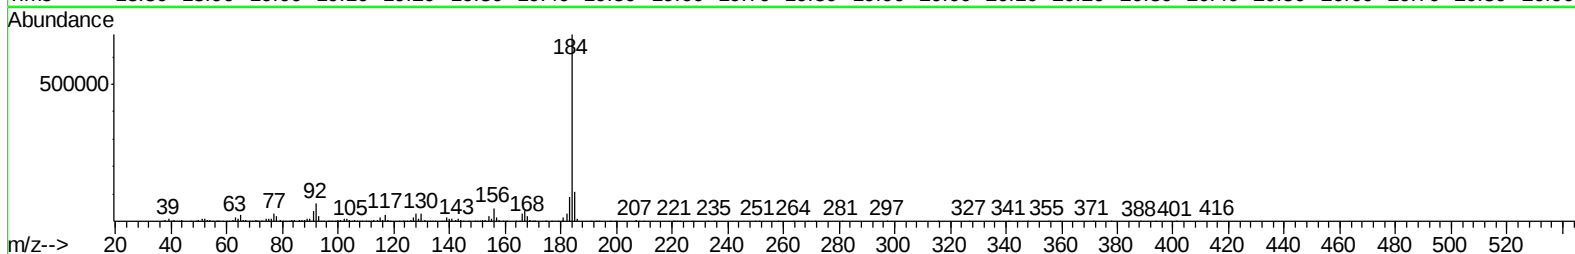


Data Path : Z:\HPCHEM1\BNA_G\Data\BG072716\
Data File : BG023277.D
Acq On : 27 Jul 2016 10:56
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 28 08:34:19 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG072616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 27 17:30:33 2016
Response via : Initial Calibration

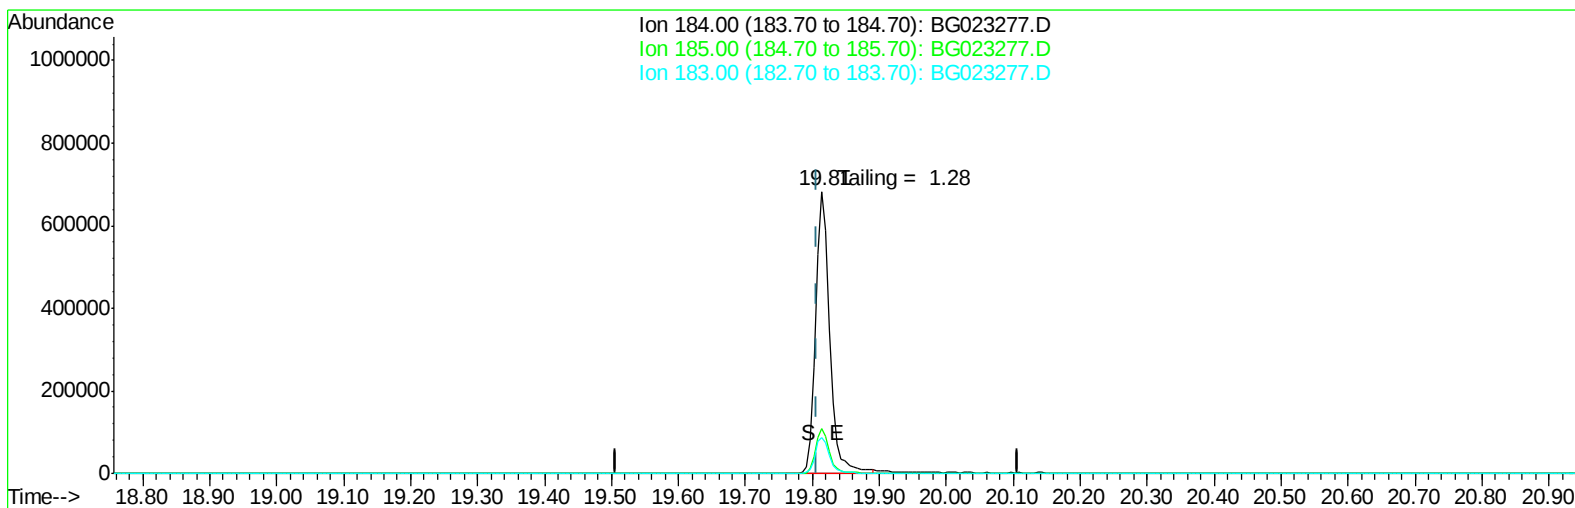

TIC: BG023277.D

(76) Benzidine




19.814min (+0.007) 32188.69ng

response 1038422

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	15.81
183.00	13.40	12.97
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG072716\
Data File : BG023277.D
Acq On : 27 Jul 2016 10:56
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 28 08:34:19 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG072616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 27 17:30:33 2016
Response via : Initial Calibration

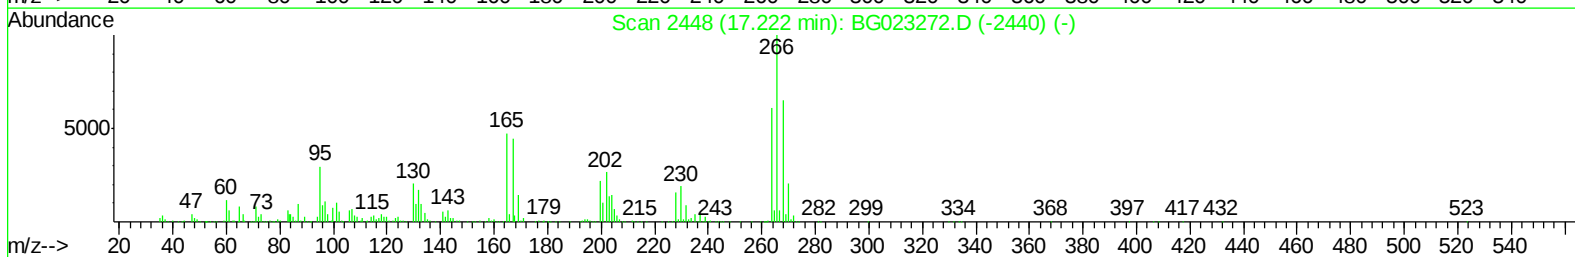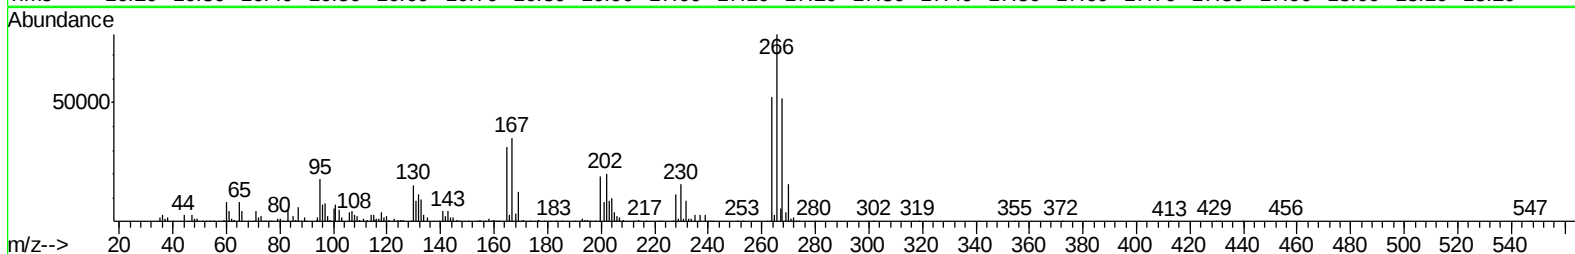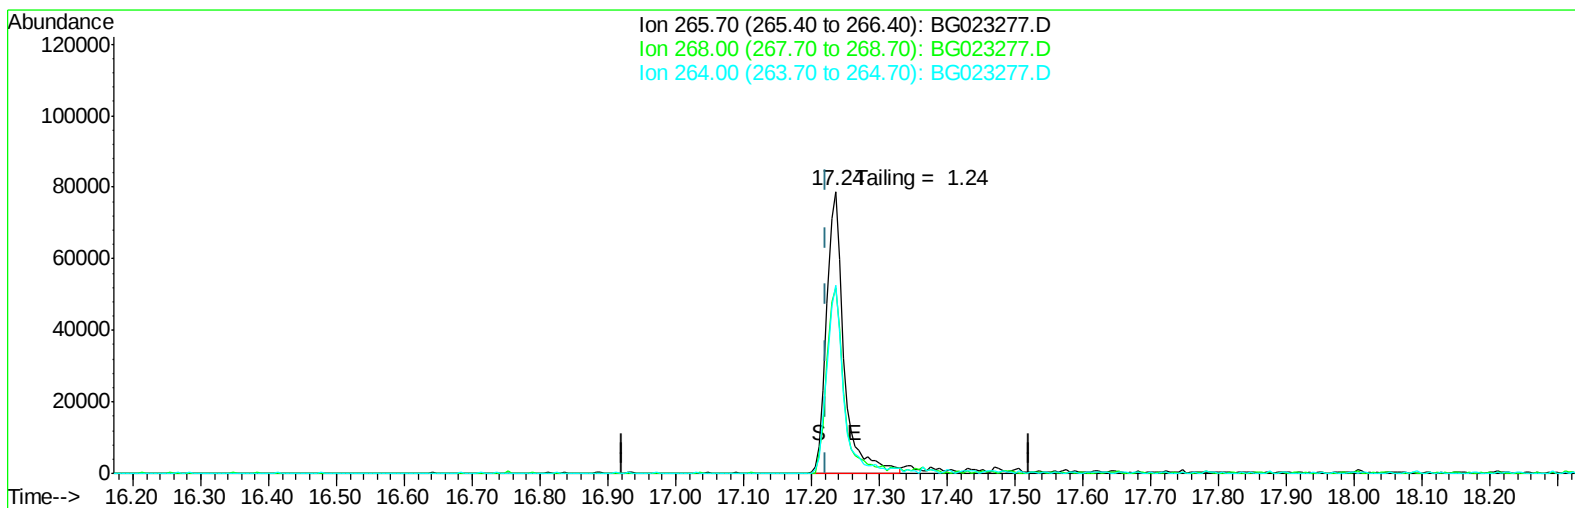

TIC: BG023277.D

(69) Pentachlorophenol (C)

17.235min (+0.014) 403710.66ng

response 139319

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	65.77
264.00	63.20	66.76
0.00	0.00	0.00