


Data Path : Z:\HPCHEM1\BNA G\DATA\BG072716\
 Data File : BG023277.D
 Acq On : 27 Jul 2016 10:56
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG072616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 27 17:30:33 2016

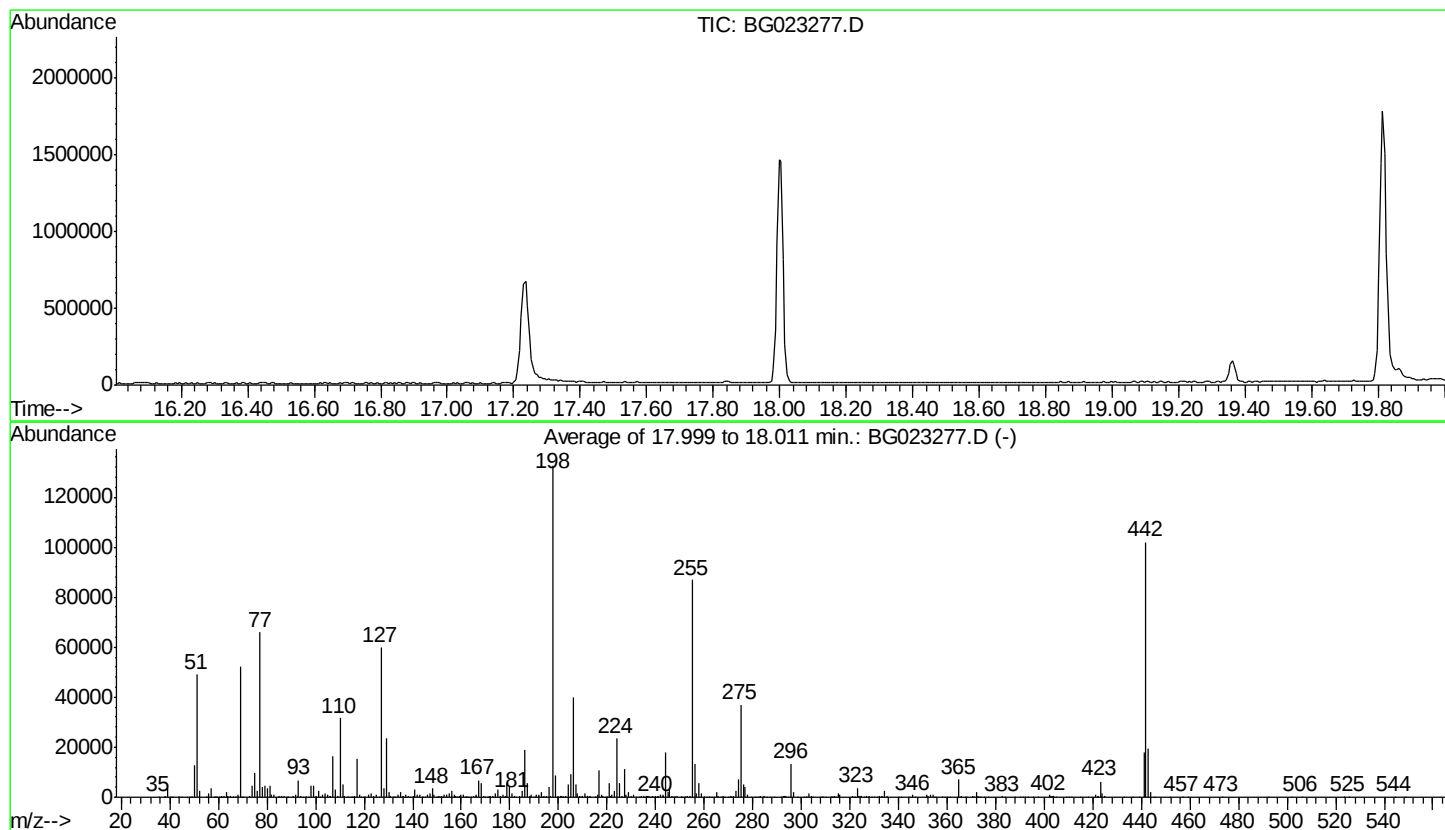

AutoFind: Scans 2581, 2582, 2583; Background Corrected with Scan 2574

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.9	48941	PASS
68	69	0.00	2	2.0	1026	PASS
69	198	0.00	100	39.6	52461	PASS
70	69	0.00	2	0.5	252	PASS
127	198	10	80	45.0	59693	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	132552	PASS
199	198	5	9	6.5	8623	PASS
275	198	10	60	27.9	36920	PASS
365	198	1	100	5.4	7095	PASS
441	442	0.01	24	17.4	17746	PASS
442	198	50	100	76.8	101866	PASS
443	442	15	24	18.9	19284	PASS