


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072722\
 Data File : BG054408.D
 Acq On : 27 Jul 2022 9:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 28 04:30:50 2022

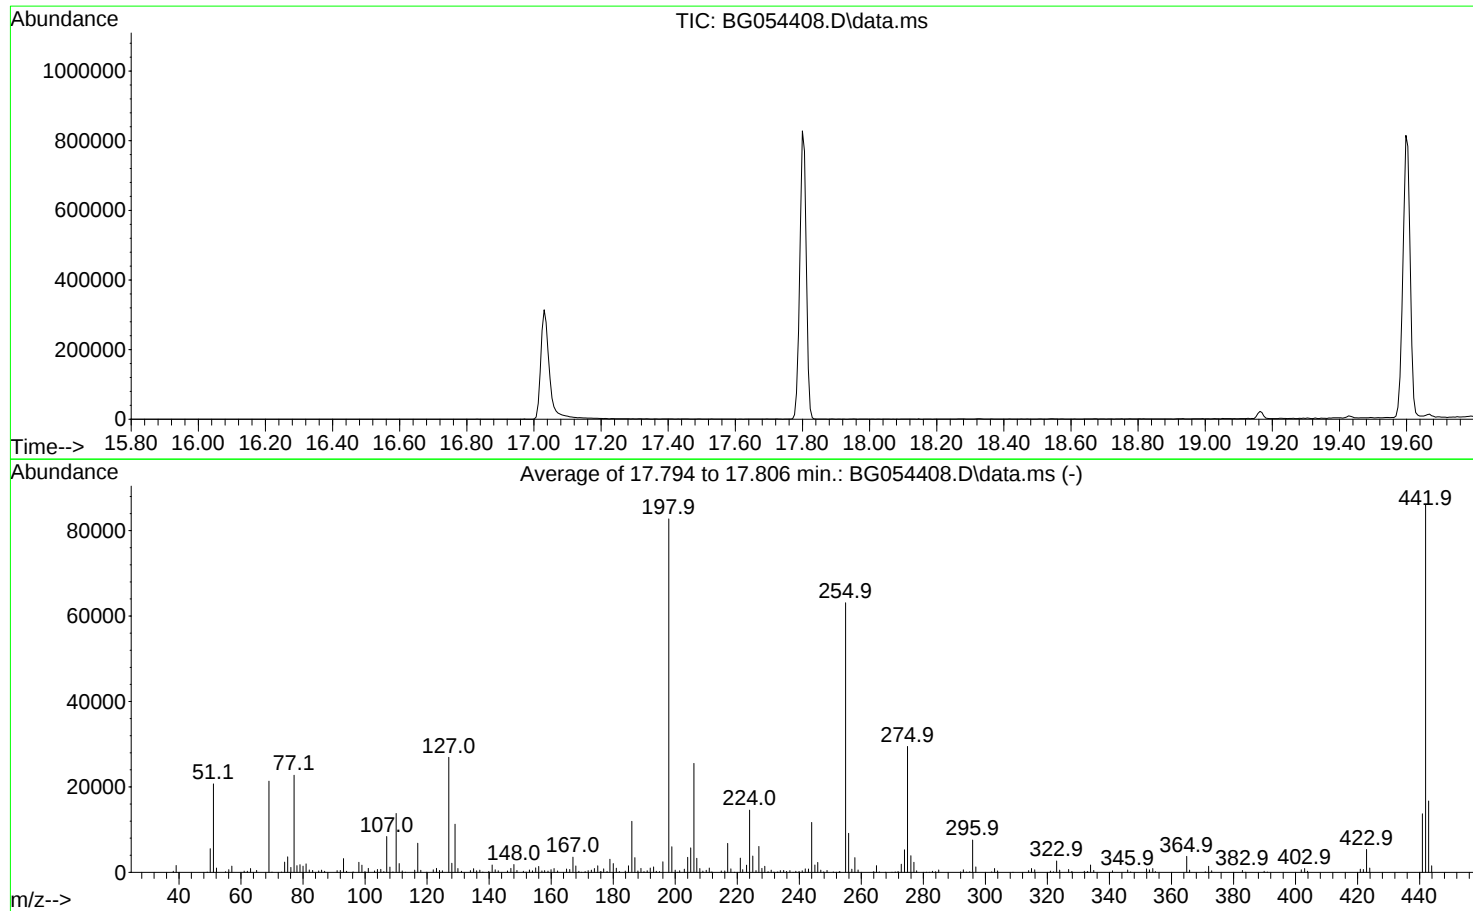




AutoFind: Scans 2520, 2521, 2522; Background Corrected with Scan 2513

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.0	20707	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	25.8	21339	PASS
70	69	0.00	2	0.3	71	PASS
127	198	10	80	32.5	26925	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	82755	PASS
199	198	5	9	7.2	5990	PASS
275	198	10	60	35.6	29472	PASS
365	198	1	100	4.5	3741	PASS
441	198	0.01	100	16.6	13726	PASS
442	442	50	100	100.0	86120	PASS
443	442	15	24	19.4	16718	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072722\
Data File : BG054408.D
Acq On : 27 Jul 2022 9:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 28 05:54:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 28 04:30:50 2022
Response via : Initial Calibration

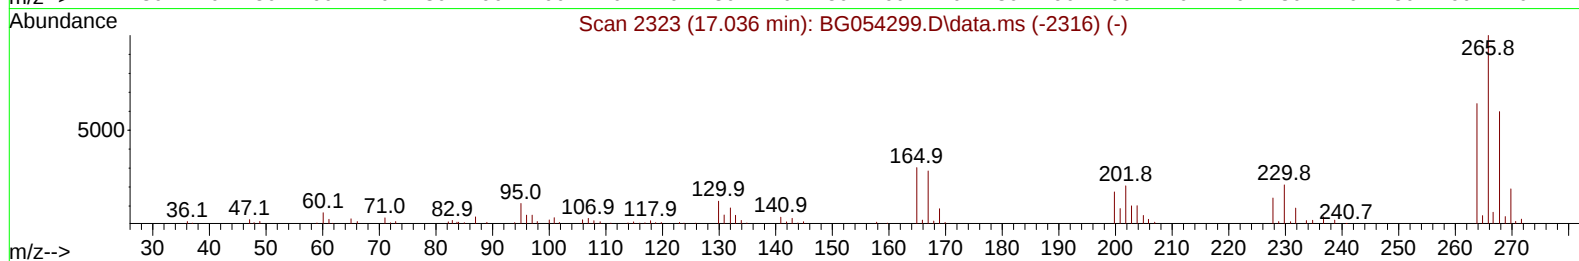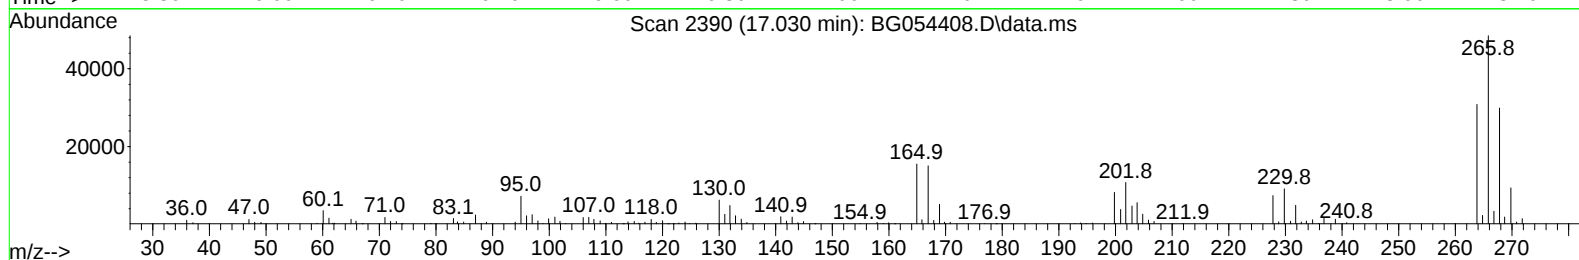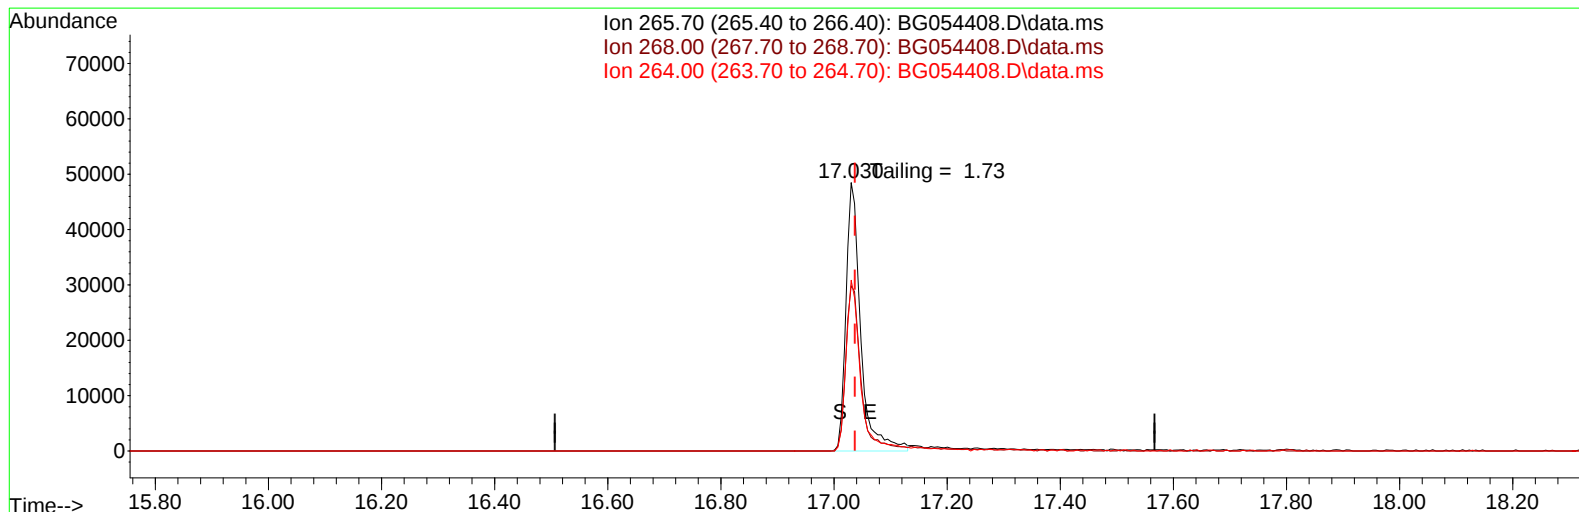

TIC: BG054408.D\data.ms

(70) Pentachlorophenol (C)

17.030min (-0.006) 34880.67 ng




response 89766

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	65.47
264.00	66.20	63.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072722\
Data File : BG054408.D
Acq On : 27 Jul 2022 9:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 28 05:54:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 28 04:30:50 2022
Response via : Initial Calibration

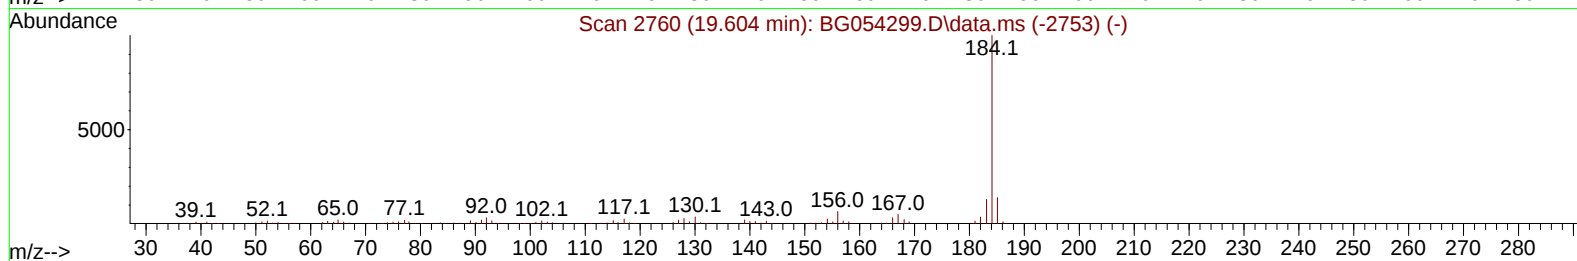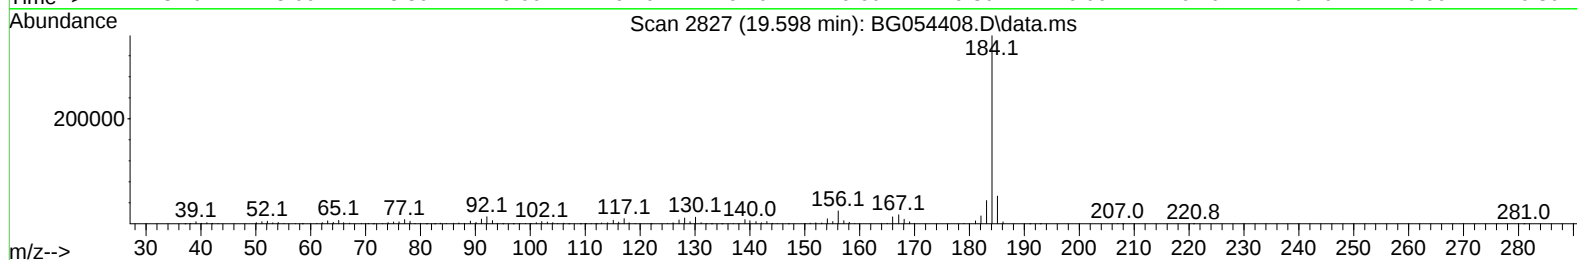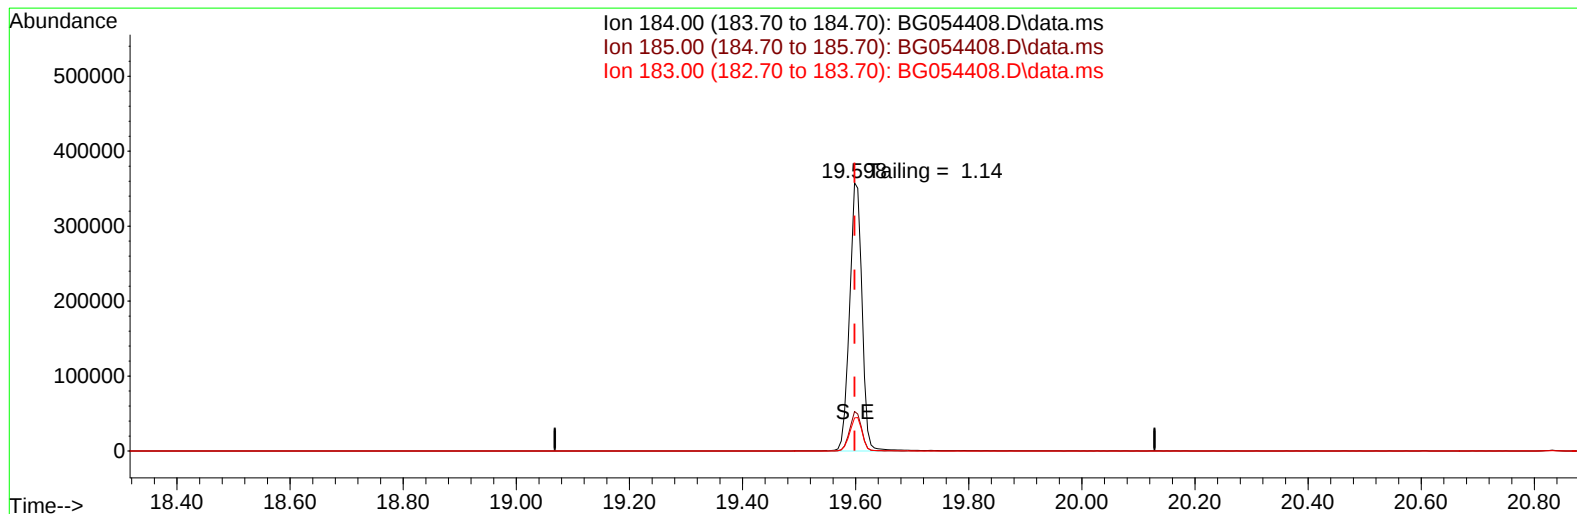

TIC: BG054408.D\data.ms

(77) Benzidine

19.598min (-0.000) 443209.09 ng

response 545826

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.73
183.00	11.10	12.34
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/27/2022	BNA_G	BG054408.D
Compound Name	Response	Retention Time
DDT	314772	20.832
DDD	8660	20.391
DDE	682	19.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9342	324114	2.88

Instrument :
BNA_G
ClientSampleId :
DFTPP