
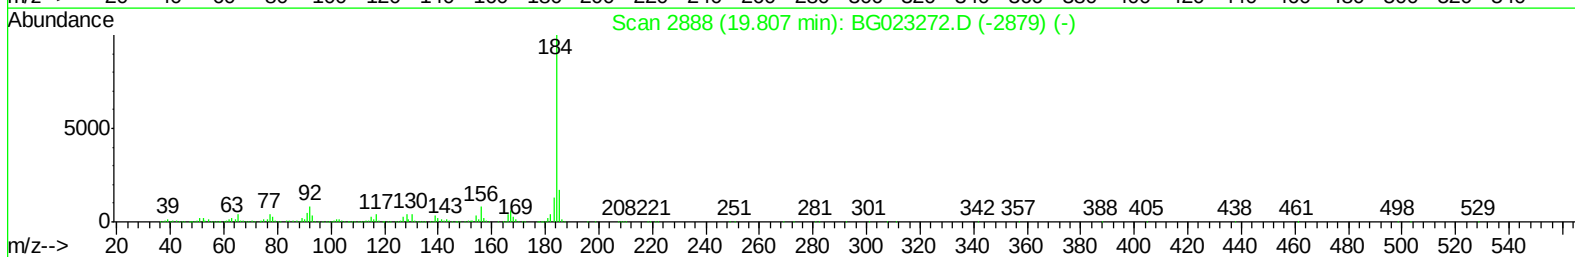
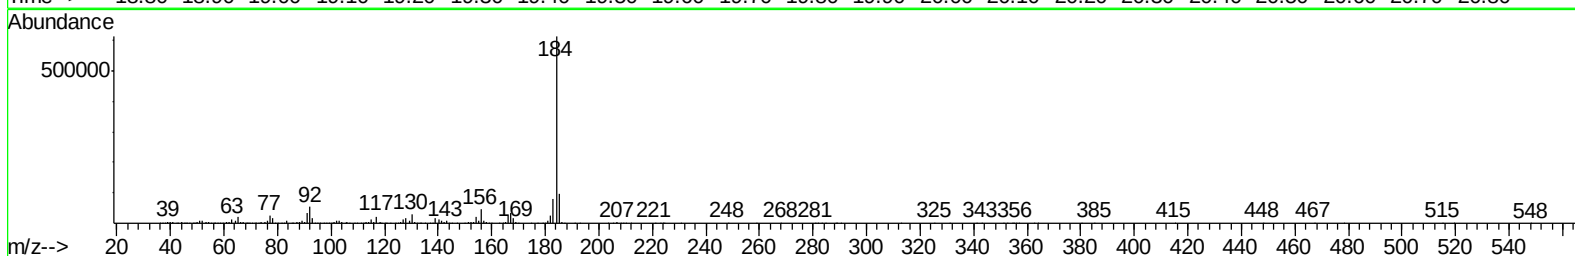


Data Path : Z:\HPCHEM1\BNA_G\Data\BG072816\
Data File : BG023305.D
Acq On : 28 Jul 2016 12:29
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 29 08:02:55 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG072616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 27 17:30:33 2016
Response via : Initial Calibration

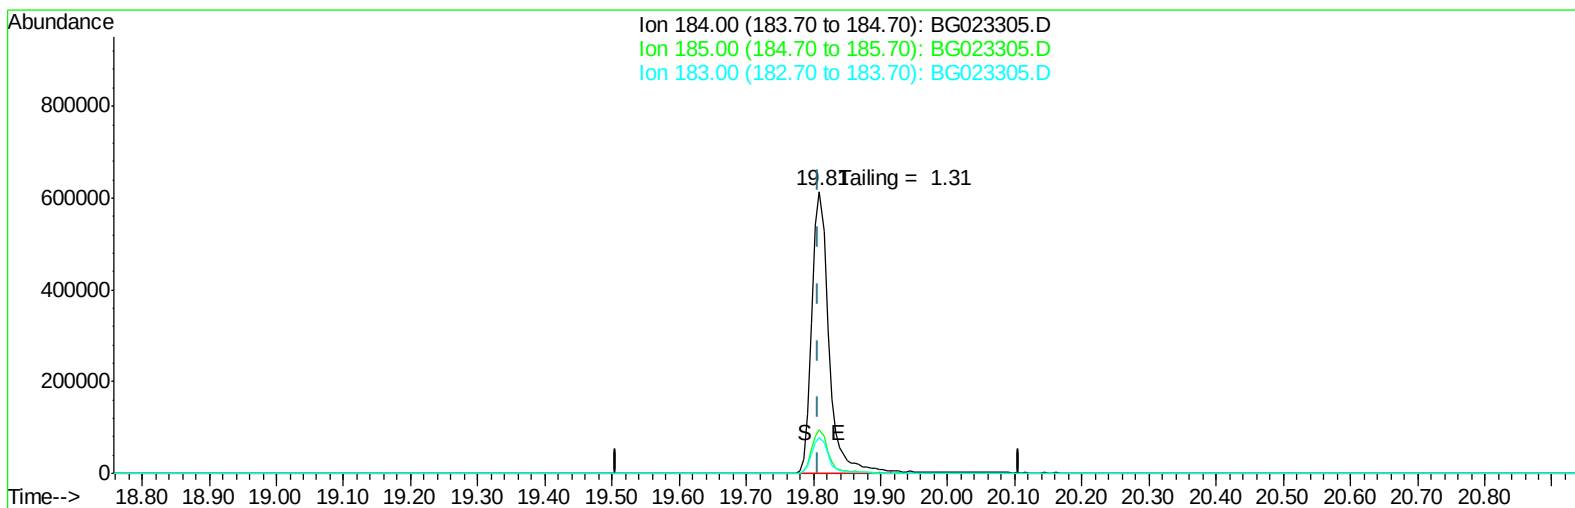

TIC: BG023305.D

(76) Benzidine




19.809min (+0.002) 24438.18ng

response 1069512

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	15.52
183.00	13.40	12.87
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG072816\
Data File : BG023305.D
Acq On : 28 Jul 2016 12:29
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 29 08:02:55 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG072616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 27 17:30:33 2016
Response via : Initial Calibration

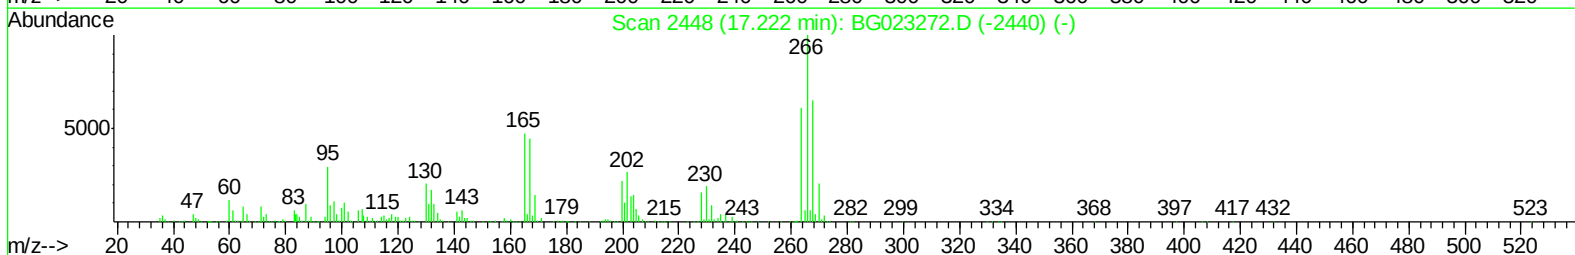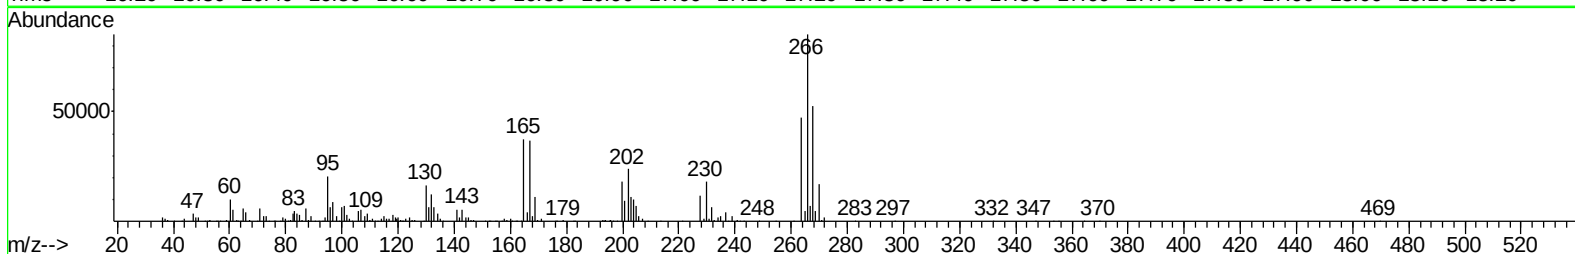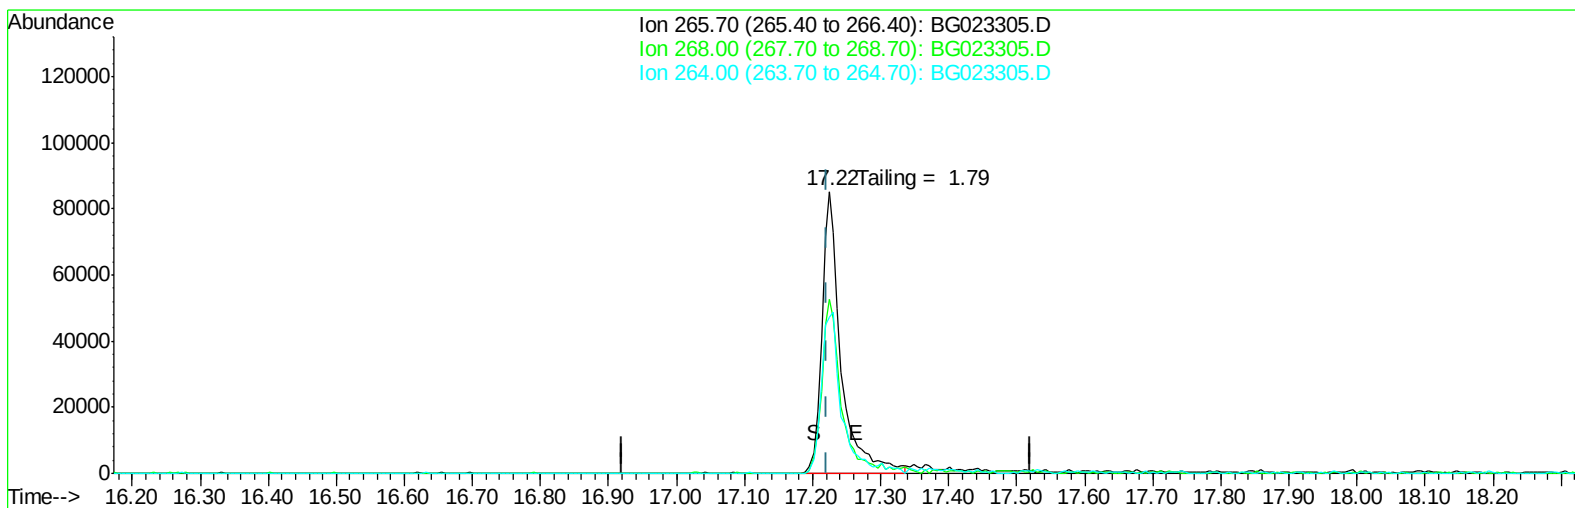

TIC: BG023305.D

(69) Pentachlorophenol (C)

17.225min (+0.004) 48383.95ng

response 166364

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	61.86
264.00	63.20	55.53
0.00	0.00	0.00