


Data Path : Z:\HPCHEM1\BNA G\Data\BG072816\
 Data File : BG023305.D
 Acq On : 28 Jul 2016 12:29
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG072616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 27 17:30:33 2016

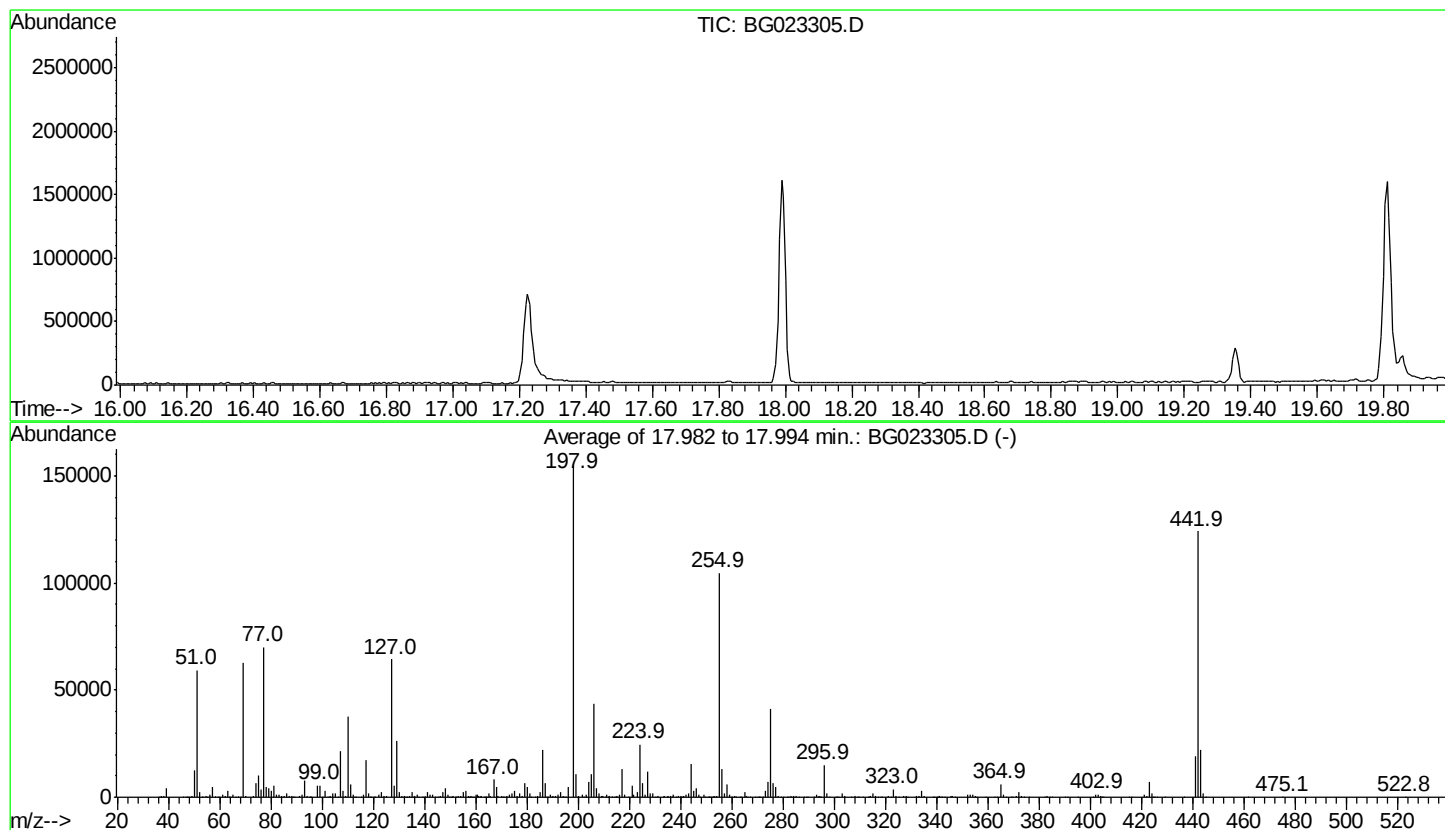

AutoFind: Scans 2578, 2579, 2580; Background Corrected with Scan 2571

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.3	59226	PASS
68	69	0.00	2	0.3	215	PASS
69	198	0.00	100	40.5	62629	PASS
70	69	0.00	2	0.6	389	PASS
127	198	10	80	41.5	64285	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	154760	PASS
199	198	5	9	7.1	11052	PASS
275	198	10	60	26.7	41248	PASS
365	198	1	100	3.9	6086	PASS
441	442	0.01	24	15.3	19028	PASS
442	198	50	100	80.3	124232	PASS
443	442	15	24	17.6	21868	PASS