
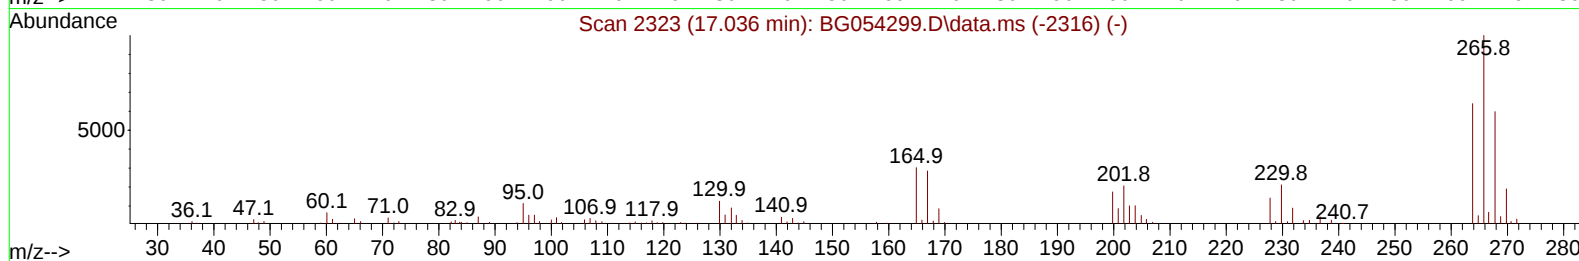
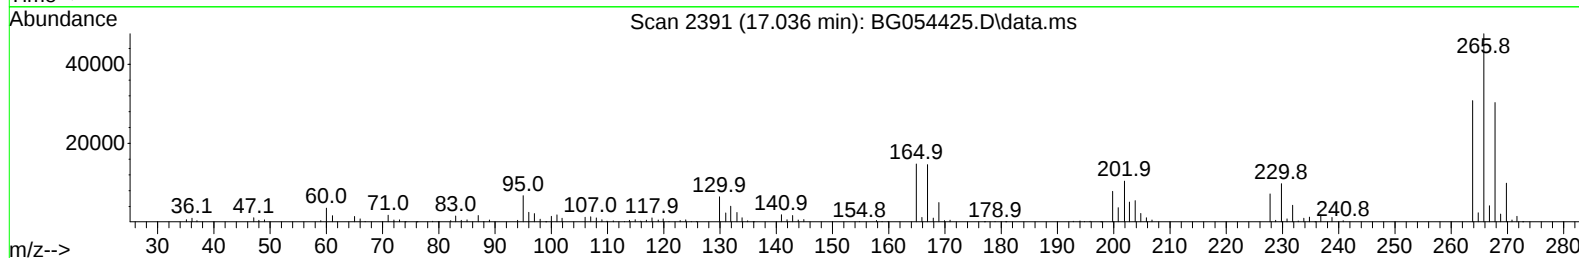


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072822\
Data File : BG054425.D
Acq On : 28 Jul 2022 10:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 29 05:49:30 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 28 04:30:50 2022
Response via : Initial Calibration

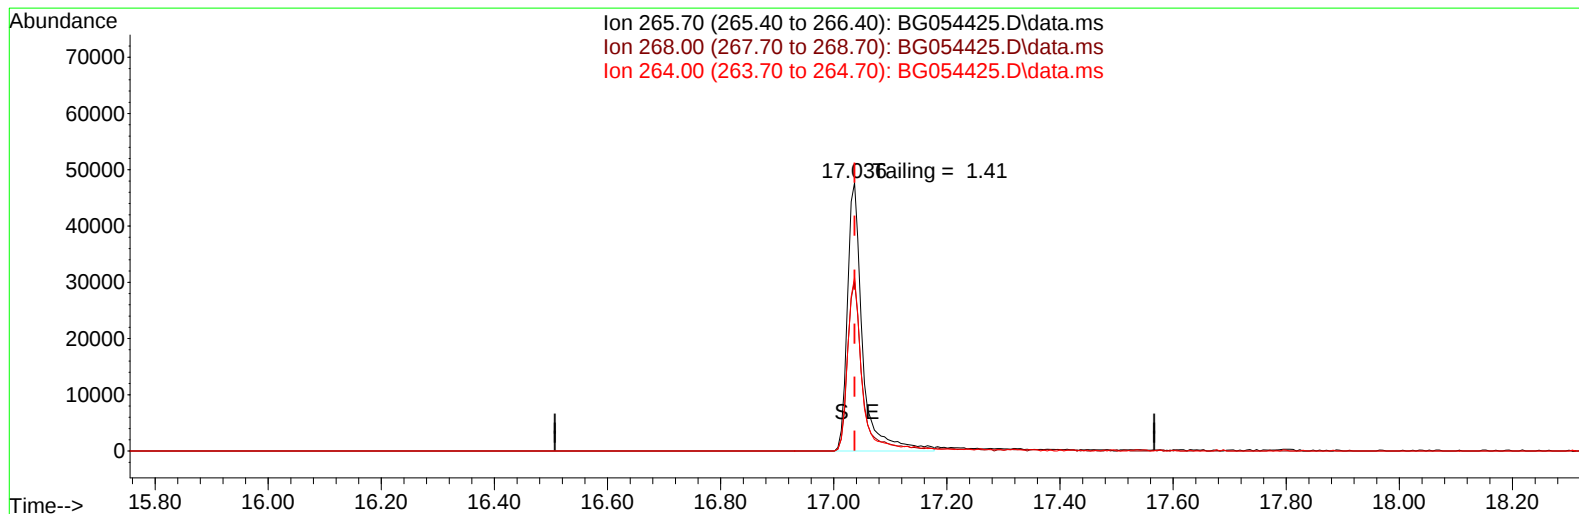

TIC: BG054425.D\data.ms

(70) Pentachlorophenol (C)




17.036min (-0.000) 24888.00 ng

response 89884

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	63.50
264.00	66.20	64.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072822\
 Data File : BG054425.D
 Acq On : 28 Jul 2022 10:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 29 05:49:30 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 28 04:30:50 2022
 Response via : Initial Calibration

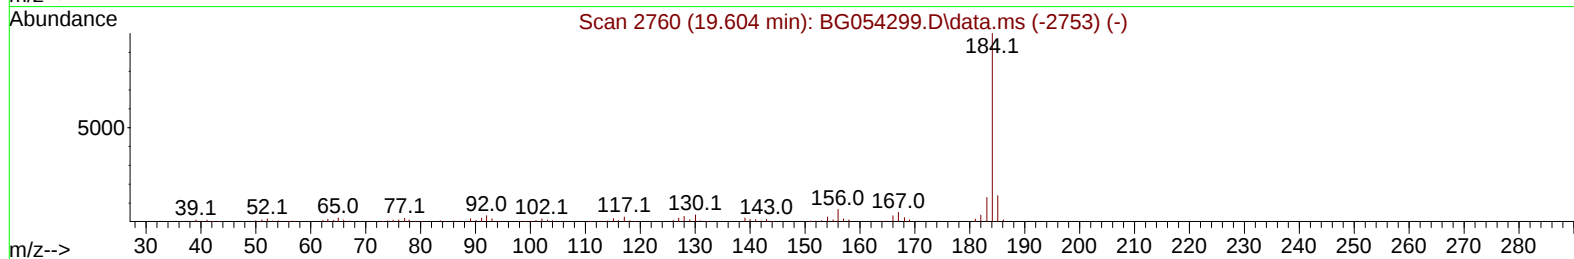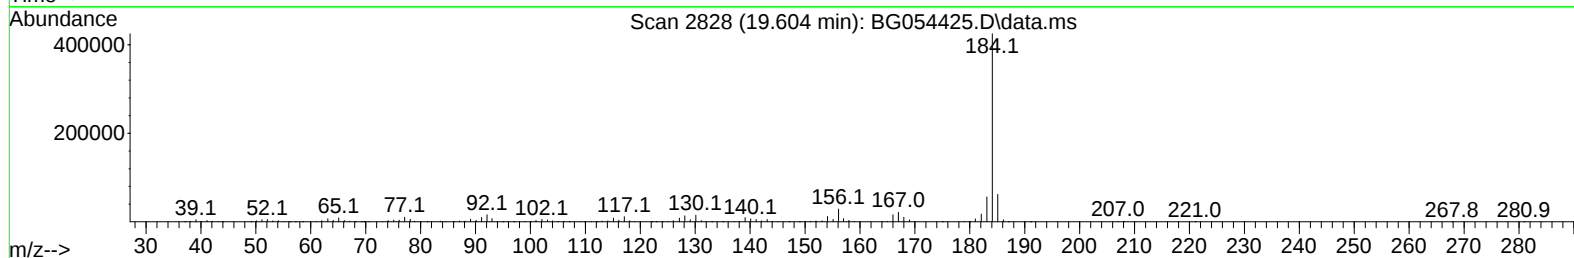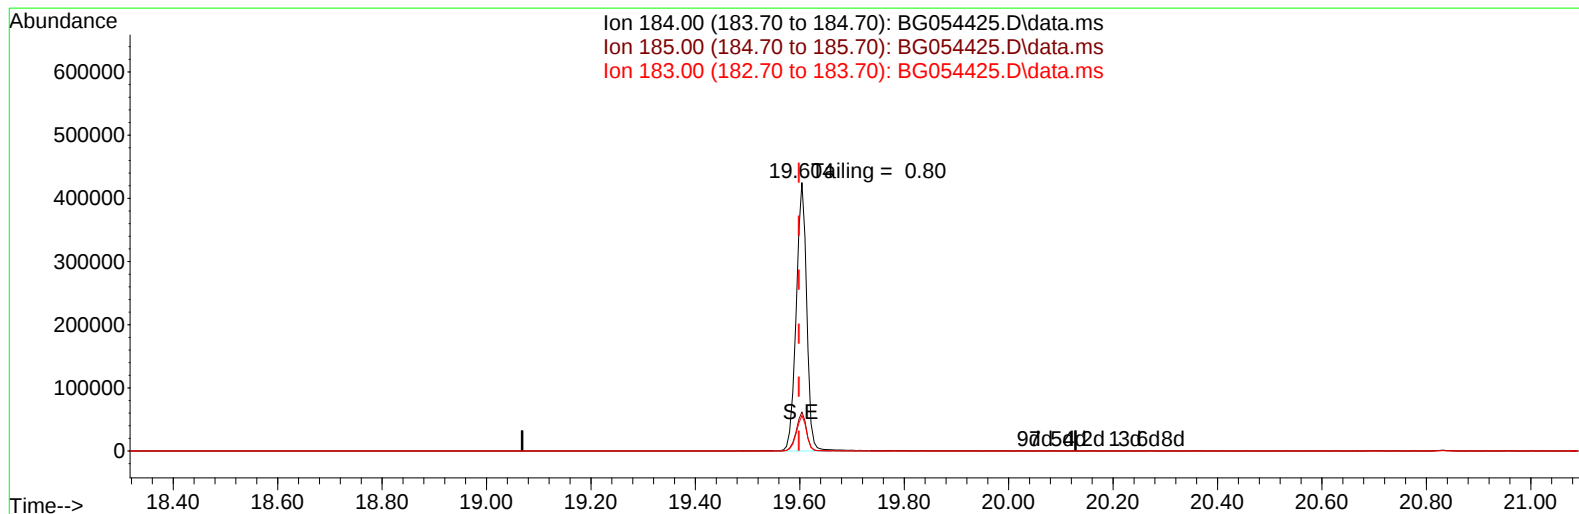

TIC: BG054425.D\data.ms

(77) Benzidine

19.604min (+ 0.006) 494135.10 ng m

response 608543

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.57
183.00	11.10	13.24
0.00	0.00	0.00