


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072822\
 Data File : BG054425.D
 Acq On : 28 Jul 2022 10:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 28 04:30:50 2022

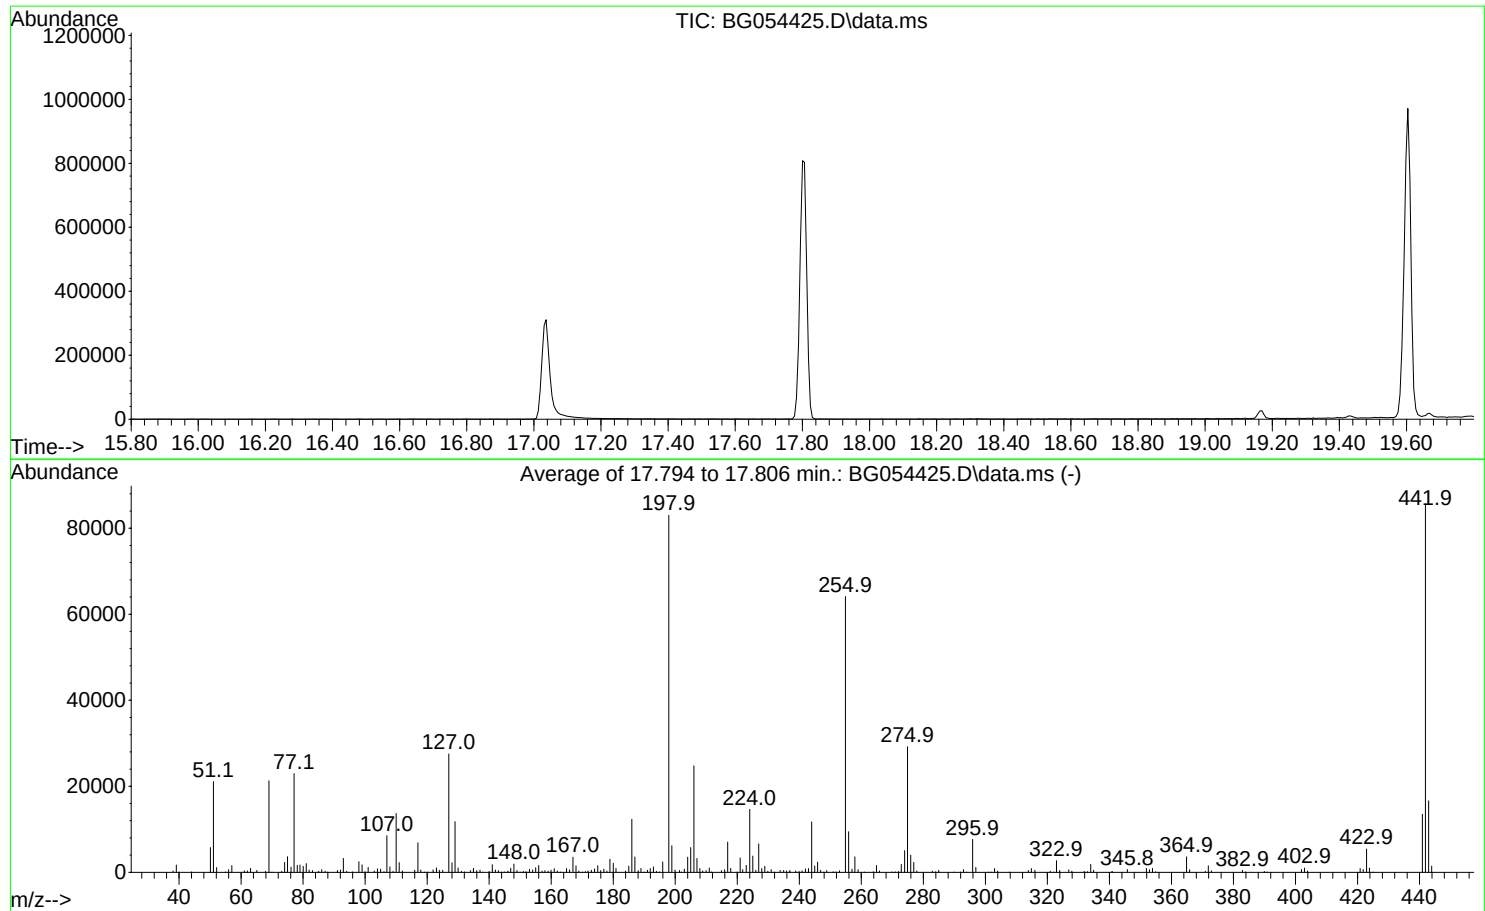




AutoFind: Scans 2520, 2521, 2522; Background Corrected with Scan 2513

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.4	21075	PASS
68	69	0.00	2	1.1	225	PASS
69	198	0.00	100	25.6	21255	PASS
70	69	0.00	2	0.3	60	PASS
127	198	10	80	33.1	27520	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	83043	PASS
199	198	5	9	7.4	6163	PASS
275	198	10	60	35.2	29203	PASS
365	198	1	100	4.3	3606	PASS
441	198	0.01	100	16.3	13496	PASS
442	442	50	100	100.0	85544	PASS
443	442	15	24	19.4	16629	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072822\
 Data File : BG054425.D
 Acq On : 28 Jul 2022 10:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Jul 29 05:49:30 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 28 04:30:50 2022
 Response via : Initial Calibration

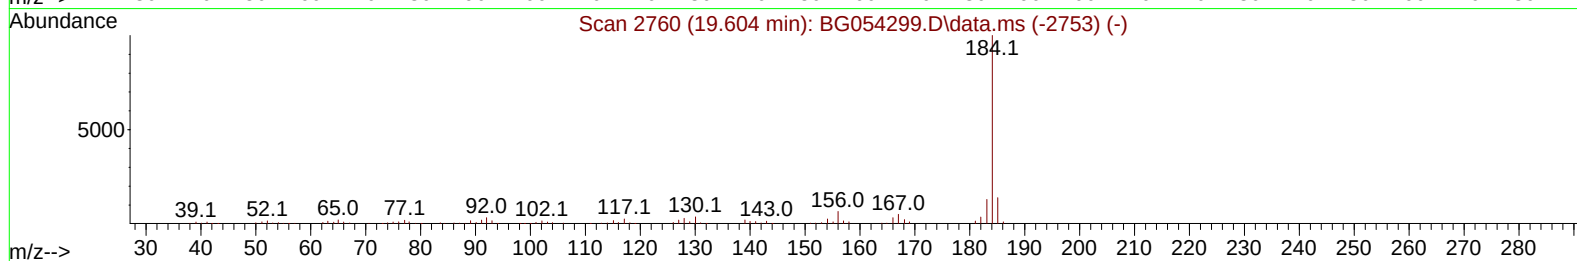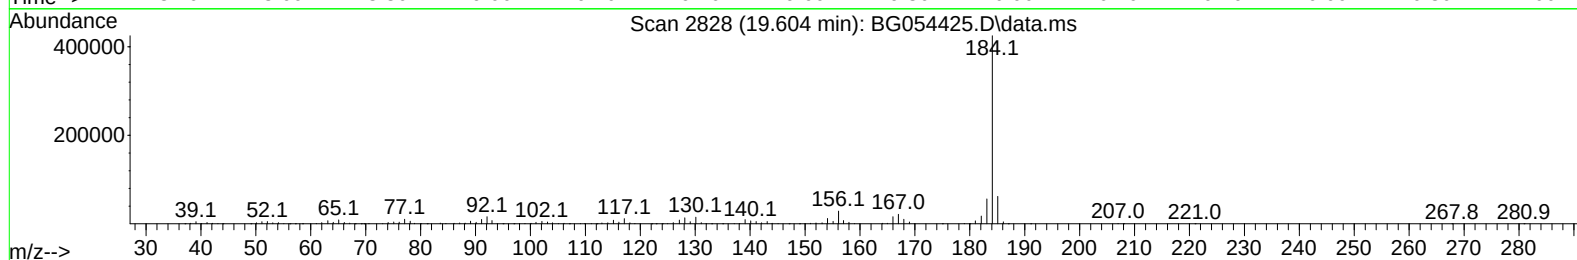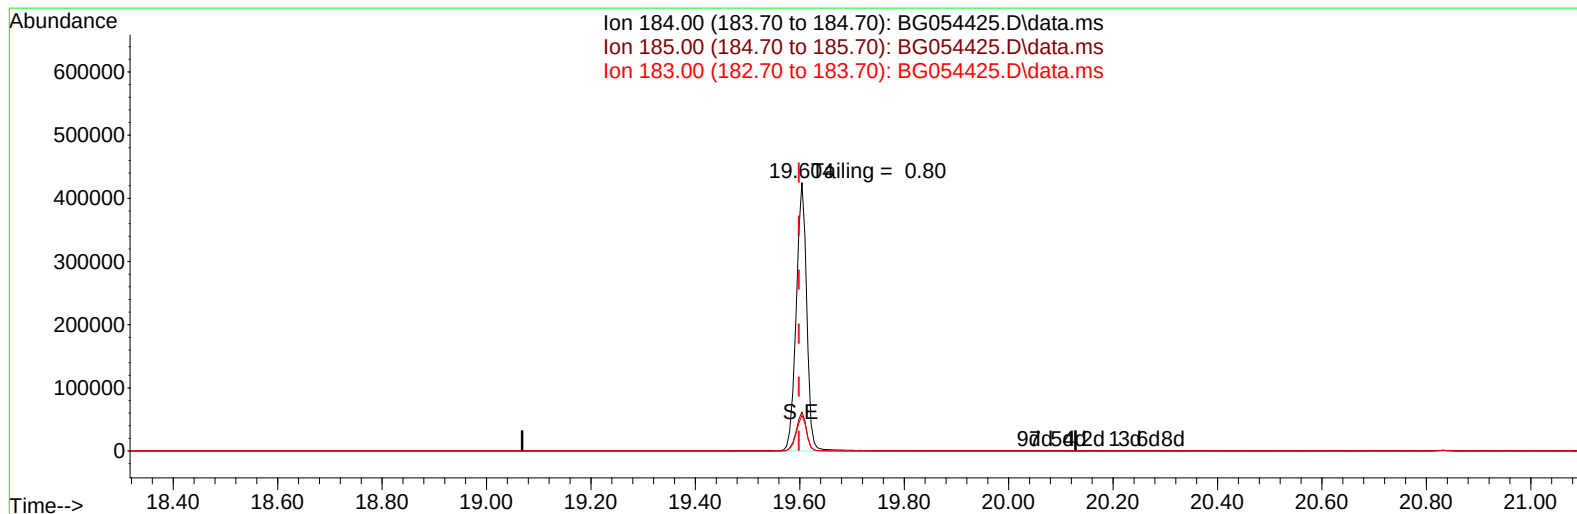

TIC: BG054425.D\data.ms

(77) Benzidine

19.604min (+ 0.006) 494135.10 ng m

response 608543

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.57
183.00	11.10	13.24
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/28/2022	BNA_G	<u>BG054425.D</u>
Compound Name	Response	Retention Time
DDT	336851	20.832
DDD	11180	20.391
DDE	909	19.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12089	348940	3.46

Instrument :
BNA_G
ClientSampleId :
DFTPP